

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100519\
 Data File : PS007038.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Oct 2019 12:37
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 00:56:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
 Quant Title : 8080.M
 QLast Update : Fri Sep 20 11:14:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
Target Compounds							
12) T	2,4,5-T	0.000	7.286	0	15611269	N.D.	7.223
15) T	Picloram	9.020	8.983	108.9E6	59633071	16.242	16.384
16) T	DCPA	0.000	8.983	0	59633071	N.D.	18.767



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100519\
Data File : PS007038.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Oct 2019 12:37
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 00:56:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
Quant Title : 8080.M
QLast Update : Fri Sep 20 11:14:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

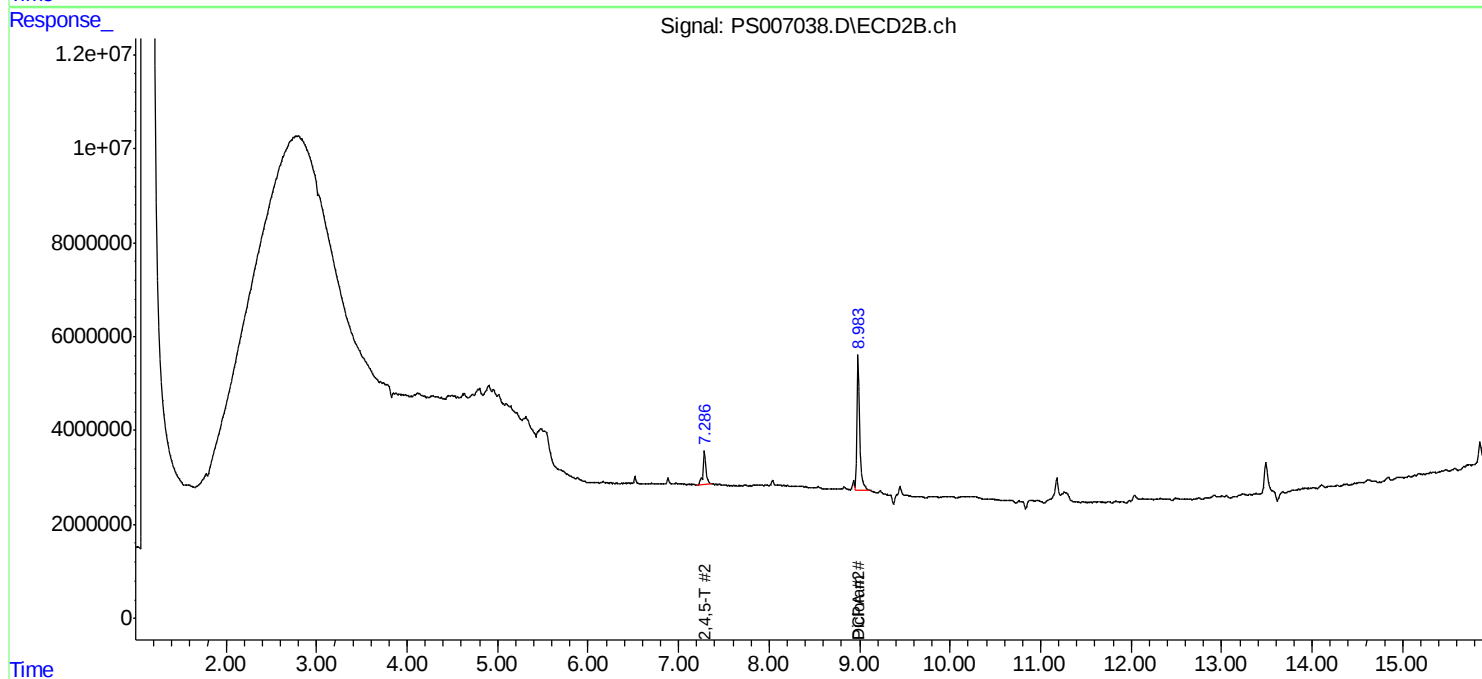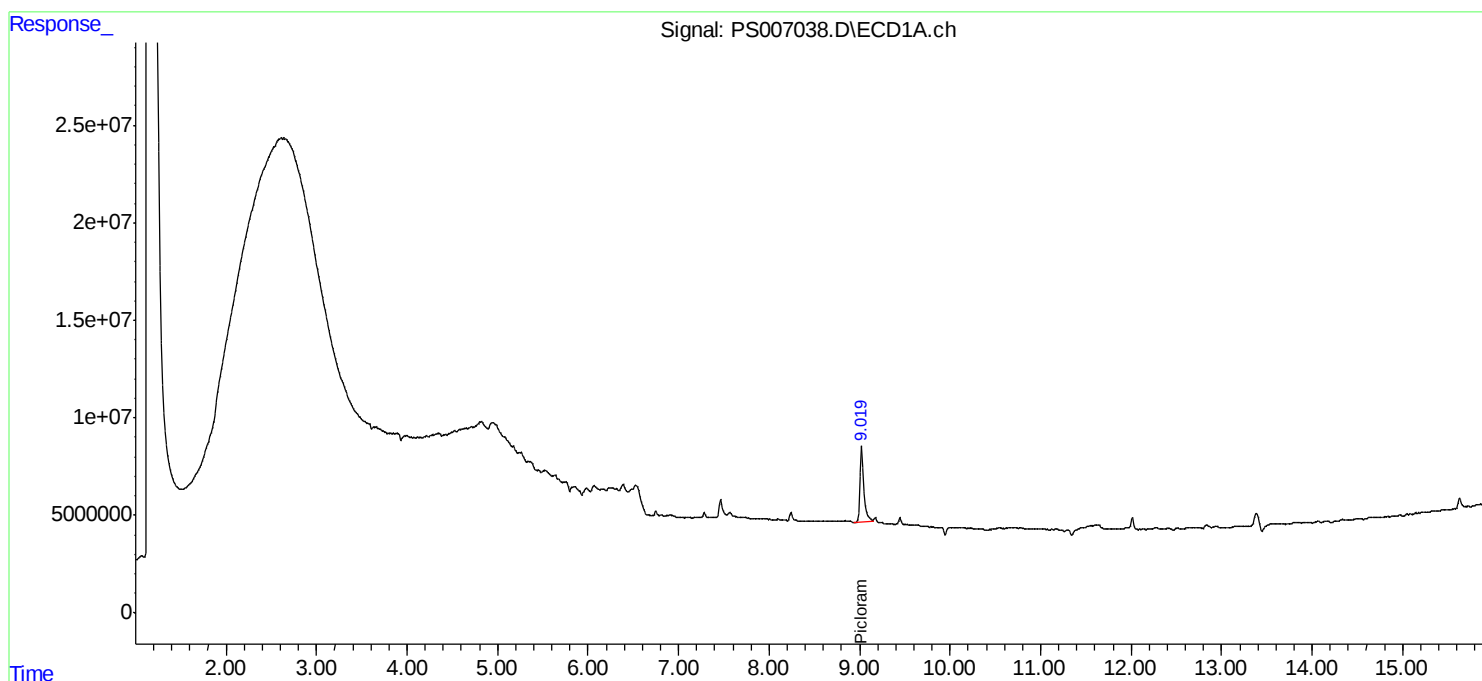


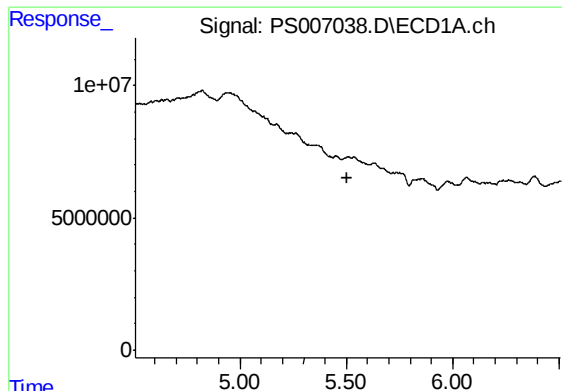

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 5.508 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

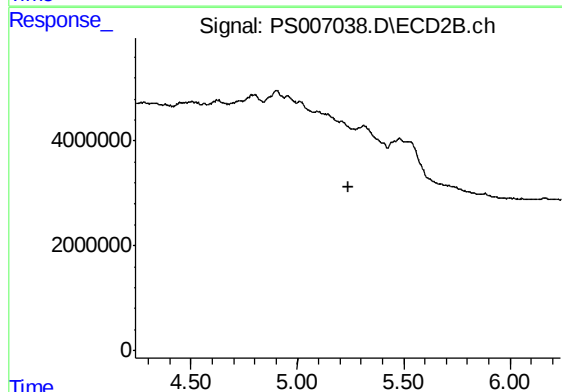


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 5.238 min
Response: 0
Conc: N.D.

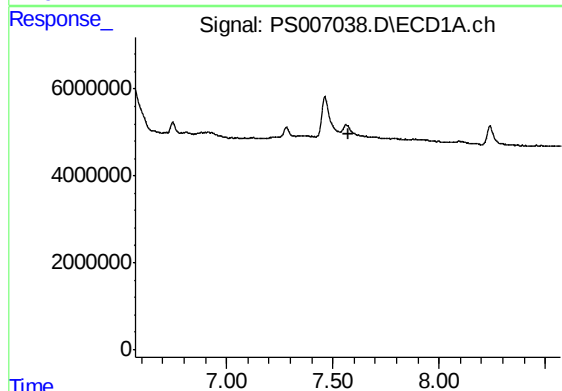


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.572 min
Response: 0
Conc: N.D.

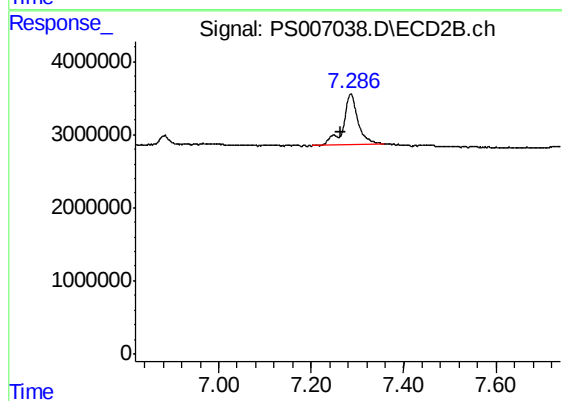

#12 2,4,5-T


R.T.: 7.286 min
Delta R.T.: 0.021 min
Response: 15611269
Conc: 7.22 ng/ml

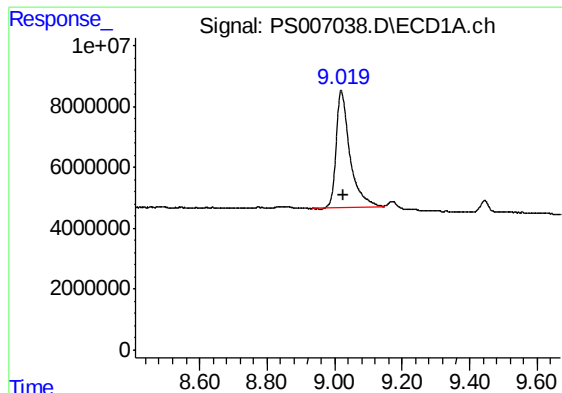

#15 Picloram


R.T.: 9.020 min
Delta R.T.: -0.005 min
Response: 108916559
Conc: 16.24 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

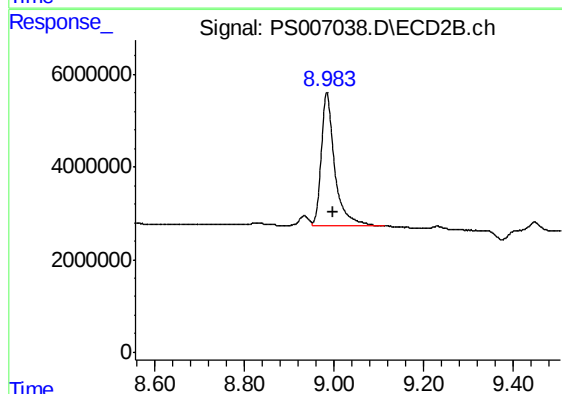


#15 Picloram

R.T.: 8.983 min
Delta R.T.: -0.015 min
Response: 59633071
Conc: 16.38 ng/ml

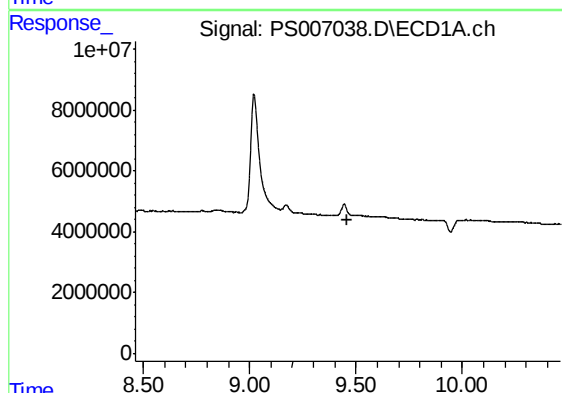

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.462 min
Response: 0
Conc: N.D.

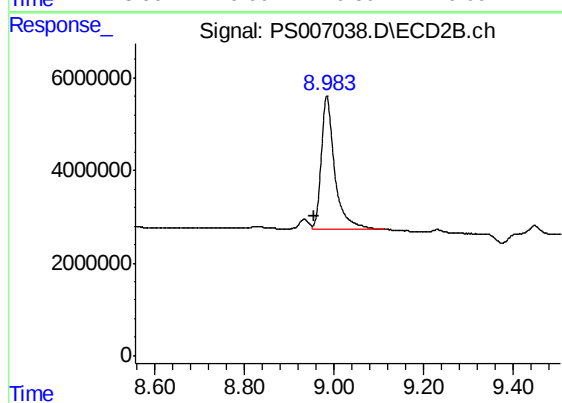

#16 DCPA

R.T.: 8.983 min
Delta R.T.: 0.027 min
Response: 59633071
Conc: 18.77 ng/ml