

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100519\
 Data File : PS007039.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Oct 2019 12:59
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 00:57:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
 Quant Title : 8080.M
 QLast Update : Fri Sep 20 11:14:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.484	5.212	403.0E6	205.8E6	441.017	447.521
Target Compounds							
9) T	2,4-D	6.549	0.000	57626769	0	70.318	N.D. #
15) T	Picloram	9.055	8.997	63551461	35716638	9.477	9.813
16) T	DCPA	0.000	8.997	0	35716638	N.D.	11.241



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100519\
Data File : PS007039.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Oct 2019 12:59
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 00:57:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
Quant Title : 8080.M
QLast Update : Fri Sep 20 11:14:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

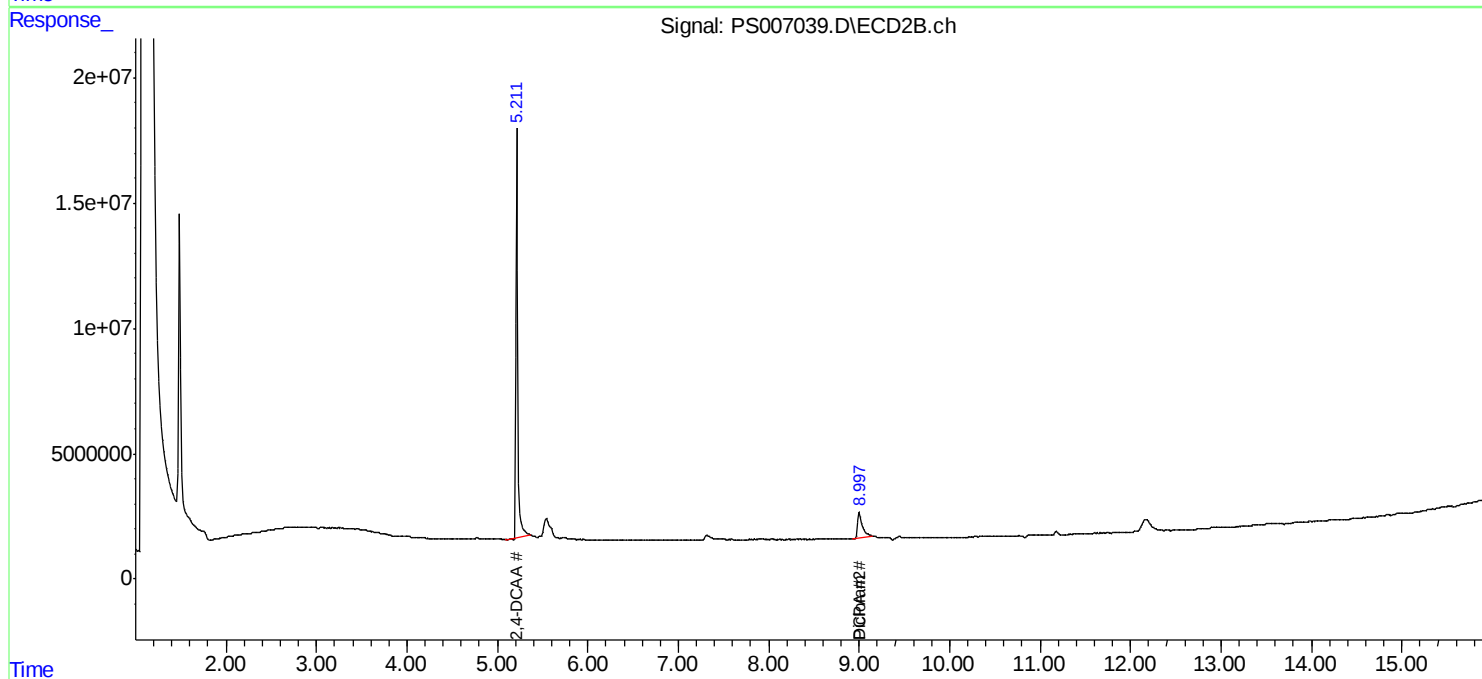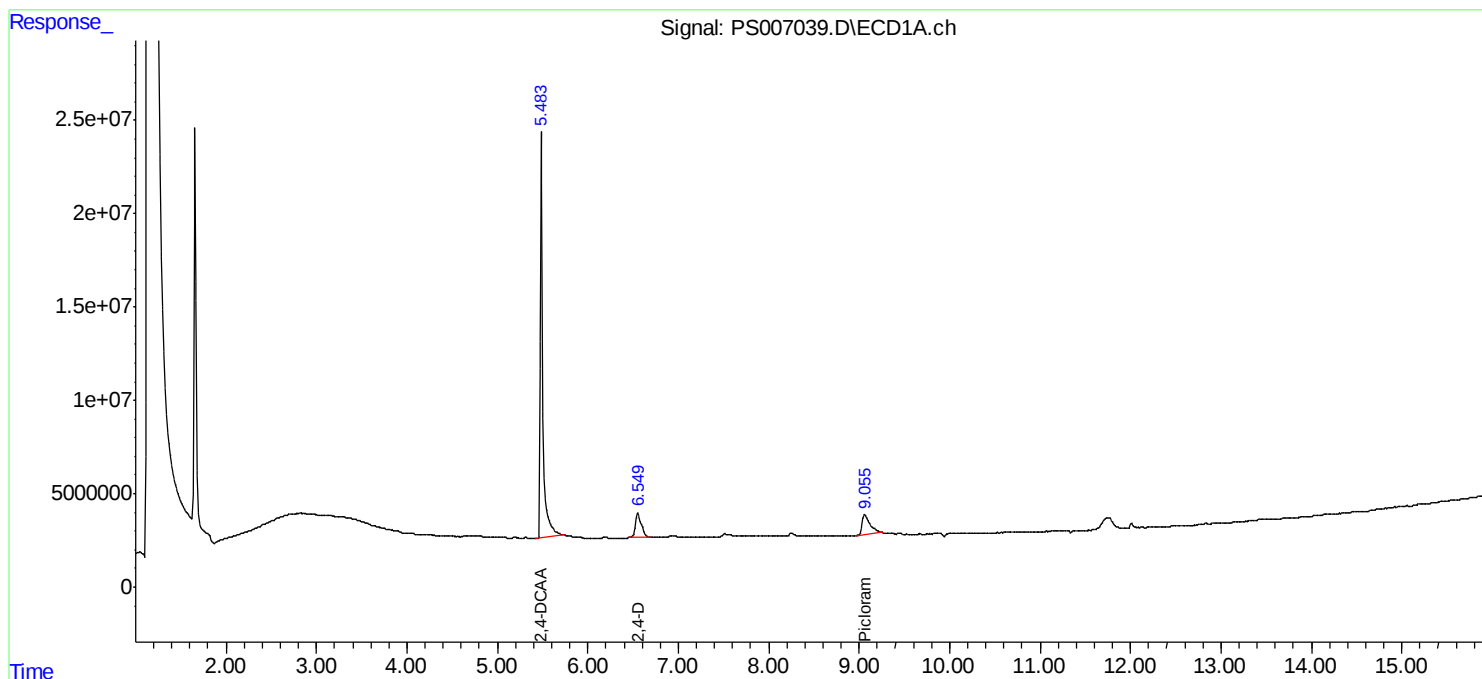


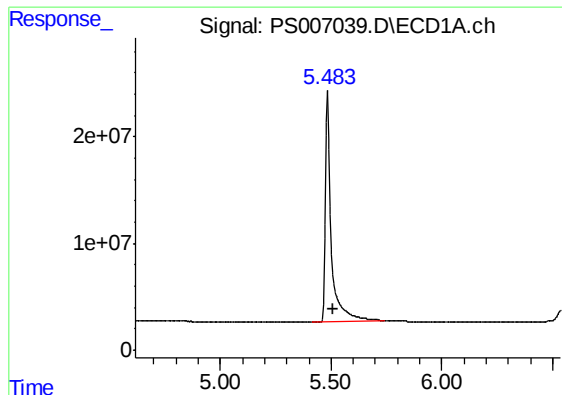

#4 2,4-DCAA


R.T.: 5.484 min
Delta R.T.: -0.024 min
Response: 403007116
Conc: 441.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

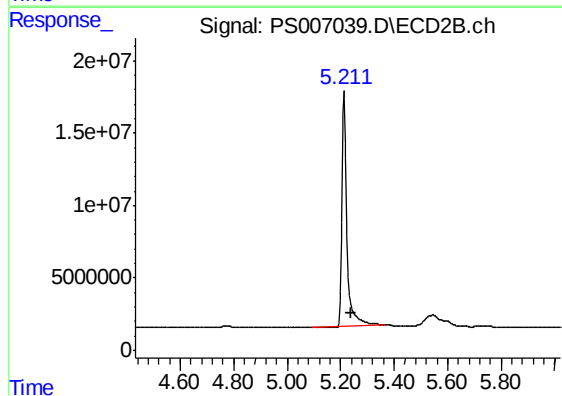


#4 2,4-DCAA

R.T.: 5.212 min
Delta R.T.: -0.026 min
Response: 205788503
Conc: 447.52 ng/ml

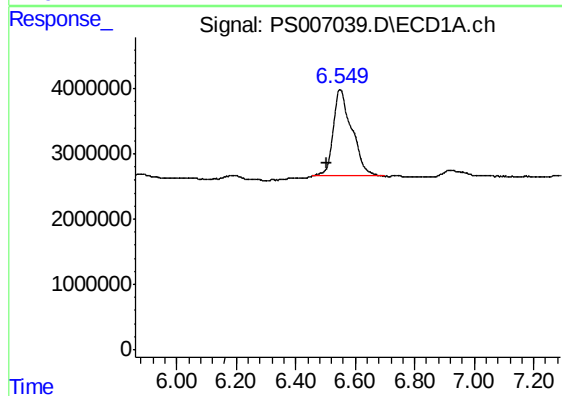


#9 2,4-D

R.T.: 6.549 min
Delta R.T.: 0.045 min
Response: 57626769
Conc: 70.32 ng/ml

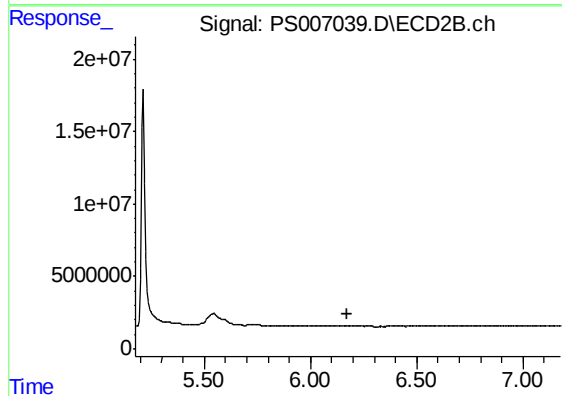

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.176 min
Response: 0
Conc: N.D.

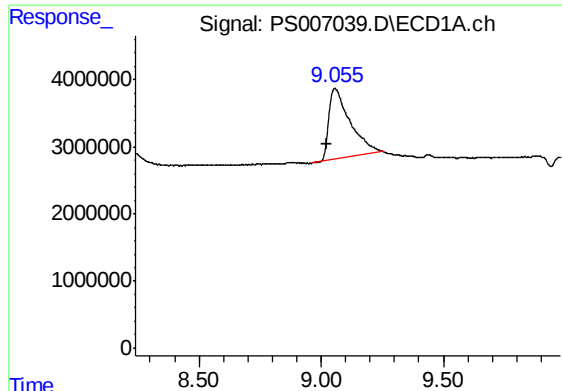

#15 Picloram


R.T.: 9.055 min
Delta R.T.: 0.030 min
Response: 63551461
Conc: 9.48 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

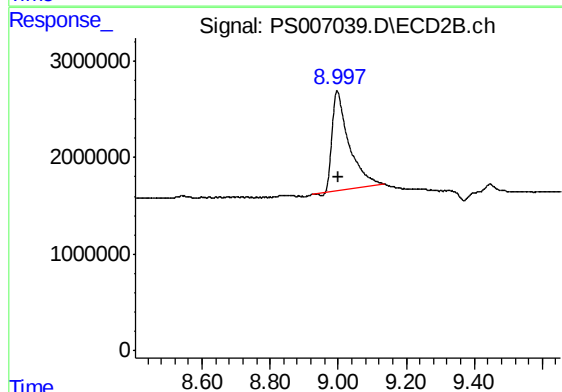


#15 Picloram

R.T.: 8.997 min
Delta R.T.: -0.001 min
Response: 35716638
Conc: 9.81 ng/ml

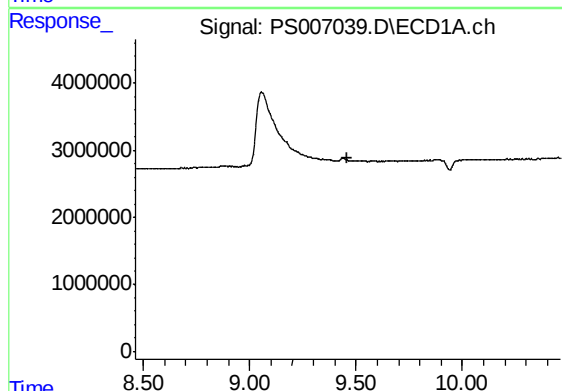

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.462 min
Response: 0
Conc: N.D.

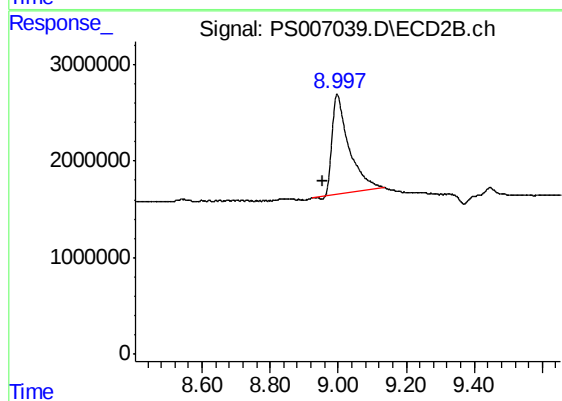

#16 DCPA

R.T.: 8.997 min
Delta R.T.: 0.042 min
Response: 35716638
Conc: 11.24 ng/ml