

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101524\
 Data File : PS027941.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 12:17
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 01:24:24 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100724.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 07 13:46:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.096	7.622	1425.7E6	448.4E6	529.152	451.243
Target Compounds							
1) T	Dalapon	2.501f	2.622	55243924	516894	12.310	<MDL #
3) T	4-Nitroph...	6.896	0.000	9274591	0	5.080	N.D. #
5) T	DICAMBA	7.328f	7.814	444873	5856869	<MDL	1.684 #
6) T	MCP	0.000	7.911	0	3466331	N.D.	1.259
7) T	MCPA	7.630f	8.134	1918585	8691906	<MDL	1.738 #
8) T	DICHLORPROP	7.979	8.564f	2038823	1346679	<MDL	1.364 #
10) T	Pentachlo...	0.000	9.328f	0	2693650	N.D.	<MDL
11) T	2,4,5-TP ...	9.032	9.744	1805142	2326529	<MDL	<MDL #
12) T	2,4,5-T	9.326	10.158	6274913	1482282	<MDL	<MDL #
13) T	2,4-DB	9.887	0.000	1900540	0	<MDL	N.D. #
14) T	DINOSEB	11.054	0.000	4393999	0	<MDL	N.D. #
15) T	Picloram	10.882	12.175	83857436	6283603	3.895	1.504 #
16) T	DCPA	11.358	12.109	3696630	1932814	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101524\
Data File : PS027941.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 12:17
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 01:24:24 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100724.M
Quant Title : 8080.M
QLast Update : Mon Oct 07 13:46:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

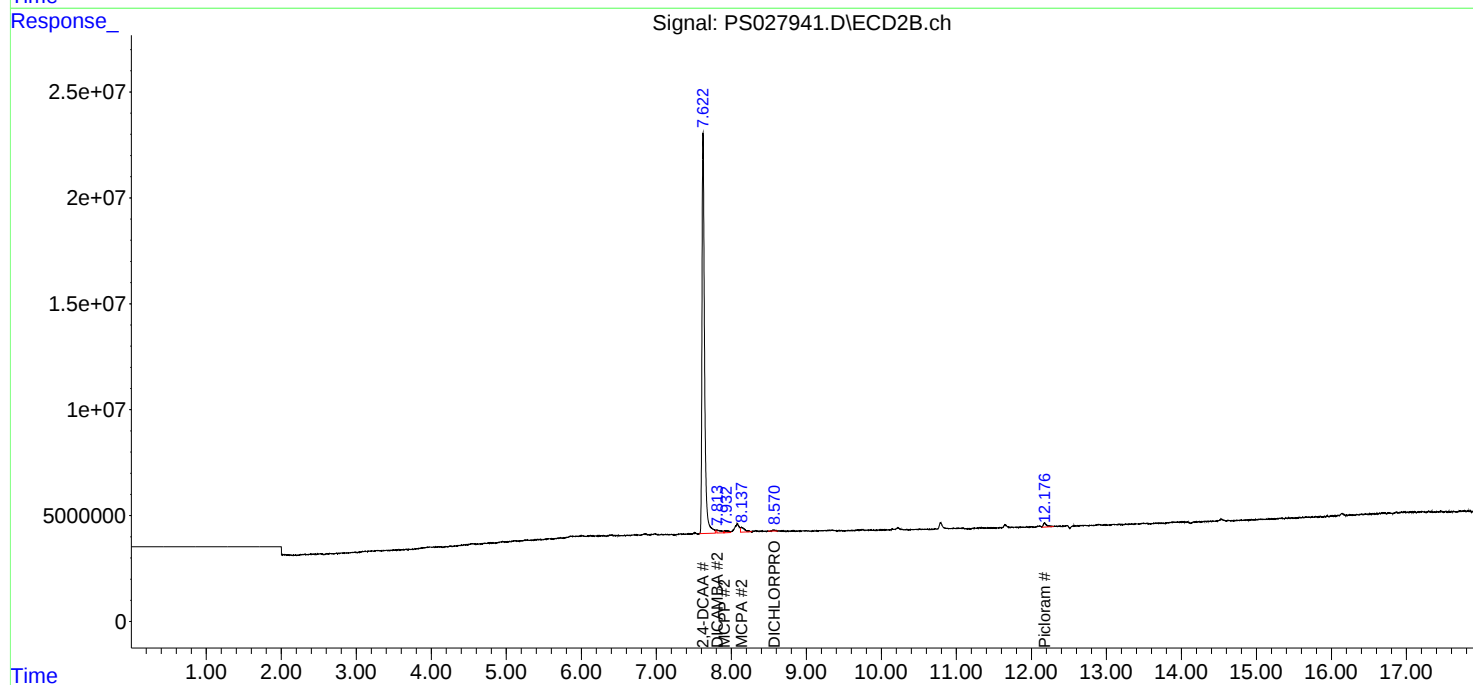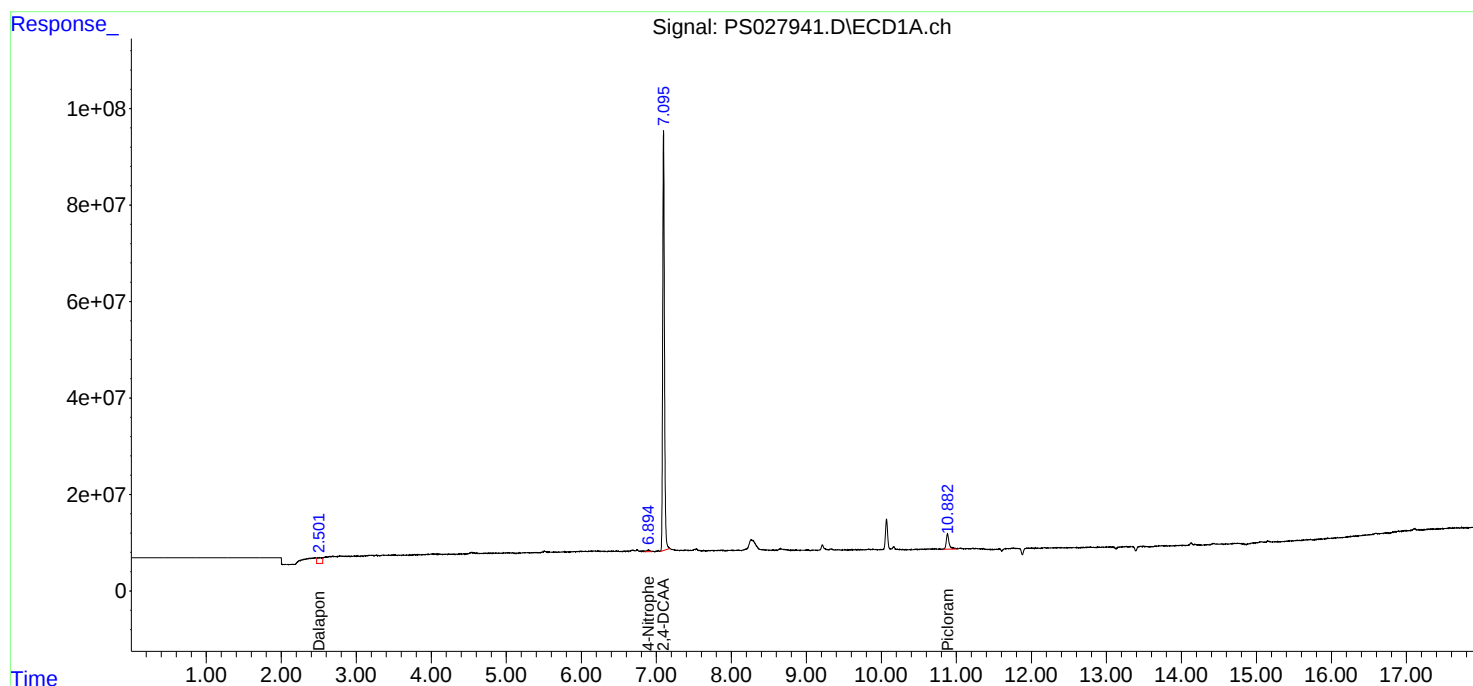


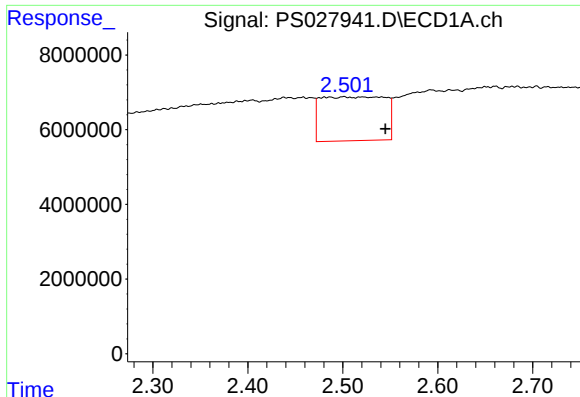

#1 Dalapon


R.T.: 2.501 min
Delta R.T.: -0.044 min
Response: 55243924
Conc: 12.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

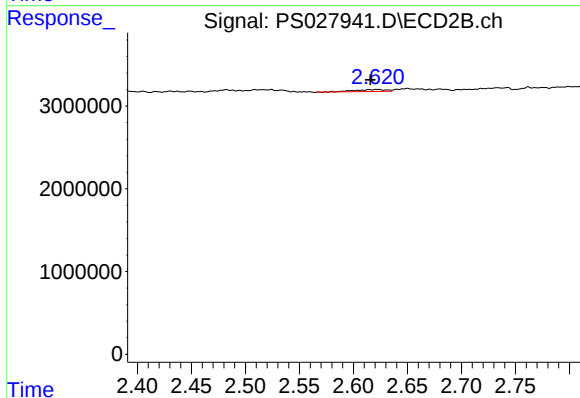


#1 Dalapon

R.T.: 2.622 min
Delta R.T.: 0.006 min
Response: 516894
Conc: N.D.

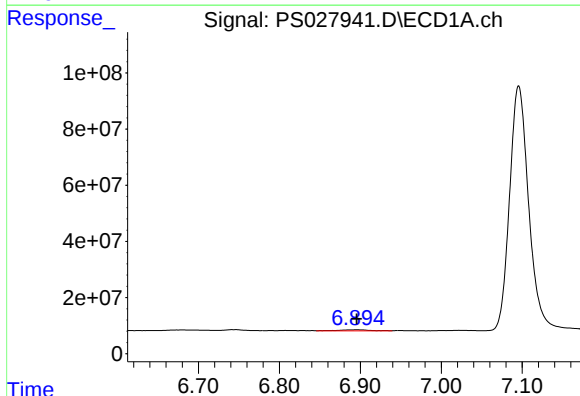


#3 4-Nitrophenol

R.T.: 6.896 min
Delta R.T.: 0.000 min
Response: 9274591
Conc: 5.08 ng/ml

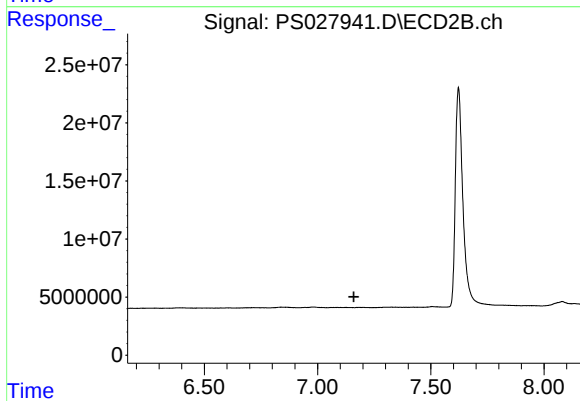

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.160 min
Response: 0
Conc: N.D.

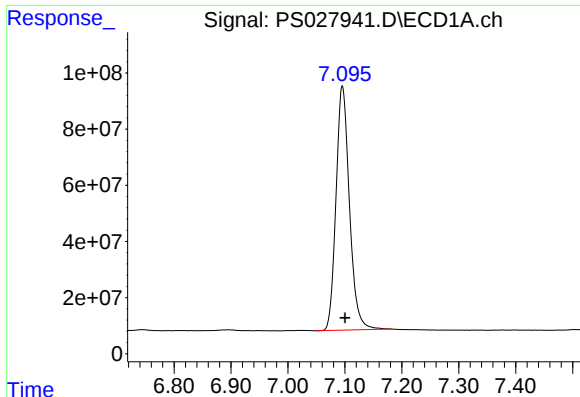

#4 2,4-DCAA


R.T.: 7.096 min
Delta R.T.: -0.004 min
Response: 1425689686
Conc: 529.15 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

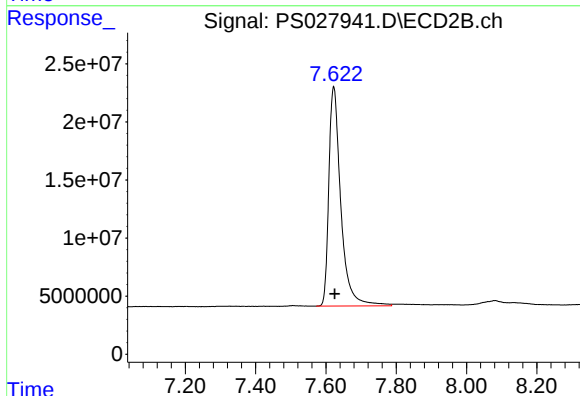


#4 2,4-DCAA

R.T.: 7.622 min
Delta R.T.: -0.003 min
Response: 448393407
Conc: 451.24 ng/ml

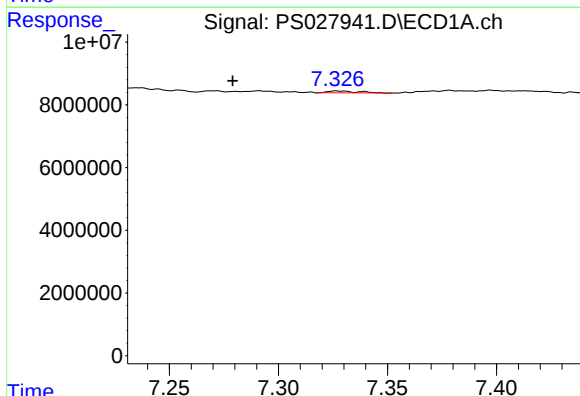


#5 DICAMBA

R.T.: 7.328 min
Delta R.T.: 0.049 min
Response: 444873
Conc: N.D.

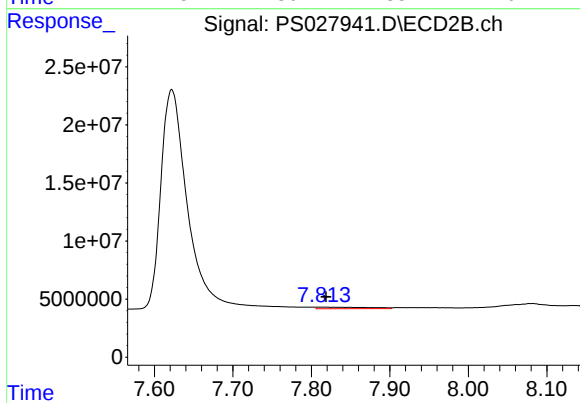

#5 DICAMBA


R.T.: 7.814 min
Delta R.T.: -0.005 min
Response: 5856869
Conc: 1.68 ng/ml

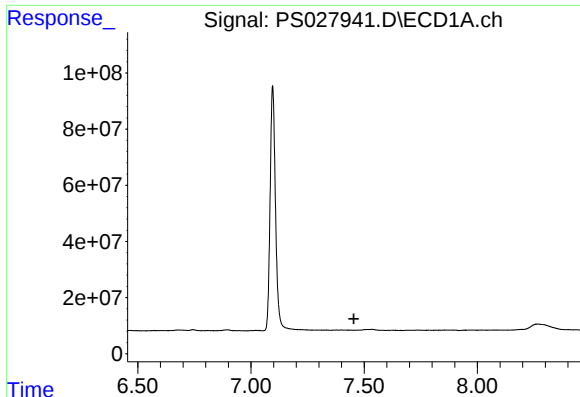

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 7.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

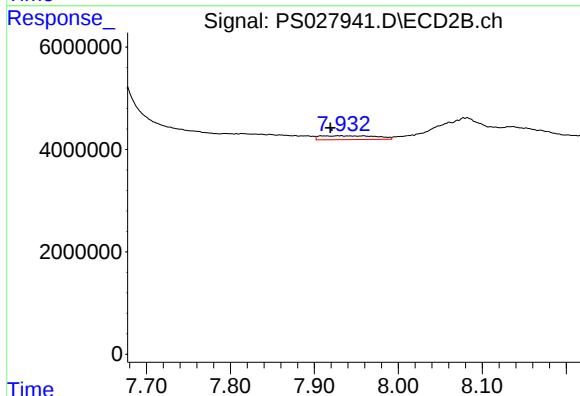


#6 MCPP

R.T.: 7.911 min
Delta R.T.: -0.008 min
Response: 3466331
Conc: 1.26 ug/ml

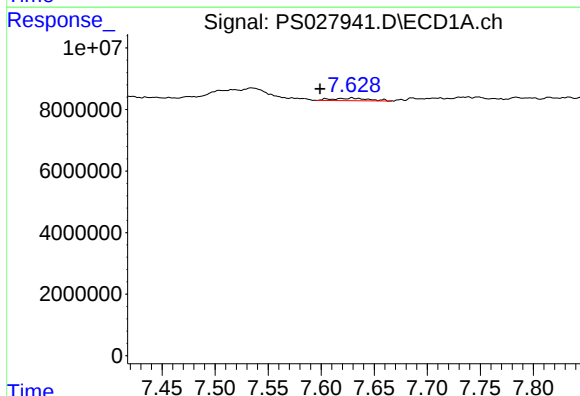


#7 MCPA

R.T.: 7.630 min
Delta R.T.: 0.031 min
Response: 1918585
Conc: N.D.

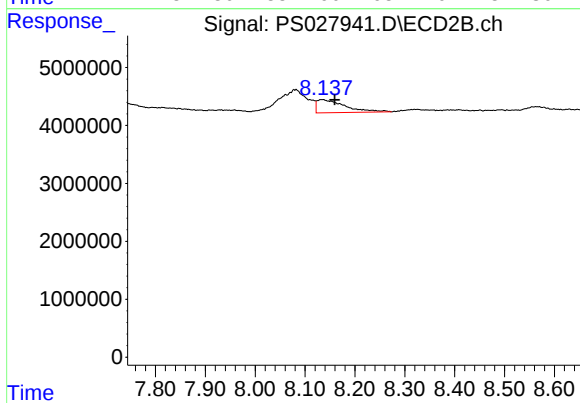

#7 MCPA


R.T.: 8.134 min
Delta R.T.: -0.025 min
Response: 8691906
Conc: 1.74 ug/ml

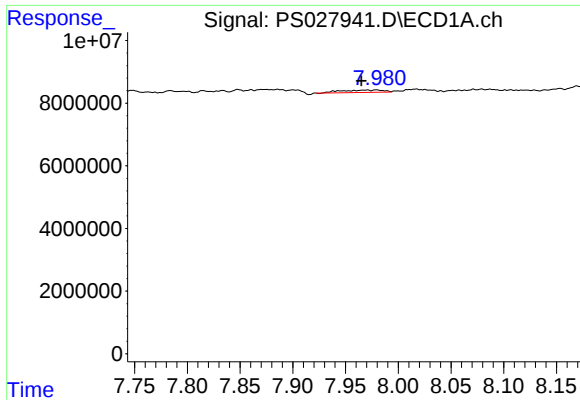

#8 DICHLORPROP


R.T.: 7.979 min
Delta R.T.: 0.014 min
Response: 2038823
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

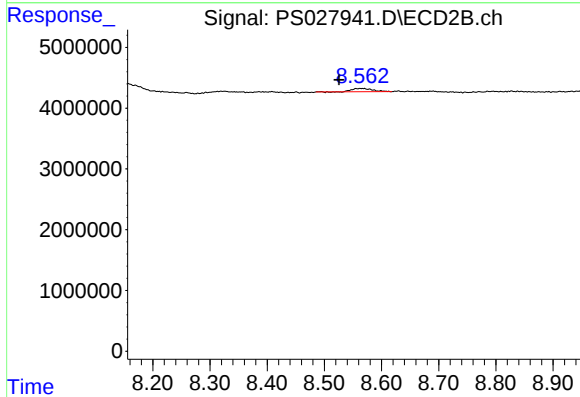


#8 DICHLORPROP

R.T.: 8.564 min
Delta R.T.: 0.039 min
Response: 1346679
Conc: 1.36 ng/ml

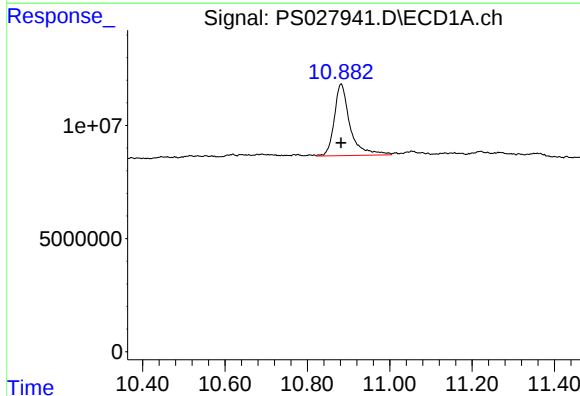

#15 Picloram

R.T.: 10.882 min
Delta R.T.: 0.000 min
Response: 83857436
Conc: 3.90 ng/ml

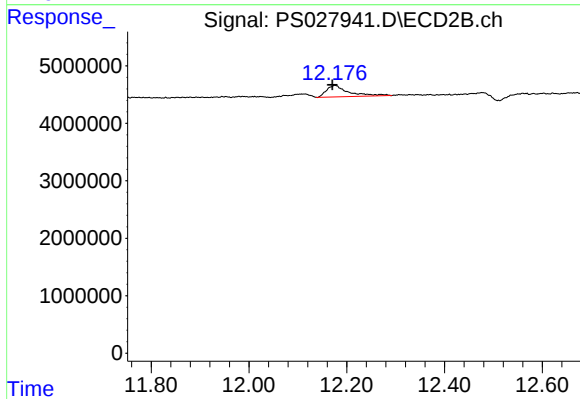

#15 Picloram

R.T.: 12.175 min
Delta R.T.: 0.005 min
Response: 6283603
Conc: 1.50 ng/ml