

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101724\
 Data File : PS027967.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2024 09:17
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 00:52:02 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100724.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 07 13:46:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.093	7.619	1464.0E6	481.7E6	543.384	484.794
Target Compounds							
1) T	Dalapon	0.000	2.594	0	569716	N.D.	<MDL
3) T	4-Nitroph...	6.884	0.000	13318684	0	7.294	N.D. #
5) T	DICAMBA	7.300	7.813	-1302337	5402288	N.D.	1.554
6) T	MCP	0.000	7.928	0	1032056	N.D.	<MDL
8) T	DICHLORPROP	7.966	8.563f	3258008	2115535	1.138	2.144 #
10) T	Pentachlo...	8.481	0.000	3999973	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.077f	9.735	4630420	910330	<MDL	<MDL #
12) T	2,4,5-T	9.321	10.158	6322247	788581	<MDL	<MDL #
13) T	2,4-DB	9.864	0.000	1690501	0	<MDL	N.D. #
14) T	DINOSEB	11.048	0.000	4348910	0	<MDL	N.D. #
15) T	Picloram	10.880	12.176	47695326	5401869	2.216	1.293 #
16) T	DCPA	11.345	12.112	2202835	2193684	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS10724\
Data File : PS027967.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2024 09:17
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 00:52:02 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100724.M
Quant Title : 8080.M
QLast Update : Mon Oct 07 13:46:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

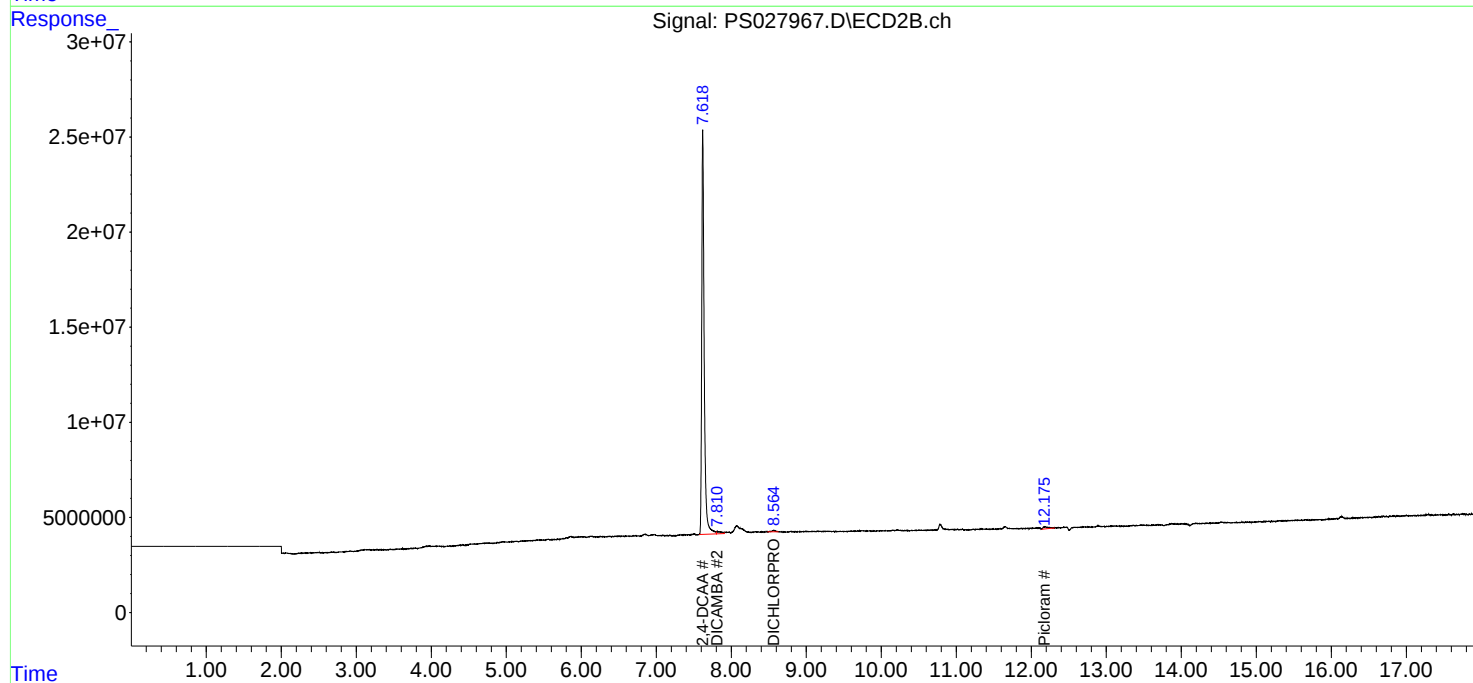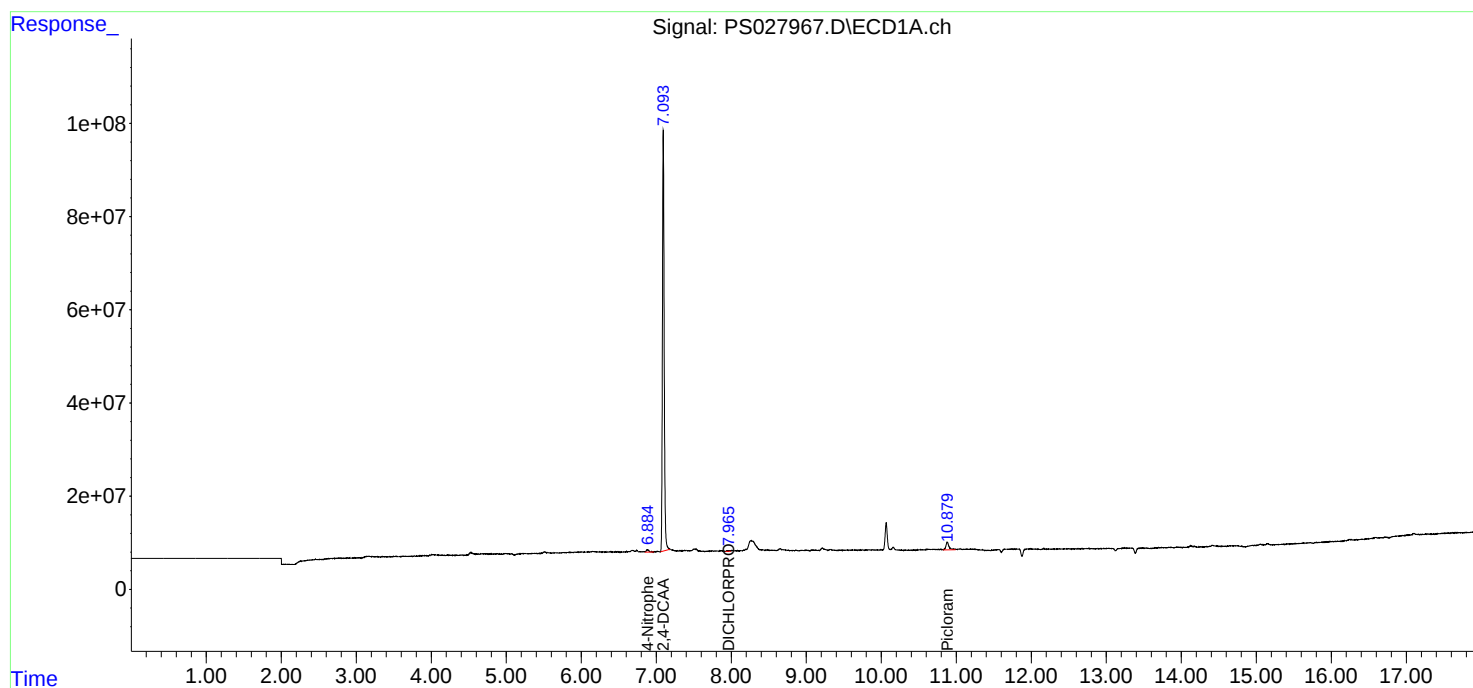


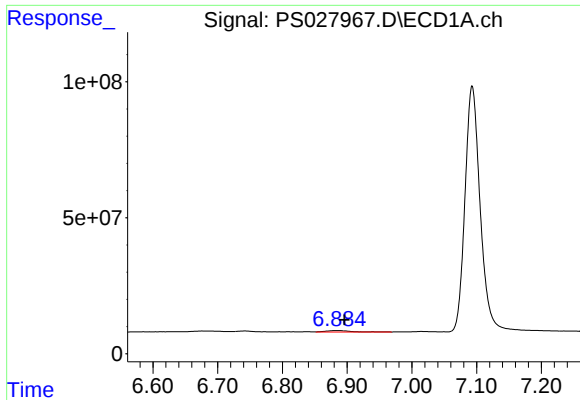

#3 4-Nitrophenol


R.T.: 6.884 min
Delta R.T.: -0.012 min
Response: 13318684
Conc: 7.29 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

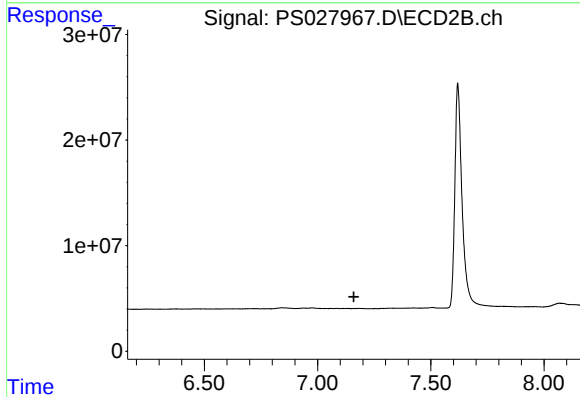


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.160 min
Response: 0
Conc: N.D.

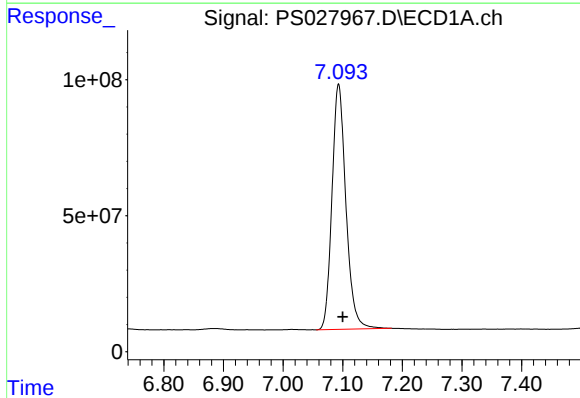


#4 2,4-DCAA

R.T.: 7.093 min
Delta R.T.: -0.007 min
Response: 1464033800
Conc: 543.38 ng/ml

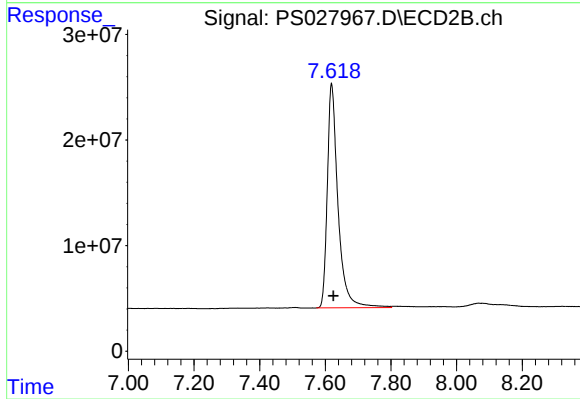

#4 2,4-DCAA


R.T.: 7.619 min
Delta R.T.: -0.006 min
Response: 481733031
Conc: 484.79 ng/ml

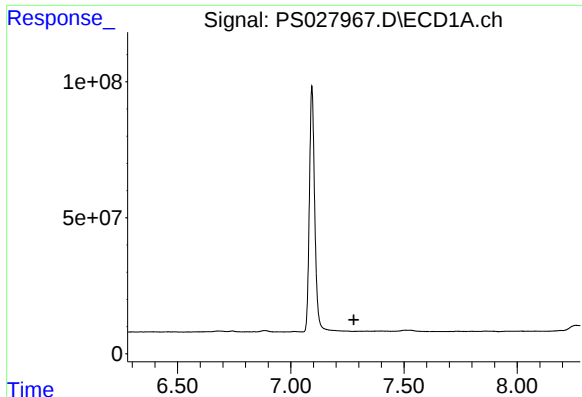

#5 DICAMBA


R.T.: 7.300 min
Delta R.T.: 0.021 min
Response: -1302337
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

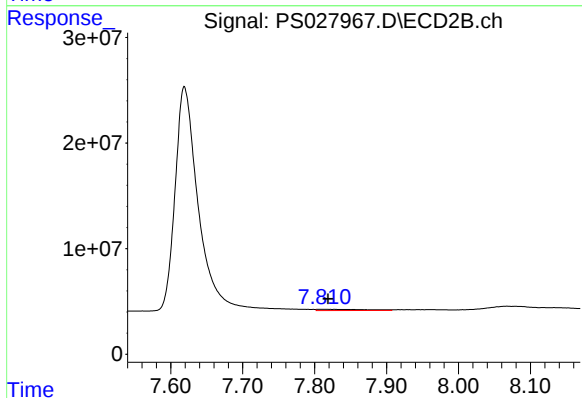


#5 DICAMBA

R.T.: 7.813 min
Delta R.T.: -0.006 min
Response: 5402288
Conc: 1.55 ng/ml

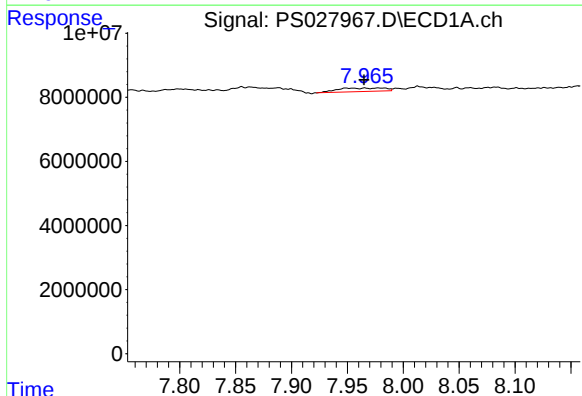


#8 DICHLORPROP

R.T.: 7.966 min
Delta R.T.: 0.000 min
Response: 3258008
Conc: 1.14 ng/ml

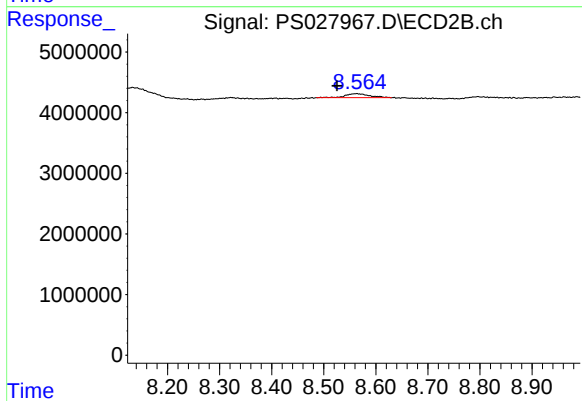

#8 DICHLORPROP


R.T.: 8.563 min
Delta R.T.: 0.037 min
Response: 2115535
Conc: 2.14 ng/ml

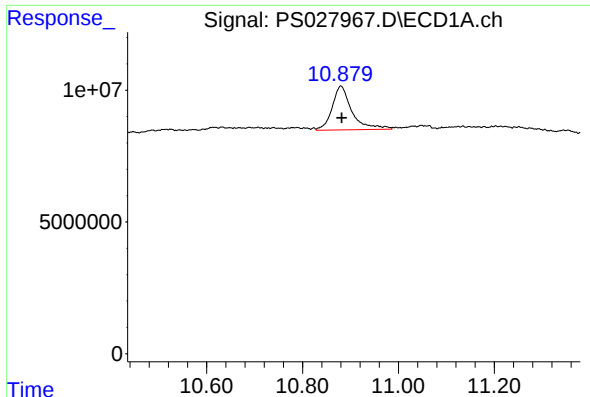

#15 Picloram

R.T.: 10.880 min
Delta R.T.: -0.002 min
Response: 47695326
Conc: 2.22 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

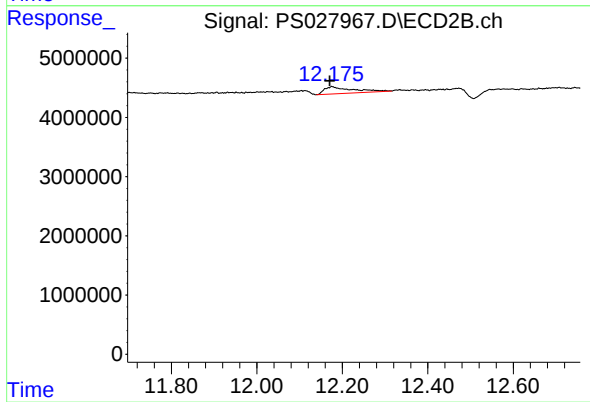

#15 Picloram

R.T.: 12.176 min
Delta R.T.: 0.006 min
Response: 5401869
Conc: 1.29 ng/ml