

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101724\
 Data File : PS027973.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2024 17:57
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 00:57:53 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100724.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 07 13:46:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.093	7.620	1493.3E6	479.5E6	554.252	482.564
Target Compounds							
1) T	Dalapon	2.528	2.603	42401886	385052	9.448	<MDL #
3) T	4-Nitroph...	6.883	0.000	16101799	0	8.819	N.D. #
5) T	DICAMBA	7.326f	7.812	-573798	6584634	N.D.	1.894
6) T	MCP	0.000	7.960f	0	1373024	N.D.	<MDL
8) T	DICHLORPROP	0.000	8.563f	0	2216365	N.D.	2.246
9) T	2,4-D	0.000	8.804f	0	769080	N.D.	<MDL
11) T	2,4,5-TP ...	9.020	9.716f	2894629	1925103	<MDL	<MDL #
12) T	2,4,5-T	9.329	10.144	1632682	947290	<MDL	<MDL #
13) T	2,4-DB	9.901	0.000	2131674	0	<MDL	N.D. #
14) T	DINOSEB	11.051	0.000	2273607	0	<MDL	N.D. #
15) T	Picloram	10.875	12.192	16830194	2039772	<MDL	<MDL #
16) T	DCPA	11.352	12.108	3533574	3540684	<MDL	<MDL #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS10724\
Data File : PS027973.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2024 17:57
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 00:57:53 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100724.M
Quant Title : 8080.M
QLast Update : Mon Oct 07 13:46:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

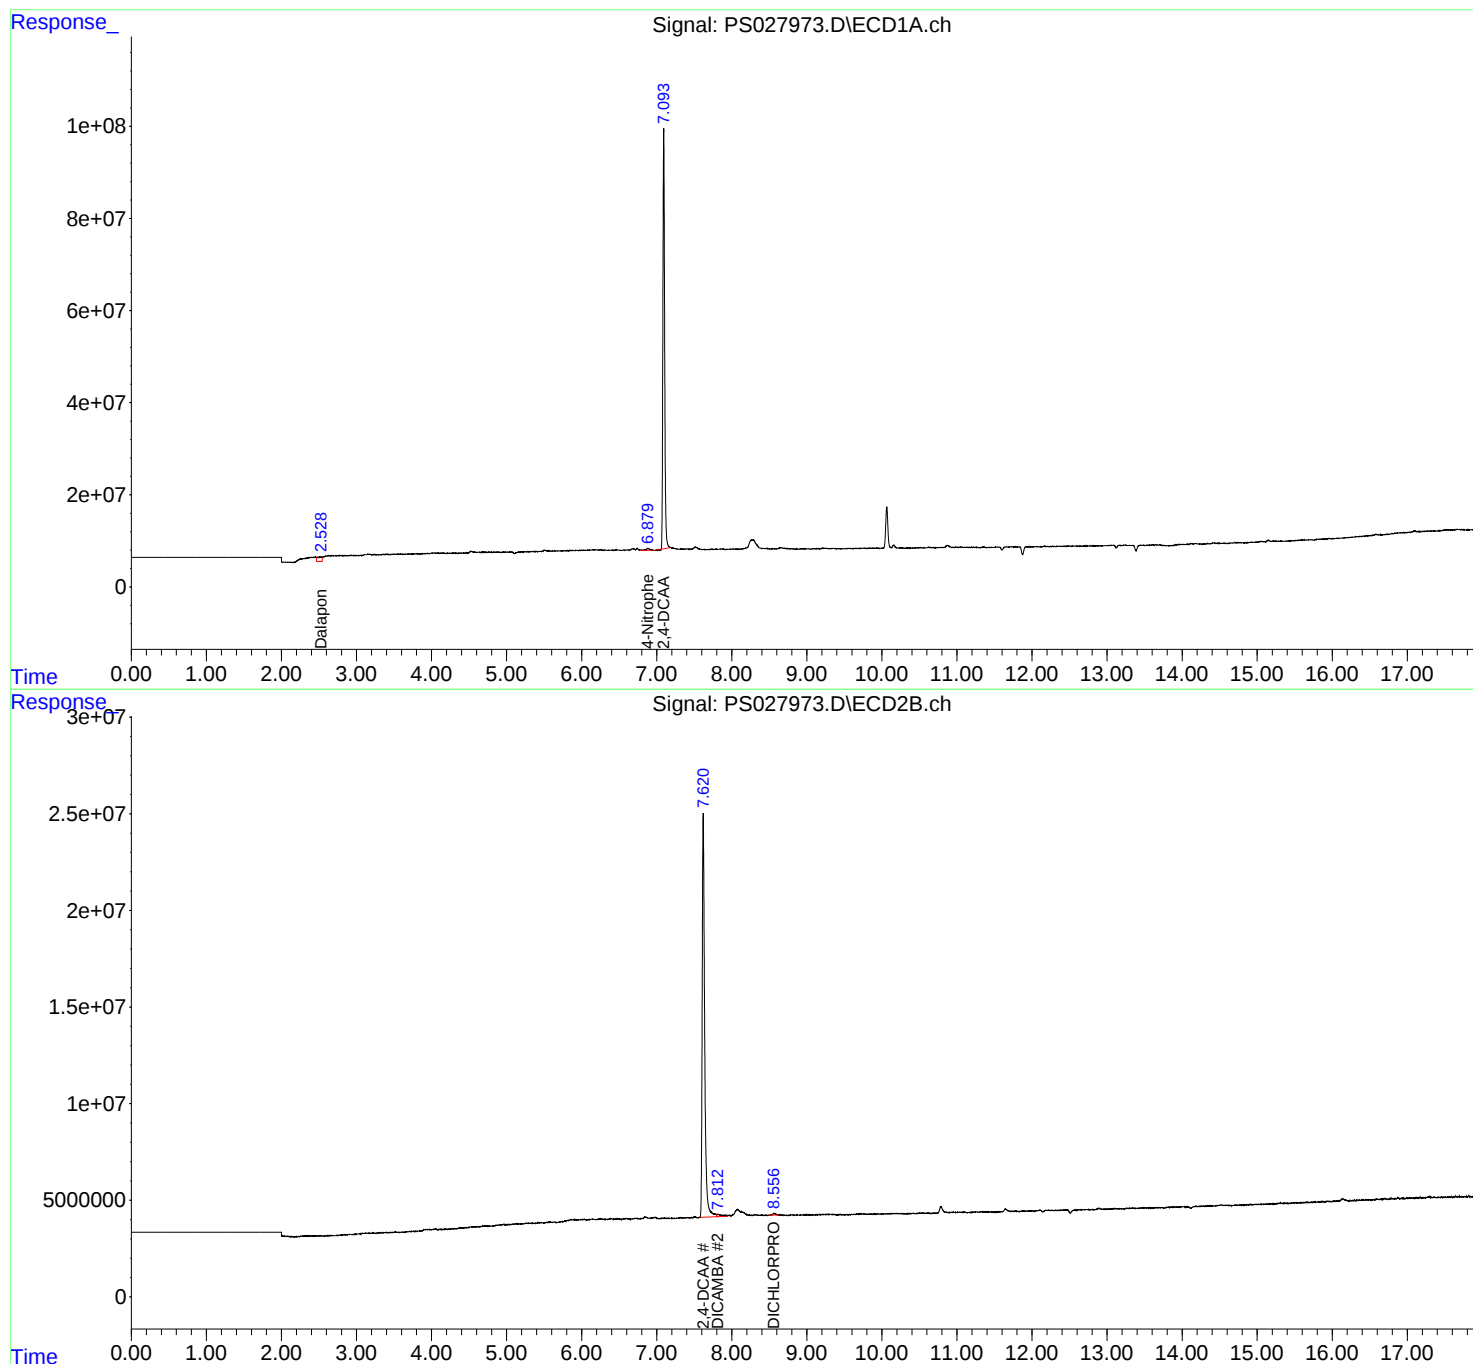


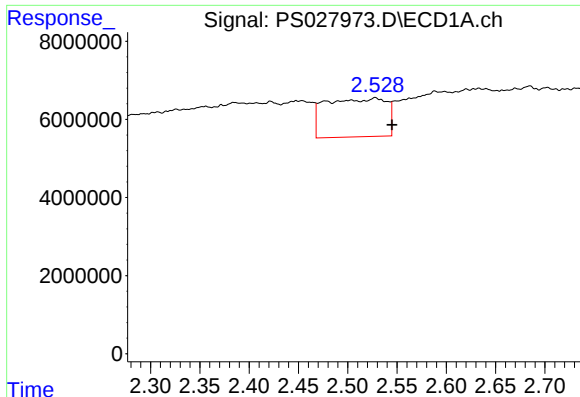

#1 Dalapon


R.T.: 2.528 min
Delta R.T.: -0.017 min
Response: 42401886
Conc: 9.45 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

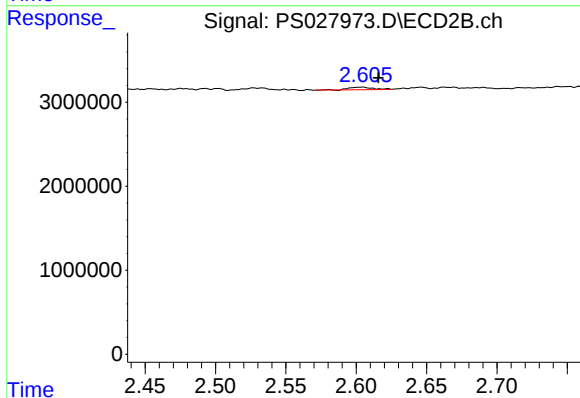


#1 Dalapon

R.T.: 2.603 min
Delta R.T.: -0.013 min
Response: 385052
Conc: N.D.

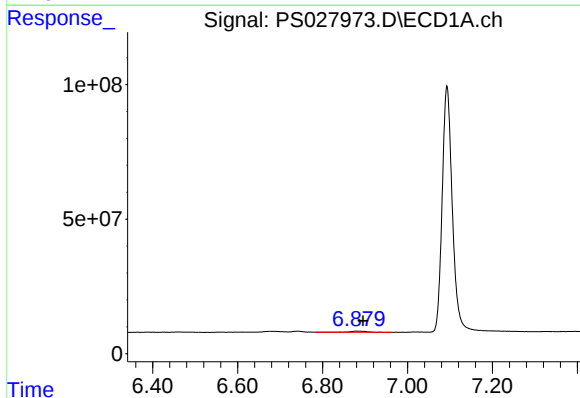


#3 4-Nitrophenol

R.T.: 6.883 min
Delta R.T.: -0.013 min
Response: 16101799
Conc: 8.82 ng/ml

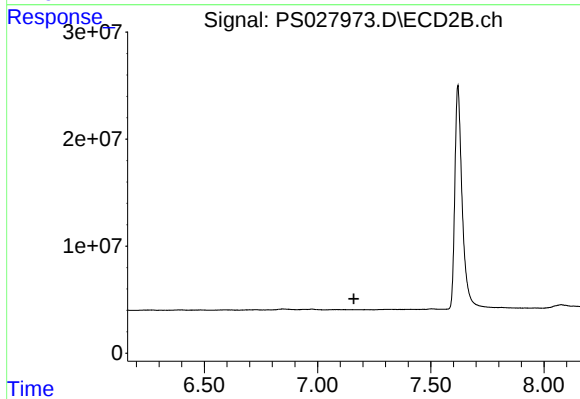

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.160 min
Response: 0
Conc: N.D.

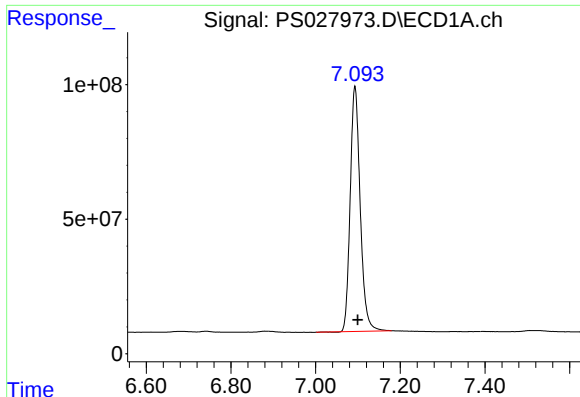

#4 2,4-DCAA


R.T.: 7.093 min
Delta R.T.: -0.007 min
Response: 1493317282
Conc: 554.25 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

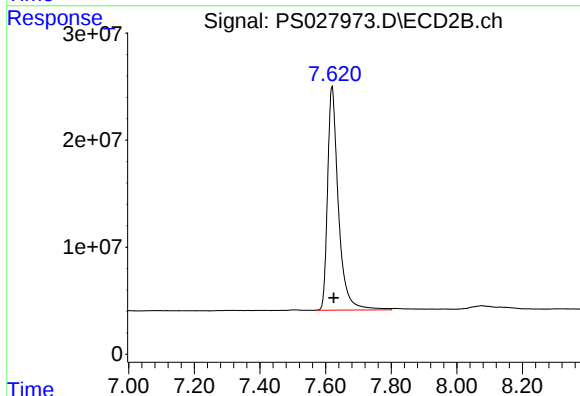


#4 2,4-DCAA

R.T.: 7.620 min
Delta R.T.: -0.005 min
Response: 479516585
Conc: 482.56 ng/ml

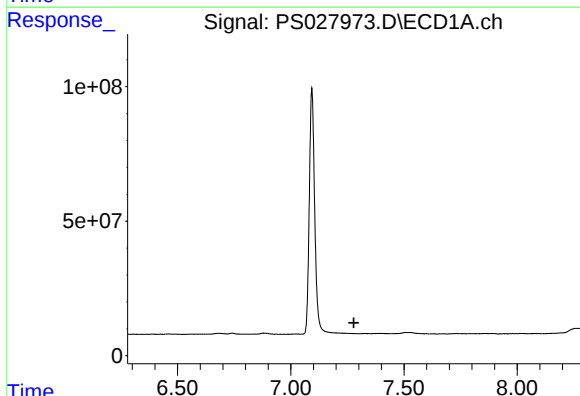


#5 DICAMBA

R.T.: 7.326 min
Delta R.T.: 0.047 min
Response: -573798
Conc: N.D.

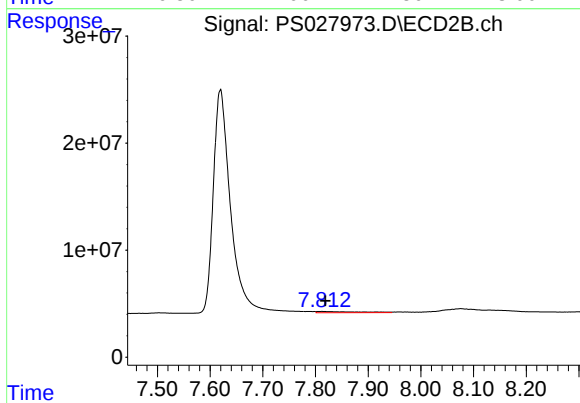

#5 DICAMBA


R.T.: 7.812 min
Delta R.T.: -0.007 min
Response: 6584634
Conc: 1.89 ng/ml

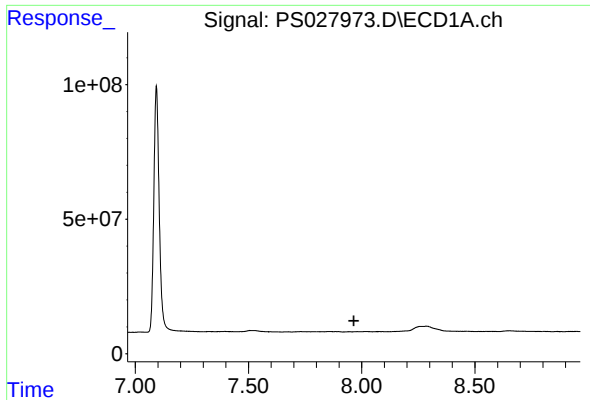

#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.965 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

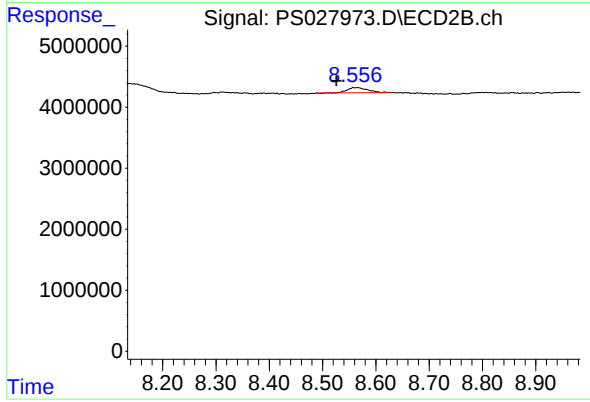

#8 DICHLORPROP

R.T.: 8.563 min
Delta R.T.: 0.037 min
Response: 2216365
Conc: 2.25 ng/ml