

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102023\
 Data File : PS024666.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Oct 2023 10:47
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 18:17:40 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 03 14:54:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	6.778	0	524407	N.D.	<MDL
Target Compounds							
1) T	Dalapon	0.000	2.562	0	2394077	N.D.	2.139
5) T	DICAMBA	0.000	6.934	0	227006	N.D.	<MDL
6) T	MCP	0.000	7.058	0	370682	N.D.	<MDL
8) T	DICHLORPROP	0.000	7.565	0	1746304	N.D.	2.322
9) T	2,4-D	7.252	7.781f	93868363	873255	33.973	<MDL #
10) T	Pentachlo...	0.000	8.261	0	584840	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.619	0	618327	N.D.	<MDL
12) T	2,4,5-T	0.000	8.988	0	616276	N.D.	<MDL
14) T	DINOSEB	0.000	9.820	0	853141	N.D.	<MDL
15) T	Picloram	9.662	10.776	16853259	18392090	<MDL	2.960 #
16) T	DCPA	0.000	10.776	0	18392090	N.D.	3.525



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102023\
Data File : PS024666.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Oct 2023 10:47
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 18:17:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
Quant Title : 8080.M
QLast Update : Tue Oct 03 14:54:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

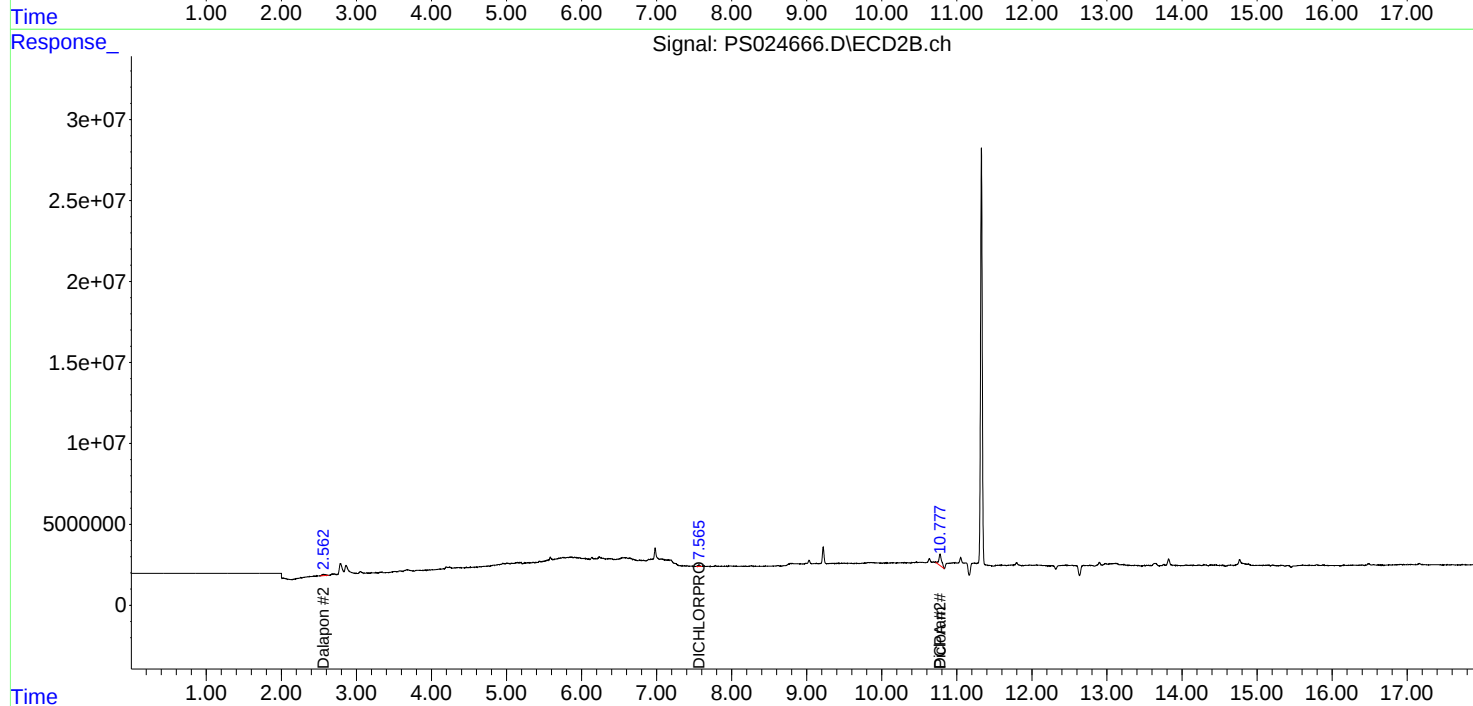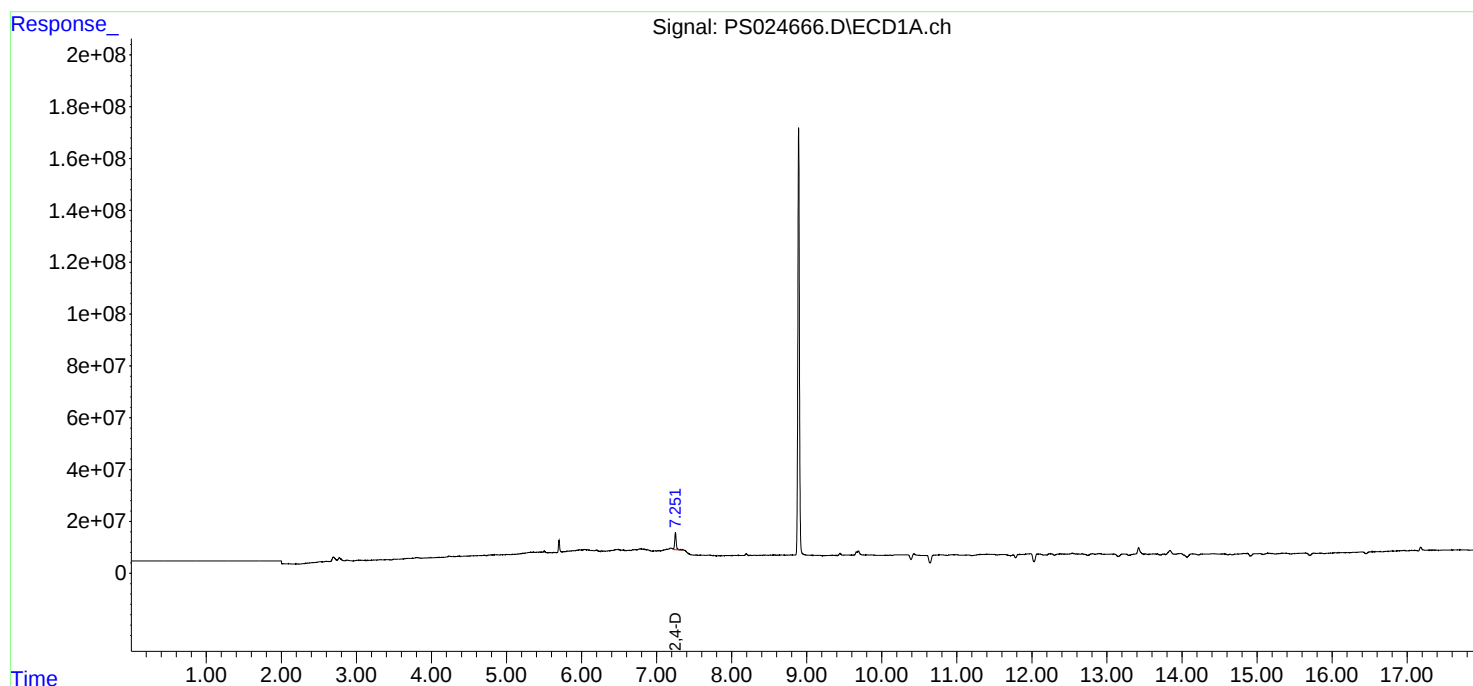


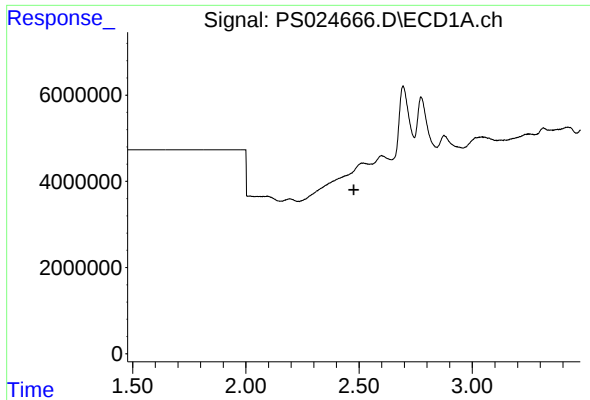

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.477 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

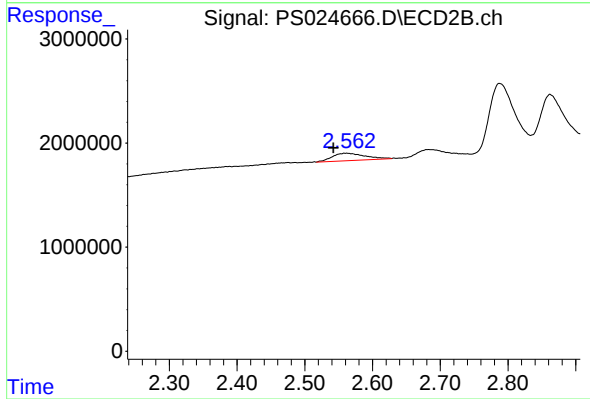


#1 Dalapon

R.T.: 2.562 min
Delta R.T.: 0.020 min
Response: 2394077
Conc: 2.14 ng/ml

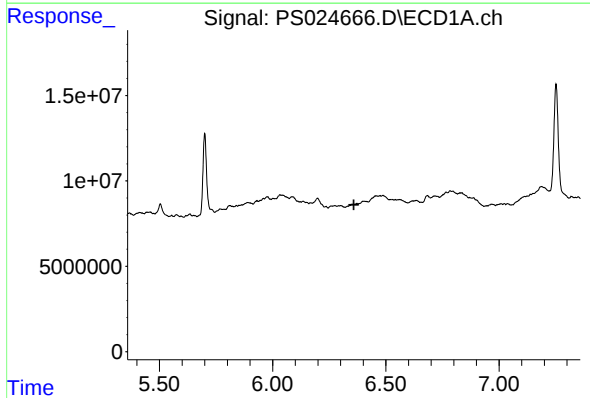


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.359 min
Response: 0
Conc: N.D.

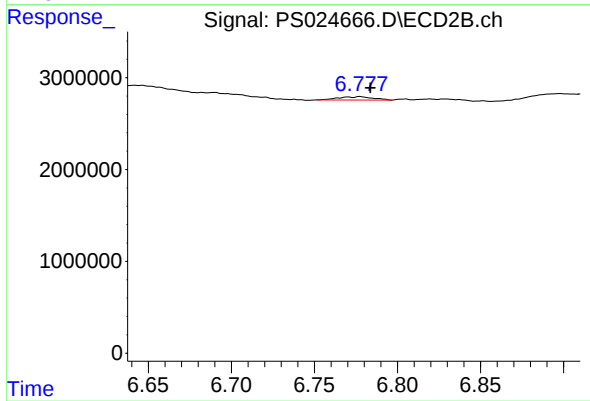

#4 2,4-DCAA


R.T.: 6.778 min
Delta R.T.: -0.006 min
Response: 524407
Conc: N.D.

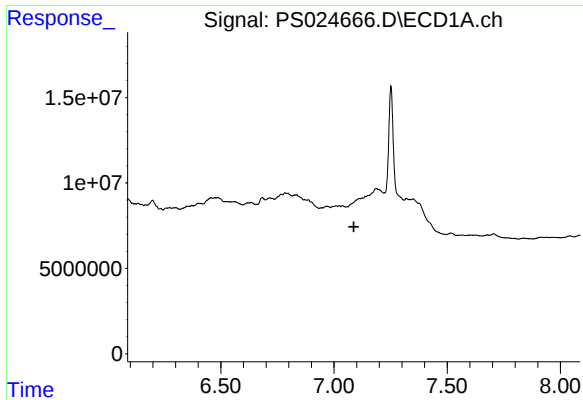

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.088 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

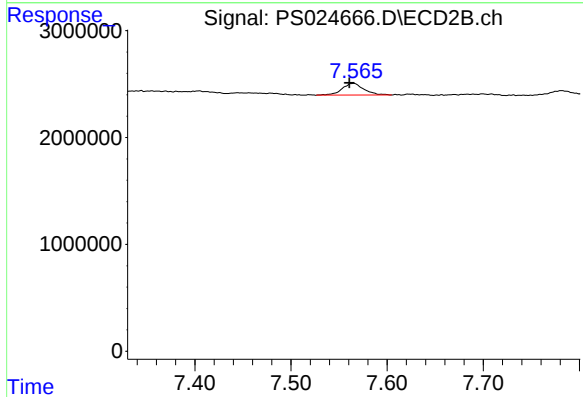


#8 DICHLORPROP

R.T.: 7.565 min
Delta R.T.: 0.004 min
Response: 1746304
Conc: 2.32 ng/ml

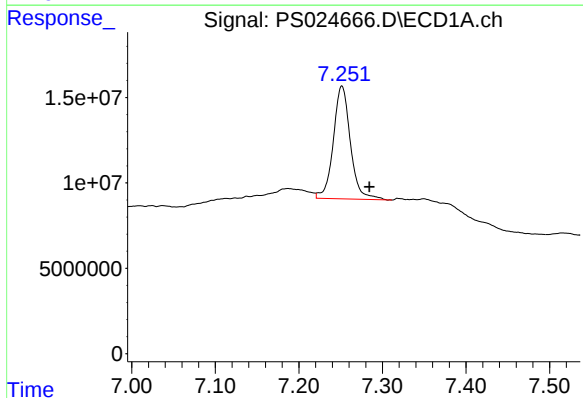


#9 2,4-D

R.T.: 7.252 min
Delta R.T.: -0.033 min
Response: 93868363
Conc: 33.97 ng/ml

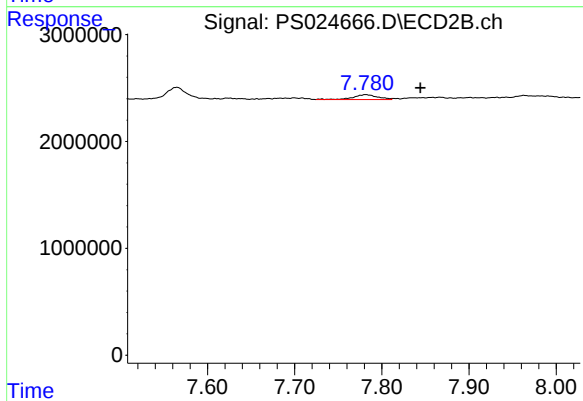

#9 2,4-D


R.T.: 7.781 min
Delta R.T.: -0.063 min
Response: 873255
Conc: N.D.

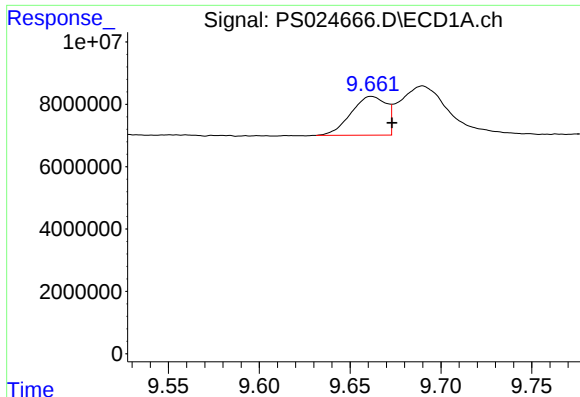

#15 Picloram


R.T.: 9.662 min
Delta R.T.: -0.011 min
Response: 16853259
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

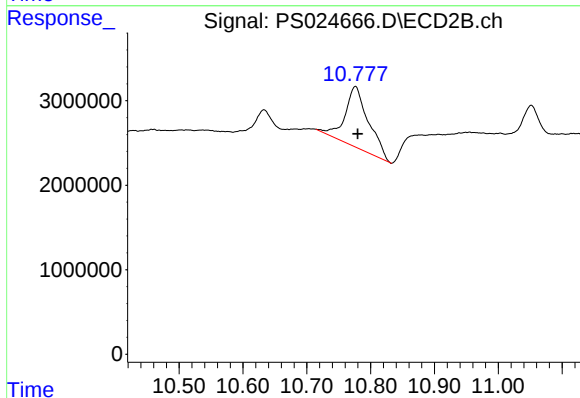


#15 Picloram

R.T.: 10.776 min
Delta R.T.: -0.004 min
Response: 18392090
Conc: 2.96 ng/ml

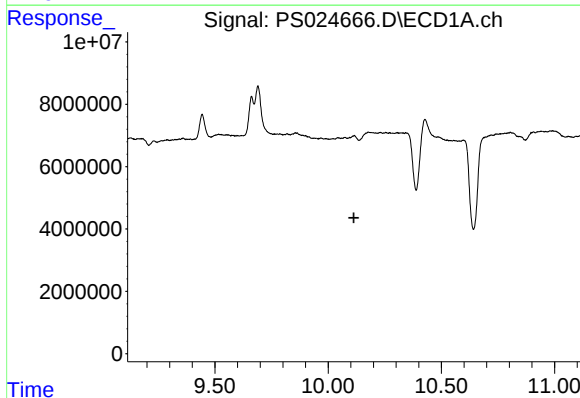

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.114 min
Response: 0
Conc: N.D.

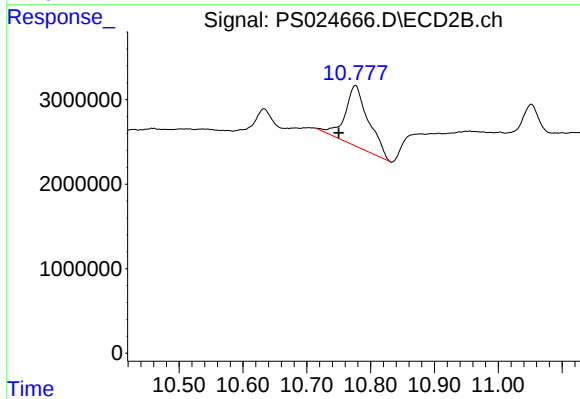

#16 DCPA

R.T.: 10.776 min
Delta R.T.: 0.026 min
Response: 18392090
Conc: 3.53 ng/ml