

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102023\
 Data File : PS024667.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Oct 2023 13:23
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 18:18:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 03 14:54:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.359	6.779	1025.2E6	337.3E6	498.335	487.962
Target Compounds							
1) T	Dalapon	2.513	2.568	8481711	4319489	3.433	3.860
7) T	MCPA	0.000	7.247	0	8681134	N.D.	2.709
8) T	DICHLORPROP	0.000	7.571	0	677960	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.619	0	471127	N.D.	<MDL
12) T	2,4,5-T	0.000	9.036	0	2225943	N.D.	<MDL
15) T	Picloram	9.694	10.780	22464411	7442654	1.288	1.198
16) T	DCPA	0.000	10.780	0	7442654	N.D.	1.426



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102023\
Data File : PS024667.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Oct 2023 13:23
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 18:18:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
Quant Title : 8080.M
QLast Update : Tue Oct 03 14:54:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

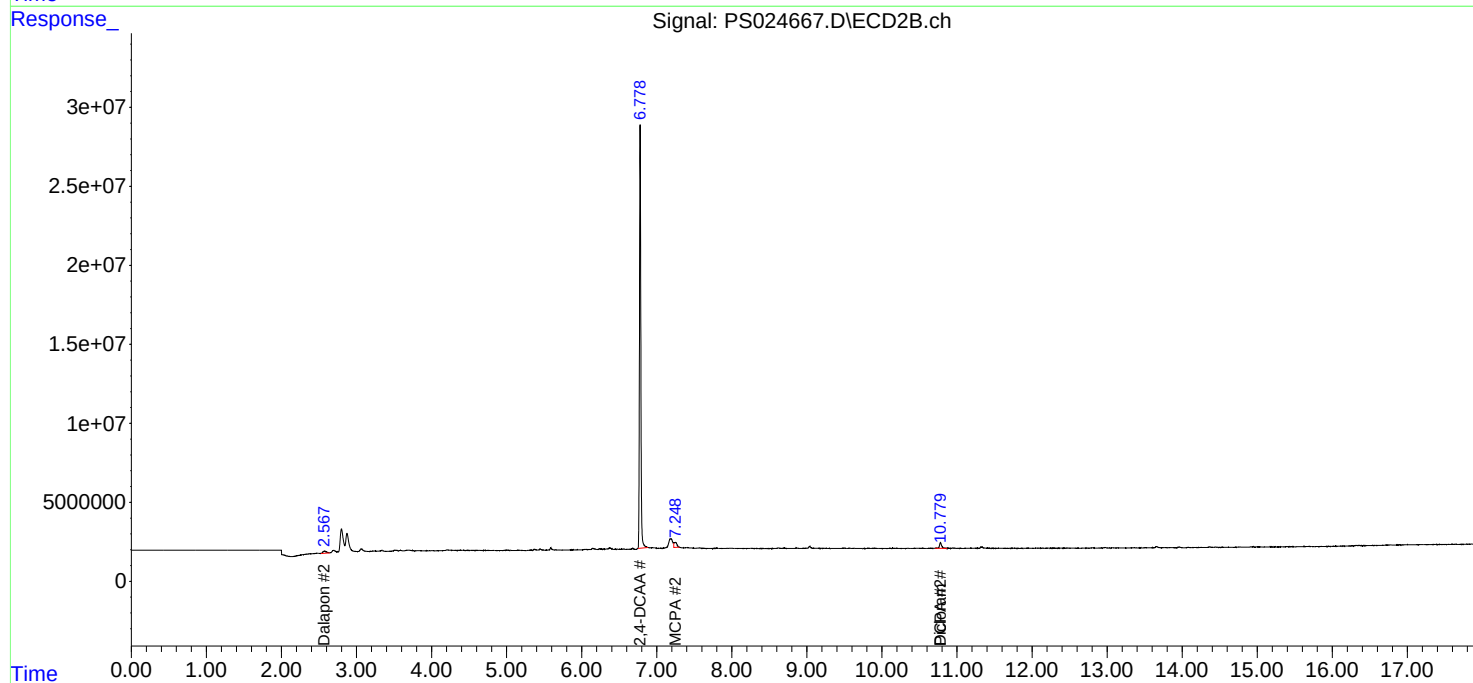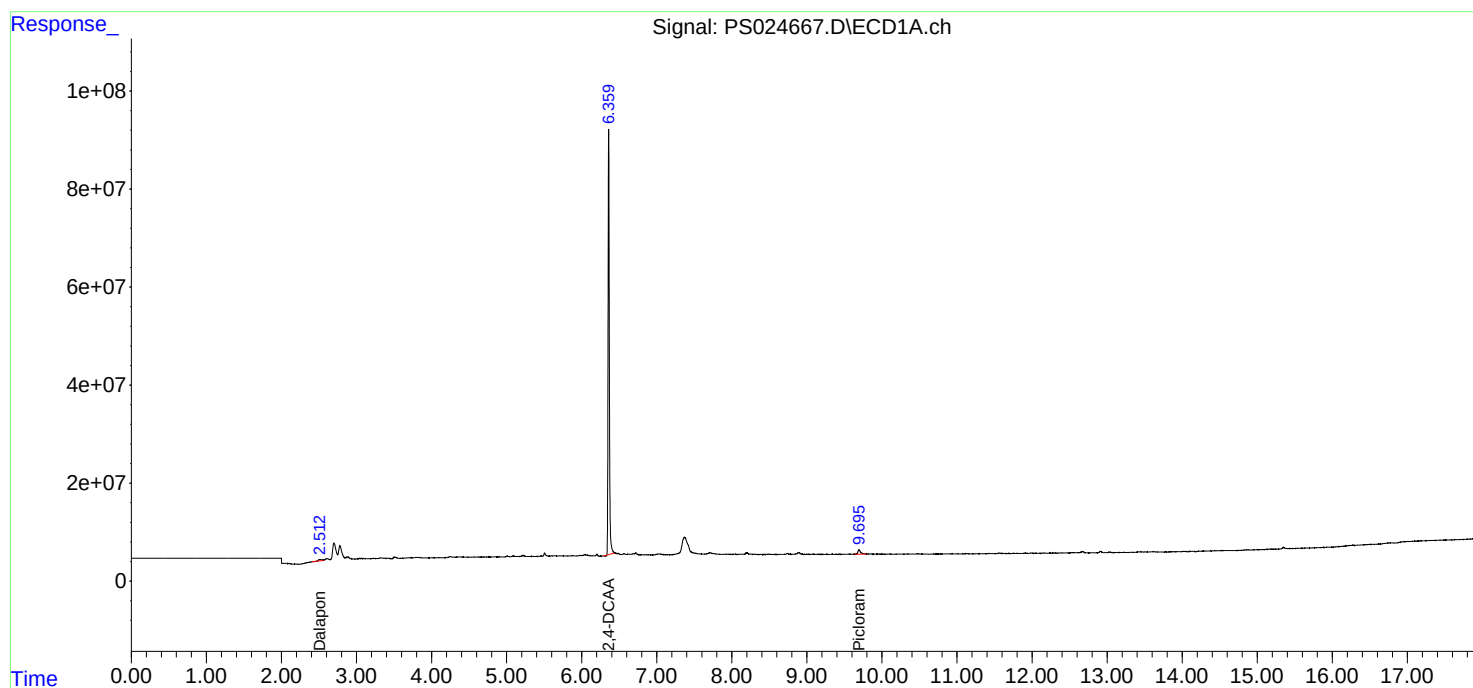


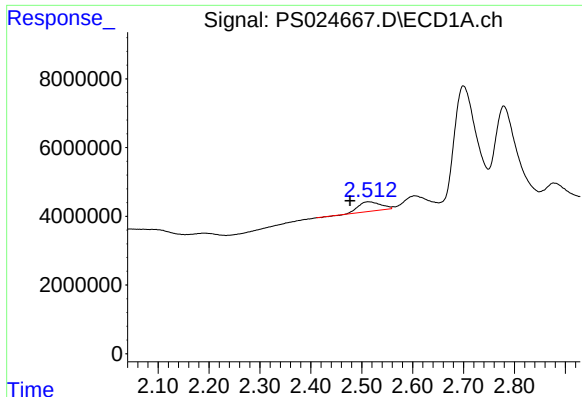

#1 Dalapon


R.T.: 2.513 min
Delta R.T.: 0.036 min
Response: 8481711
Conc: 3.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

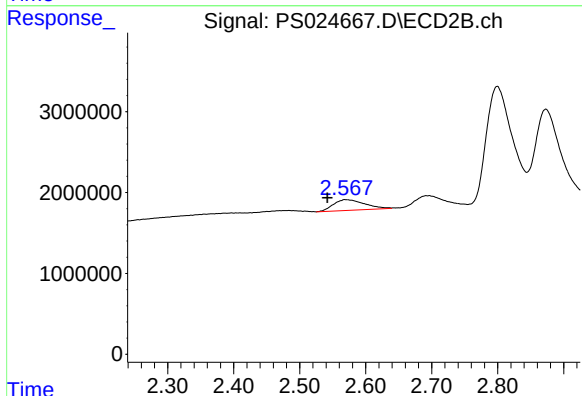


#1 Dalapon

R.T.: 2.568 min
Delta R.T.: 0.026 min
Response: 4319489
Conc: 3.86 ng/ml

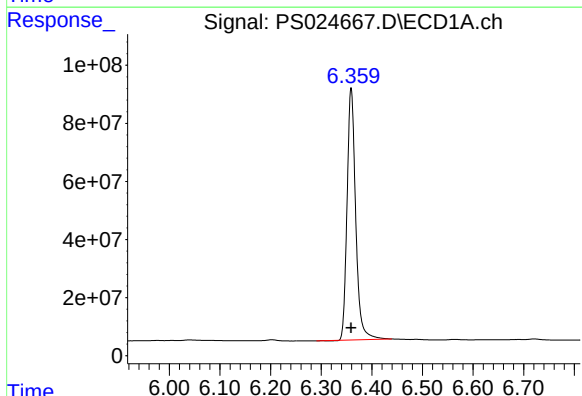


#4 2,4-DCAA

R.T.: 6.359 min
Delta R.T.: 0.000 min
Response: 1025239303
Conc: 498.34 ng/ml

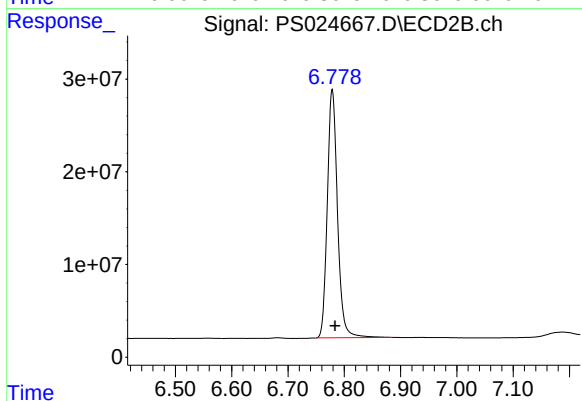

#4 2,4-DCAA


R.T.: 6.779 min
Delta R.T.: -0.005 min
Response: 337323784
Conc: 487.96 ng/ml

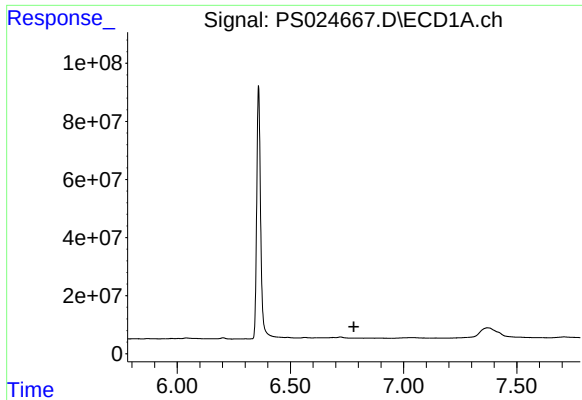

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.780 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

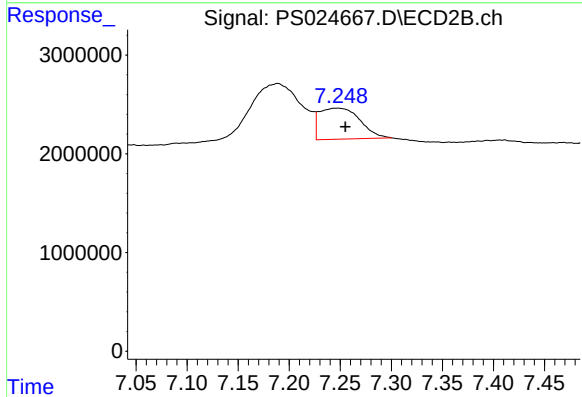


#7 MCPA

R.T.: 7.247 min
Delta R.T.: -0.008 min
Response: 8681134
Conc: 2.71 ug/ml

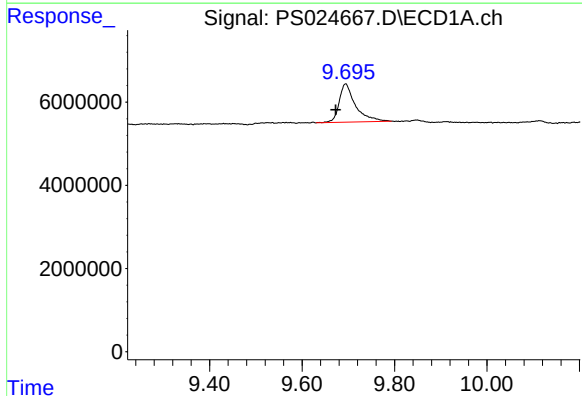


#15 Picloram

R.T.: 9.694 min
Delta R.T.: 0.021 min
Response: 22464411
Conc: 1.29 ng/ml

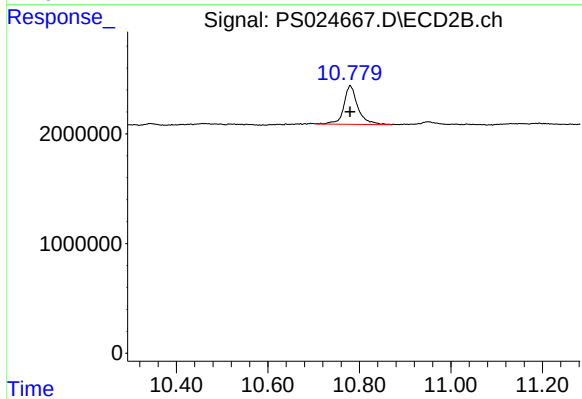

#15 Picloram


R.T.: 10.780 min
Delta R.T.: 0.000 min
Response: 7442654
Conc: 1.20 ng/ml

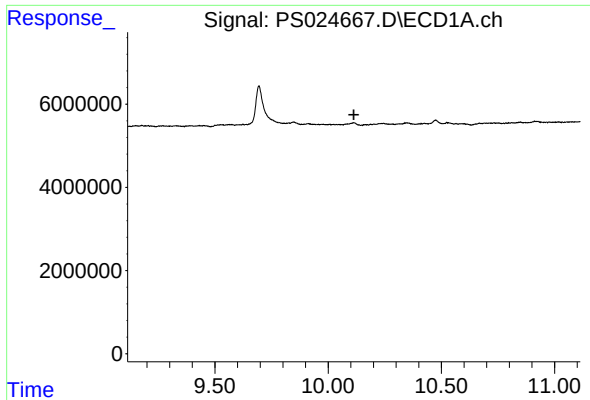

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.114 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

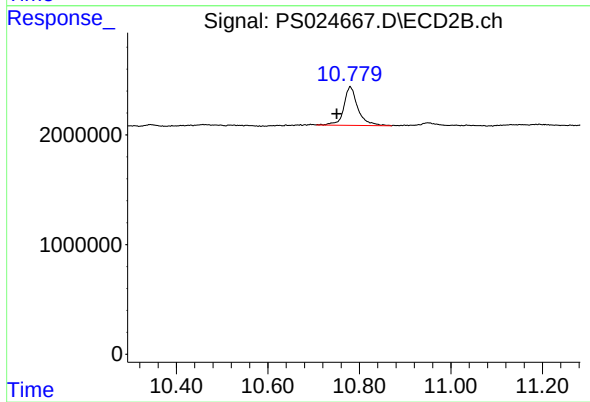

#16 DCPA

R.T.: 10.780 min
Delta R.T.: 0.030 min
Response: 7442654
Conc: 1.43 ng/ml