

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102023\
 Data File : PS024676.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Oct 2023 19:31
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 00:36:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 03 14:54:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.359	6.779	1030.1E6	343.8E6	500.695	497.344
Target Compounds							
1) T	Dalapon	0.000	2.568	0	3044142	N.D.	2.720
3) T	4-Nitroph...	6.199	0.000	10549426	0	7.793	N.D. #
5) T	DICAMBA	0.000	6.979	0	1110655	N.D.	<MDL
6) T	MCP	6.686	7.091f	1481285	331030	<MDL	<MDL #
7) T	MCPA	0.000	7.252	0	7424657	N.D.	2.317
8) T	DICHLORPROP	0.000	7.569	0	4396916	N.D.	5.847
9) T	2,4-D	0.000	7.784f	0	1341084	N.D.	1.457
11) T	2,4,5-TP ...	0.000	8.622	0	406908	N.D.	<MDL
12) T	2,4,5-T	0.000	9.033	0	722190	N.D.	<MDL
13) T	2,4-DB	0.000	9.490	0	928480	N.D.	1.822
15) T	Picloram	0.000	10.777	0	1585540	N.D.	<MDL
16) T	DCPA	0.000	10.777	0	1585540	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102023\
Data File : PS024676.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Oct 2023 19:31
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 00:36:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
Quant Title : 8080.M
QLast Update : Tue Oct 03 14:54:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

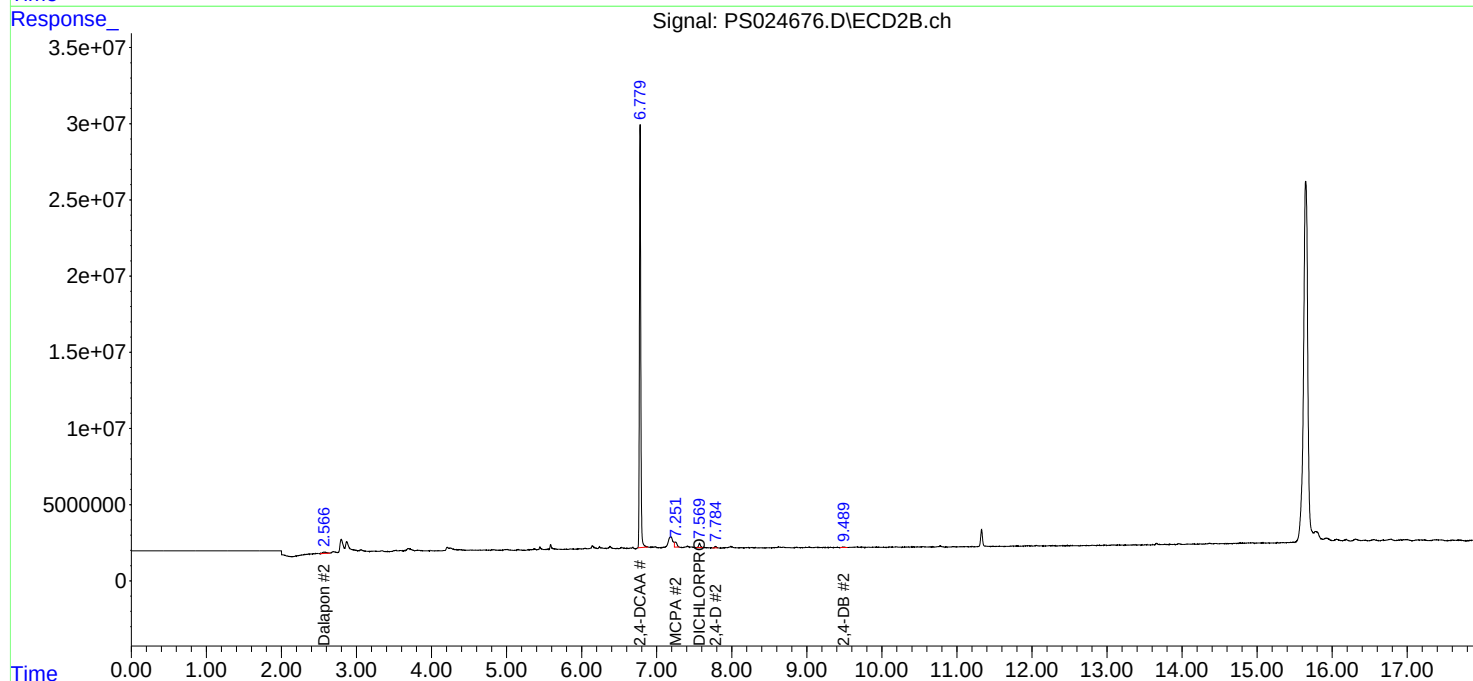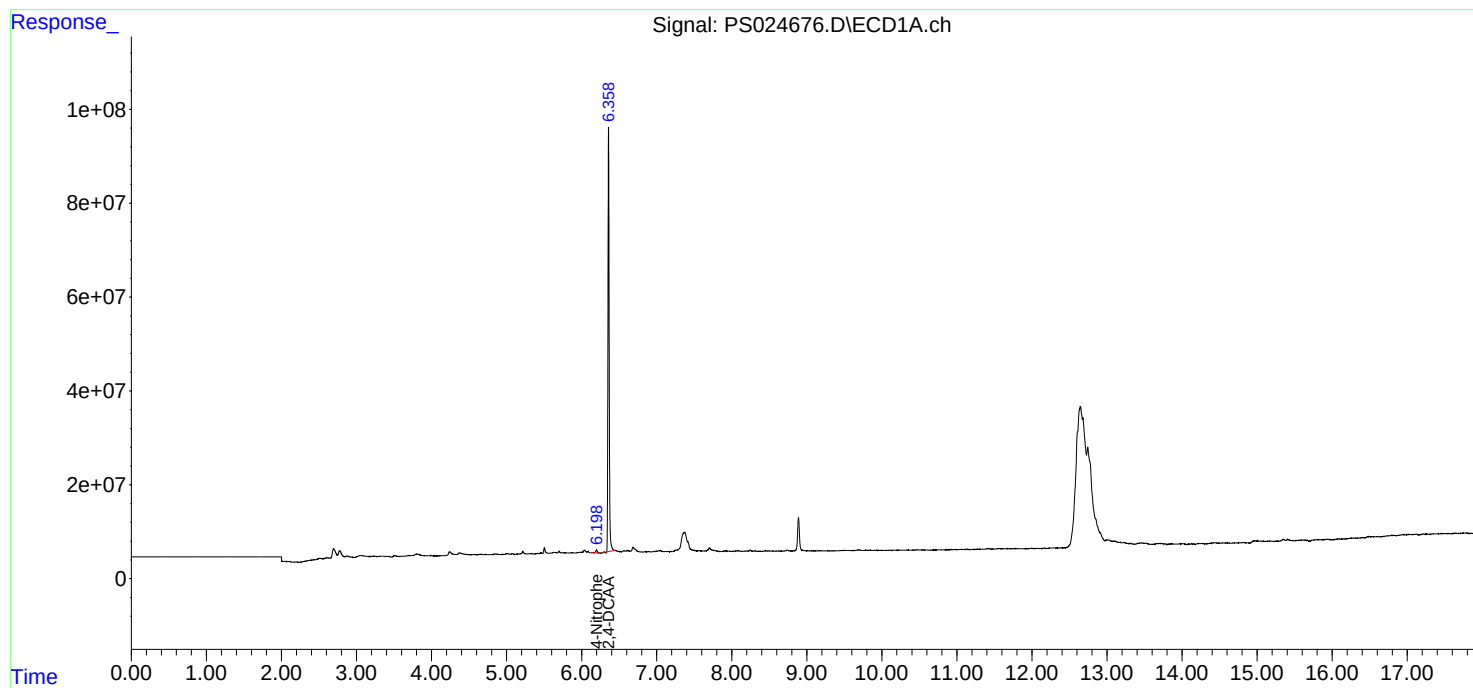


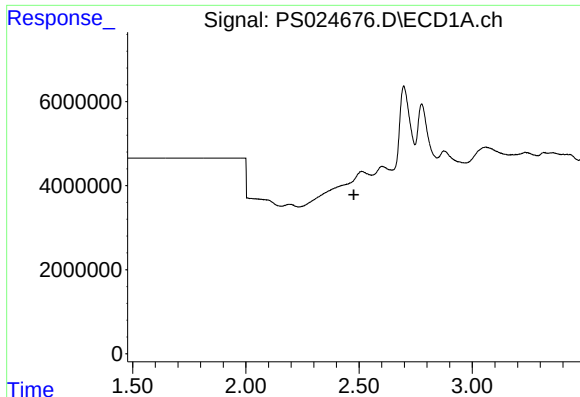

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.477 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

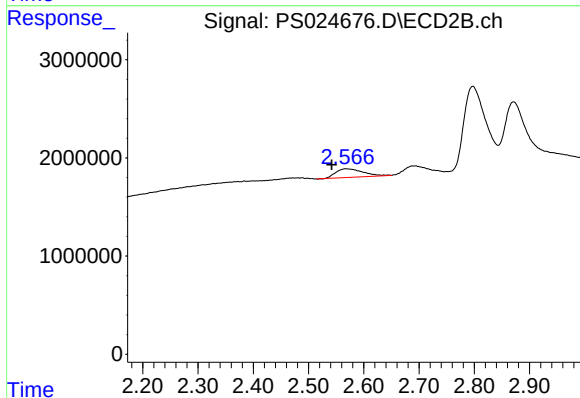


#1 Dalapon

R.T.: 2.568 min
Delta R.T.: 0.025 min
Response: 3044142
Conc: 2.72 ng/ml

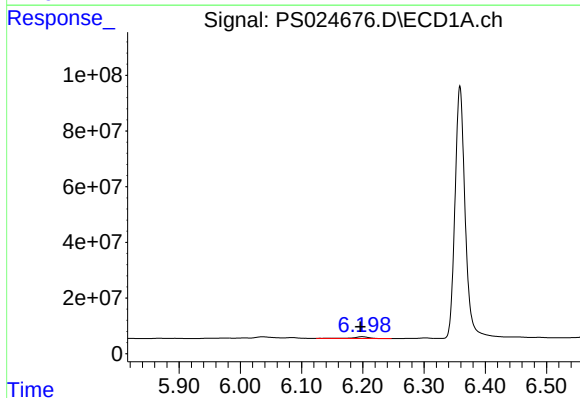


#3 4-Nitrophenol

R.T.: 6.199 min
Delta R.T.: 0.003 min
Response: 10549426
Conc: 7.79 ng/ml

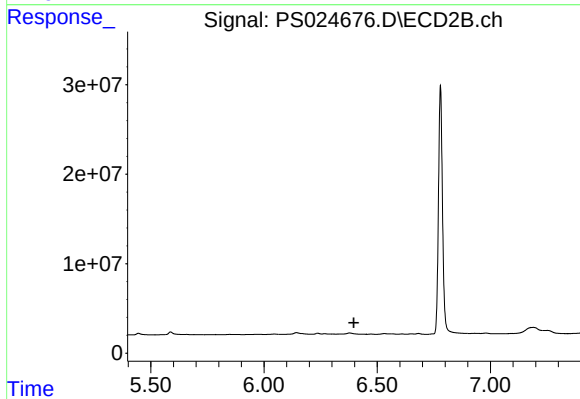

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.397 min
Response: 0
Conc: N.D.

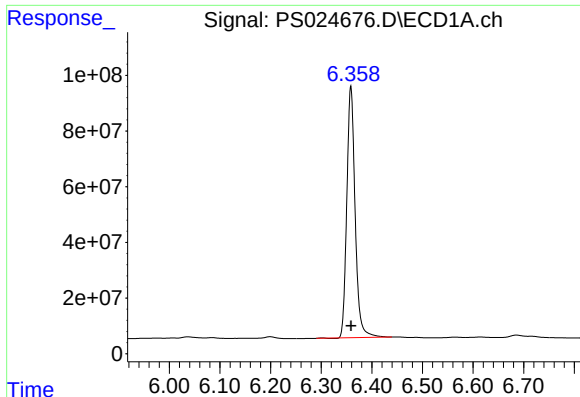

#4 2,4-DCAA


R.T.: 6.359 min
Delta R.T.: 0.000 min
Response: 1030095445
Conc: 500.70 ng/ml

Instrument :
ECD_S
ClientSampleId :

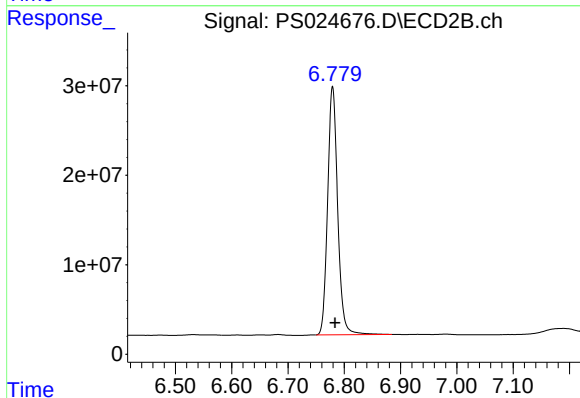


#4 2,4-DCAA

R.T.: 6.779 min
Delta R.T.: -0.004 min
Response: 343808956
Conc: 497.34 ng/ml

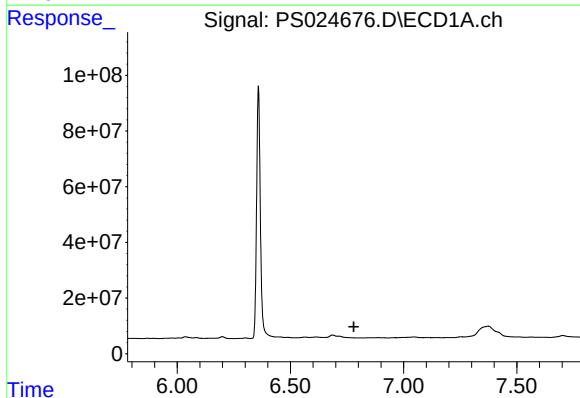


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 6.780 min
Response: 0
Conc: N.D.

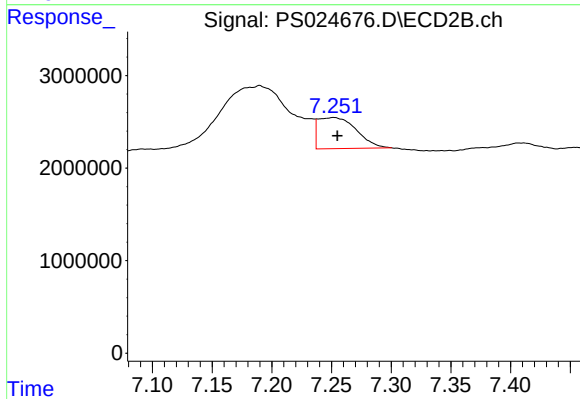

#7 MCPA


R.T.: 7.252 min
Delta R.T.: -0.003 min
Response: 7424657
Conc: 2.32 ug/ml

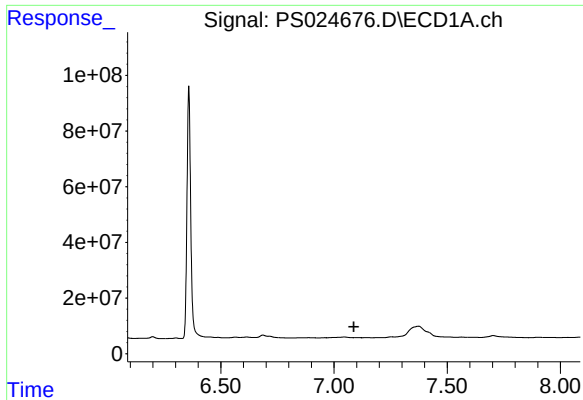

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.088 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

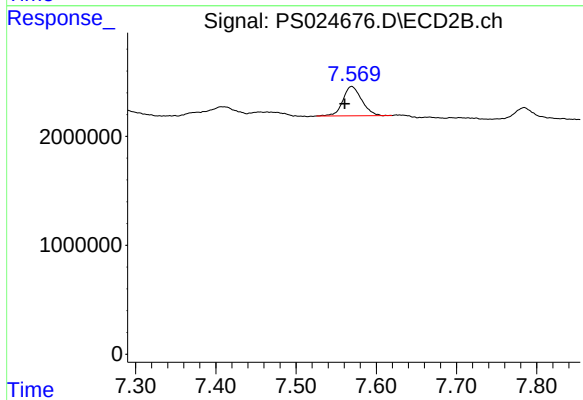


#8 DICHLORPROP

R.T.: 7.569 min
Delta R.T.: 0.009 min
Response: 4396916
Conc: 5.85 ng/ml

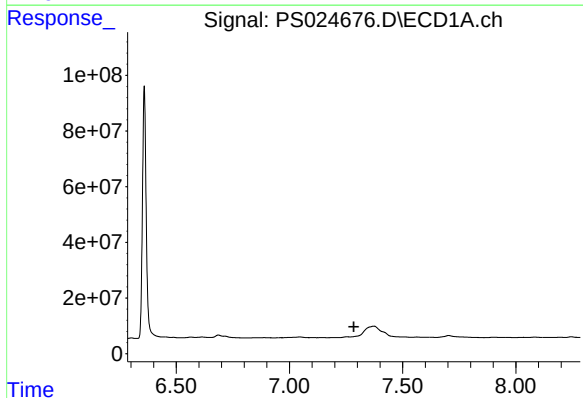


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 7.284 min
Response: 0
Conc: N.D.

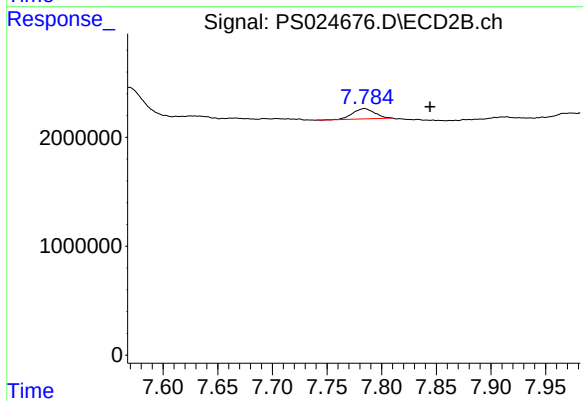

#9 2,4-D


R.T.: 7.784 min
Delta R.T.: -0.060 min
Response: 1341084
Conc: 1.46 ng/ml

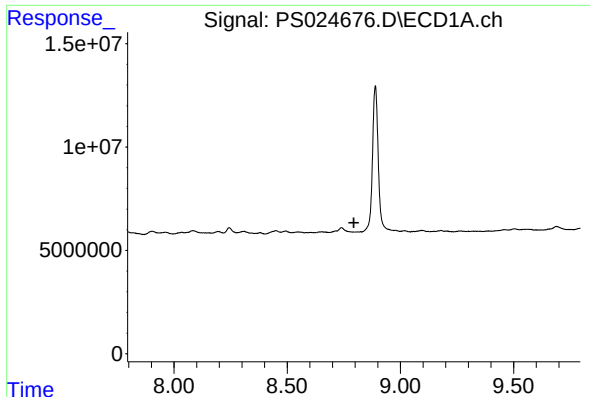

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 8.795 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

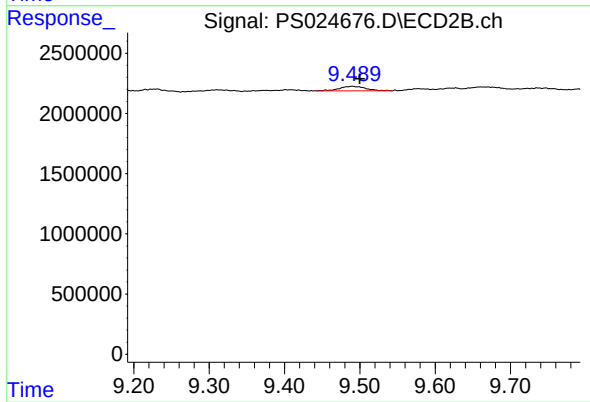

#13 2,4-DB

R.T.: 9.490 min
Delta R.T.: -0.010 min
Response: 928480
Conc: 1.82 ng/ml