

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110425\
 Data File : PS032265.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Nov 2025 09:07
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 00:24:13 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.301	0.000	1190312	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	2.673	0.000	46189471	0	6.434	N.D. #
2) T	3,5-DICHL...	6.444	0.000	7452964	0	1.153	N.D. #
5) T	DICAMBA	7.470	7.819	1313083	5063081	<MDL	<MDL #
6) T	MCP	7.636	7.915	382824	3216198	<MDL	<MDL #
7) T	MCPA	7.791	0.000	225003	0	<MDL	N.D. #
8) T	DICHLORPROP	8.188	0.000	1895907	0	<MDL	N.D. #
10) T	Pentachlo...	8.709	9.368	3398958	4494163	<MDL	<MDL #
11) T	2,4,5-TP ...	9.301	9.793f	8263909	-2885148	<MDL	N.D. #
12) T	2,4,5-T	9.613f	10.180	8718176	3557929	<MDL	<MDL #
13) T	2,4-DB	10.152	10.756	468037	2866751	<MDL	<MDL #
14) T	DINOSEB	11.356	11.125	83879622	2873826	4.031	<MDL #
15) T	Picloram	11.168	12.194f	910922	26631076	<MDL	<MDL #
16) T	DCPA	11.648	0.000	6644120	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110425\
Data File : PS032265.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Nov 2025 09:07
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 00:24:13 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

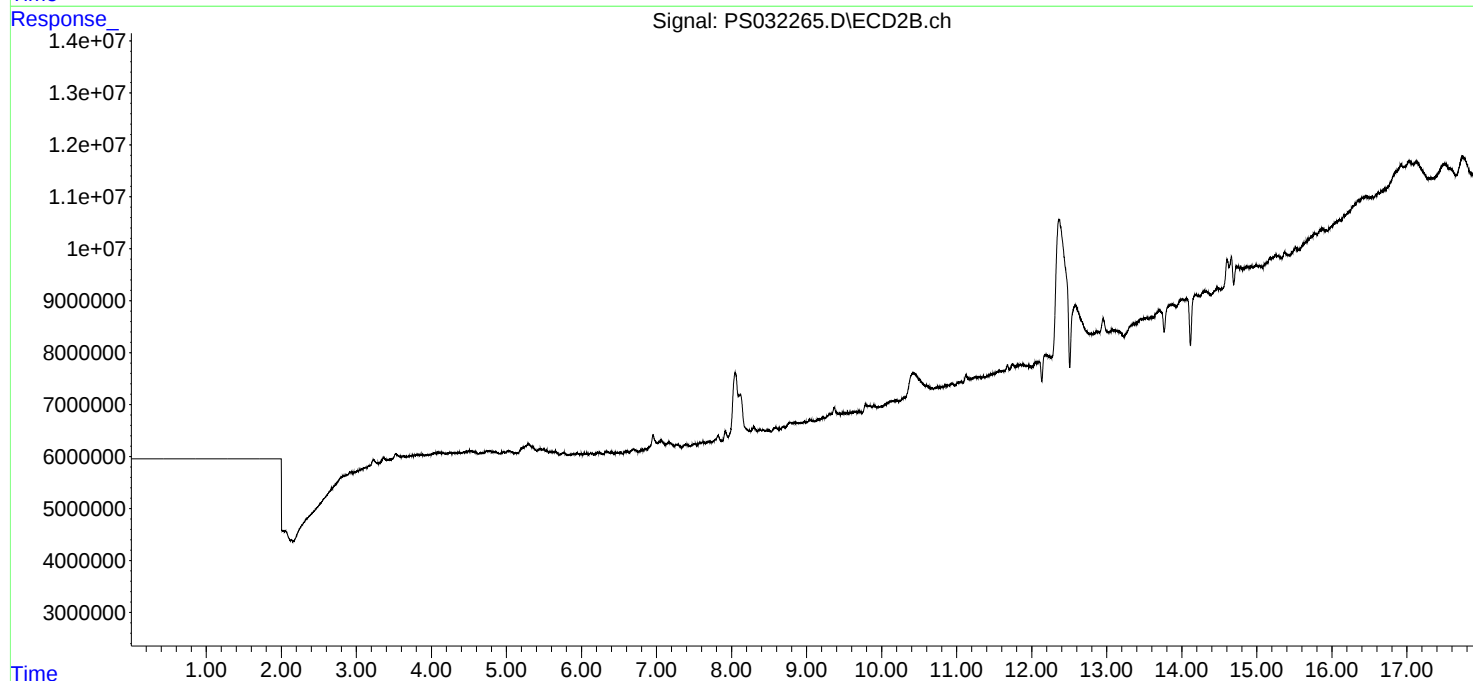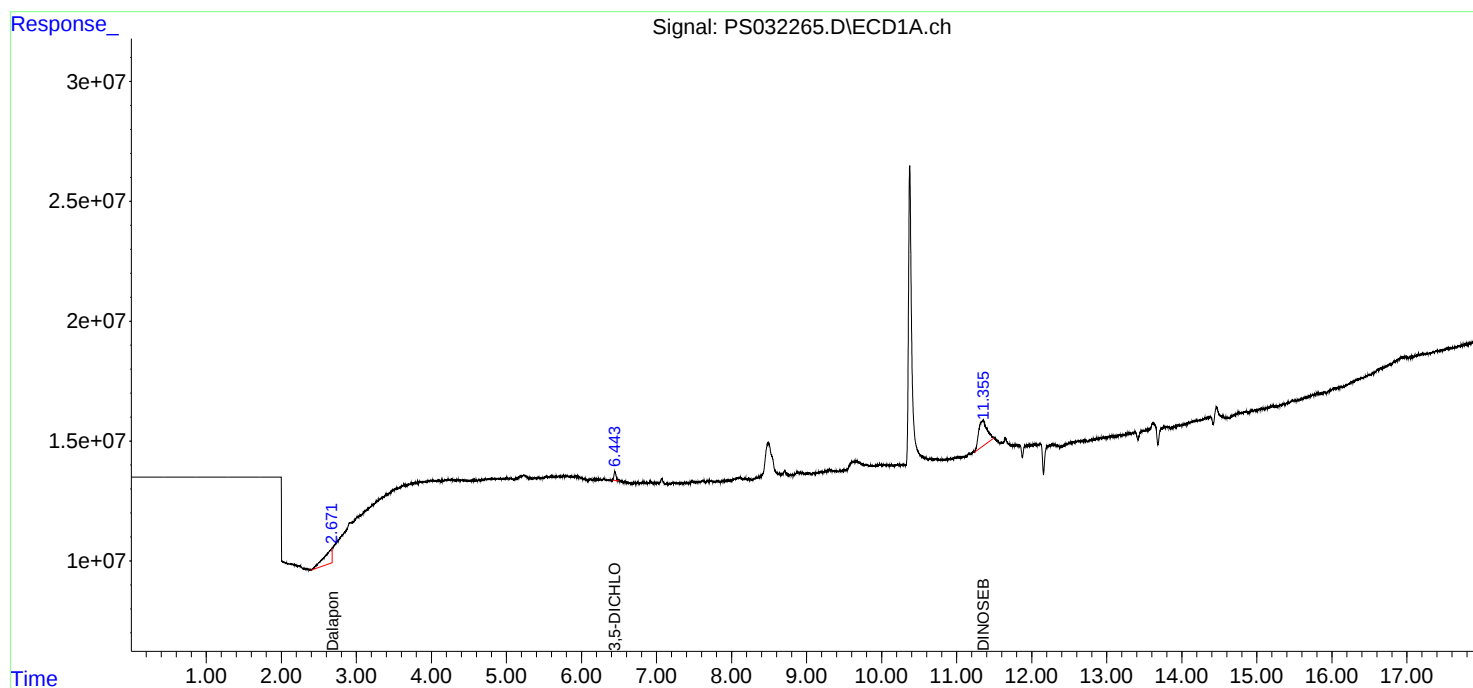


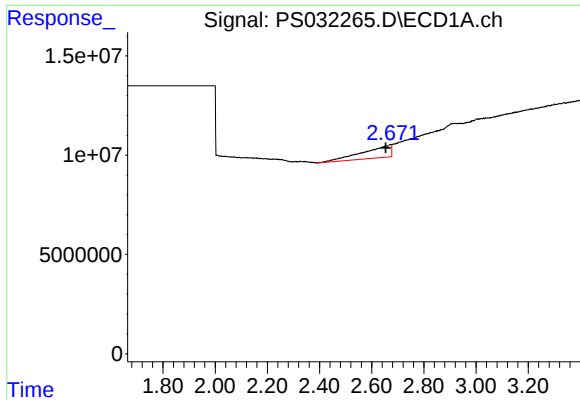

#1 Dalapon


R.T.: 2.673 min
Delta R.T.: 0.019 min
Response: 46189471
Conc: 6.43 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

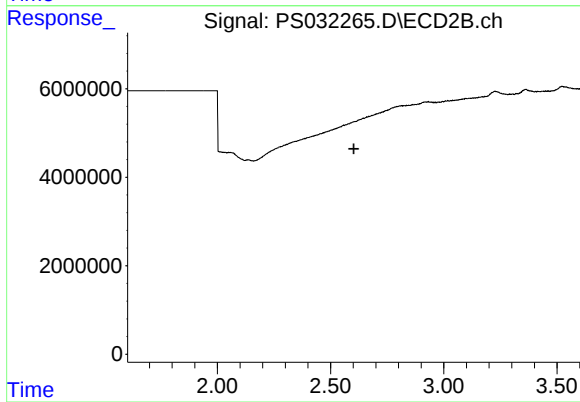


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.603 min
Response: 0
Conc: N.D.

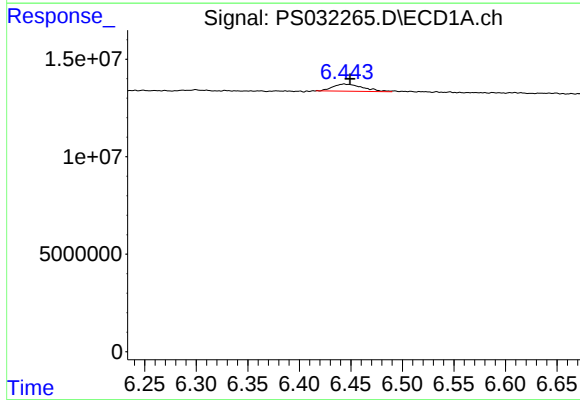


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.444 min
Delta R.T.: -0.006 min
Response: 7452964
Conc: 1.15 ng/ml

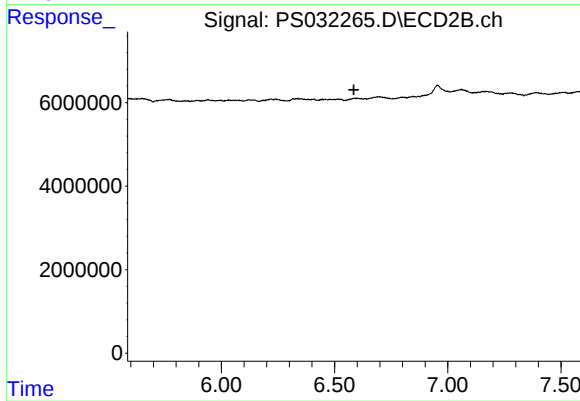

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T. : 6.585 min
Response: 0
Conc: N.D.

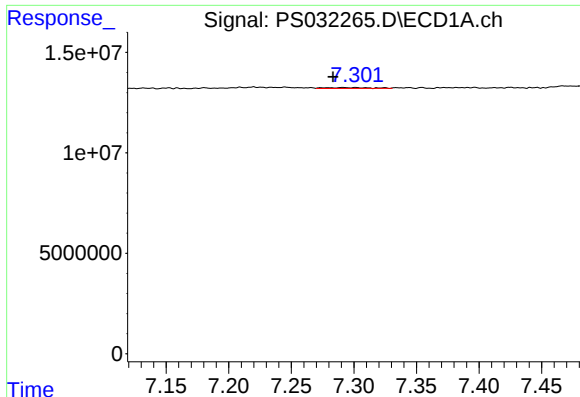

#4 2,4-DCAA


R.T.: 7.301 min
Delta R.T.: 0.017 min
Response: 1190312
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

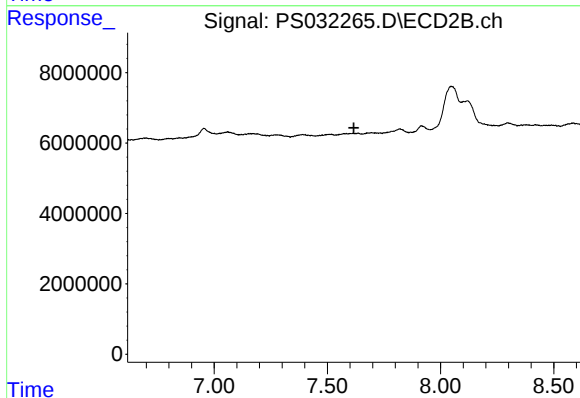


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.617 min
Response: 0
Conc: N.D.

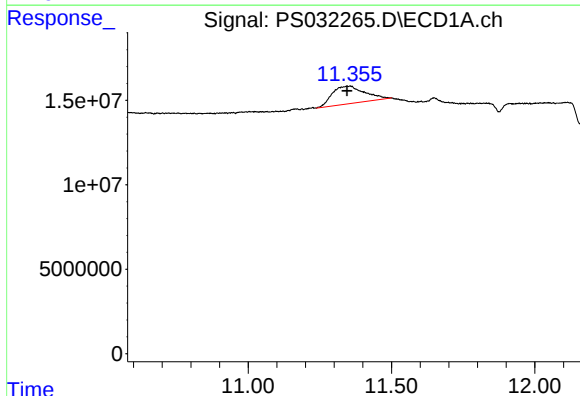

#14 DINOSEB

R.T.: 11.356 min
Delta R.T.: 0.011 min
Response: 83879622
Conc: 4.03 ng/ml

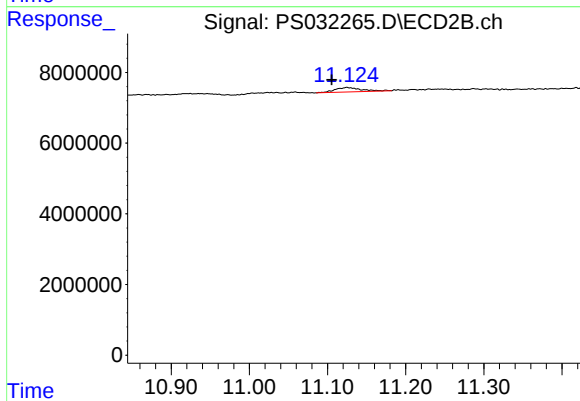

#14 DINOSEB

R.T.: 11.125 min
Delta R.T.: 0.020 min
Response: 2873826
Conc: N.D.