

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS110425\  
 Data File : PS032275.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 04 Nov 2025 13:48  
 Operator : AR\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Nov 05 00:26:36 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS110325.M  
 Quant Title : 8080.M  
 QLast Update : Tue Nov 04 04:59:50 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound     | RT#1    | RT#2    | Resp#1   | Resp#2   | ng/ml   | ng/ml    |
|-----------------------------|--------------|---------|---------|----------|----------|---------|----------|
| -----                       |              |         |         |          |          |         |          |
| System Monitoring Compounds |              |         |         |          |          |         |          |
| 4) S                        | 2,4-DCAA     | 7.277   | 7.612   | 1843.1E6 | 1784.4E6 | 406.743 | 489.471  |
| Target Compounds            |              |         |         |          |          |         |          |
| 1) T                        | Dalapon      | 0.000   | 2.638f  | 0        | 38173192 | N.D.    | 5.489    |
| 2) T                        | 3,5-DICHL... | 6.434   | 0.000   | 2319720  | 0        | <MDL    | N.D. #   |
| 5) T                        | DICAMBA      | 7.458   | 0.000   | 946039   | 0        | <MDL    | N.D. #   |
| 6) T                        | MCP          | 7.642   | 7.905   | 55312    | 3999420  | <MDL    | <MDL #   |
| 7) T                        | MCPA         | 7.816   | 8.105f  | 2096316  | 3278497  | <MDL    | <MDL #   |
| 8) T                        | DICHLORPROP  | 8.176   | 0.000   | 837060   | 0        | <MDL    | N.D. #   |
| 9) T                        | 2,4-D        | 8.384f  | 8.819f  | 243750   | 4758445  | <MDL    | <MDL #   |
| 10) T                       | Pentachlo... | 8.701   | 9.358   | 459850   | 6297532  | <MDL    | <MDL #   |
| 11) T                       | 2,4,5-TP ... | 9.275   | 0.000   | 3931093  | 0        | <MDL    | N.D. #   |
| 12) T                       | 2,4,5-T      | 9.594   | 10.195  | 1106864  | 21338286 | <MDL    | <MDL #   |
| 13) T                       | 2,4-DB       | 10.159  | 10.756  | 2537496  | 49488836 | <MDL    | 13.122 # |
| 14) T                       | DINOSEB      | 11.342  | 0.000   | 1112151  | 0        | <MDL    | N.D. #   |
| 15) T                       | Picloram     | 11.212f | 0.000   | 7249139  | 0        | <MDL    | N.D. #   |
| 16) T                       | DCPA         | 0.000   | 12.095f | 0        | 4414654  | N.D.    | <MDL     |
| -----                       |              |         |         |          |          |         |          |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS110425\  
Data File : PS032275.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Nov 2025 13:48  
Operator : AR\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :  
I.BLK

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Nov 05 00:26:36 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS110325.M  
Quant Title : 8080.M  
QLast Update : Tue Nov 04 04:59:50 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

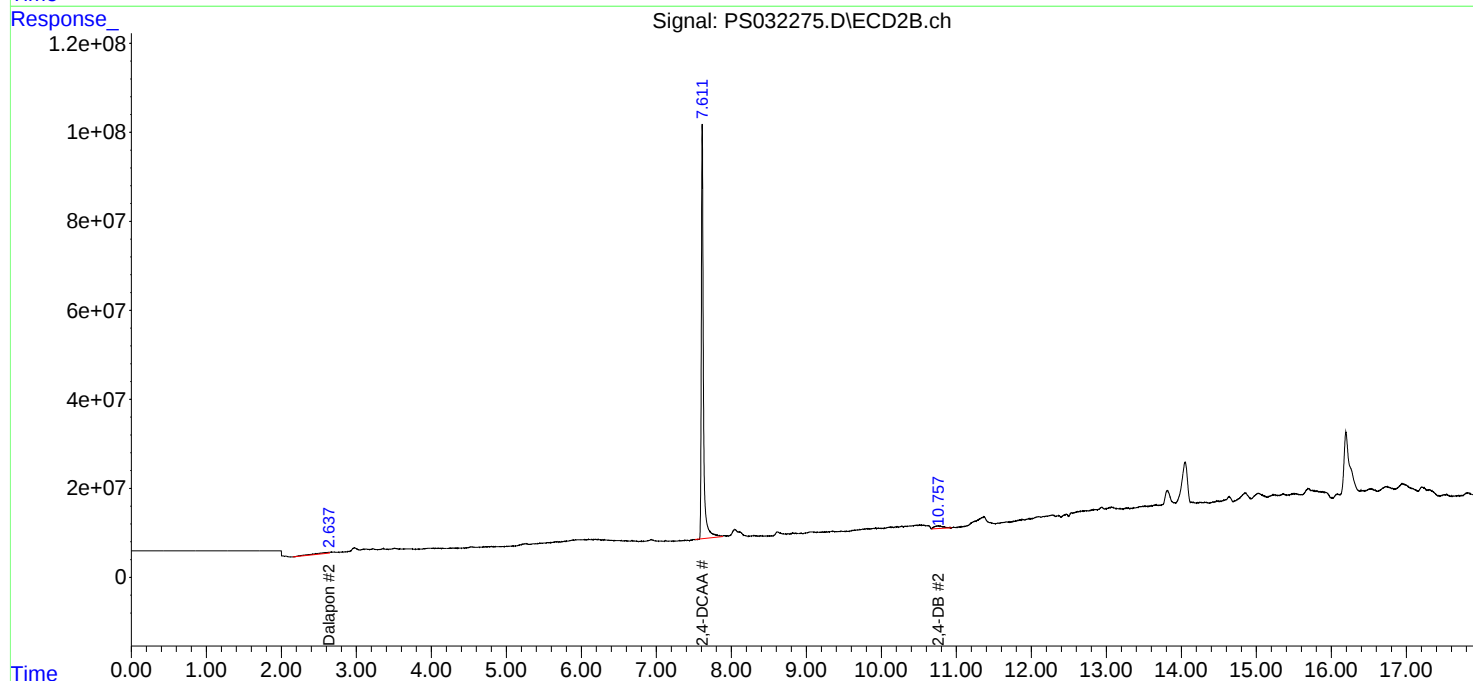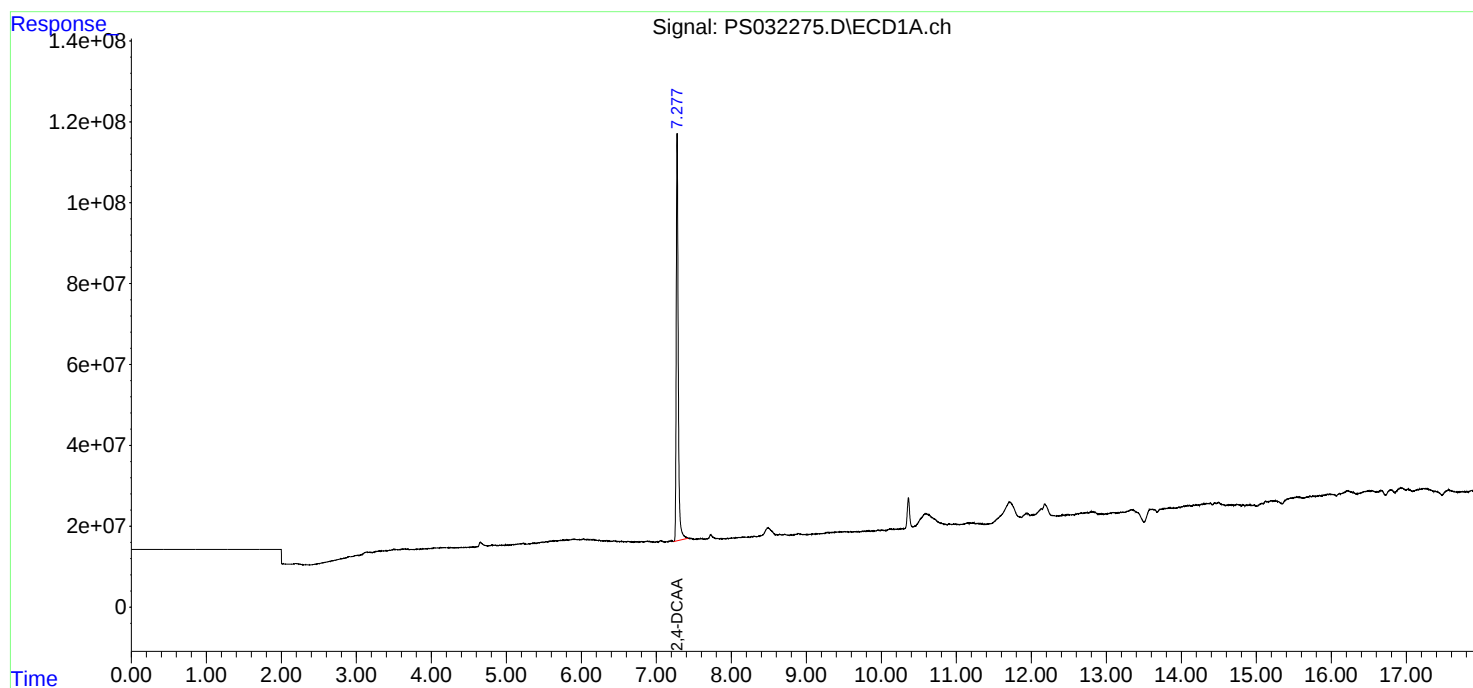


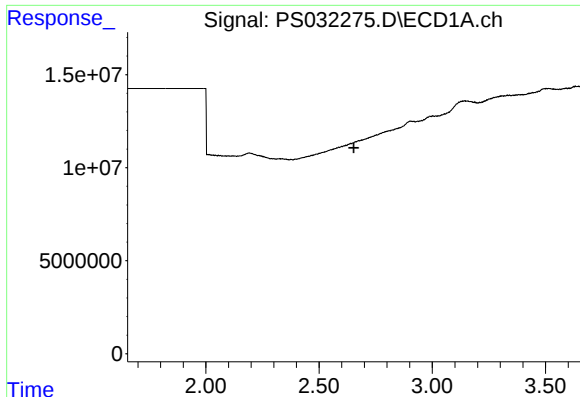

#1 Dalapon


R.T.: 0.000 min  
Exp R.T.: 2.654 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :  
I.BLK

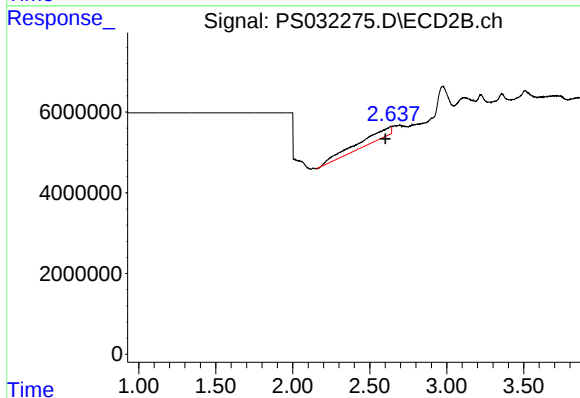


#1 Dalapon

R.T.: 2.638 min  
Delta R.T.: 0.035 min  
Response: 38173192  
Conc: 5.49 ng/ml

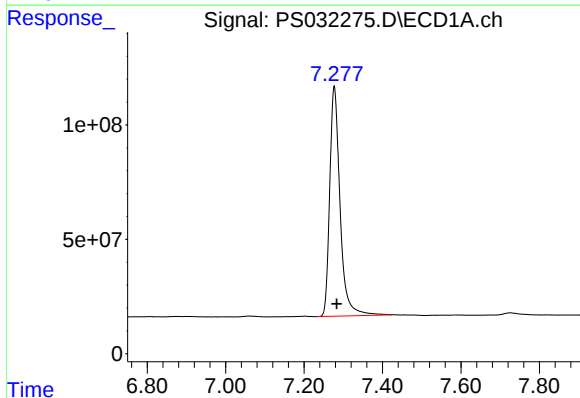


#4 2,4-DCAA

R.T.: 7.277 min  
Delta R.T.: -0.006 min  
Response: 1843065952  
Conc: 406.74 ng/ml

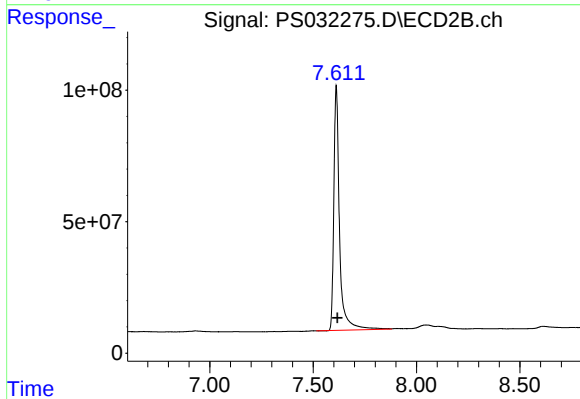

#4 2,4-DCAA


R.T.: 7.612 min  
Delta R.T.: -0.006 min  
Response: 1784365262  
Conc: 489.47 ng/ml

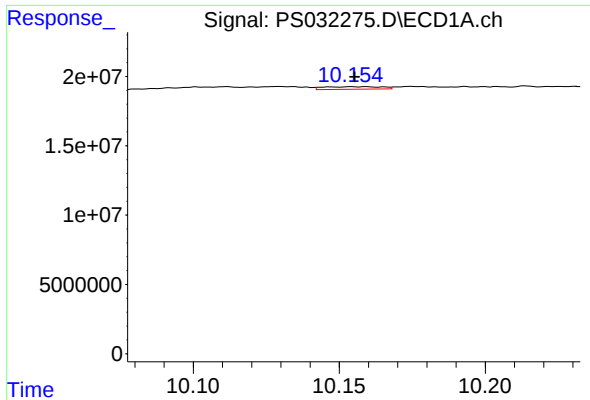

#13 2,4-DB

R.T.: 10.159 min  
Delta R.T.: 0.004 min  
Response: 2537496  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :  
I.BLK

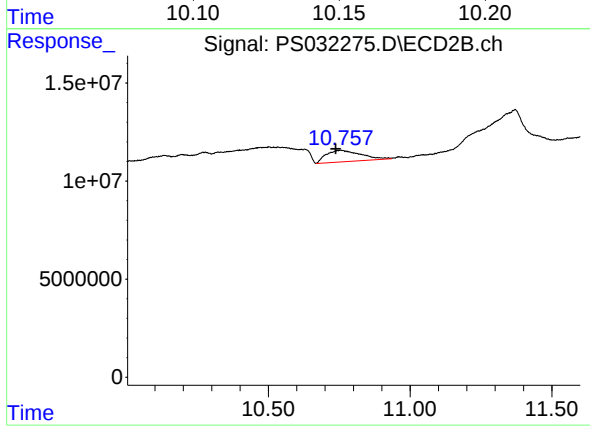

#13 2,4-DB

R.T.: 10.756 min  
Delta R.T.: 0.019 min  
Response: 49488836  
Conc: 13.12 ng/ml