

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111124\
 Data File : PS028393.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Nov 2024 10:24
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 11 23:08:28 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110924.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 08 17:46:43 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.247	7.752	1410.8E6	752.2E6	511.038	472.080
Target Compounds							
2) T	3,5-DICHL...	6.433	0.000	670966	0	<MDL	N.D. #
3) T	4-Nitroph...	7.037	0.000	9028183	0	4.869	N.D. #
6) T	MCP	7.674f	0.000	19335008	0	2.364	N.D. #
7) T	MCPA	7.818f	8.270f	532440	8578904	<MDL	1.071 #
8) T	DICHLORPROP	8.137	8.721f	147457	7571348	<MDL	4.251 #
11) T	2,4,5-TP ...	9.239	9.937f	1449593	3912024	<MDL	<MDL #
12) T	2,4,5-T	9.558	10.329	434885	6549628	<MDL	<MDL #
13) T	2,4-DB	10.105	0.000	1154971	0	<MDL	N.D. #
15) T	Picloram	11.147	12.375	17088300	15041859	<MDL	1.045 #
16) T	DCPA	11.632	12.375f	2135555	15041859	<MDL	1.342 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111124\
Data File : PS028393.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Nov 2024 10:24
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 11 23:08:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110924.M
Quant Title : 8080.M
QLast Update : Fri Nov 08 17:46:43 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

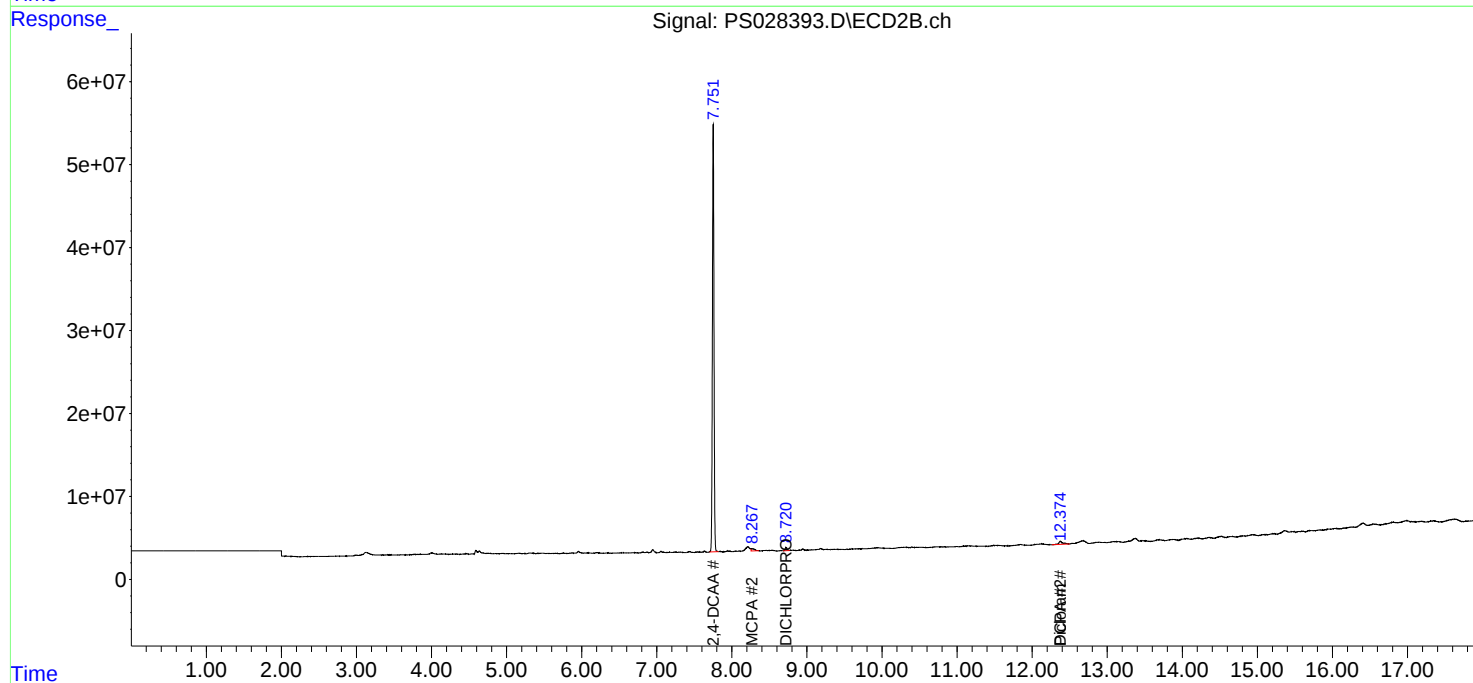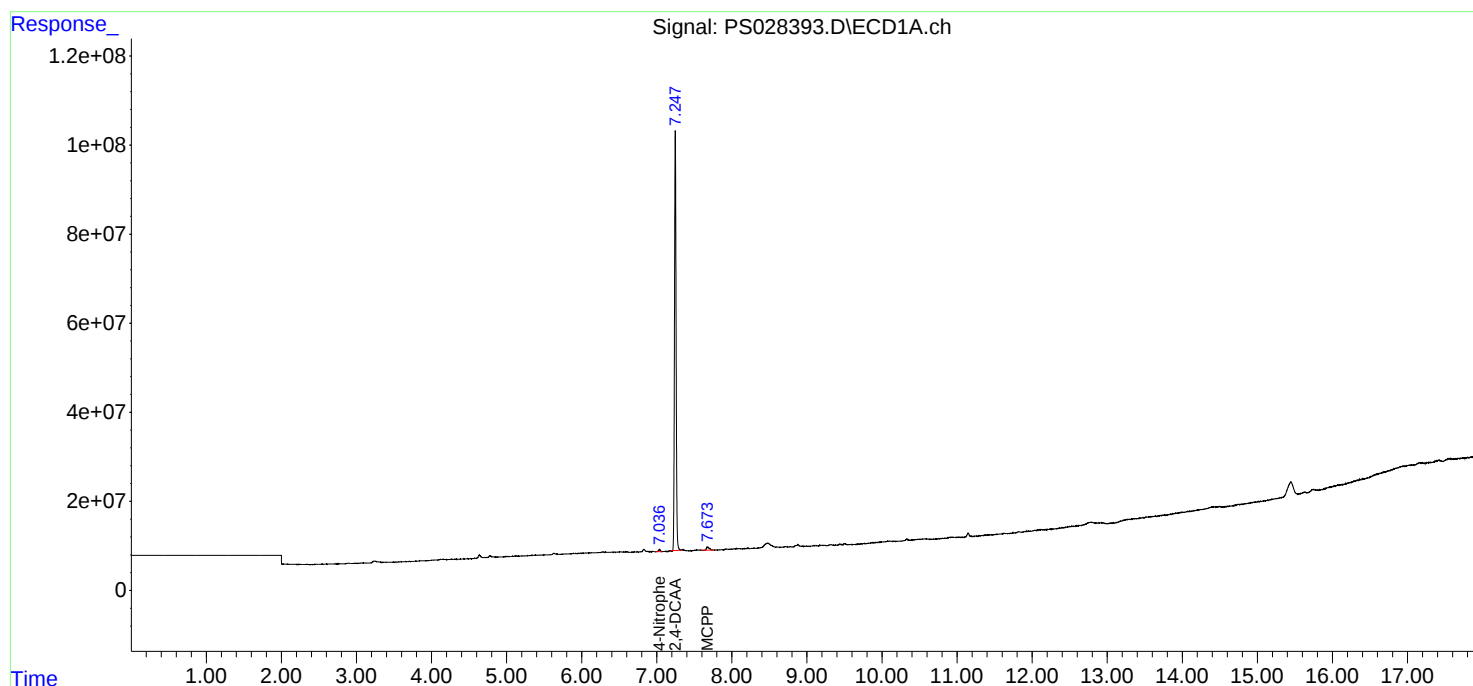


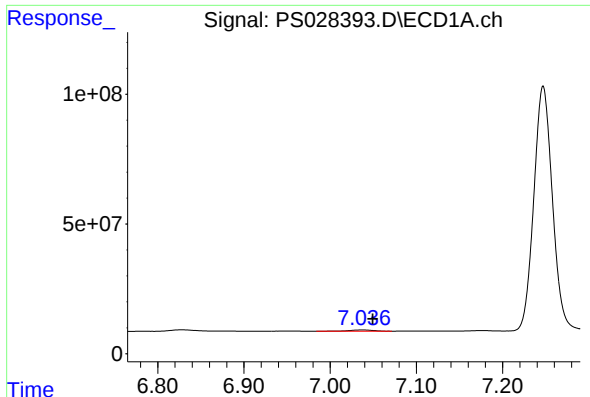

#3 4-Nitrophenol


R.T.: 7.037 min
Delta R.T.: -0.012 min
Response: 9028183
Conc: 4.87 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

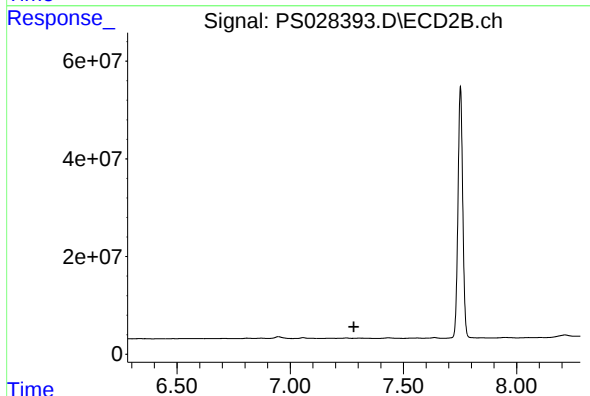


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.281 min
Response: 0
Conc: N.D.

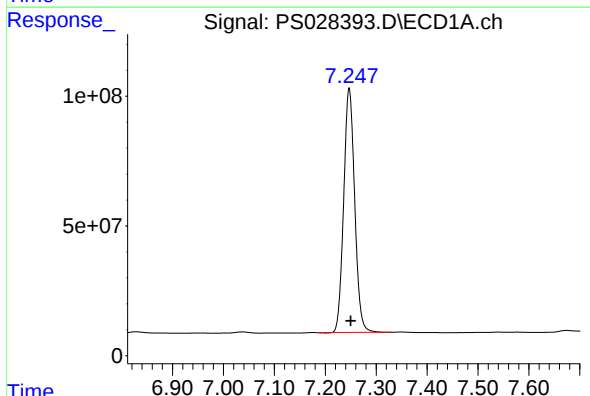


#4 2,4-DCAA

R.T.: 7.247 min
Delta R.T.: -0.003 min
Response: 1410849503
Conc: 511.04 ng/ml

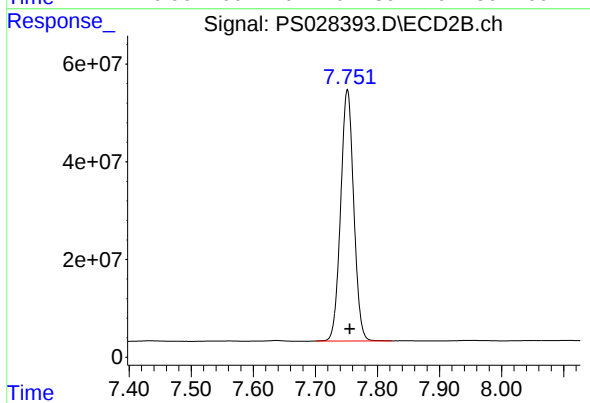

#4 2,4-DCAA


R.T.: 7.752 min
Delta R.T.: -0.004 min
Response: 752222628
Conc: 472.08 ng/ml

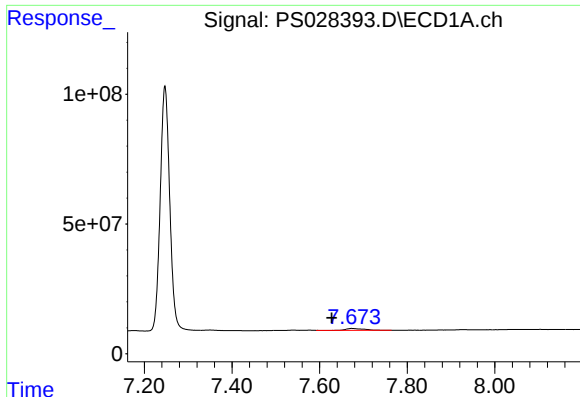

#6 MCPP


R.T.: 7.674 min
Delta R.T.: 0.047 min
Response: 19335008
Conc: 2.36 ug/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

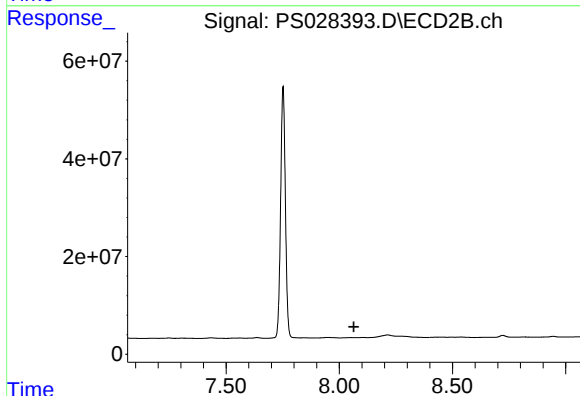


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 8.064 min
Response: 0
Conc: N.D.

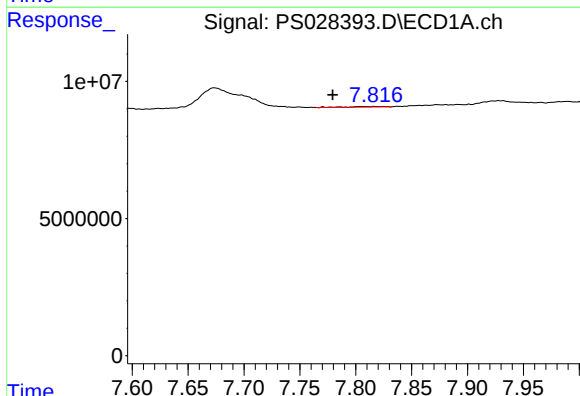


#7 MCPA

R.T.: 7.818 min
Delta R.T.: 0.038 min
Response: 532440
Conc: N.D.

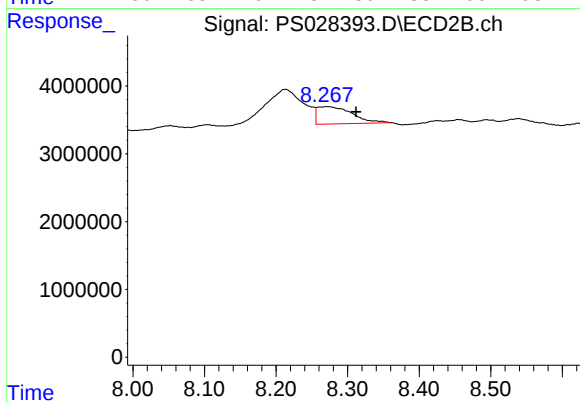

#7 MCPA


R.T.: 8.270 min
Delta R.T.: -0.041 min
Response: 8578904
Conc: 1.07 ug/ml

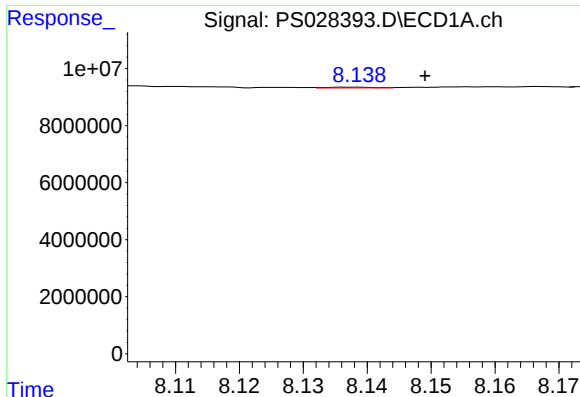

#8 DICHLORPROP


R.T.: 8.137 min
Delta R.T.: -0.012 min
Response: 147457
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

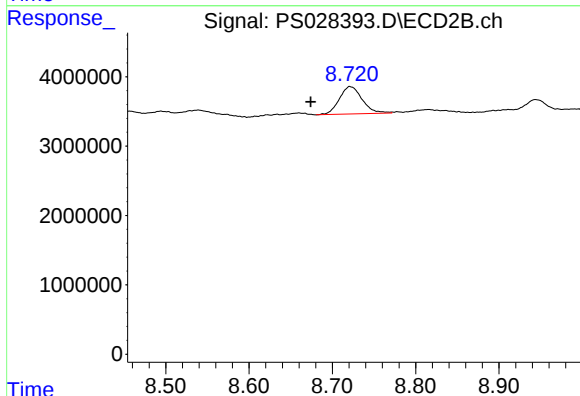


#8 DICHLORPROP

R.T.: 8.721 min
Delta R.T.: 0.047 min
Response: 7571348
Conc: 4.25 ng/ml

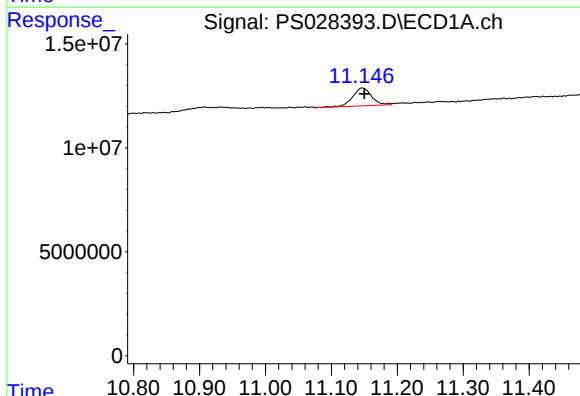


#15 Picloram

R.T.: 11.147 min
Delta R.T.: -0.003 min
Response: 17088300
Conc: N.D.

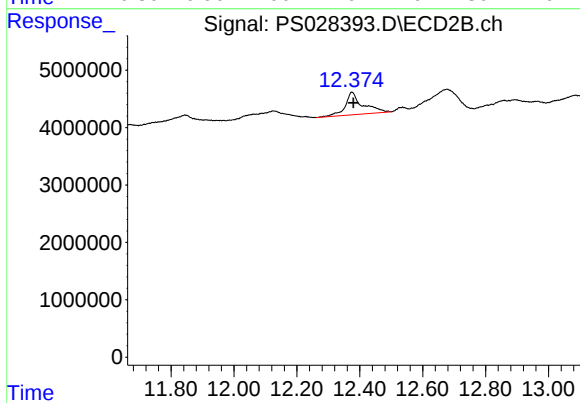

#15 Picloram


R.T.: 12.375 min
Delta R.T.: -0.004 min
Response: 15041859
Conc: 1.05 ng/ml

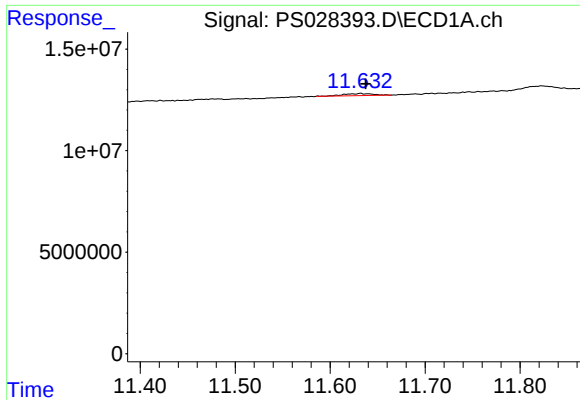

#16 DCPA

R.T.: 11.632 min
Delta R.T.: -0.006 min
Response: 2135555
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

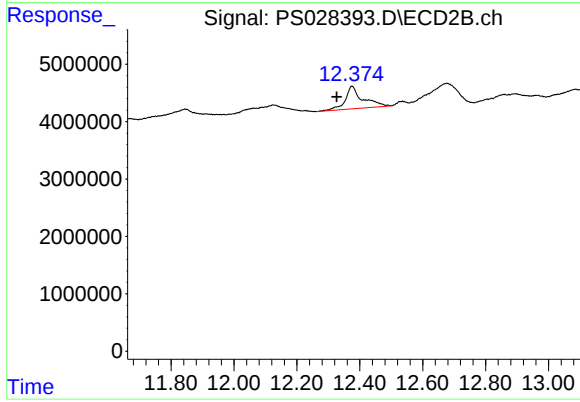

#16 DCPA

R.T.: 12.375 min
Delta R.T.: 0.049 min
Response: 15041859
Conc: 1.34 ng/ml