

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111124\
 Data File : PS028405.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Nov 2024 16:09
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 11 23:19:06 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110924.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 08 17:46:43 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.247	7.752	1410.9E6	751.7E6	511.039	471.753
Target Compounds							
1) T	Dalapon	2.658	0.000	2123875	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.407	0.000	936638	0	<MDL	N.D. #
3) T	4-Nitroph...	7.039	0.000	7148152	0	3.855	N.D. #
5) T	DICAMBA	7.438	7.951	227530	3092874	<MDL	<MDL #
6) T	MCPD	7.673f	8.108f	20868120	2830027	2.552	<MDL #
7) T	MCPA	0.000	8.274f	0	16829215	N.D.	2.102
8) T	DICHLORPROP	8.108f	8.722f	3773080	9257642	1.217	5.197 #
10) T	Pentachlo...	0.000	9.524	0	2372935	N.D.	<MDL
11) T	2,4,5-TP ...	9.252	9.932	2743044	15257792	<MDL	1.440 #
12) T	2,4,5-T	9.557	10.303f	9887181	4988647	<MDL	<MDL #
14) T	DINOSEB	11.338	0.000	5401085	0	<MDL	N.D. #
15) T	Picloram	11.139	12.374	50582545	22902701	1.611	1.591
16) T	DCPA	11.624	12.374f	3974087	22902701	<MDL	2.043 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111124\
Data File : PS028405.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Nov 2024 16:09
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 11 23:19:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110924.M
Quant Title : 8080.M
QLast Update : Fri Nov 08 17:46:43 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

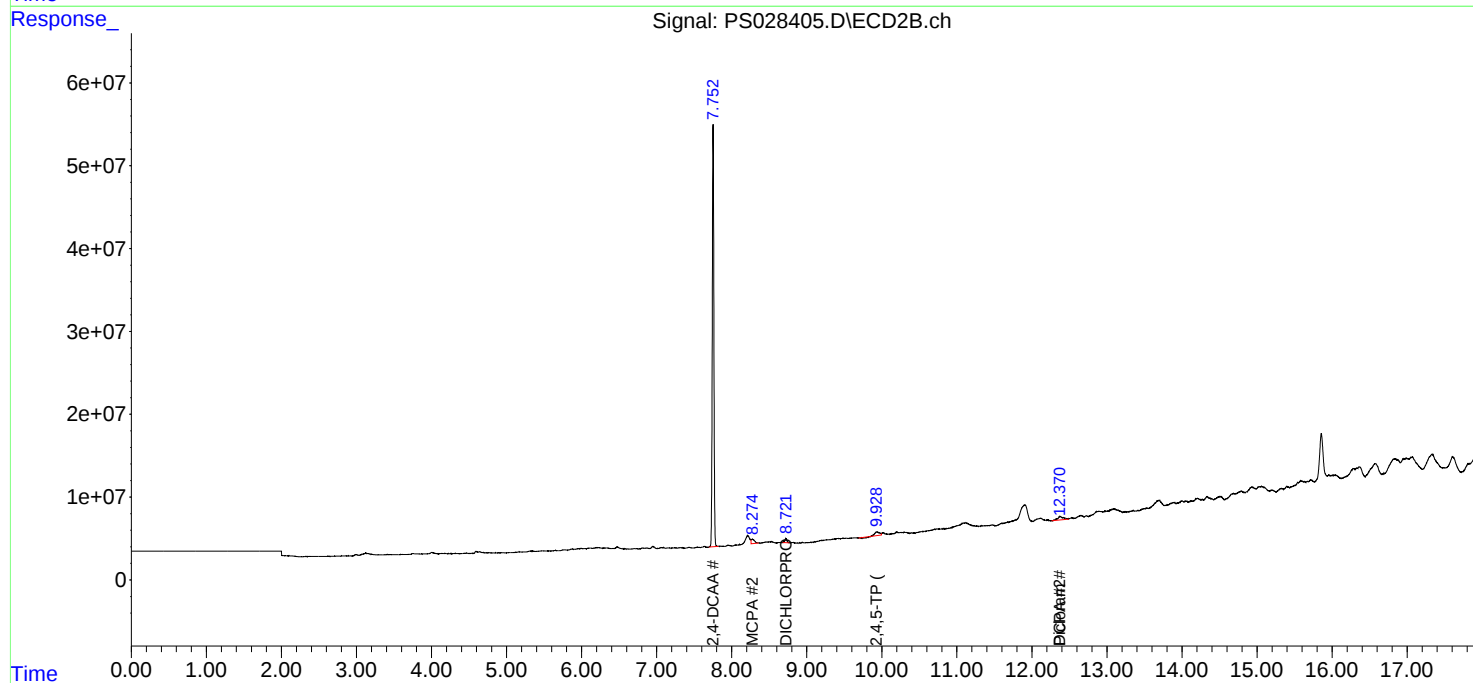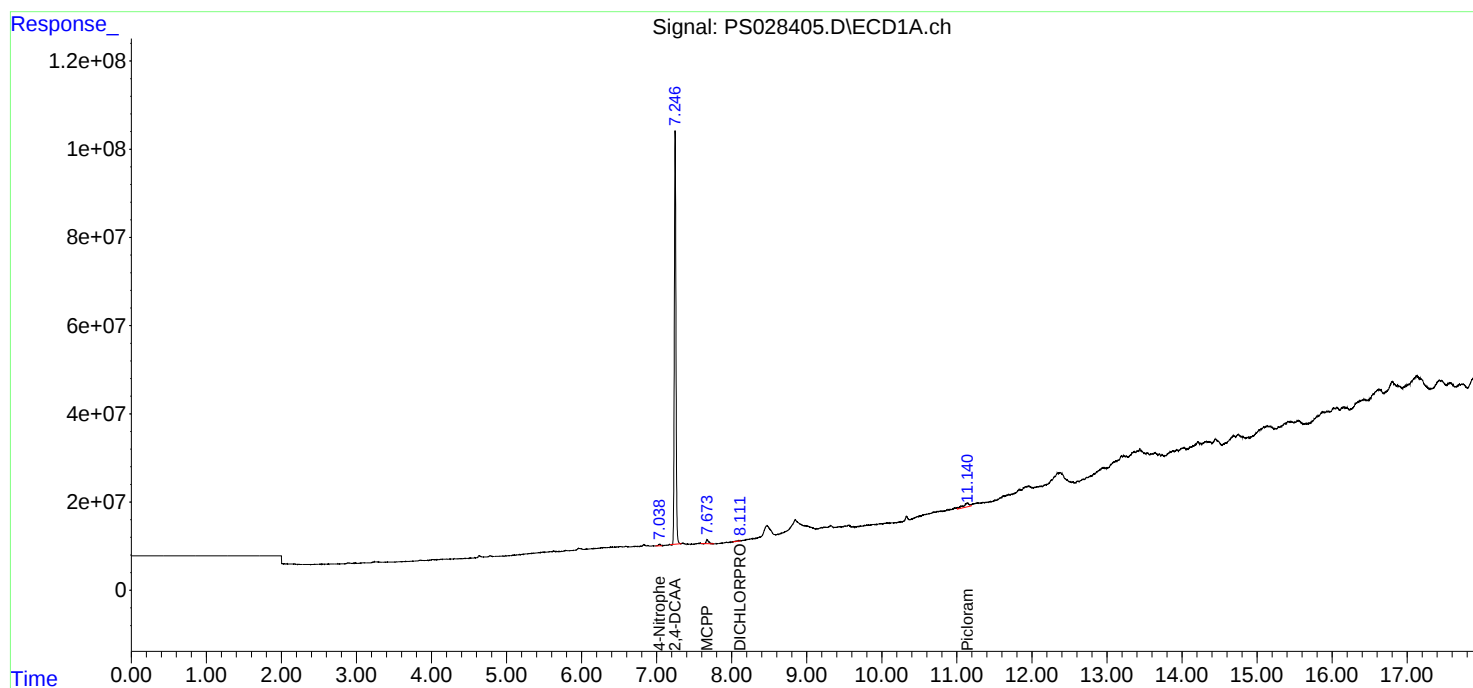


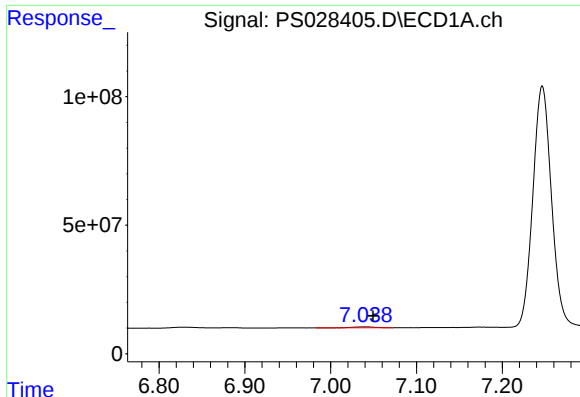

#3 4-Nitrophenol


R.T.: 7.039 min
Delta R.T.: -0.010 min
Response: 7148152
Conc: 3.86 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

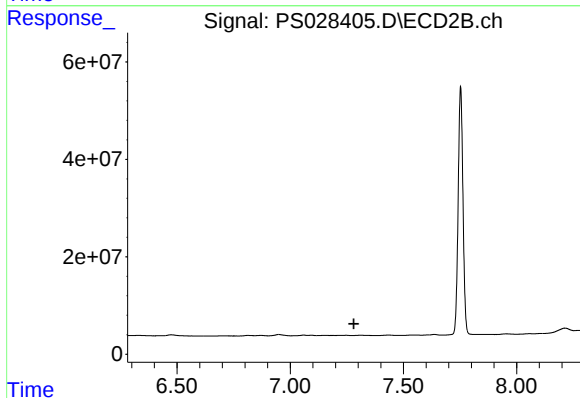


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.281 min
Response: 0
Conc: N.D.

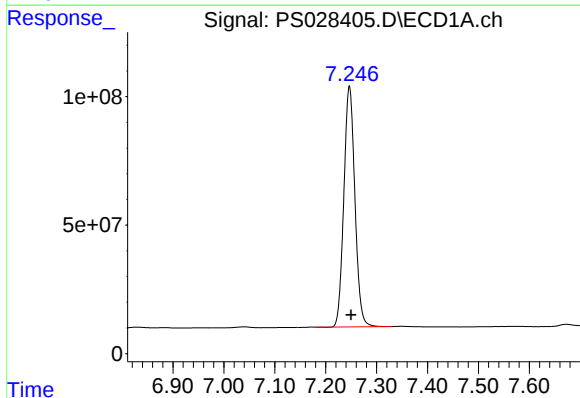


#4 2,4-DCAA

R.T.: 7.247 min
Delta R.T.: -0.003 min
Response: 1410854111
Conc: 511.04 ng/ml

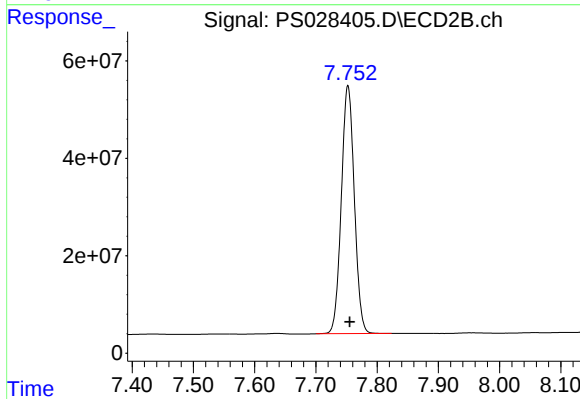

#4 2,4-DCAA


R.T.: 7.752 min
Delta R.T.: -0.003 min
Response: 751701019
Conc: 471.75 ng/ml

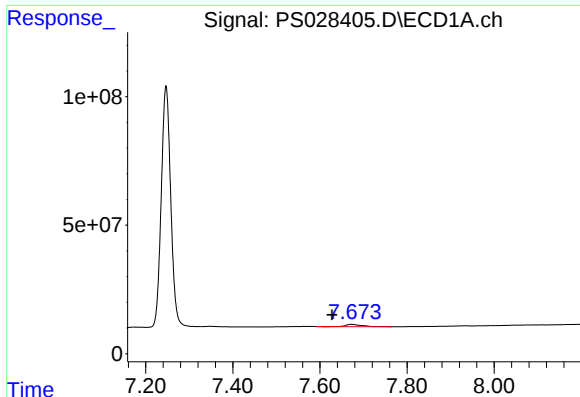

#6 MCPP


R.T.: 7.673 min
Delta R.T.: 0.045 min
Response: 20868120
Conc: 2.55 ug/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

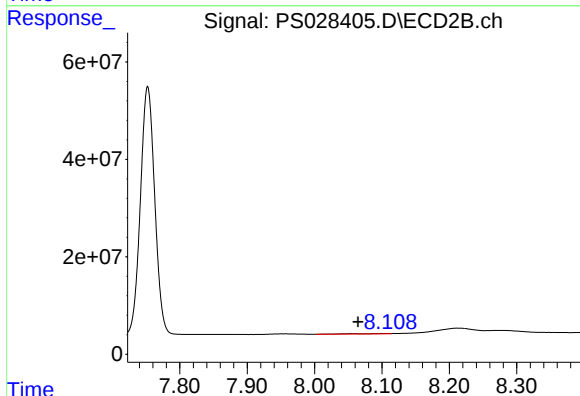


#6 MCPP

R.T.: 8.108 min
Delta R.T.: 0.044 min
Response: 2830027
Conc: N.D.

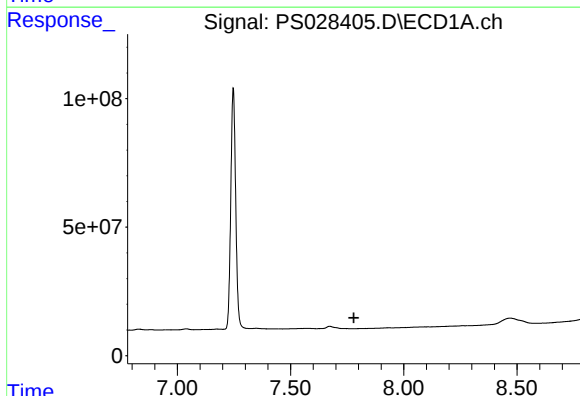


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.779 min
Response: 0
Conc: N.D.

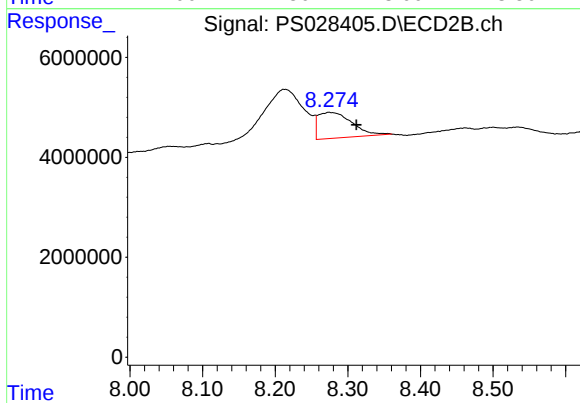

#7 MCPA


R.T.: 8.274 min
Delta R.T.: -0.038 min
Response: 16829215
Conc: 2.10 ug/ml

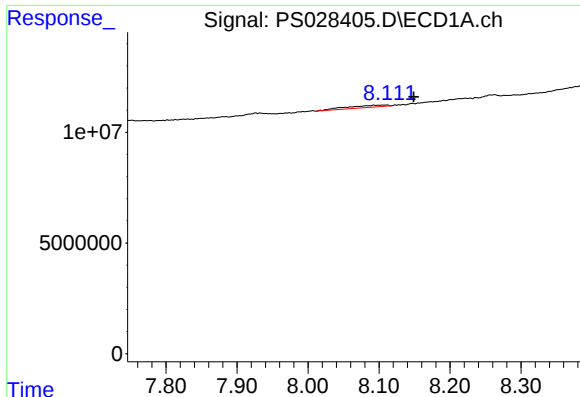

#8 DICHLORPROP


R.T.: 8.108 min
Delta R.T.: -0.041 min
Response: 3773080
Conc: 1.22 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

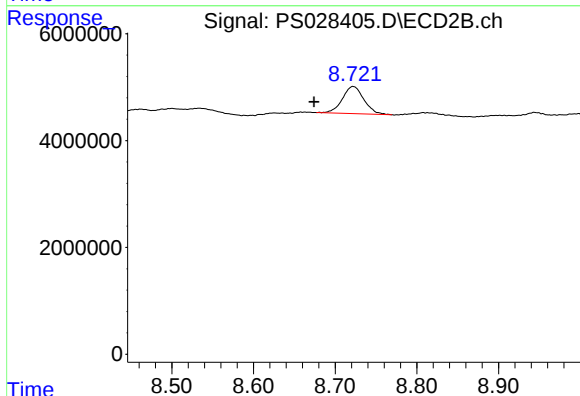


#8 DICHLORPROP

R.T.: 8.722 min
Delta R.T.: 0.048 min
Response: 9257642
Conc: 5.20 ng/ml

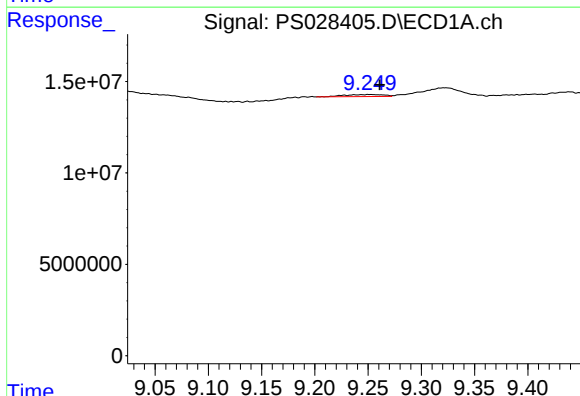


#11 2,4,5-TP (SILVEX)

R.T.: 9.252 min
Delta R.T.: -0.009 min
Response: 2743044
Conc: N.D.

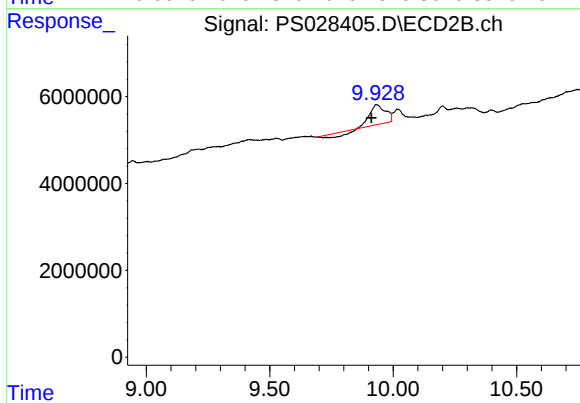

#11 2,4,5-TP (SILVEX)


R.T.: 9.932 min
Delta R.T.: 0.021 min
Response: 15257792
Conc: 1.44 ng/ml

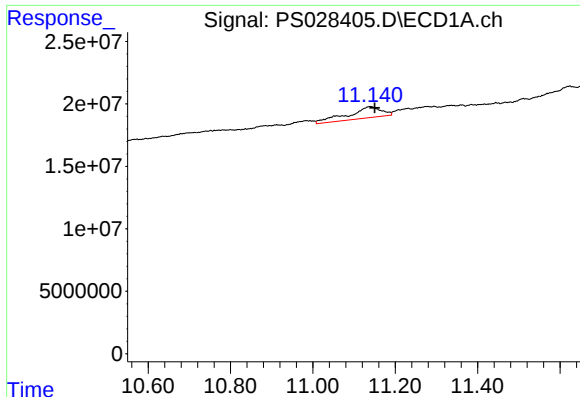

#15 Picloram


R.T.: 11.139 min
Delta R.T.: -0.011 min
Response: 50582545
Conc: 1.61 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

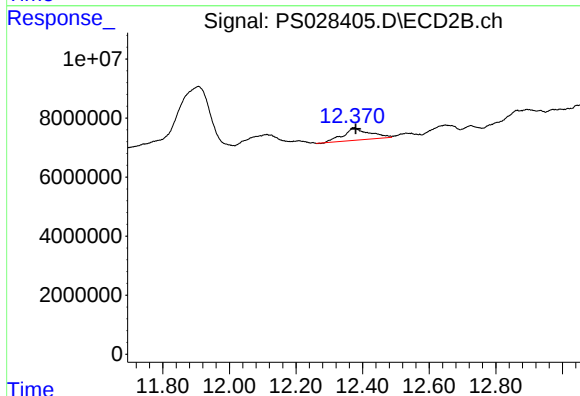


#15 Picloram

R.T.: 12.374 min
Delta R.T.: -0.006 min
Response: 22902701
Conc: 1.59 ng/ml

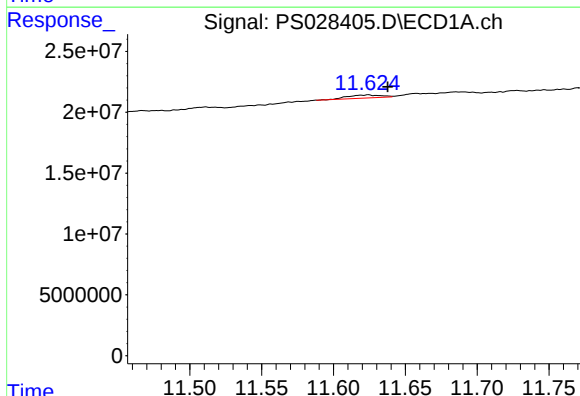

#16 DCPA

R.T.: 11.624 min
Delta R.T.: -0.014 min
Response: 3974087
Conc: N.D.

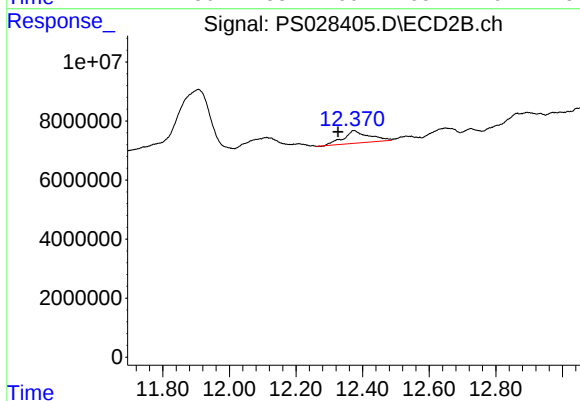

#16 DCPA

R.T.: 12.374 min
Delta R.T.: 0.047 min
Response: 22902701
Conc: 2.04 ng/ml