

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111124\
 Data File : PS028417.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Nov 2024 20:58
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 11 23:31:06 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110924.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 08 17:46:43 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.245	7.751	1417.0E6	745.5E6	513.251	467.848
Target Compounds							
1) T	Dalapon	2.676f	0.000	831594	0	<MDL	N.D. #
3) T	4-Nitroph...	7.038	0.000	5595950	0	3.018	N.D. #
5) T	DICAMBA	0.000	7.948	0	4313720	N.D.	<MDL
6) T	MCP	7.672f	0.000	24507953	0	2.997	N.D. #
7) T	MCPA	0.000	8.273f	0	9442582	N.D.	1.179
8) T	DICHLORPROP	0.000	8.720f	0	11255092	N.D.	6.319
10) T	Pentachlo...	0.000	9.529	0	1132225	N.D.	<MDL
11) T	2,4,5-TP ...	9.310f	0.000	6494770	0	<MDL	N.D. #
12) T	2,4,5-T	9.555	10.312	941892	3952469	<MDL	<MDL #
14) T	DINOSEB	11.354	0.000	3451569	0	<MDL	N.D. #
15) T	Picloram	11.145	12.374	49477853	9214880	1.575	<MDL #
16) T	DCPA	11.615	12.374f	2903662	9214880	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111124\
Data File : PS028417.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Nov 2024 20:58
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 11 23:31:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110924.M
Quant Title : 8080.M
QLast Update : Fri Nov 08 17:46:43 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

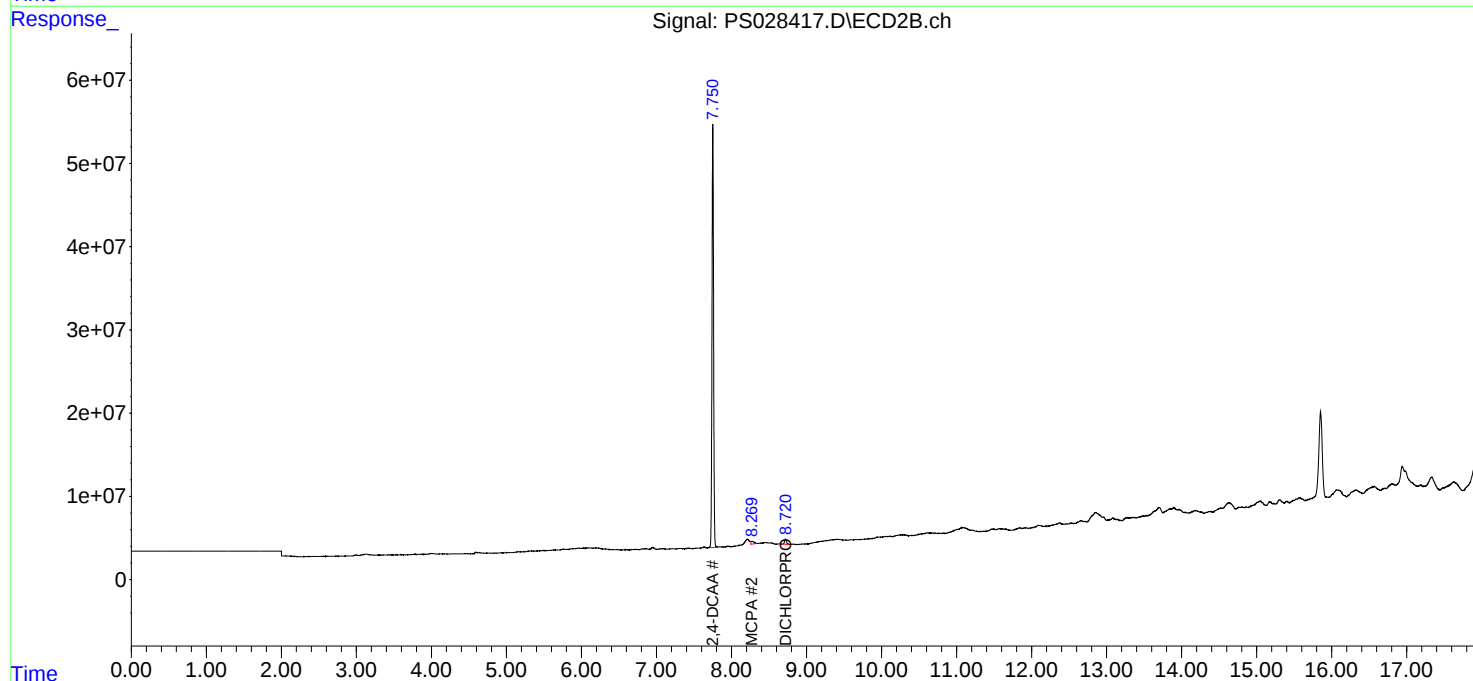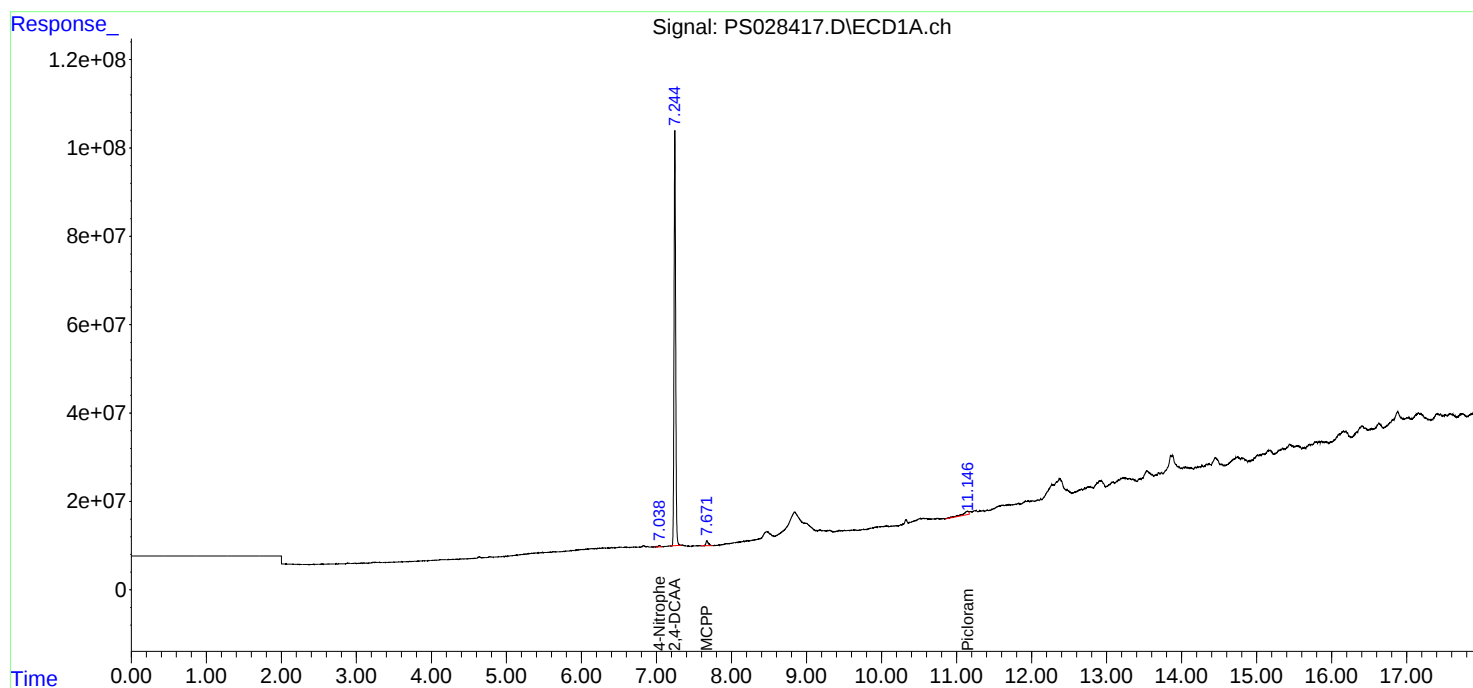


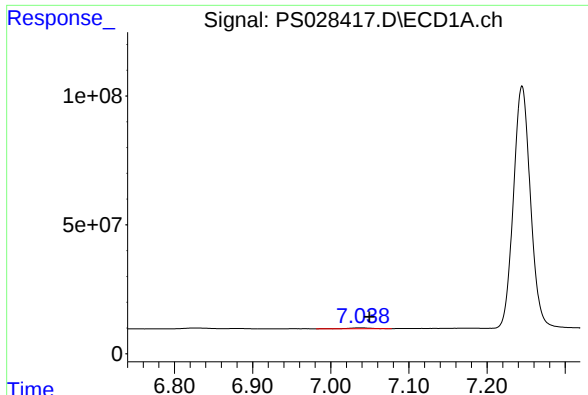

#3 4-Nitrophenol


R.T.: 7.038 min
Delta R.T.: -0.011 min
Response: 5595950
Conc: 3.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

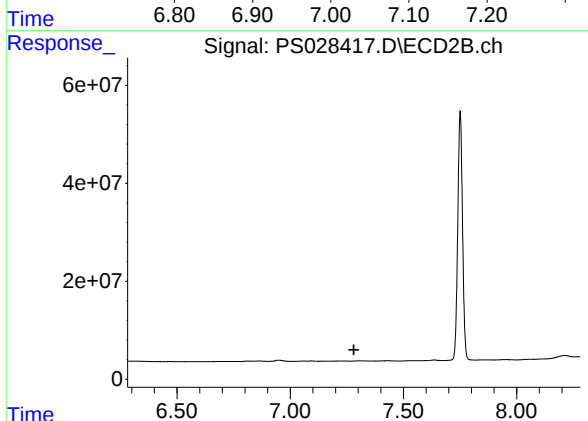


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.281 min
Response: 0
Conc: N.D.

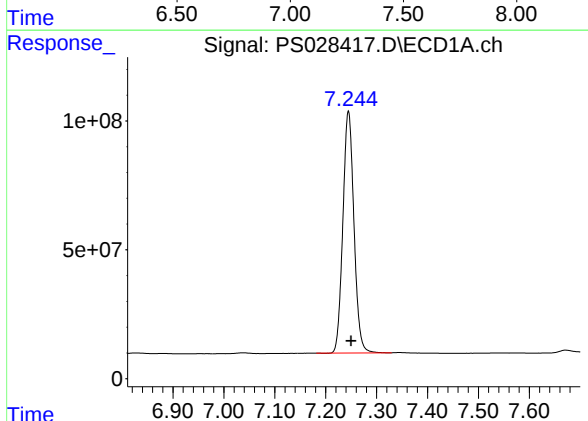


#4 2,4-DCAA

R.T.: 7.245 min
Delta R.T.: -0.005 min
Response: 1416961208
Conc: 513.25 ng/ml

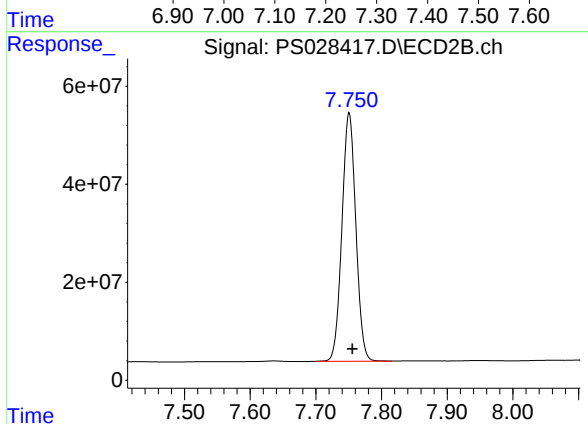

#4 2,4-DCAA


R.T.: 7.751 min
Delta R.T.: -0.005 min
Response: 745478861
Conc: 467.85 ng/ml

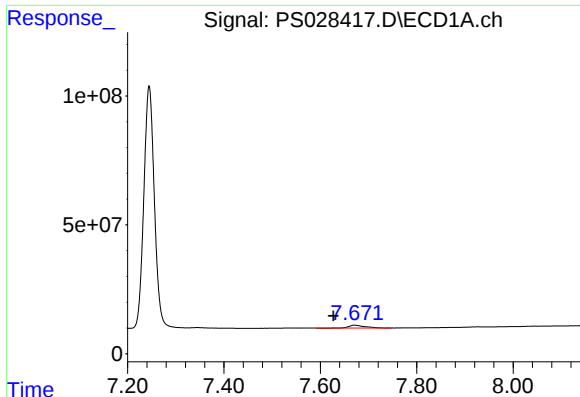

#6 MCPP


R.T.: 7.672 min
Delta R.T.: 0.044 min
Response: 24507953
Conc: 3.00 ug/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

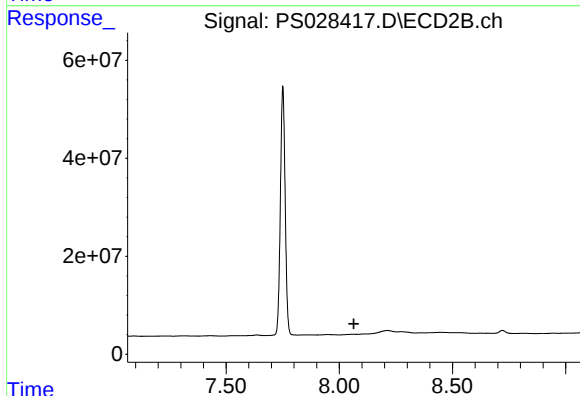


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 8.064 min
Response: 0
Conc: N.D.

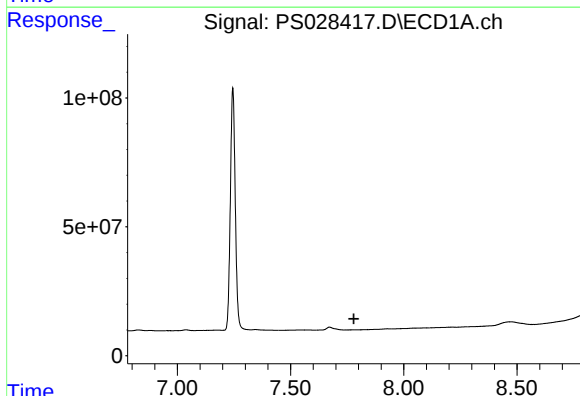


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.779 min
Response: 0
Conc: N.D.

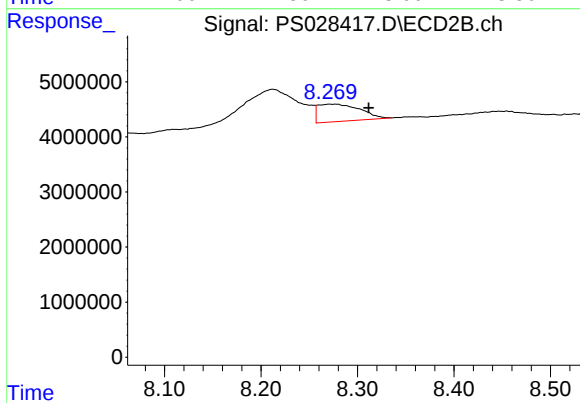

#7 MCPA


R.T.: 8.273 min
Delta R.T.: -0.039 min
Response: 9442582
Conc: 1.18 ug/ml

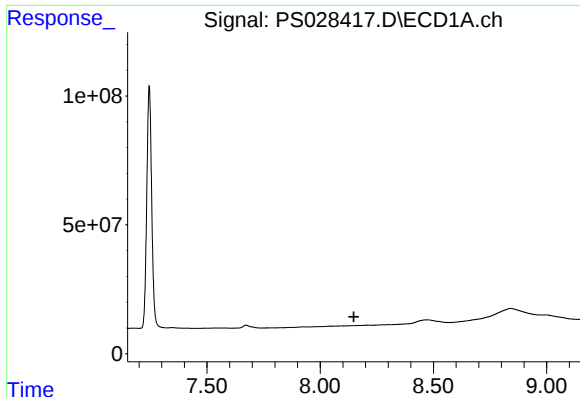

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.149 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

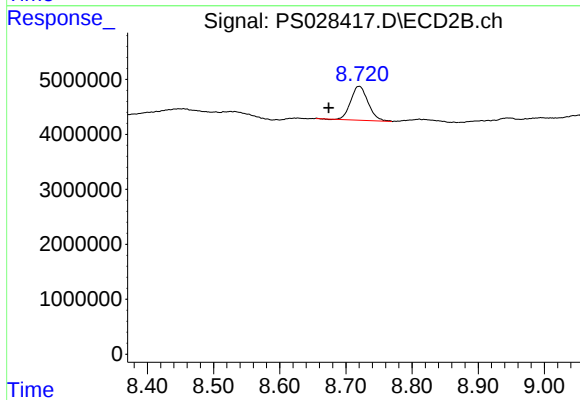


#8 DICHLORPROP

R.T.: 8.720 min
Delta R.T.: 0.046 min
Response: 11255092
Conc: 6.32 ng/ml

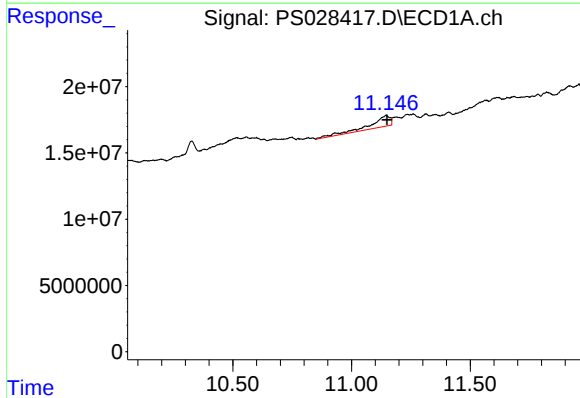

#15 Picloram

R.T.: 11.145 min
Delta R.T.: -0.005 min
Response: 49477853
Conc: 1.58 ng/ml

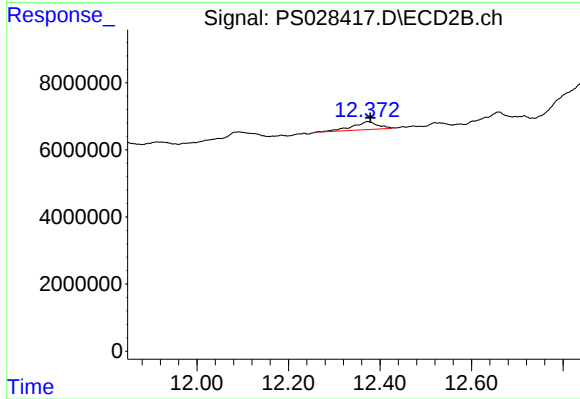

#15 Picloram

R.T.: 12.374 min
Delta R.T.: -0.005 min
Response: 9214880
Conc: N.D.