

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111124\
 Data File : PS028426.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2024 00:34
 Operator : AR\AJ
 Sample : P4602-28
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CC0Q4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 00:42:26 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110924.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 08 17:46:43 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	7.234	0.000	45649085	0	16.535	N.D.	#
Target Compounds								
5) T	DICAMBA	7.466f	7.945	1670990	6935111	<MDL	<MDL	#
6) T	MCPD	7.667f	8.079	63078601	2436024	7.713	<MDL	#
7) T	MCPA	7.767	8.295	3855107	15316825	<MDL	1.913	#
8) T	DICHLORPROP	8.108f	8.718f	21668909	28450023	6.991	15.972	#
9) T	2,4-D	0.000	8.995	0	4802189	N.D.	2.483	
10) T	Pentachlo...	8.675	9.531	860927	14741605	<MDL	<MDL	#
12) T	2,4,5-T	9.588f	0.000	8577441	0	<MDL	N.D.	#
13) T	2,4-DB	0.000	10.925	0	2861122	N.D.	2.159	
14) T	DINOSEB	11.330	0.000	25014451	0	1.543	N.D.	#
15) T	Picloram	11.141	12.374	83950601	5222918	2.673	<MDL	#
16) T	DCPA	11.604f	12.334	22960067	8287512	<MDL	<MDL	#


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111124\
Data File : PS028426.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2024 00:34
Operator : AR\AJ
Sample : P4602-28
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CC0Q4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 00:42:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110924.M
Quant Title : 8080.M
QLast Update : Fri Nov 08 17:46:43 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

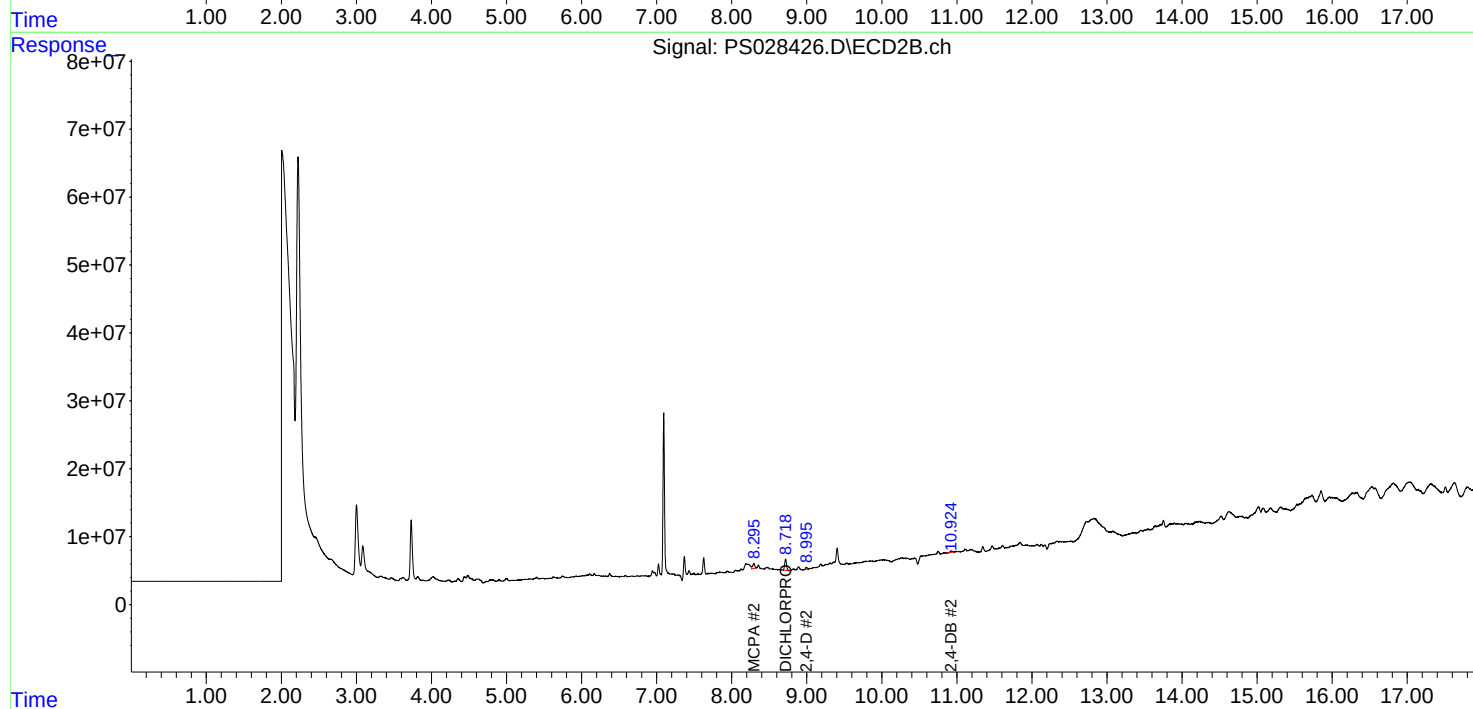


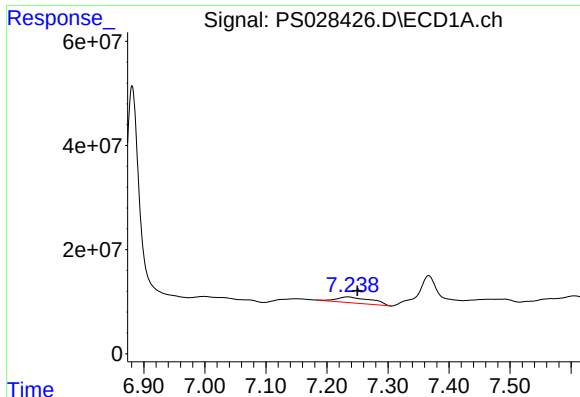

#4 2,4-DCAA


R.T.: 7.234 min
Delta R.T.: -0.016 min
Response: 45649085
Conc: 16.54 ng/ml

Instrument :
ECD_S
ClientSampleId :
CC0Q4

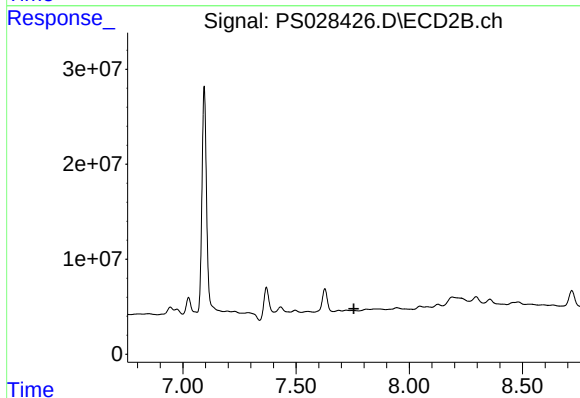


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.755 min
Response: 0
Conc: N.D.

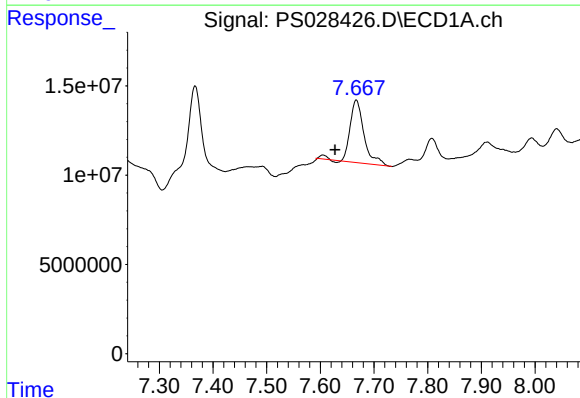


#6 MCPP

R.T.: 7.667 min
Delta R.T.: 0.039 min
Response: 63078601
Conc: 7.71 ug/ml

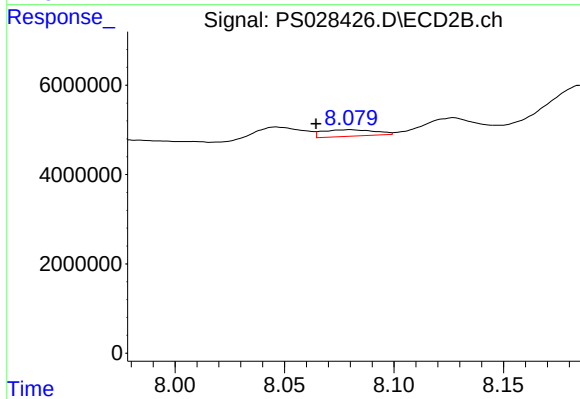

#6 MCPP


R.T.: 8.079 min
Delta R.T.: 0.015 min
Response: 2436024
Conc: N.D.

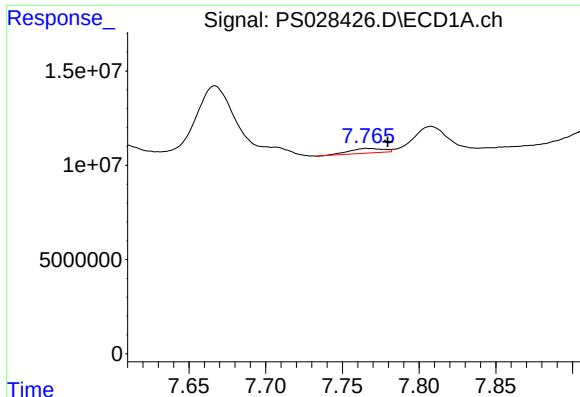

#7 MCPA


R.T.: 7.767 min
Delta R.T.: -0.013 min
Response: 3855107
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CC0Q4

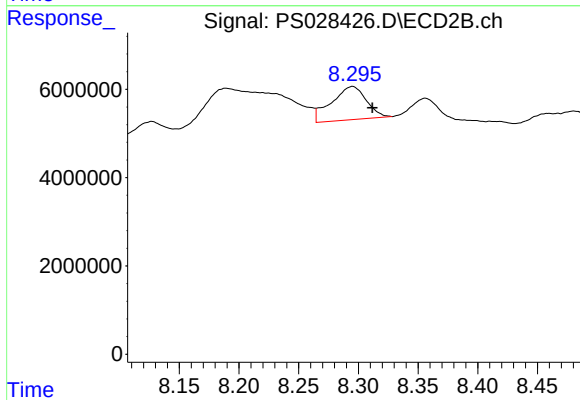


#7 MCPA

R.T.: 8.295 min
Delta R.T.: -0.017 min
Response: 15316825
Conc: 1.91 ug/ml

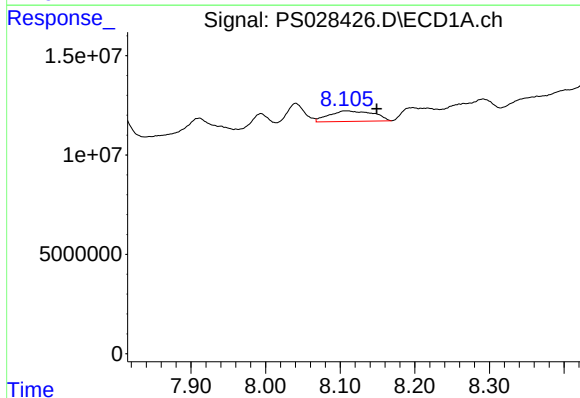


#8 DICHLORPROP

R.T.: 8.108 min
Delta R.T.: -0.041 min
Response: 21668909
Conc: 6.99 ng/ml

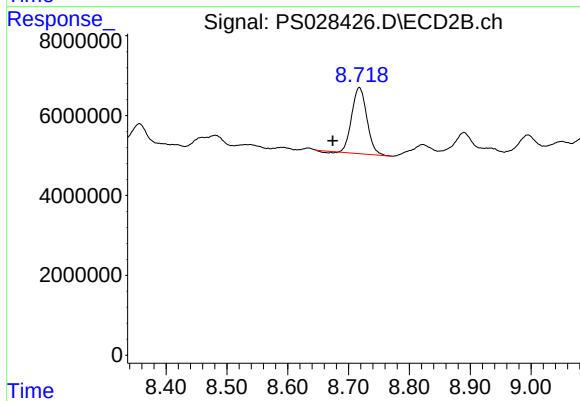

#8 DICHLORPROP


R.T.: 8.718 min
Delta R.T.: 0.044 min
Response: 28450023
Conc: 15.97 ng/ml

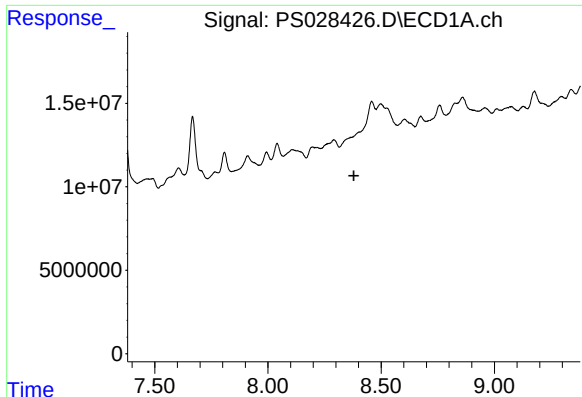

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.380 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CC0Q4

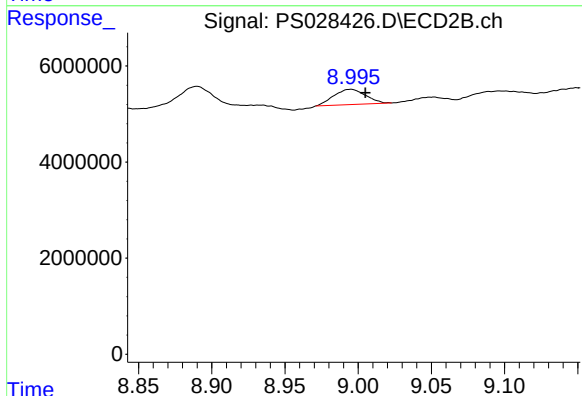


#9 2,4-D

R.T.: 8.995 min
Delta R.T.: -0.010 min
Response: 4802189
Conc: 2.48 ng/ml

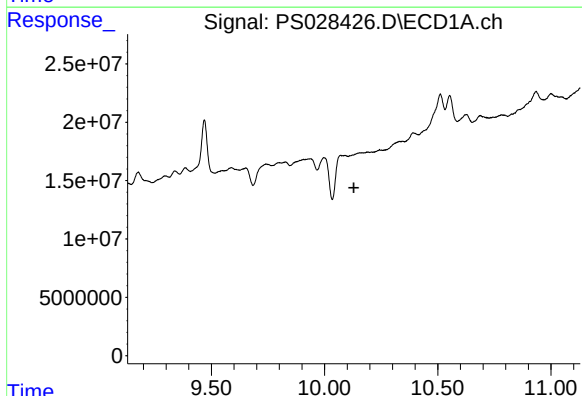


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 10.130 min
Response: 0
Conc: N.D.

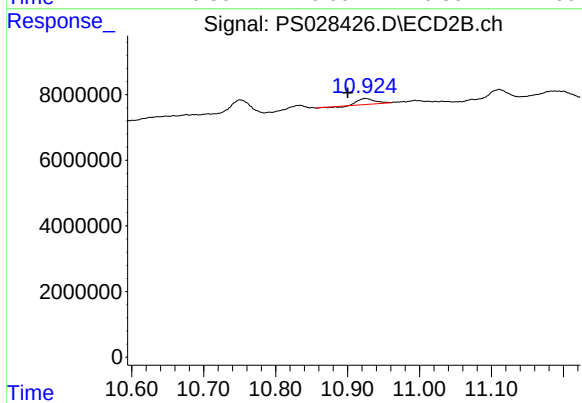

#13 2,4-DB


R.T.: 10.925 min
Delta R.T.: 0.025 min
Response: 2861122
Conc: 2.16 ng/ml

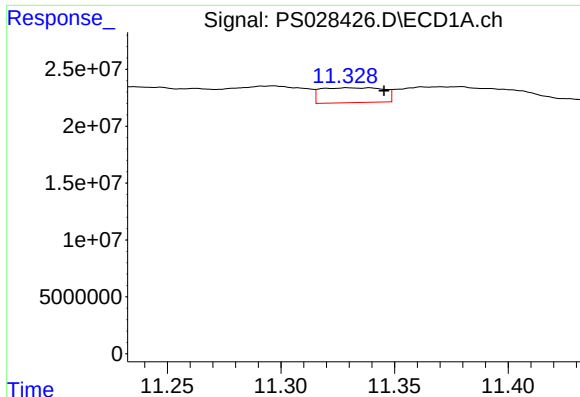

#14 DINOSEB


R.T.: 11.330 min
Delta R.T.: -0.015 min
Response: 25014451
Conc: 1.54 ng/ml

Instrument :
ECD_S
ClientSampleId :
CC0Q4

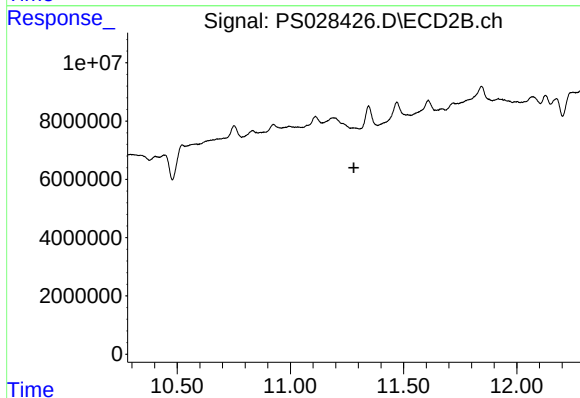


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.280 min
Response: 0
Conc: N.D.

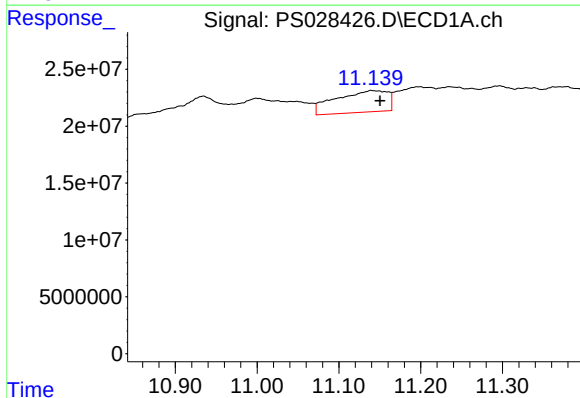

#15 Picloram

R.T.: 11.141 min
Delta R.T.: -0.010 min
Response: 83950601
Conc: 2.67 ng/ml

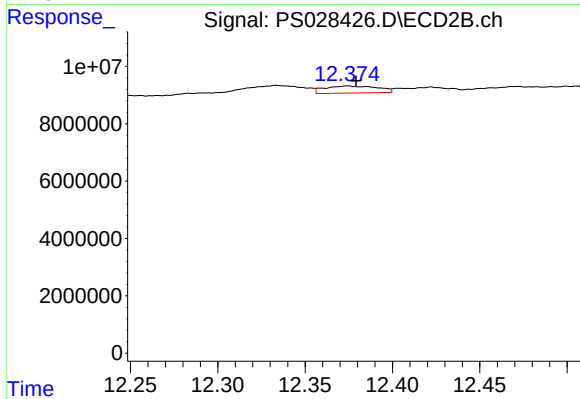

#15 Picloram

R.T.: 12.374 min
Delta R.T.: -0.005 min
Response: 5222918
Conc: N.D.