

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111124\
 Data File : PS028429.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2024 01:47
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 02:17:06 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110924.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 08 17:46:43 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.244	7.749	1401.6E6	735.0E6	507.701	461.293
Target Compounds							
1) T	Dalapon	2.649	0.000	913022	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.397	0.000	1085036	0	<MDL	N.D. #
3) T	4-Nitroph...	7.034	0.000	8371355	0	4.515	N.D. #
5) T	DICAMBA	0.000	7.950	0	4282674	N.D.	<MDL
6) T	MCPD	7.671f	8.103f	25650052	4600812	3.136	<MDL #
7) T	MCPA	0.000	8.277f	0	9176905	N.D.	1.146
8) T	DICHLORPROP	0.000	8.719f	0	10942516	N.D.	6.143
10) T	Pentachlo...	0.000	9.537	0	7630076	N.D.	<MDL
11) T	2,4,5-TP ...	9.239	0.000	1146168	0	<MDL	N.D. #
12) T	2,4,5-T	9.590f	10.284f	6844462	26805110	<MDL	2.583 #
14) T	DINOSEB	11.329	0.000	9481860	0	<MDL	N.D. #
15) T	Picloram	11.142	12.368	23343898	15768447	<MDL	1.096 #
16) T	DCPA	11.603f	12.368f	5443450	15768447	<MDL	1.407 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111124\
Data File : PS028429.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2024 01:47
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 02:17:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110924.M
Quant Title : 8080.M
QLast Update : Fri Nov 08 17:46:43 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

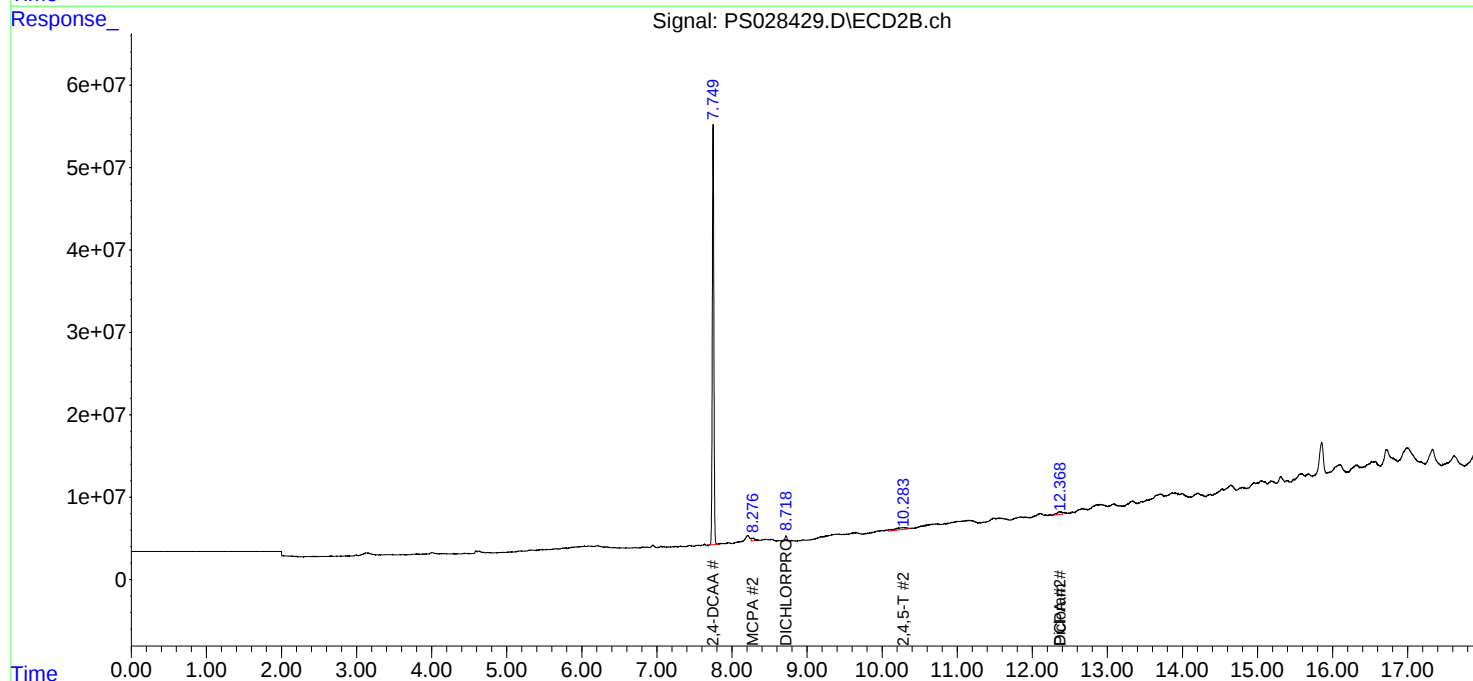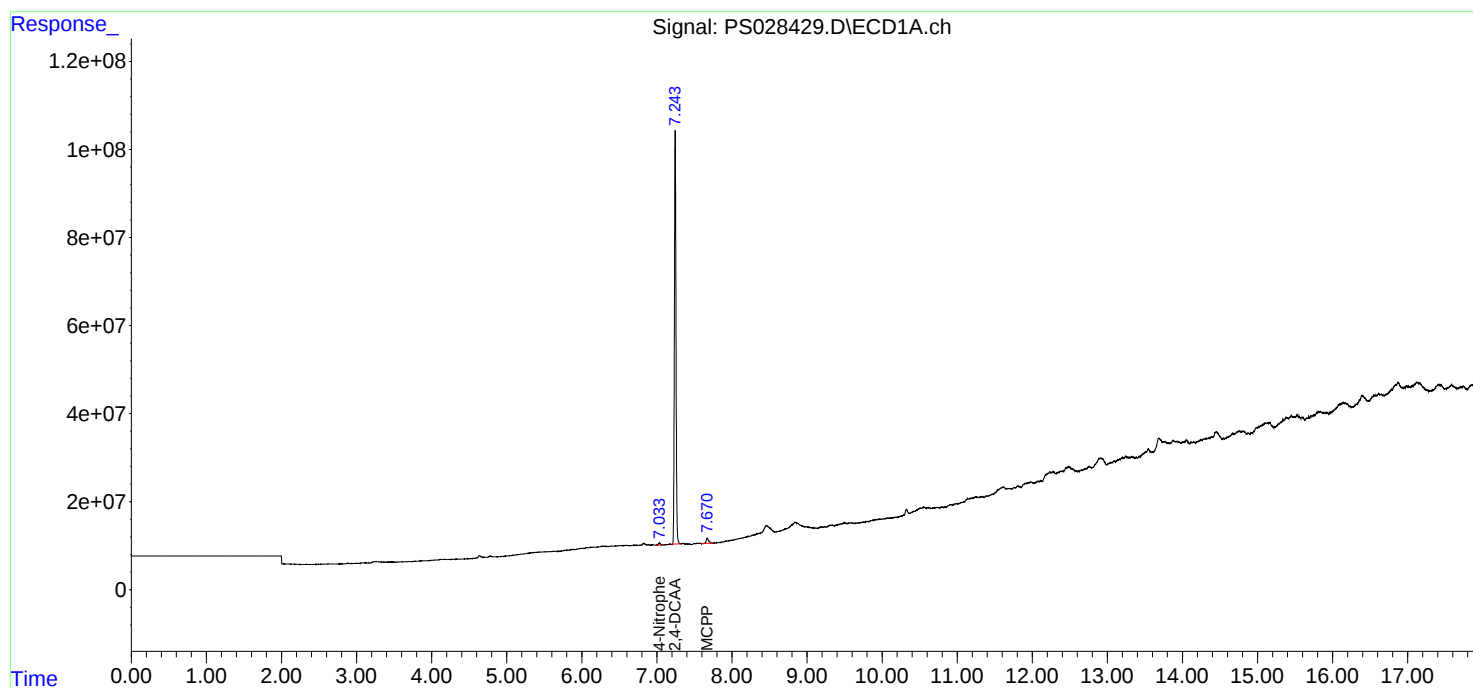


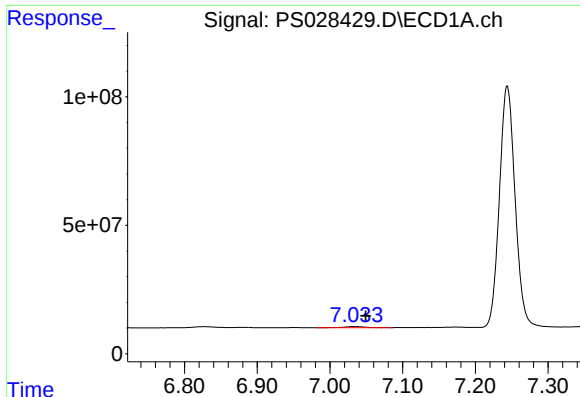

#3 4-Nitrophenol


R.T.: 7.034 min
Delta R.T.: -0.015 min
Response: 8371355
Conc: 4.51 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

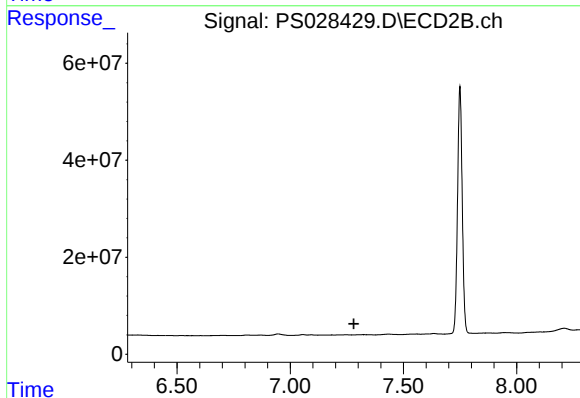


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 7.281 min
Response: 0
Conc: N.D.

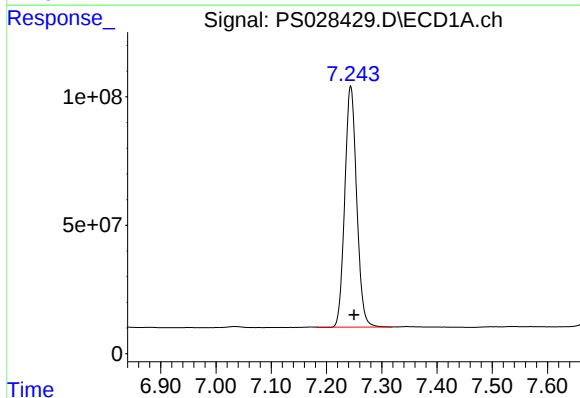


#4 2,4-DCAA

R.T.: 7.244 min
Delta R.T.: -0.006 min
Response: 1401637232
Conc: 507.70 ng/ml

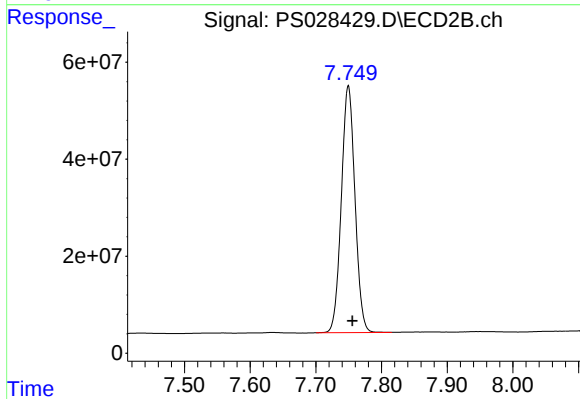

#4 2,4-DCAA


R.T.: 7.749 min
Delta R.T.: -0.006 min
Response: 735034310
Conc: 461.29 ng/ml

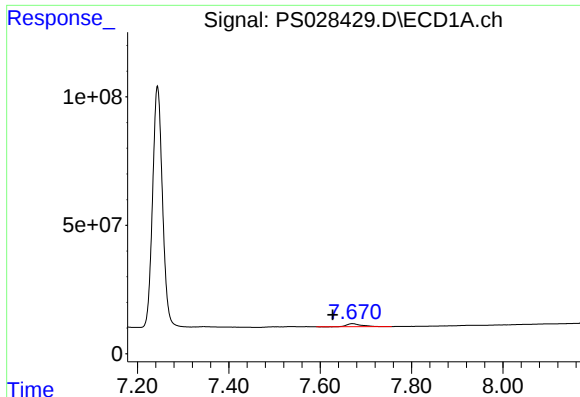

#6 MCPP


R.T.: 7.671 min
Delta R.T.: 0.043 min
Response: 25650052
Conc: 3.14 ug/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

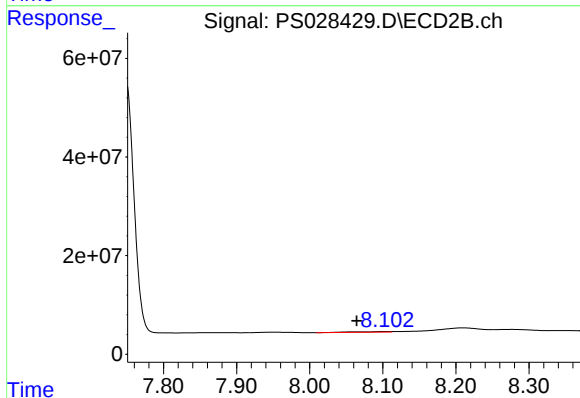


#6 MCPP

R.T.: 8.103 min
Delta R.T.: 0.038 min
Response: 4600812
Conc: N.D.

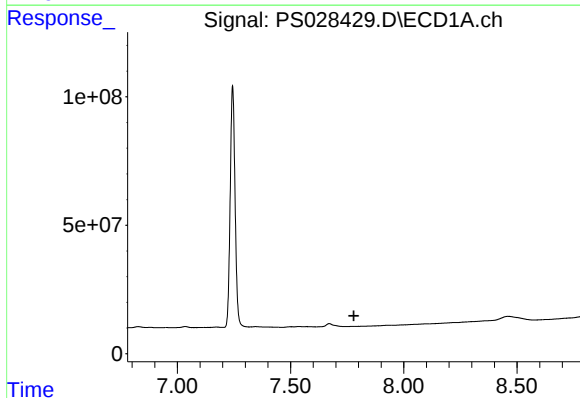


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.779 min
Response: 0
Conc: N.D.

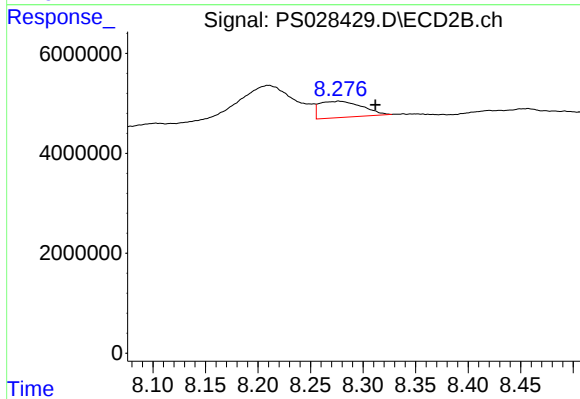

#7 MCPA


R.T.: 8.277 min
Delta R.T.: -0.035 min
Response: 9176905
Conc: 1.15 ug/ml

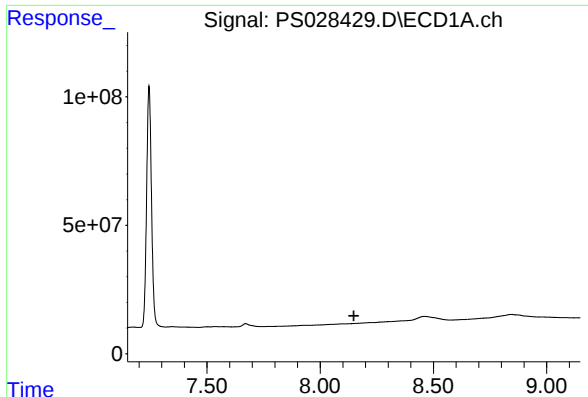

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.149 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

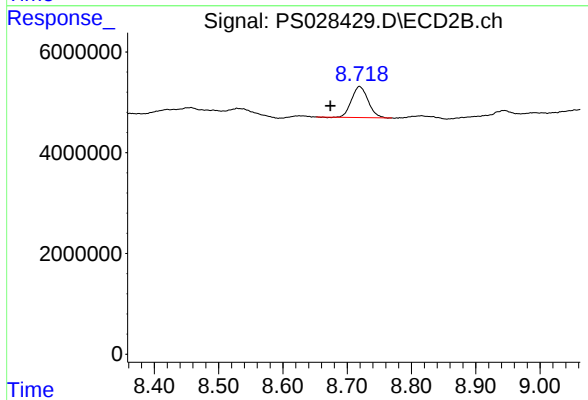


#8 DICHLORPROP

R.T.: 8.719 min
Delta R.T.: 0.045 min
Response: 10942516
Conc: 6.14 ng/ml

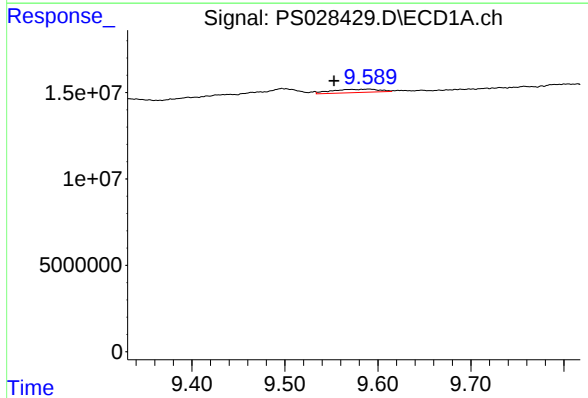


#12 2,4,5-T

R.T.: 9.590 min
Delta R.T.: 0.037 min
Response: 6844462
Conc: N.D.

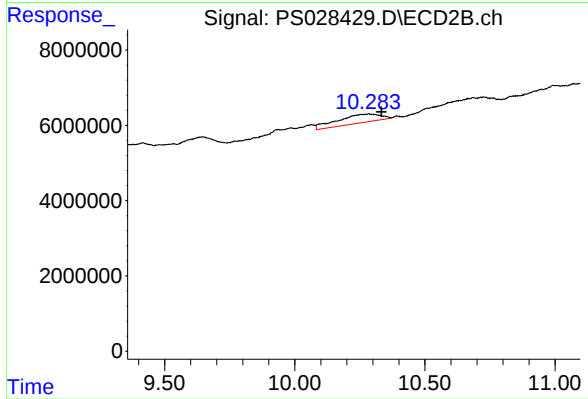

#12 2,4,5-T


R.T.: 10.284 min
Delta R.T.: -0.050 min
Response: 26805110
Conc: 2.58 ng/ml

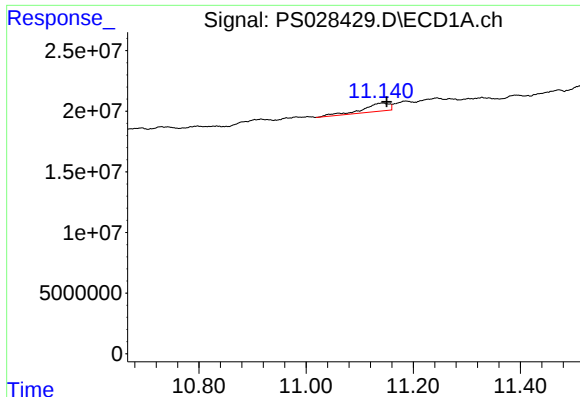

#15 Picloram


R.T.: 11.142 min
Delta R.T.: -0.008 min
Response: 23343898
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

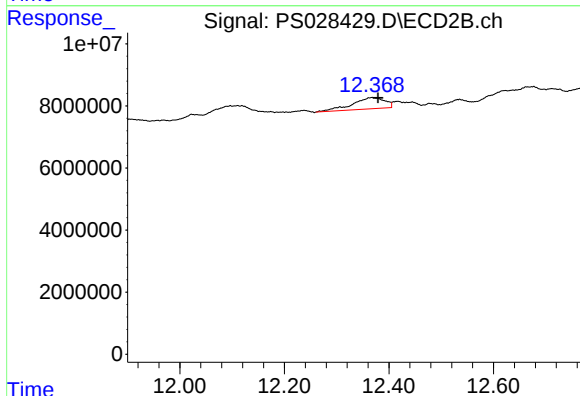


#15 Picloram

R.T.: 12.368 min
Delta R.T.: -0.011 min
Response: 15768447
Conc: 1.10 ng/ml

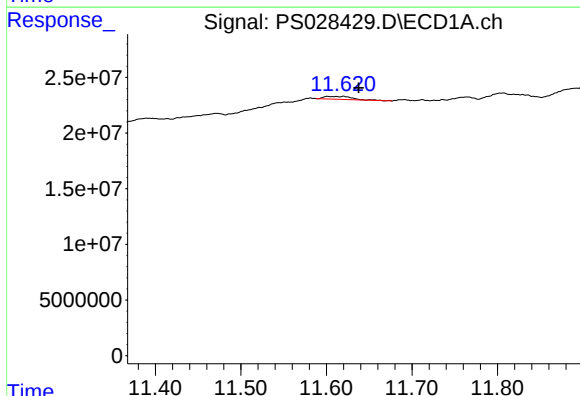

#16 DCPA

R.T.: 11.603 min
Delta R.T.: -0.035 min
Response: 5443450
Conc: N.D.

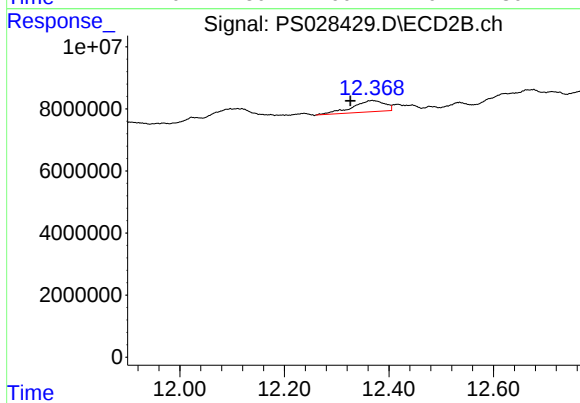

#16 DCPA

R.T.: 12.368 min
Delta R.T.: 0.042 min
Response: 15768447
Conc: 1.41 ng/ml