

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111124\
 Data File : PS028441.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2024 06:35
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 06:56:06 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110924.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 08 17:46:43 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.242	7.748	1405.9E6	725.4E6	509.235	455.240
Target Compounds							
1) T	Dalapon	2.651	0.000	535854	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.402	0.000	546798	0	<MDL	N.D. #
3) T	4-Nitroph...	7.031	0.000	11496894	0	6.200	N.D. #
5) T	DICAMBA	7.451	7.940	-358258	2823809	N.D.	<MDL
6) T	MCPD	7.668f	0.000	43121459	0	5.272	N.D. #
7) T	MCPA	7.794	8.267f	466349	10896065	<MDL	1.361 #
8) T	DICHLORPROP	8.159	8.716f	679230	17103035	<MDL	9.602 #
10) T	Pentachlo...	8.708f	0.000	2625536	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.307f	0.000	12063800	0	<MDL	N.D. #
12) T	2,4,5-T	9.552	10.324	741172	5235247	<MDL	<MDL #
15) T	Picloram	11.138	12.368	10359311	11546057	<MDL	<MDL #
16) T	DCPA	0.000	12.368f	0	11546057	N.D.	1.030



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111124\
Data File : PS028441.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2024 06:35
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 06:56:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110924.M
Quant Title : 8080.M
QLast Update : Fri Nov 08 17:46:43 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

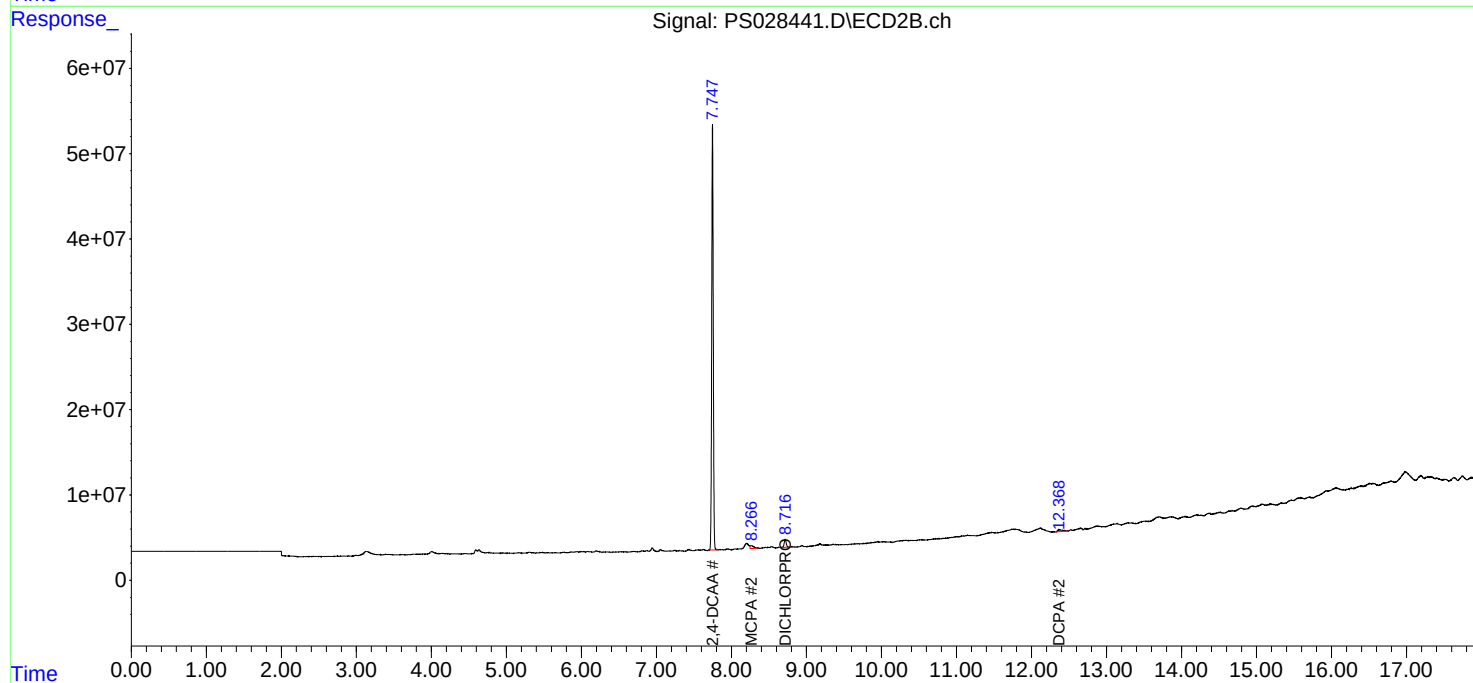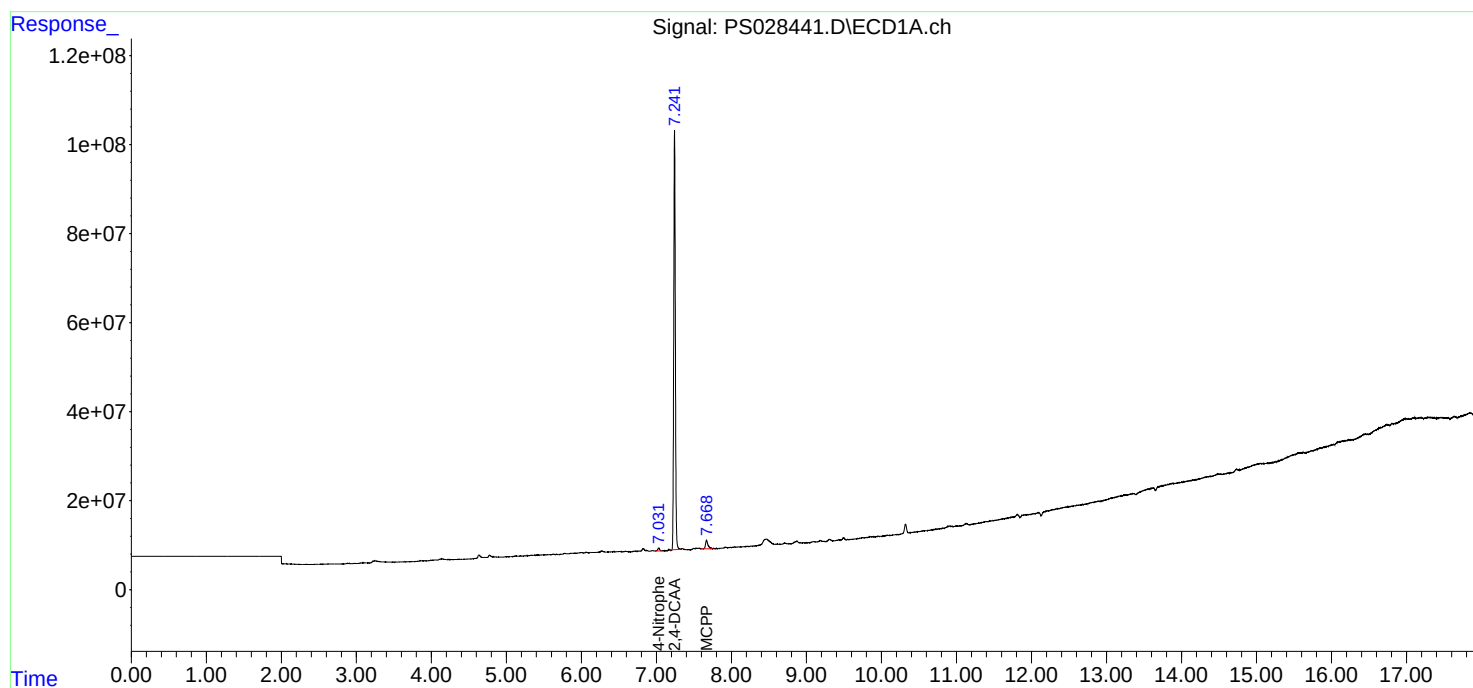


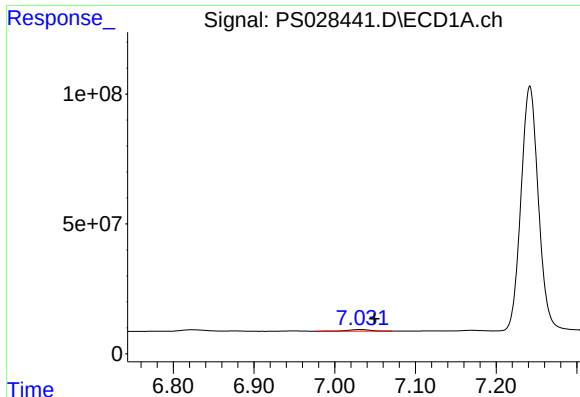

#3 4-Nitrophenol


R.T.: 7.031 min
Delta R.T.: -0.019 min
Response: 11496894
Conc: 6.20 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

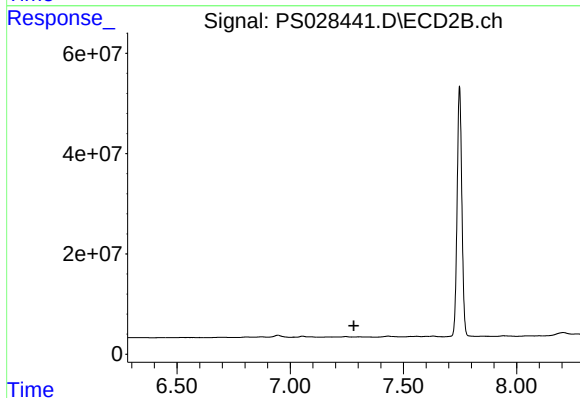


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 7.281 min
Response: 0
Conc: N.D.

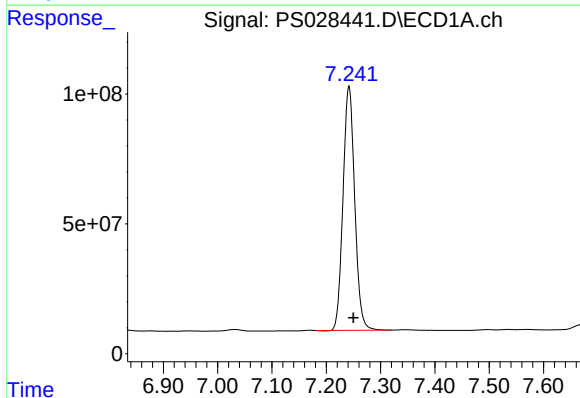


#4 2,4-DCAA

R.T.: 7.242 min
Delta R.T.: -0.008 min
Response: 1405871707
Conc: 509.23 ng/ml

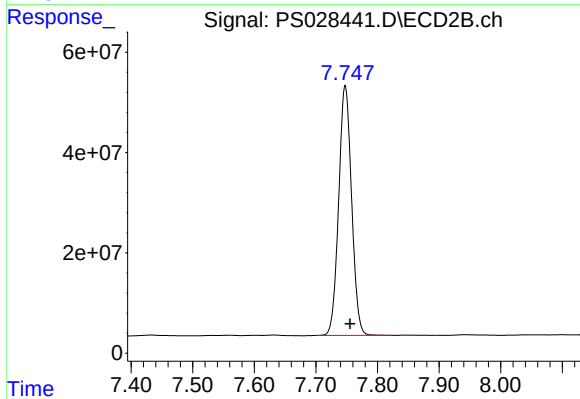

#4 2,4-DCAA


R.T.: 7.748 min
Delta R.T.: -0.008 min
Response: 725389010
Conc: 455.24 ng/ml

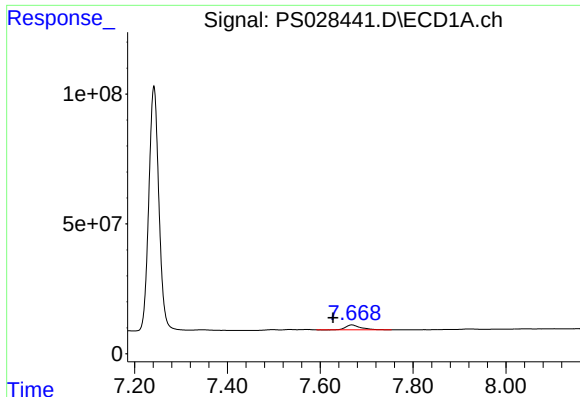

#6 MCPP


R.T.: 7.668 min
Delta R.T.: 0.040 min
Response: 43121459
Conc: 5.27 ug/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

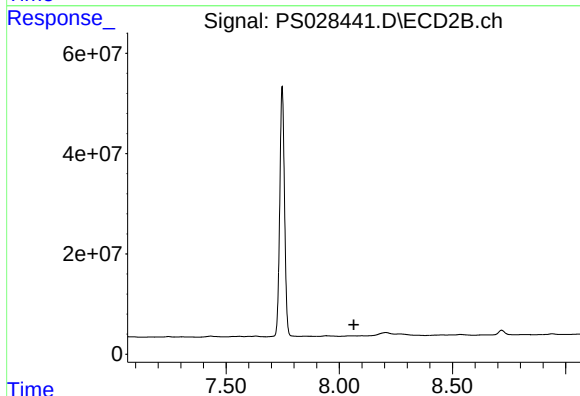


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 8.064 min
Response: 0
Conc: N.D.

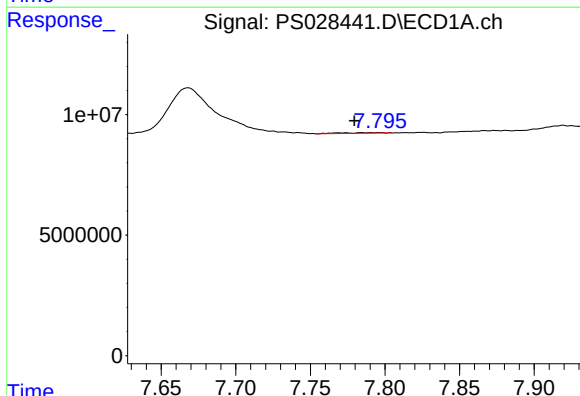


#7 MCPA

R.T.: 7.794 min
Delta R.T.: 0.014 min
Response: 466349
Conc: N.D.

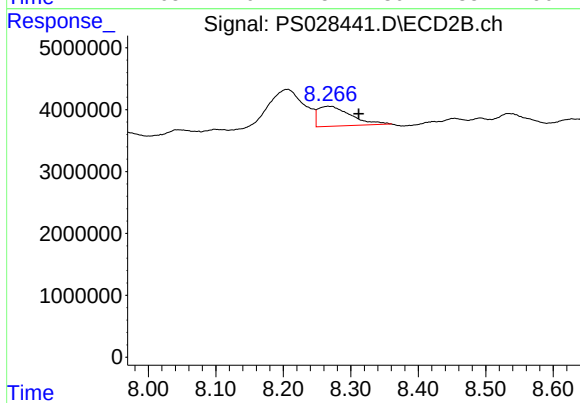

#7 MCPA


R.T.: 8.267 min
Delta R.T.: -0.045 min
Response: 10896065
Conc: 1.36 ug/ml

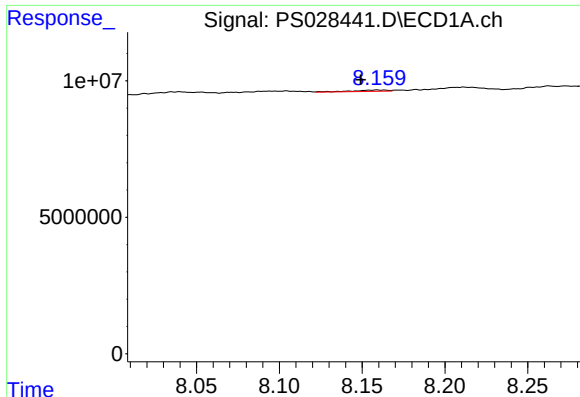

#8 DICHLORPROP


R.T.: 8.159 min
Delta R.T.: 0.010 min
Response: 679230
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

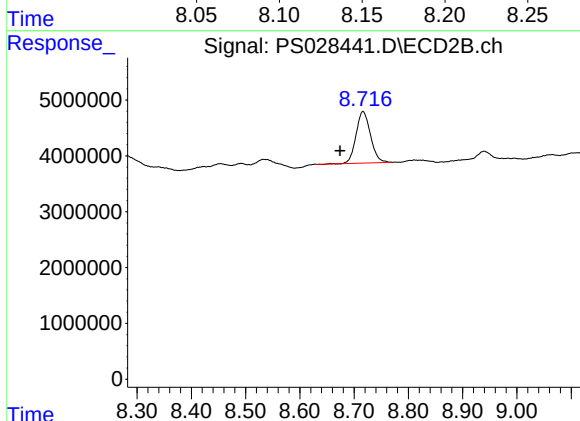


#8 DICHLORPROP

R.T.: 8.716 min
Delta R.T.: 0.042 min
Response: 17103035
Conc: 9.60 ng/ml

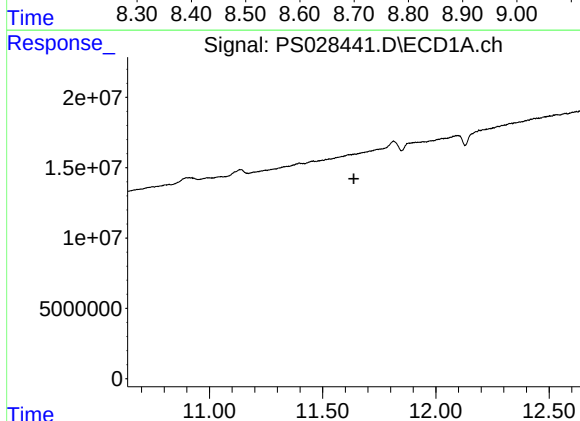

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.638 min
Response: 0
Conc: N.D.

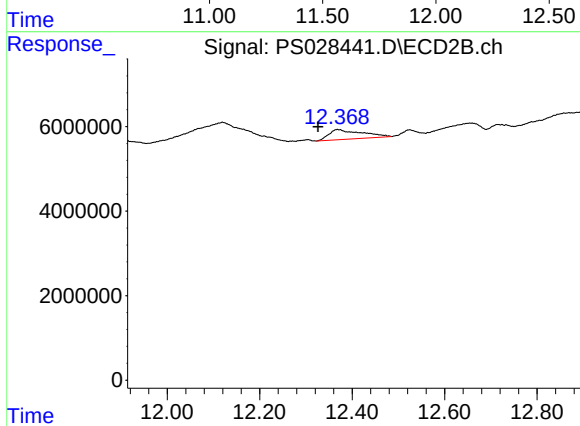

#16 DCPA

R.T.: 12.368 min
Delta R.T.: 0.042 min
Response: 11546057
Conc: 1.03 ng/ml