

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111124\
 Data File : PS028447.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2024 09:28
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 14:09:43 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110924.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 08 17:46:43 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.244	7.748	1371.0E6	710.3E6	496.594	445.760
Target Compounds							
2) T	3,5-DICHL...	6.407	0.000	470003	0	<MDL	N.D. #
3) T	4-Nitroph...	7.039	0.000	6325553	0	3.411	N.D. #
5) T	DICAMBA	0.000	7.944	0	2538583	N.D.	<MDL
6) T	MCP	7.671f	8.057	16192887	849204	1.980	<MDL #
7) T	MCPA	0.000	8.345f	0	961187	N.D.	<MDL
8) T	DICHLORPROP	0.000	8.717f	0	6365424	N.D.	3.574
10) T	Pentachlo...	8.678	0.000	545893	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.285	9.957f	92823355	3777551	4.904	<MDL #
12) T	2,4,5-T	0.000	10.317	0	6932509	N.D.	<MDL
14) T	DINOSEB	11.339	0.000	1978403	0	<MDL	N.D. #
15) T	Picloram	11.150	12.370	21574625	32016672	<MDL	2.225 #
16) T	DCPA	11.630	12.370f	2624116	32016672	<MDL	2.856 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111124\
Data File : PS028447.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2024 09:28
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 14:09:43 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110924.M
Quant Title : 8080.M
QLast Update : Fri Nov 08 17:46:43 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

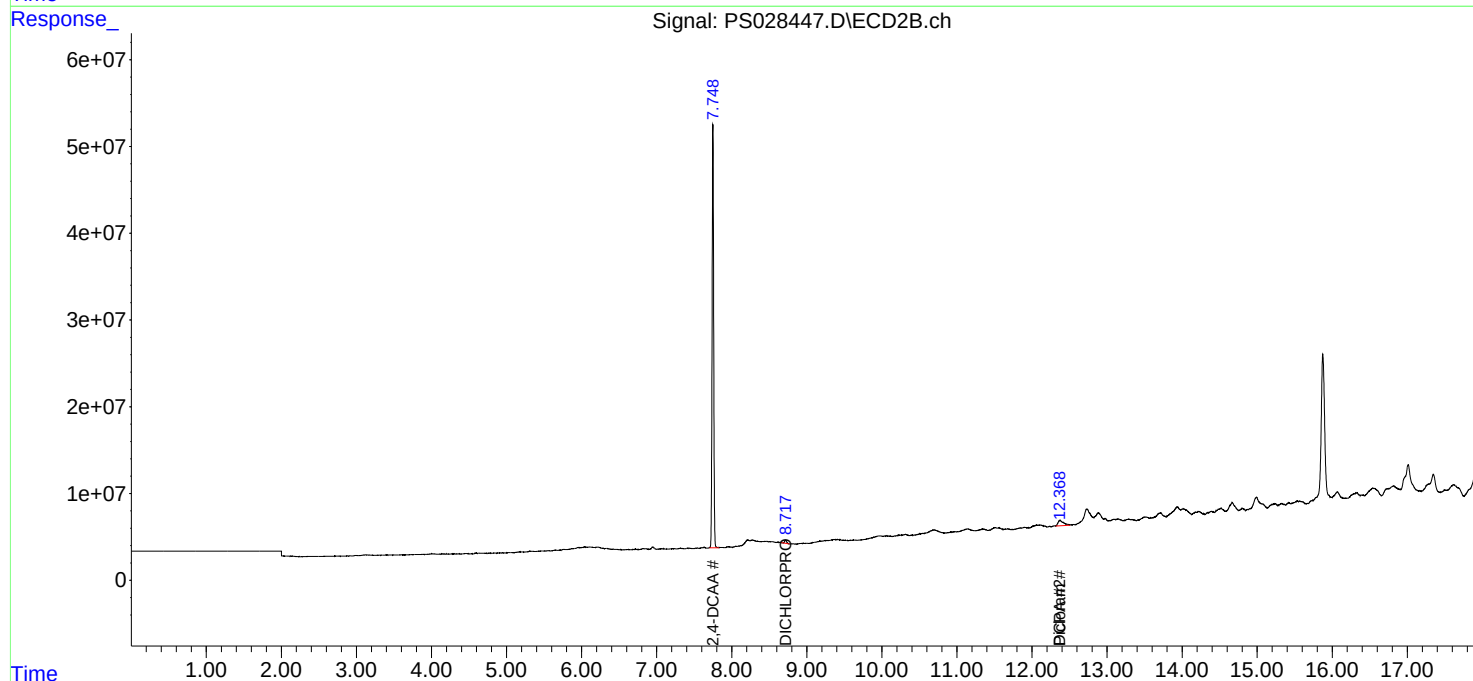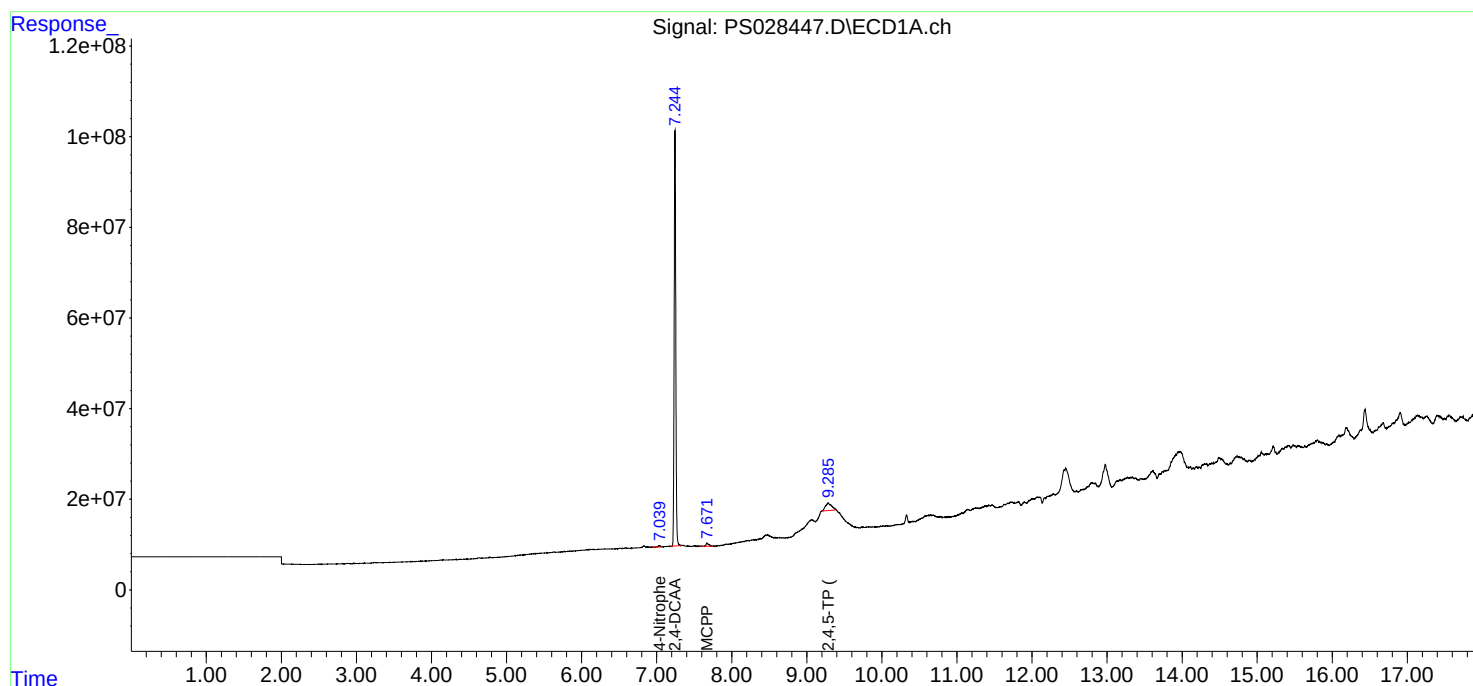


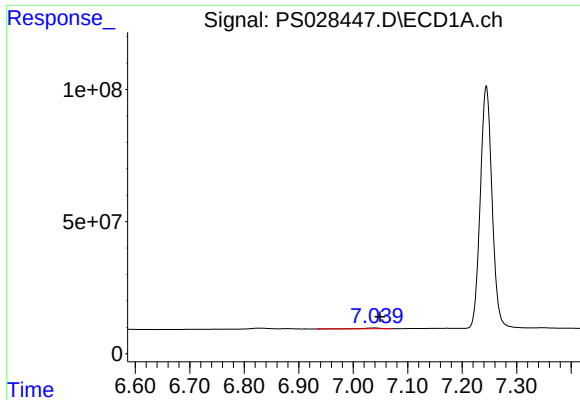

#3 4-Nitrophenol


R.T.: 7.039 min
Delta R.T.: -0.011 min
Response: 6325553
Conc: 3.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

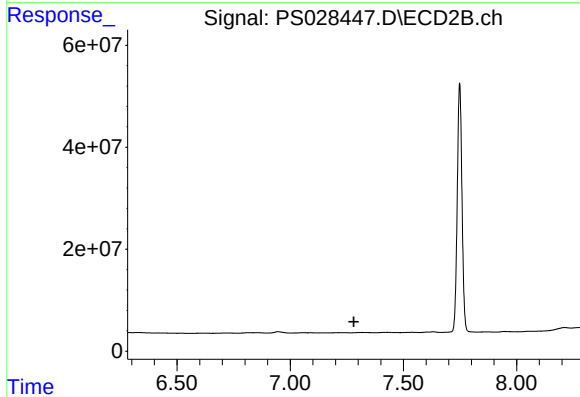


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.281 min
Response: 0
Conc: N.D.

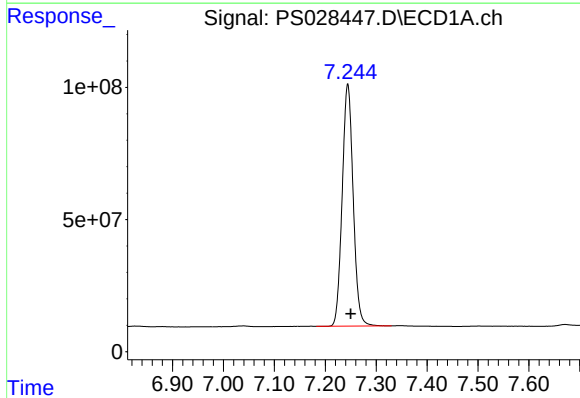


#4 2,4-DCAA

R.T.: 7.244 min
Delta R.T.: -0.006 min
Response: 1370975098
Conc: 496.59 ng/ml

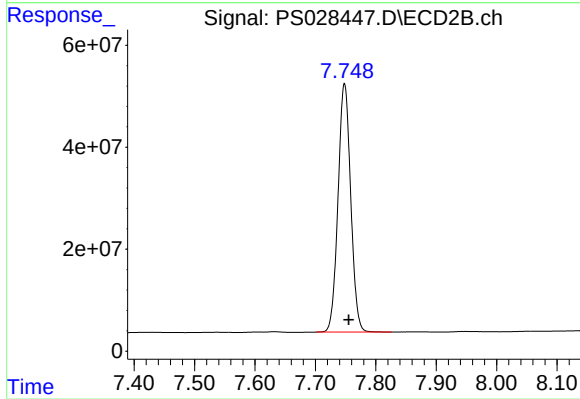

#4 2,4-DCAA


R.T.: 7.748 min
Delta R.T.: -0.007 min
Response: 710282798
Conc: 445.76 ng/ml

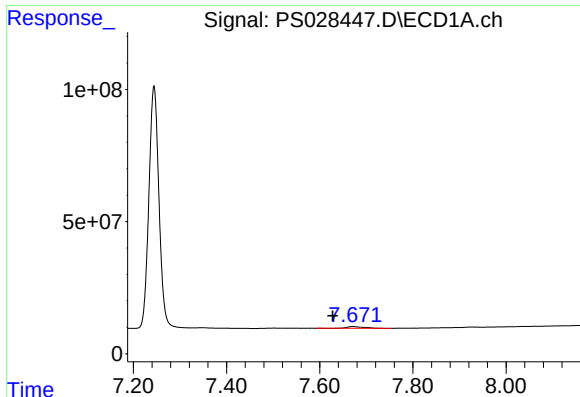

#6 MCP


R.T.: 7.671 min
Delta R.T.: 0.044 min
Response: 16192887
Conc: 1.98 ug/ml

Instrument :
ECD_S
ClientSampleId :

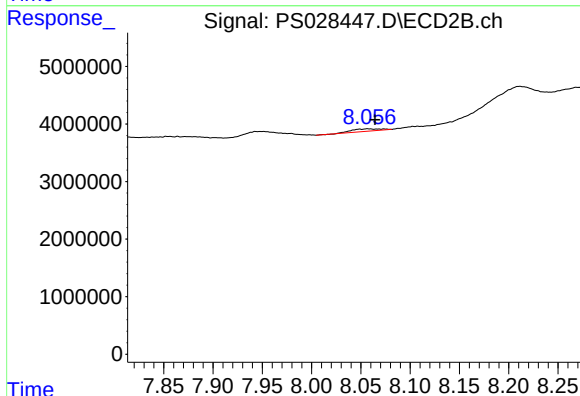


#6 MCP

R.T.: 8.057 min
Delta R.T.: -0.008 min
Response: 849204
Conc: N.D.

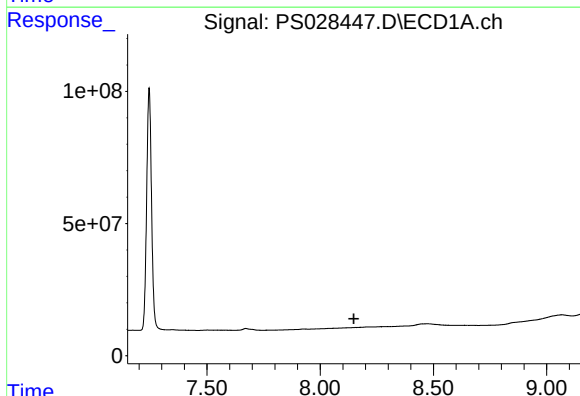


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.149 min
Response: 0
Conc: N.D.

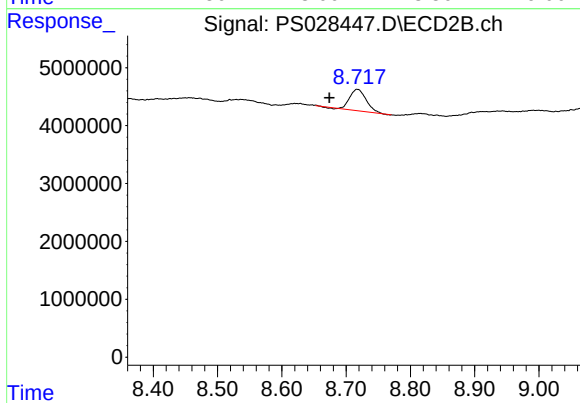

#8 DICHLORPROP


R.T.: 8.717 min
Delta R.T.: 0.043 min
Response: 6365424
Conc: 3.57 ng/ml

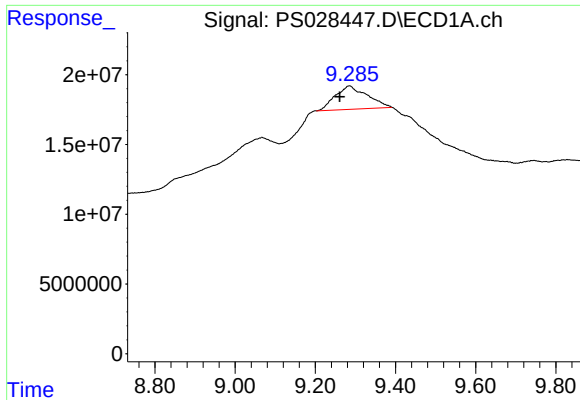

#11 2,4,5-TP (SILVEX)


R.T.: 9.285 min
Delta R.T.: 0.024 min
Response: 92823355
Conc: 4.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

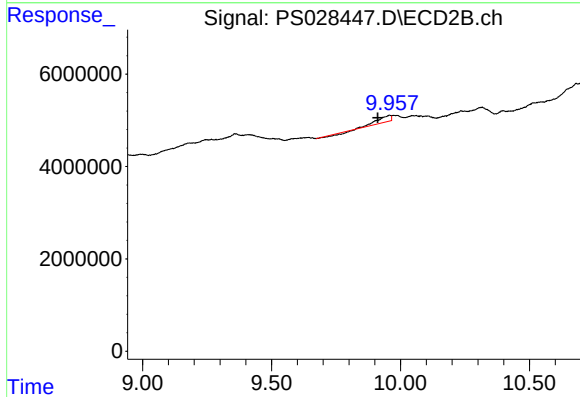


#11 2,4,5-TP (SILVEX)

R.T.: 9.957 min
Delta R.T.: 0.045 min
Response: 3777551
Conc: N.D.

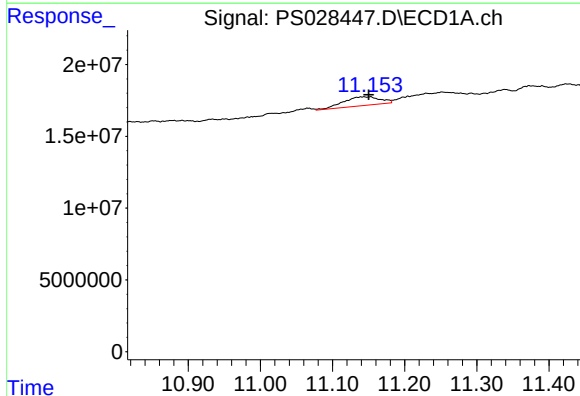


#15 Picloram

R.T.: 11.150 min
Delta R.T.: 0.000 min
Response: 21574625
Conc: N.D.

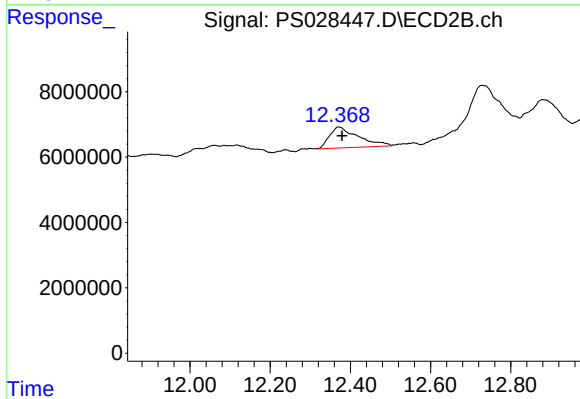

#15 Picloram


R.T.: 12.370 min
Delta R.T.: -0.010 min
Response: 32016672
Conc: 2.22 ng/ml

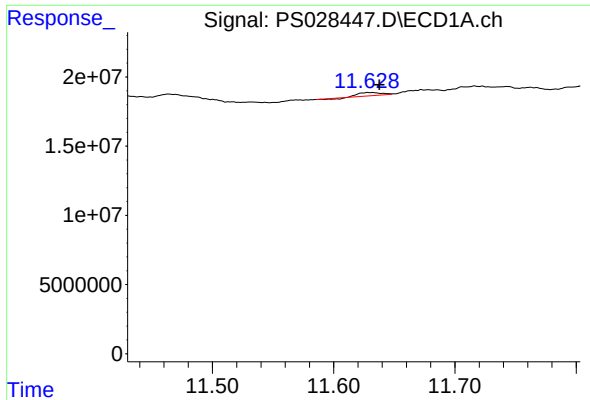

#16 DCPA

R.T.: 11.630 min
Delta R.T.: -0.007 min
Response: 2624116
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

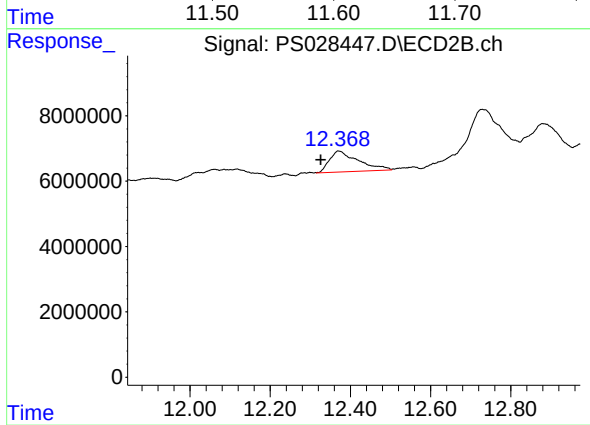

#16 DCPA

R.T.: 12.370 min
Delta R.T.: 0.043 min
Response: 32016672
Conc: 2.86 ng/ml