

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111522\
 Data File : PS021165.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Nov 2022 09:08
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 20:20:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102822.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 31 10:07:57 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.422	0.000	394526	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	2.501	0.000	315888	0	<MDL	N.D. #
3) T	4-Nitroph...	6.242	0.000	2514049	0	1.672	N.D. #
5) T	DICAMBA	6.555	0.000	199327	0	<MDL	N.D. #
6) T	MCP	6.685	0.000	1259223	0	<MDL	N.D. #
7) T	MCPA	6.866	7.296	198792	3599205	<MDL	<MDL #
8) T	DICHLORPROP	0.000	7.675	0	938028	N.D.	<MDL
10) T	Pentachlo...	7.575	0.000	898978	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.121	0.000	2684667	0	<MDL	N.D. #
12) T	2,4,5-T	8.390	0.000	2422704	0	<MDL	N.D. #
13) T	2,4-DB	8.855	0.000	273858	0	<MDL	N.D. #
14) T	DINOSEB	10.012f	0.000	694480	0	<MDL	N.D. #
15) T	Picloram	9.760	10.949	1261196	14007798	<MDL	1.104 #
16) T	DCPA	10.204	10.864	466055	721565	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111522\
Data File : PS021165.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Nov 2022 09:08
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 20:20:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102822.M
Quant Title : 8080.M
QLast Update : Mon Oct 31 10:07:57 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

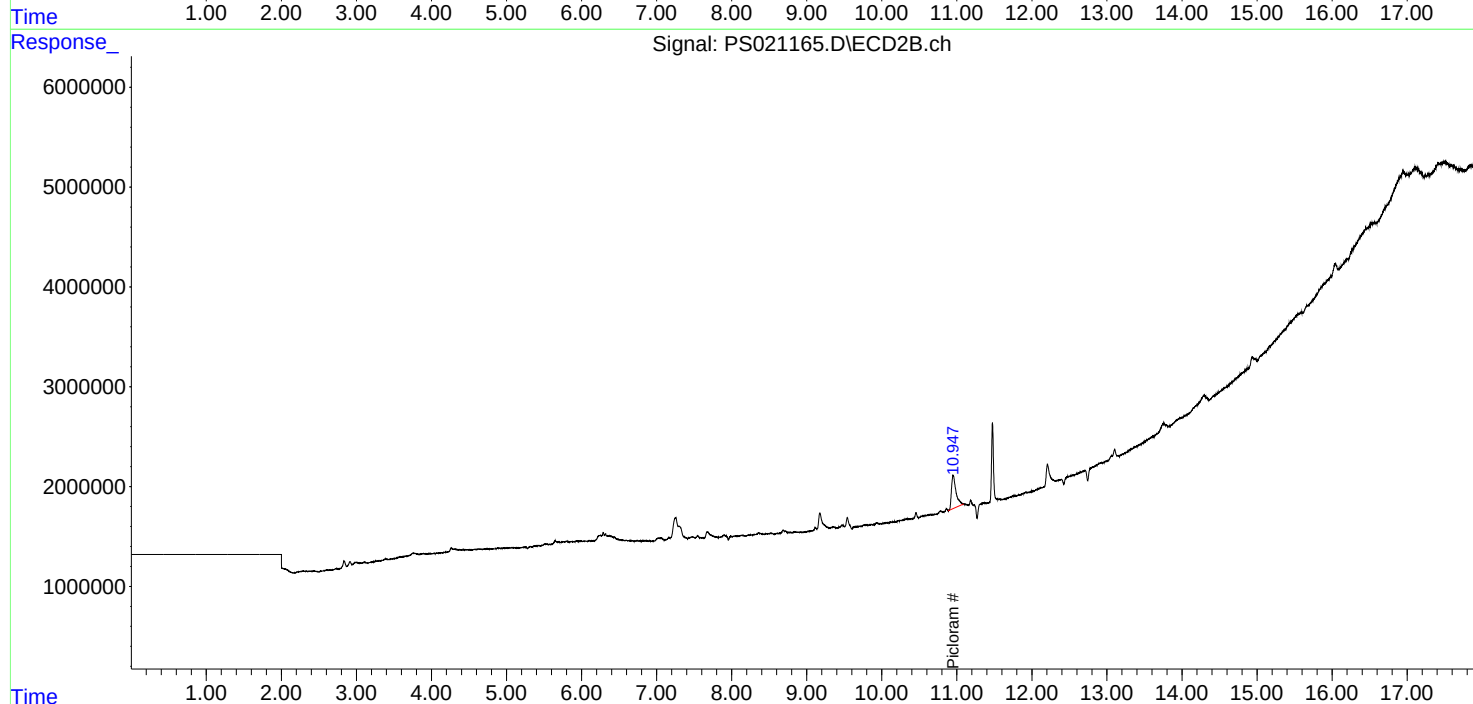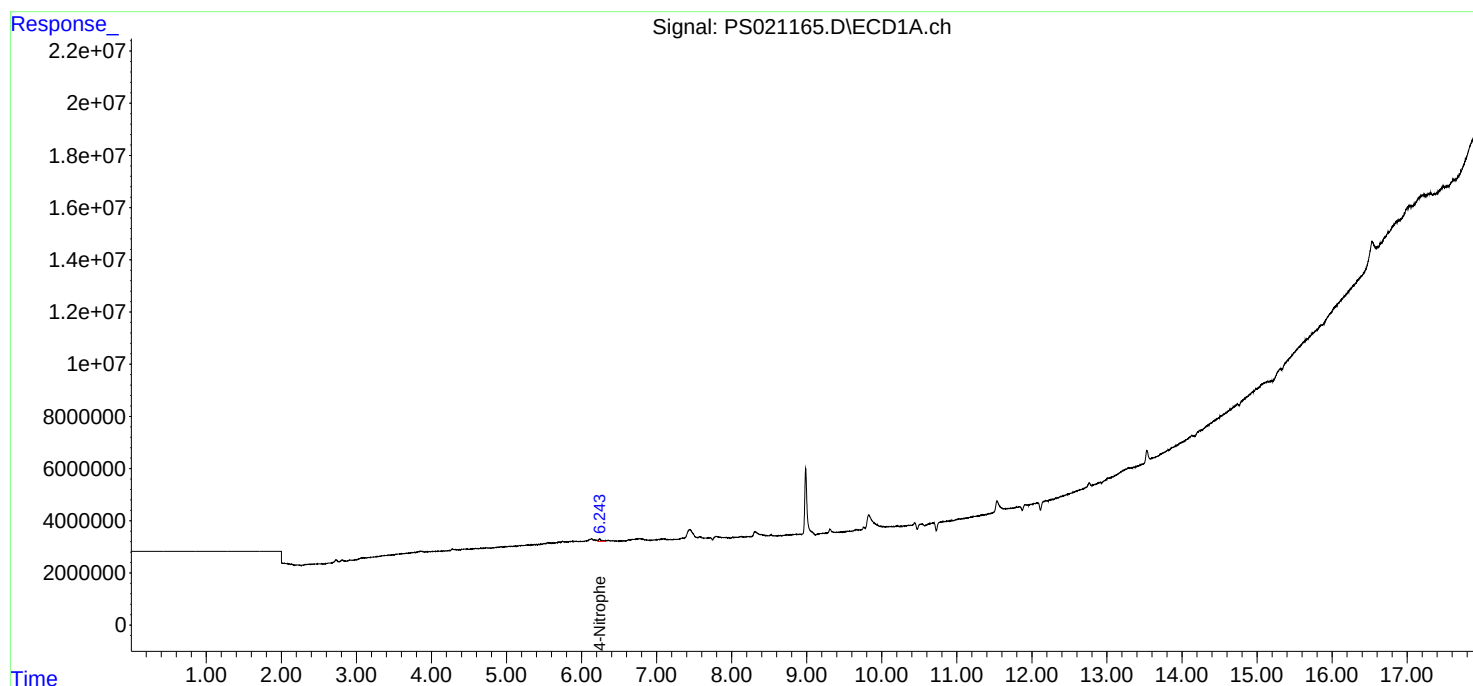


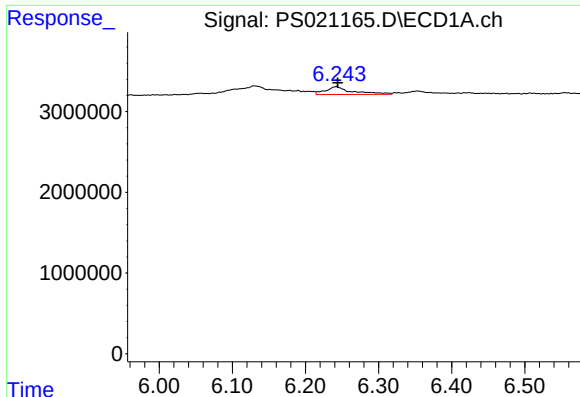

#3 4-Nitrophenol


R.T.: 6.242 min
Delta R.T.: -0.002 min
Response: 2514049
Conc: 1.67 ng/ml

Instrument :
ECD_S
ClientSampleId :

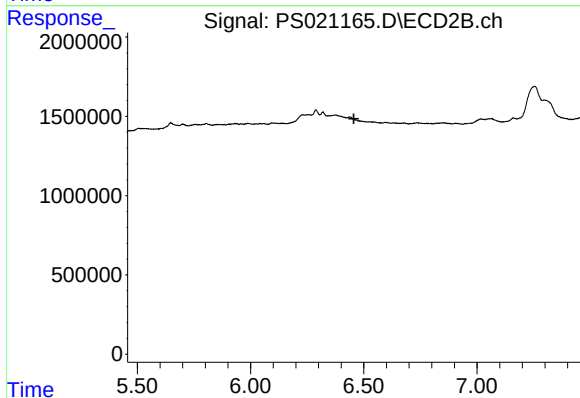


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.456 min
Response: 0
Conc: N.D.

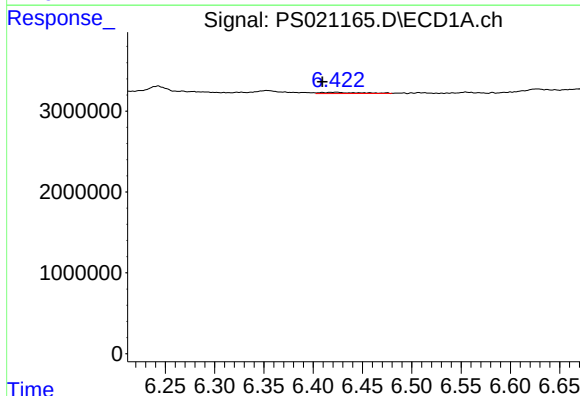


#4 2,4-DCAA

R.T.: 6.422 min
Delta R.T.: 0.013 min
Response: 394526
Conc: N.D.

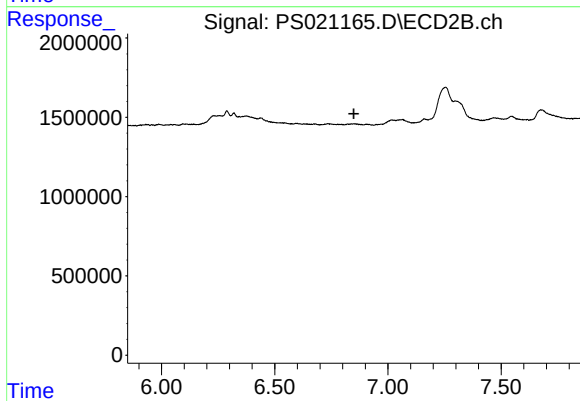

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.850 min
Response: 0
Conc: N.D.

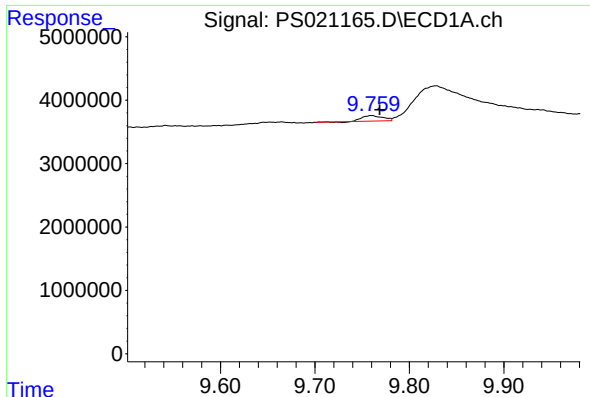

#15 Picloram

R.T.: 9.760 min
Delta R.T.: -0.009 min
Response: 1261196
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

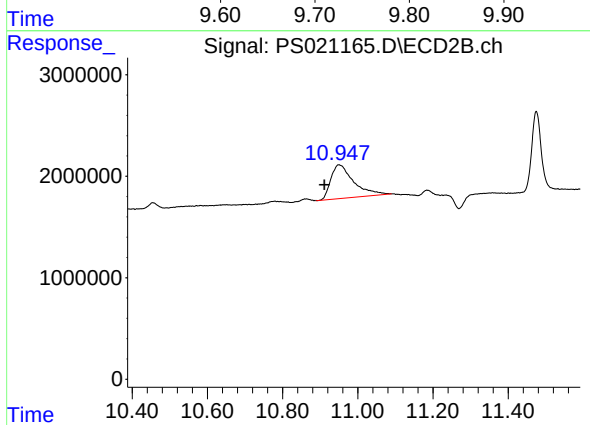

#15 Picloram

R.T.: 10.949 min
Delta R.T.: 0.038 min
Response: 14007798
Conc: 1.10 ng/ml