

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111522\
 Data File : PS021170.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Nov 2022 14:05
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 20:23:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102822.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 31 10:07:57 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.411	6.844	1048.3E6	788.5E6	502.277	570.095
Target Compounds							
1) T	Dalapon	2.487	0.000	385954	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.795	0.000	418752	0	<MDL	N.D. #
3) T	4-Nitroph...	6.252	0.000	5469716	0	3.637	N.D. #
5) T	DICAMBA	0.000	7.005	0	31534989	N.D.	5.078
6) T	MCPD	6.675	7.133	4842472	26582625	<MDL	5.595 #
7) T	MCPA	6.782f	0.000	13628927	0	1.453	N.D. #
8) T	DICHLORPROP	7.095f	7.667	2692295	3937459	1.179	2.557 #
9) T	2,4-D	7.379	0.000	3377147	0	1.208	N.D. #
10) T	Pentachlo...	7.588	8.359	2219834	4949572	<MDL	<MDL #
11) T	2,4,5-TP ...	8.122	8.723	3146673	630514	<MDL	<MDL #
12) T	2,4,5-T	8.394	9.109	8187330	5279611	<MDL	<MDL #
13) T	2,4-DB	8.904	9.626	492961	893648	<MDL	<MDL #
14) T	DINOSEB	10.013f	0.000	1812720	0	<MDL	N.D. #
15) T	Picloram	9.761	10.935	396050	33262480	<MDL	2.622 #
16) T	DCPA	10.211	10.862	1081112	1632394	<MDL	<MDL #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111522\
Data File : PS021170.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Nov 2022 14:05
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 20:23:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102822.M
Quant Title : 8080.M
QLast Update : Mon Oct 31 10:07:57 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

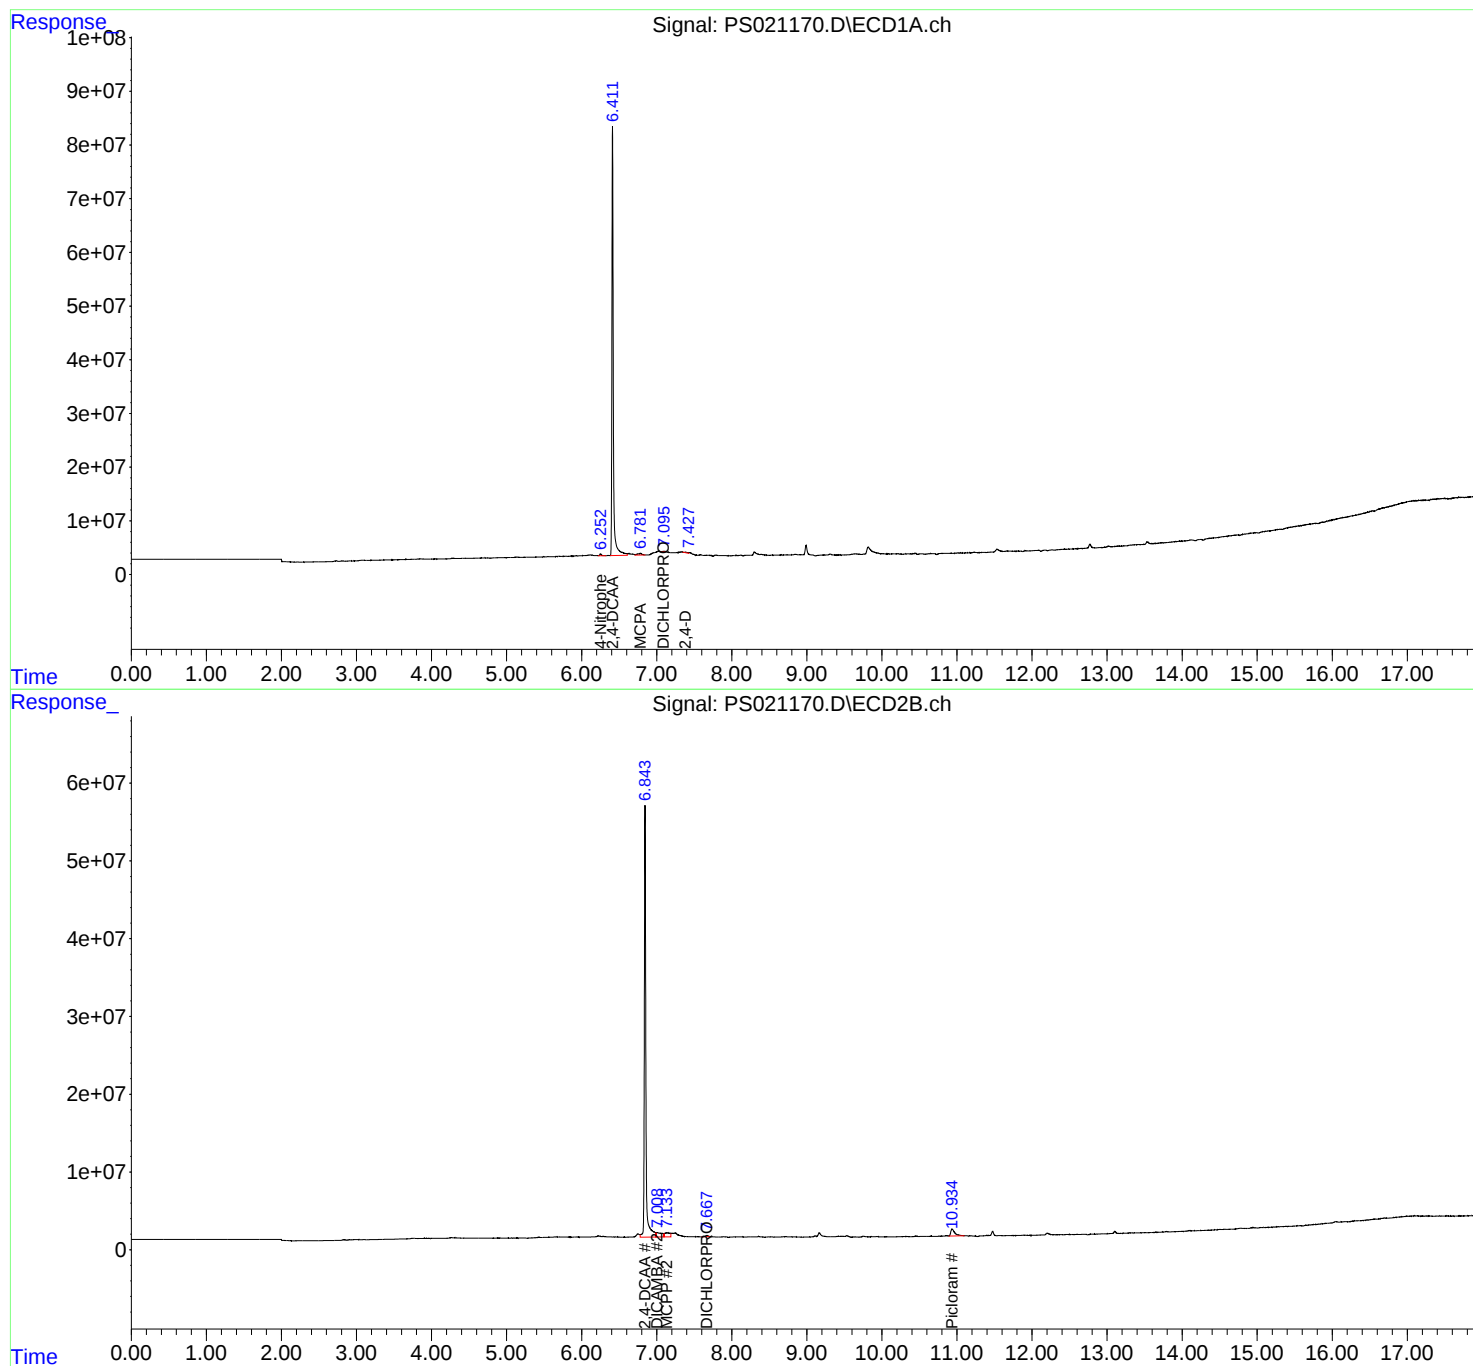


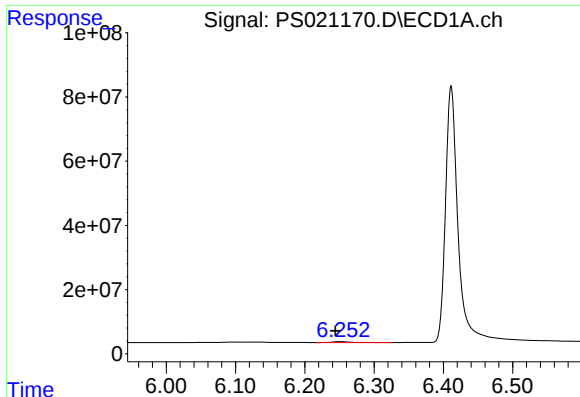

#3 4-Nitrophenol


R.T.: 6.252 min
Delta R.T.: 0.008 min
Response: 5469716
Conc: 3.64 ng/ml

Instrument :
ECD_S
ClientSampleId :

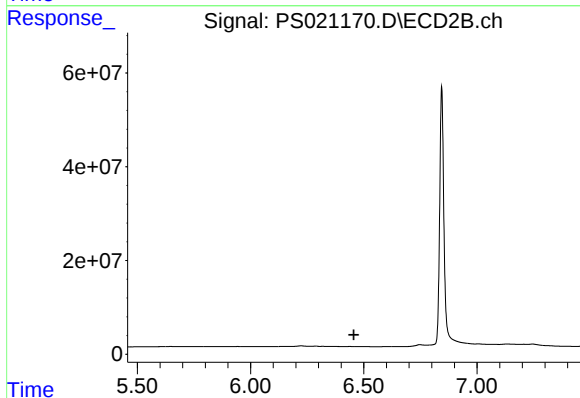


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.456 min
Response: 0
Conc: N.D.

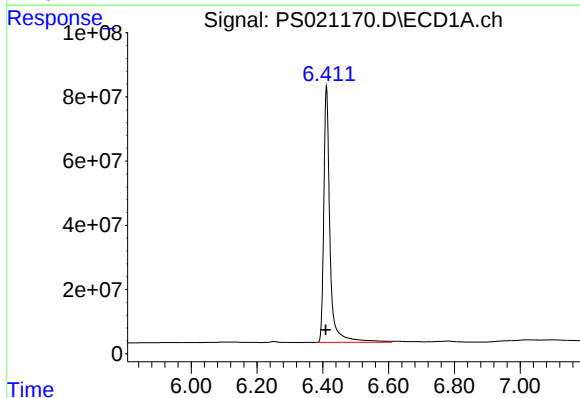


#4 2,4-DCAA

R.T.: 6.411 min
Delta R.T.: 0.002 min
Response: 1048290547
Conc: 502.28 ng/ml

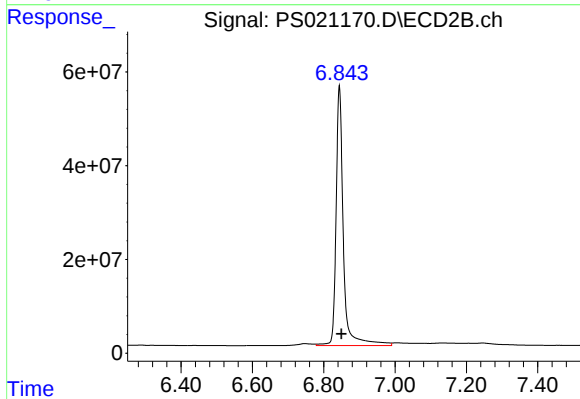

#4 2,4-DCAA


R.T.: 6.844 min
Delta R.T.: -0.006 min
Response: 788524878
Conc: 570.10 ng/ml

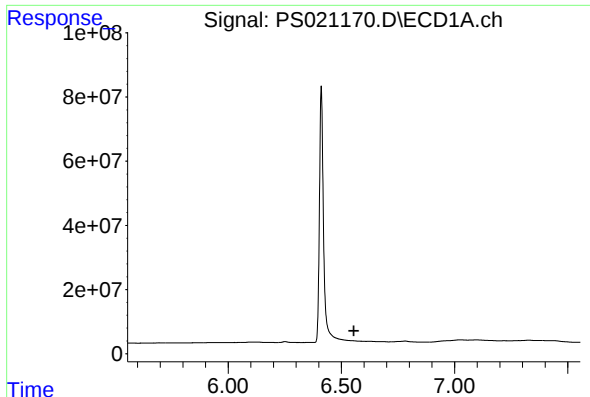

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.555 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

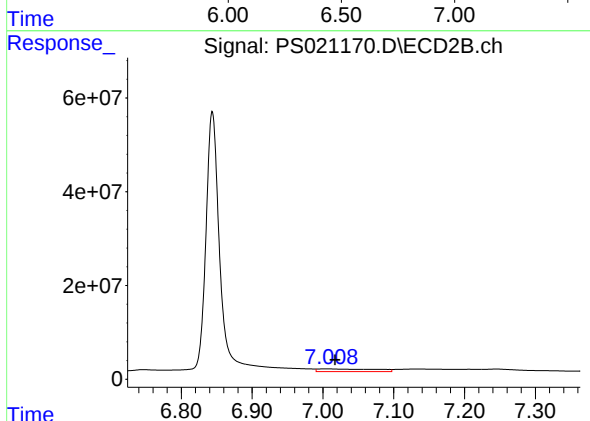


#5 DICAMBA

R.T.: 7.005 min
Delta R.T.: -0.012 min
Response: 31534989
Conc: 5.08 ng/ml

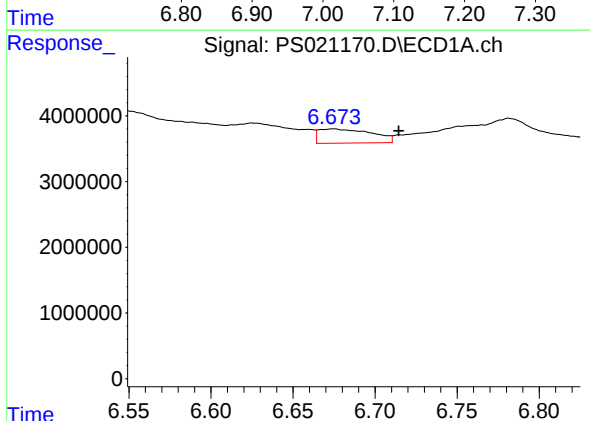


#6 MCP

R.T.: 6.675 min
Delta R.T.: -0.040 min
Response: 4842472
Conc: N.D.

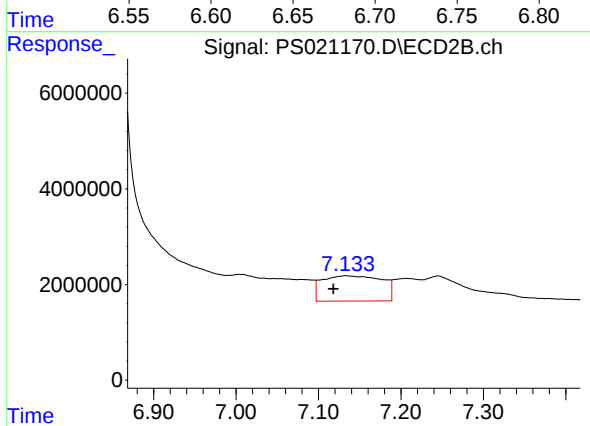

#6 MCP


R.T.: 7.133 min
Delta R.T.: 0.015 min
Response: 26582625
Conc: 5.60 ug/ml

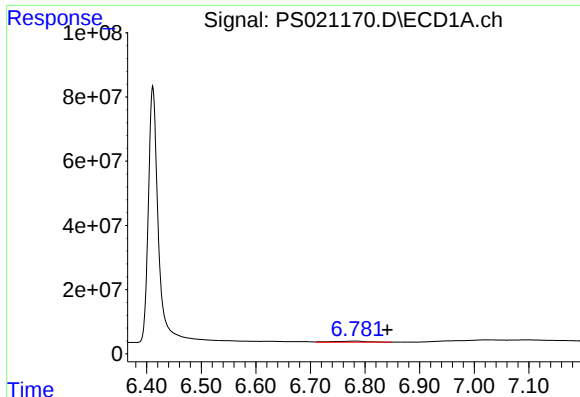

#7 MCPA


R.T.: 6.782 min
Delta R.T.: -0.059 min
Response: 13628927
Conc: 1.45 ug/ml

Instrument :
ECD_S
ClientSampleId :

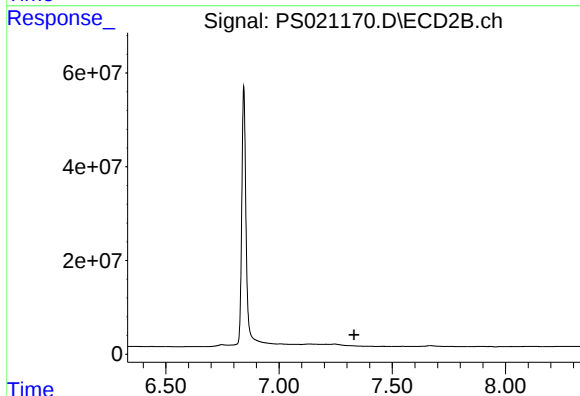


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.331 min
Response: 0
Conc: N.D.

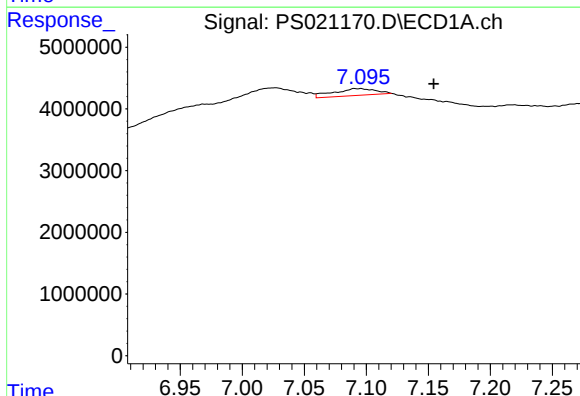


#8 DICHLORPROP

R.T.: 7.095 min
Delta R.T.: -0.059 min
Response: 2692295
Conc: 1.18 ng/ml

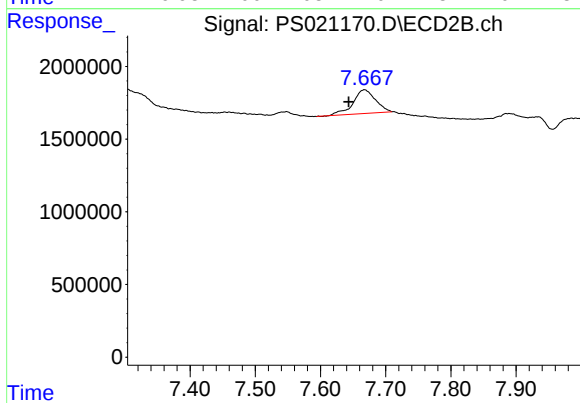

#8 DICHLORPROP


R.T.: 7.667 min
Delta R.T.: 0.024 min
Response: 3937459
Conc: 2.56 ng/ml

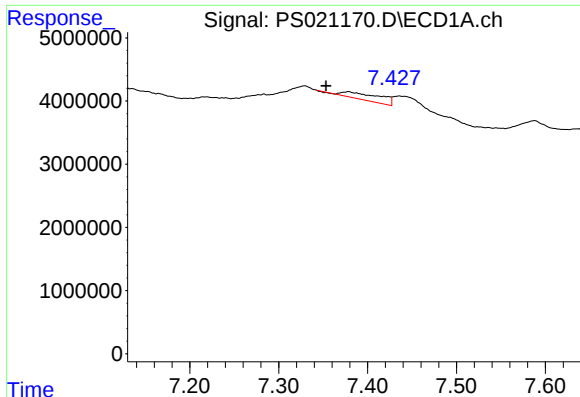

#9 2,4-D


R.T.: 7.379 min
Delta R.T.: 0.025 min
Response: 3377147
Conc: 1.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

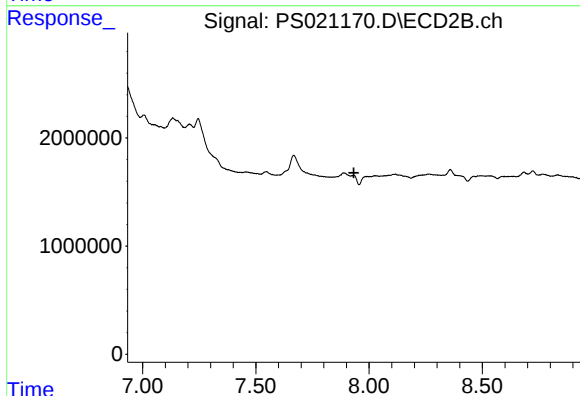


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.933 min
Response: 0
Conc: N.D.

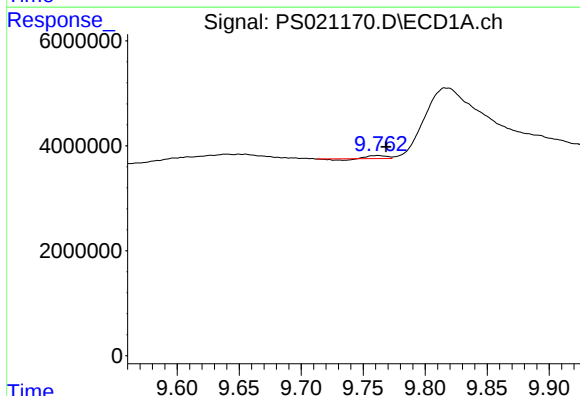

#15 Picloram

R.T.: 9.761 min
Delta R.T.: -0.007 min
Response: 396050
Conc: N.D.

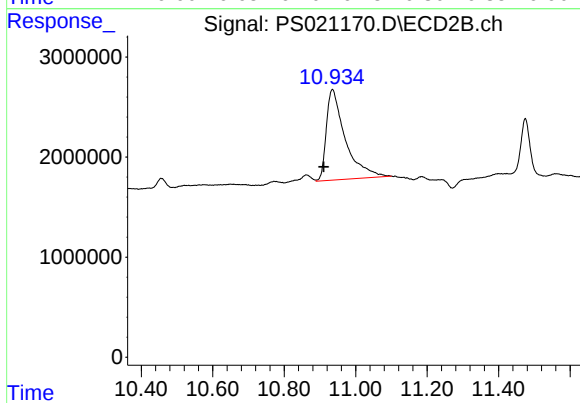

#15 Picloram

R.T.: 10.935 min
Delta R.T.: 0.024 min
Response: 33262480
Conc: 2.62 ng/ml