

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121919\
 Data File : PS008098.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2019 14:08
 Operator : SM\AJ
 Sample : PB125584TB
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 16:24:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121819.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 18 11:09:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.431	5.158	451.5E6	248.2E6	301.370	338.238
Target Compounds							
2) T	3,5-DICHL...	0.000	4.492	0	27459092	N.D.	29.120
5) T	DICAMBA	5.517	0.000	48494331	0	8.761	N.D. #
7) T	MCPA	5.891	5.525	30682149	22345309	5.375	7.483 #
10) T	Pentachlo...	0.000	6.370	0	17991095	N.D.	1.769
11) T	2,4,5-TP ...	0.000	6.760	0	18546447	N.D.	4.585
14) T	DINOSEB	0.000	7.945	0	7178554	N.D.	2.826
15) T	Picloram	0.000	8.930	0	5786049	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121919\
Data File : PS008098.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2019 14:08
Operator : SM\AJ
Sample : PB125584TB
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 16:24:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121819.M
Quant Title : 8080.M
QLast Update : Wed Dec 18 11:09:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

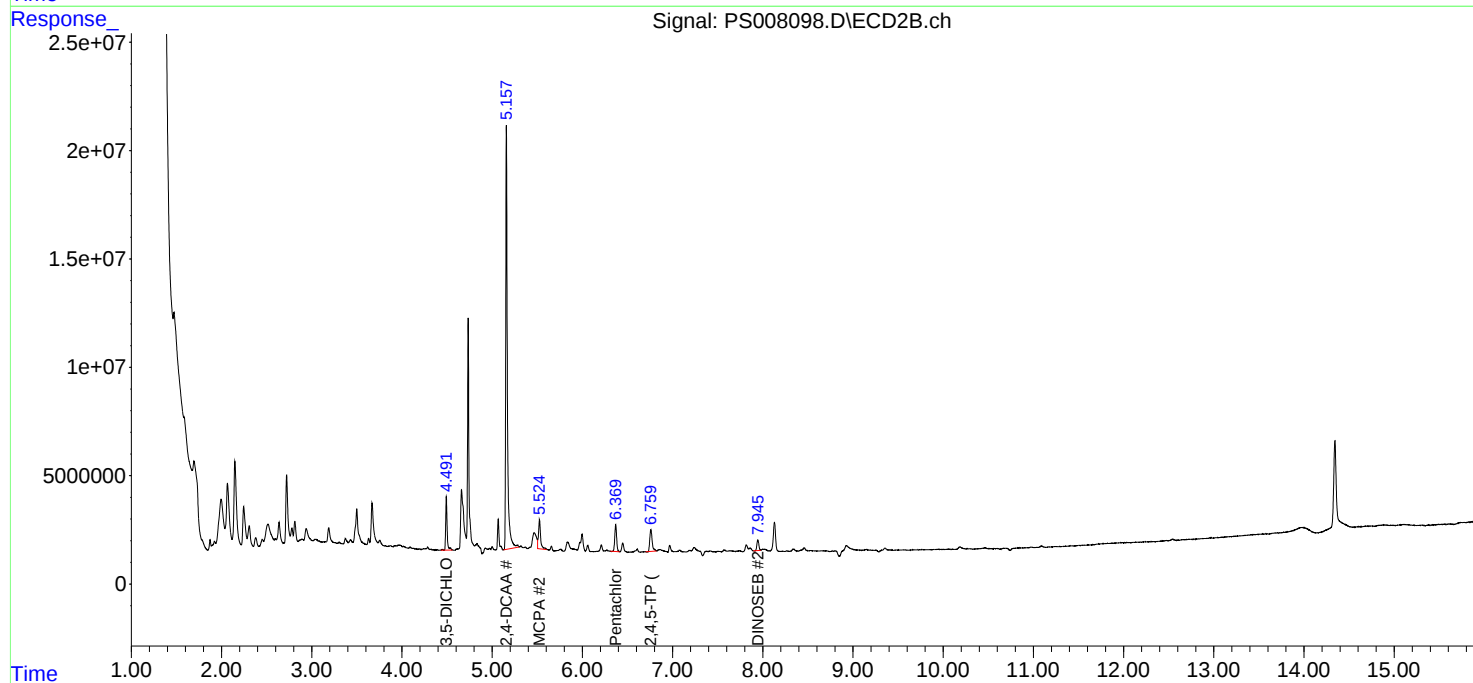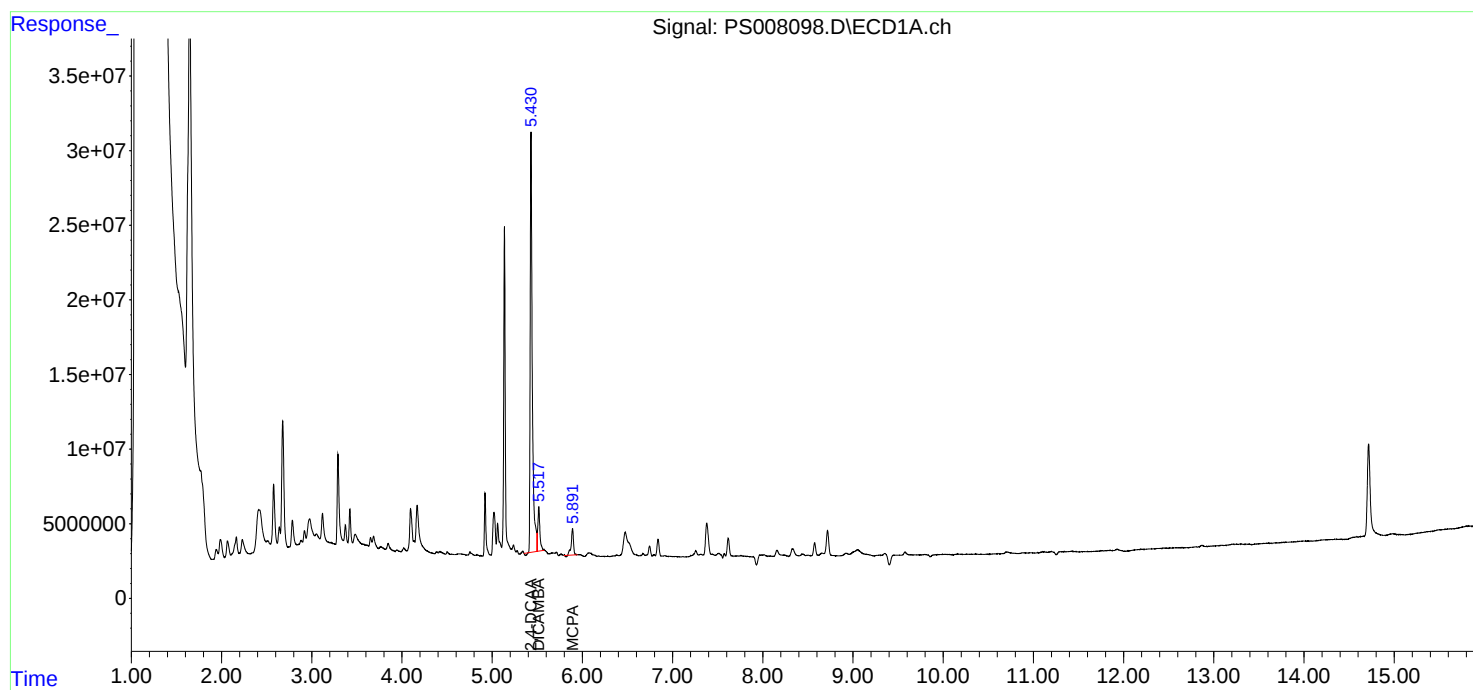


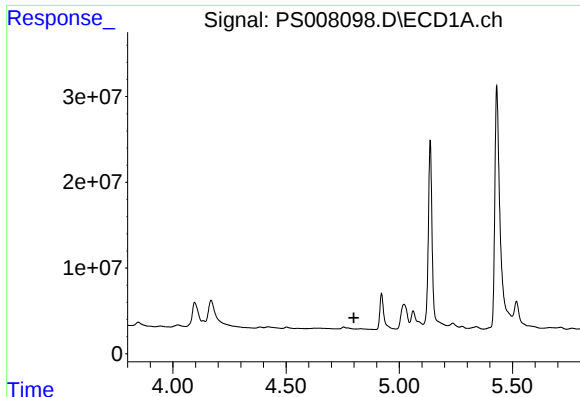

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.800 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

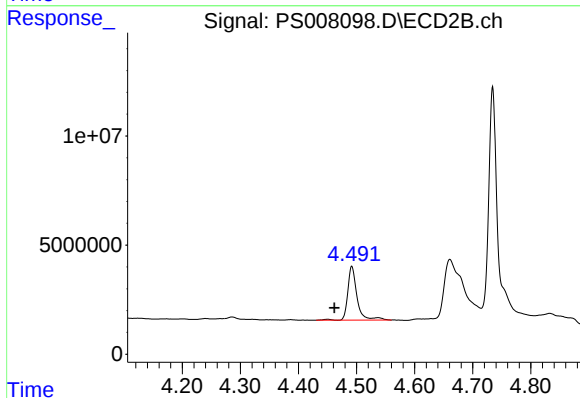


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.492 min
Delta R.T.: 0.030 min
Response: 27459092
Conc: 29.12 ng/ml

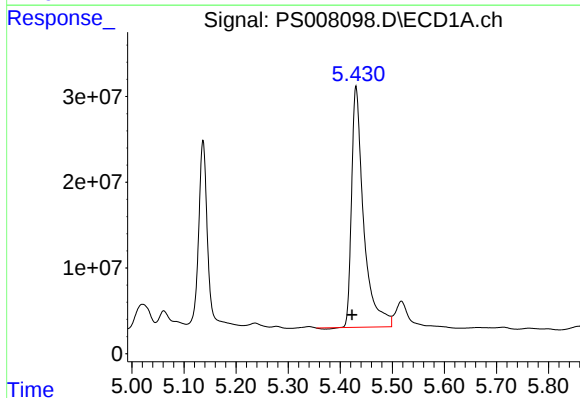


#4 2,4-DCAA

R.T.: 5.431 min
Delta R.T.: 0.008 min
Response: 451484308
Conc: 301.37 ng/ml

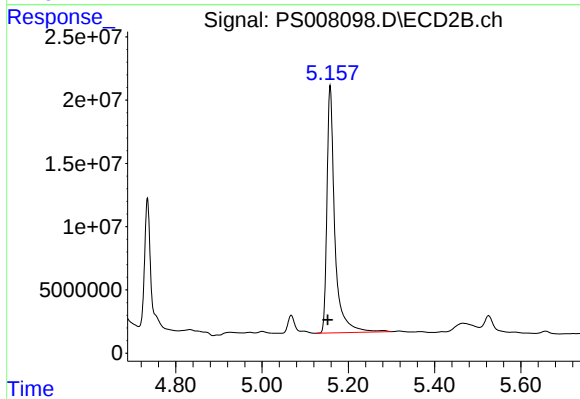

#4 2,4-DCAA


R.T.: 5.158 min
Delta R.T.: 0.006 min
Response: 248244339
Conc: 338.24 ng/ml

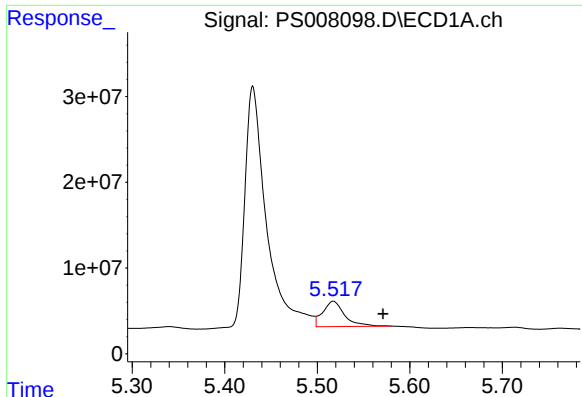

#5 DICAMBA


R.T.: 5.517 min
Delta R.T.: -0.054 min
Response: 48494331
Conc: 8.76 ng/ml

Instrument :
ECD_S
ClientSampleId :

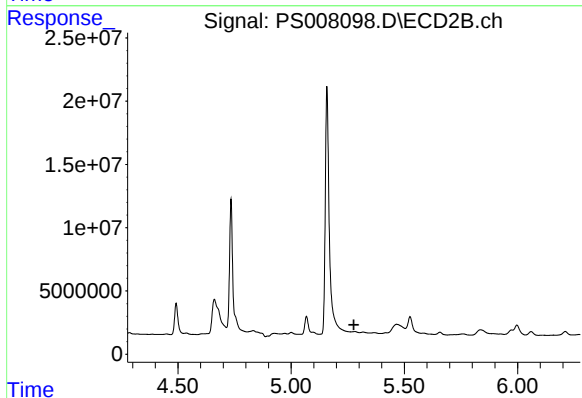


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.277 min
Response: 0
Conc: N.D.

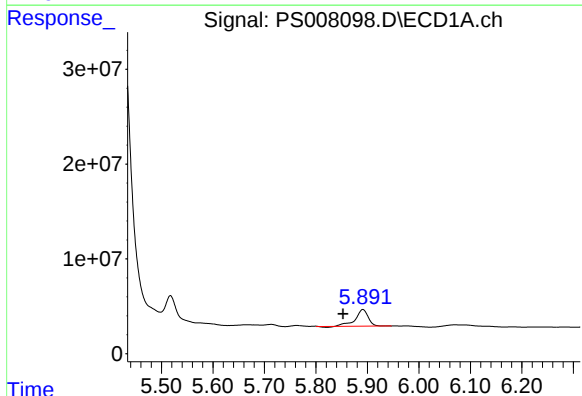


#7 MCPA

R.T.: 5.891 min
Delta R.T.: 0.039 min
Response: 30682149
Conc: 5.38 ug/ml

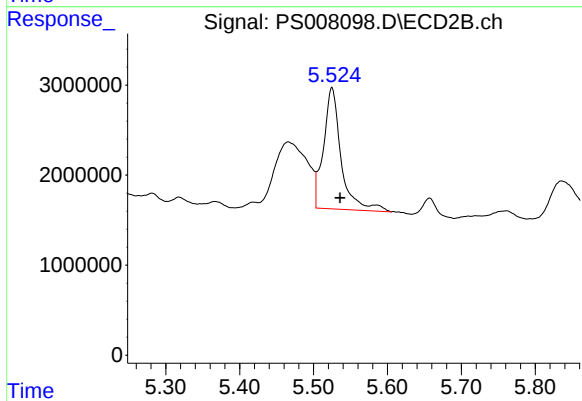

#7 MCPA


R.T.: 5.525 min
Delta R.T.: -0.011 min
Response: 22345309
Conc: 7.48 ug/ml

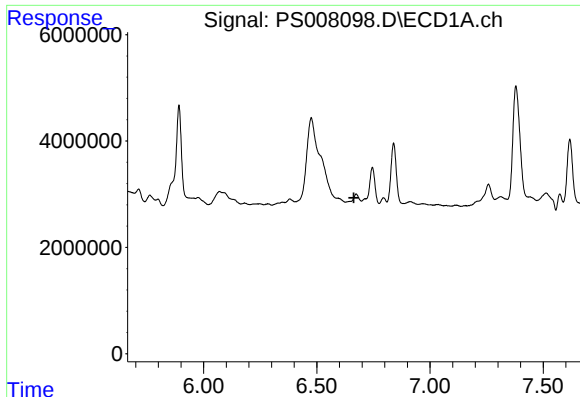

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.663 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

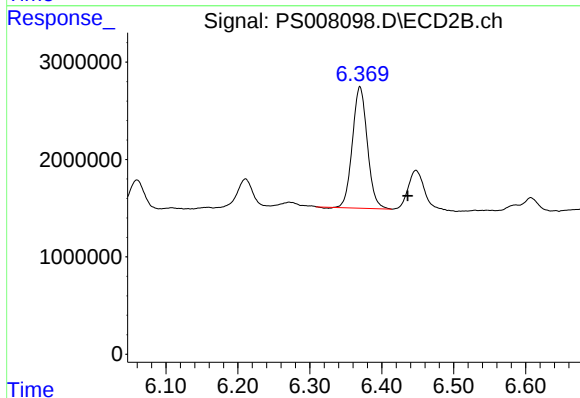


#10 Pentachlorophenol

R.T.: 6.370 min
Delta R.T.: -0.066 min
Response: 17991095
Conc: 1.77 ng/ml

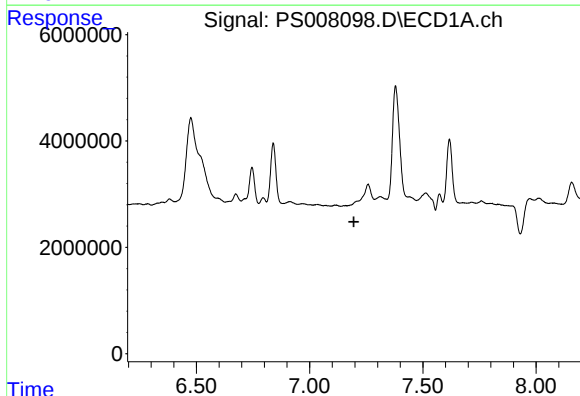


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.195 min
Response: 0
Conc: N.D.

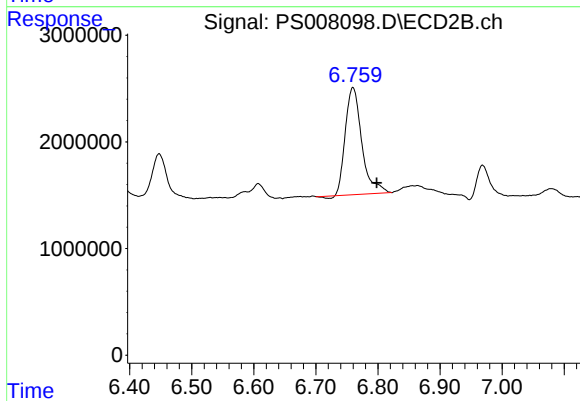

#11 2,4,5-TP (SILVEX)


R.T.: 6.760 min
Delta R.T.: -0.038 min
Response: 18546447
Conc: 4.59 ng/ml

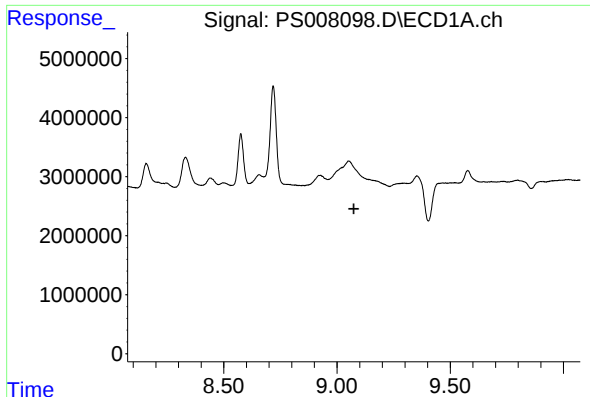

#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 9.075 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

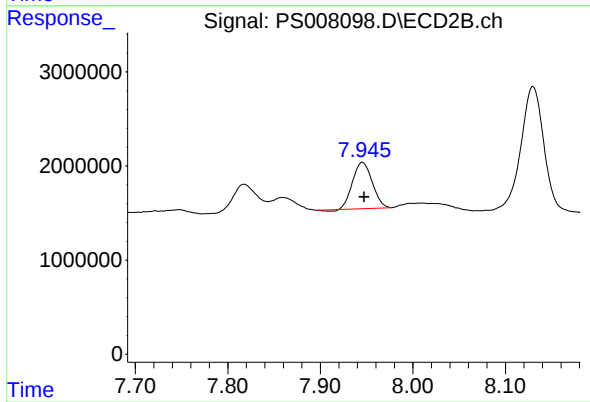

#14 DINOSEB

R.T.: 7.945 min
Delta R.T.: -0.002 min
Response: 7178554
Conc: 2.83 ng/ml