

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121919\
 Data File : PS008104.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2019 16:41
 Operator : SM\AJ
 Sample : K6318-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 05:35:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121819.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 18 11:09:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.438	5.167	954.9E6	497.1E6	637.377	677.308
Target Compounds							
2) T	3,5-DICHL...	0.000	4.502	0	51264343	N.D.	54.365
5) T	DICAMBA	5.528	5.306	40157139	8291776	7.255	3.001 #
6) T	MCP	0.000	5.306	0	8291776	N.D.	4.243
7) T	MCPA	0.000	5.479	0	34949517	N.D.	11.703
8) T	DICHLORPROP	0.000	5.840	0	7582691	N.D.	11.055
9) T	2,4-D	0.000	6.009	0	10386334	N.D.	12.766
10) T	Pentachlo...	0.000	6.381	0	11400366	N.D.	1.121
11) T	2,4,5-TP ...	0.000	6.765	0	37715910	N.D.	9.324
12) T	2,4,5-T	7.402	0.000	91912075	0	10.771	N.D. #
14) T	DINOSEB	0.000	7.999	0	11818463	N.D.	4.652



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121919\
Data File : PS008104.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2019 16:41
Operator : SM\AJ
Sample : K6318-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 05:35:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121819.M
Quant Title : 8080.M
QLast Update : Wed Dec 18 11:09:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

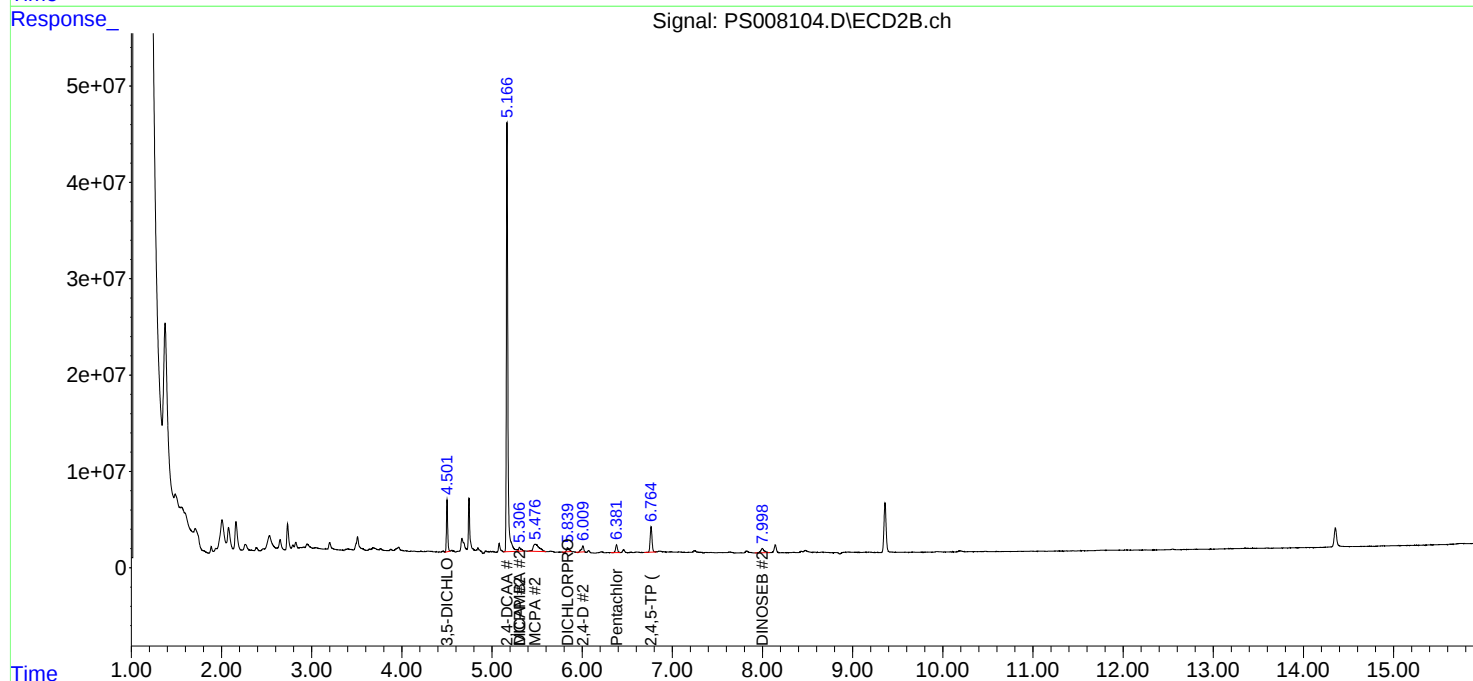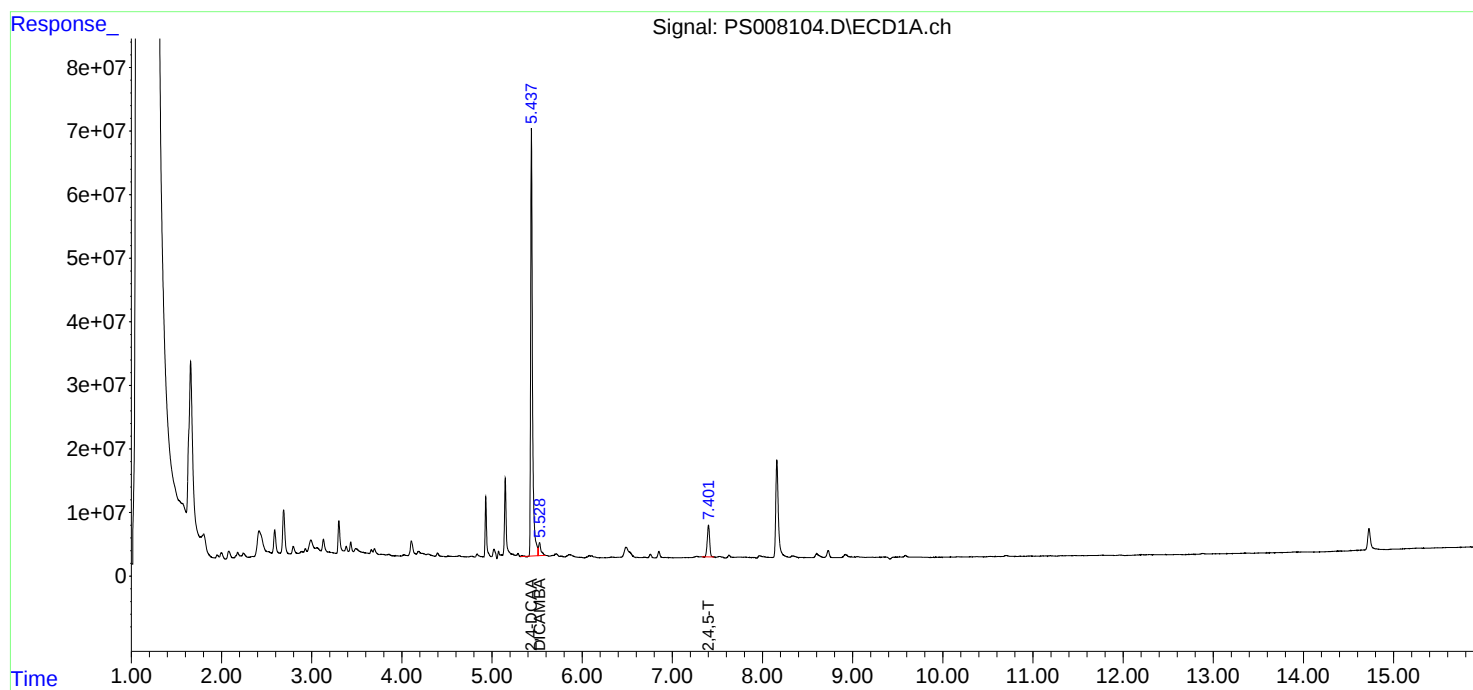


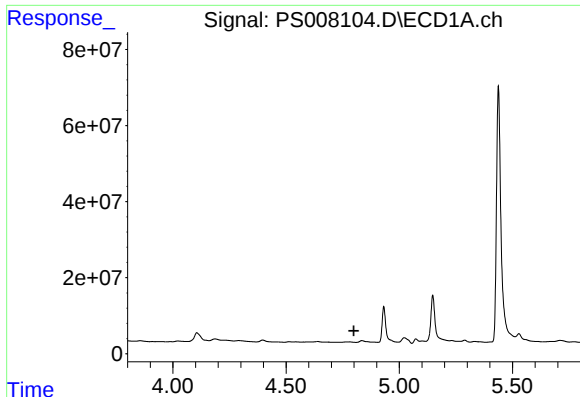

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.800 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

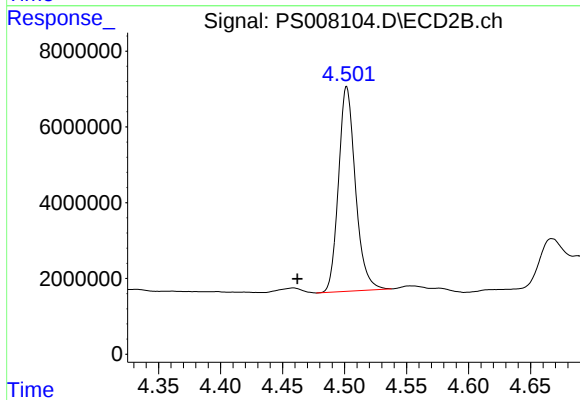


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.502 min
Delta R.T.: 0.040 min
Response: 51264343
Conc: 54.36 ng/ml

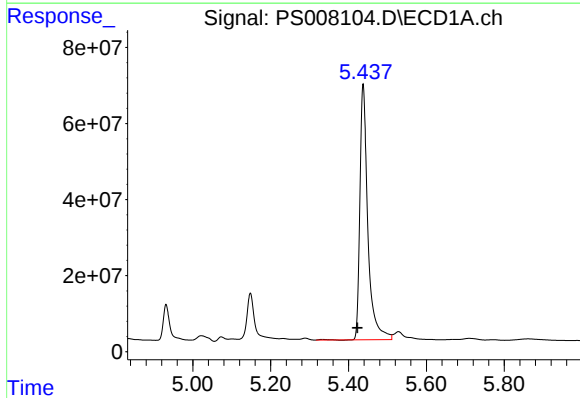


#4 2,4-DCAA

R.T.: 5.438 min
Delta R.T.: 0.015 min
Response: 954858745
Conc: 637.38 ng/ml

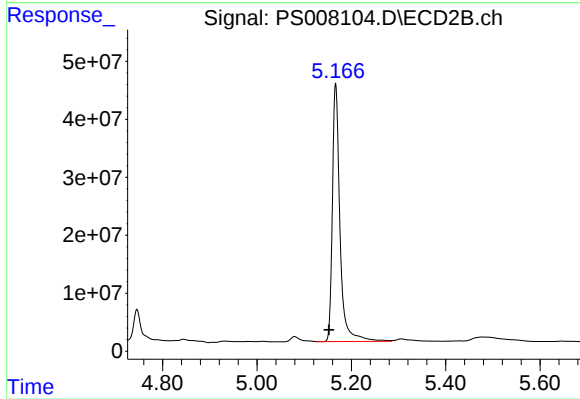

#4 2,4-DCAA


R.T.: 5.167 min
Delta R.T.: 0.015 min
Response: 497099727
Conc: 677.31 ng/ml

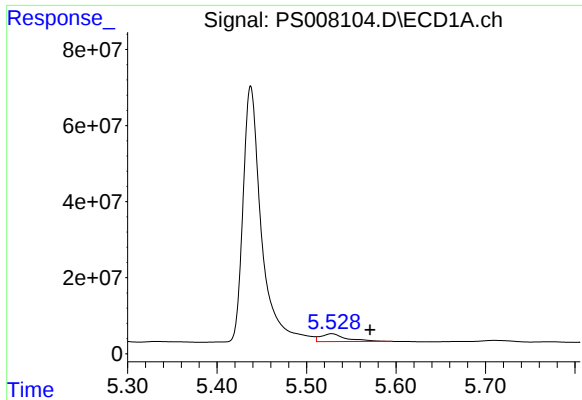

#5 DICAMBA


R.T.: 5.528 min
Delta R.T.: -0.043 min
Response: 40157139
Conc: 7.26 ng/ml

Instrument :
ECD_S
ClientSampleId :

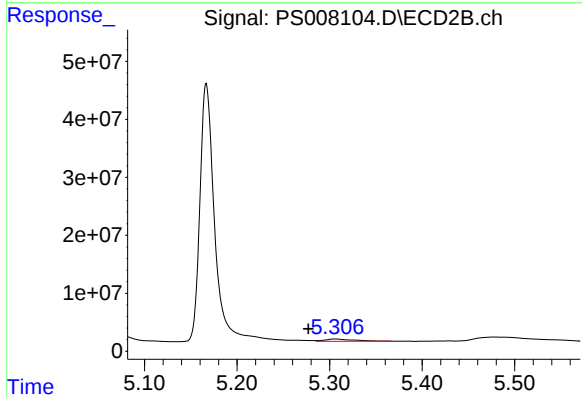


#5 DICAMBA

R.T.: 5.306 min
Delta R.T.: 0.029 min
Response: 8291776
Conc: 3.00 ng/ml

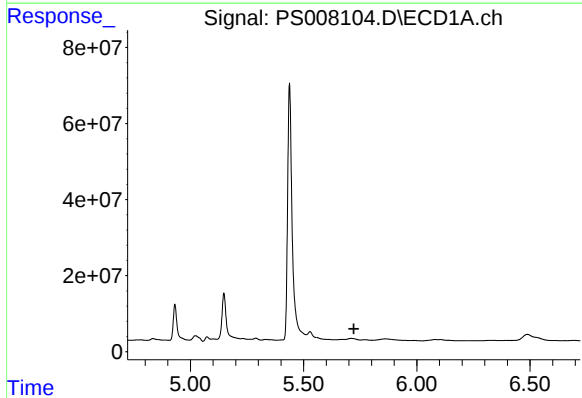


#6 MCP

R.T.: 0.000 min
Exp R.T. : 5.722 min
Response: 0
Conc: N.D.

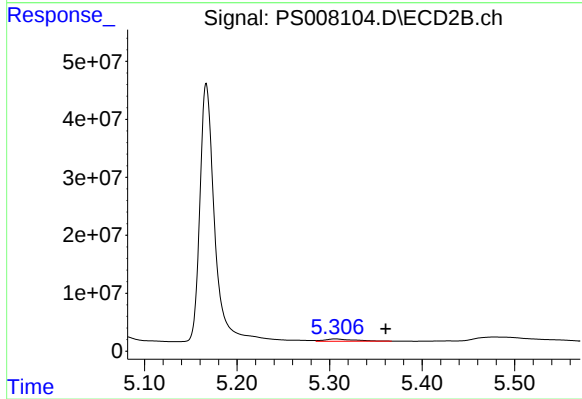

#6 MCP


R.T.: 5.306 min
Delta R.T.: -0.055 min
Response: 8291776
Conc: 4.24 ug/ml

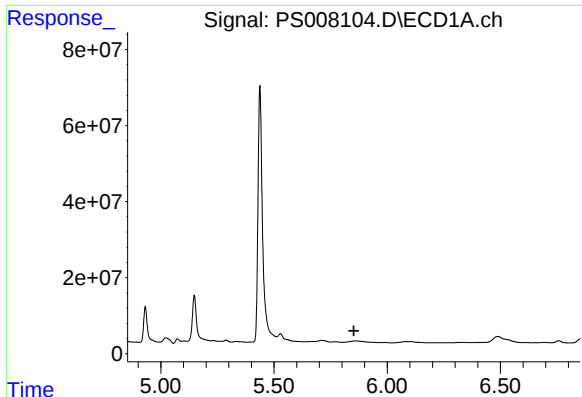

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 5.853 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

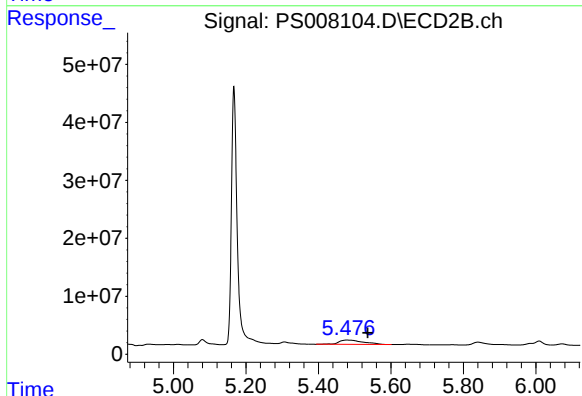


#7 MCPA

R.T.: 5.479 min
Delta R.T.: -0.057 min
Response: 34949517
Conc: 11.70 ug/ml

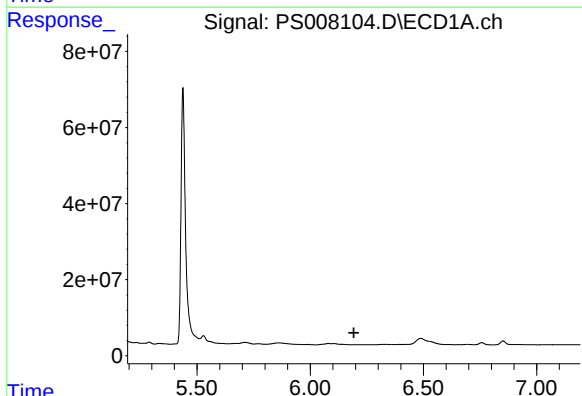


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 6.193 min
Response: 0
Conc: N.D.

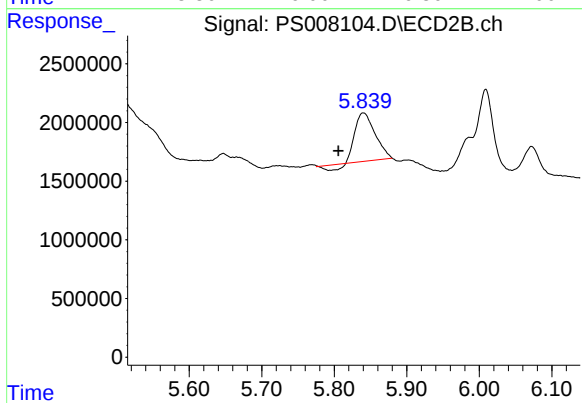

#8 DICHLORPROP


R.T.: 5.840 min
Delta R.T.: 0.035 min
Response: 7582691
Conc: 11.05 ng/ml

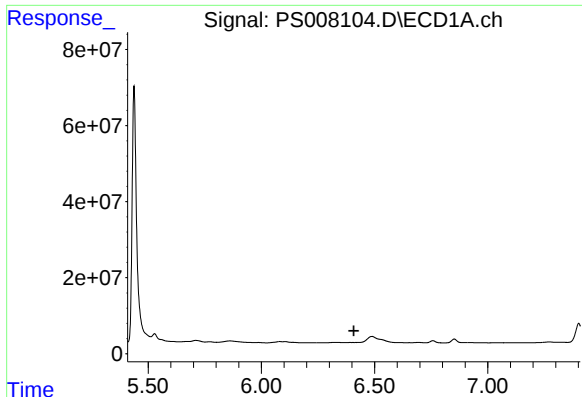

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.409 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

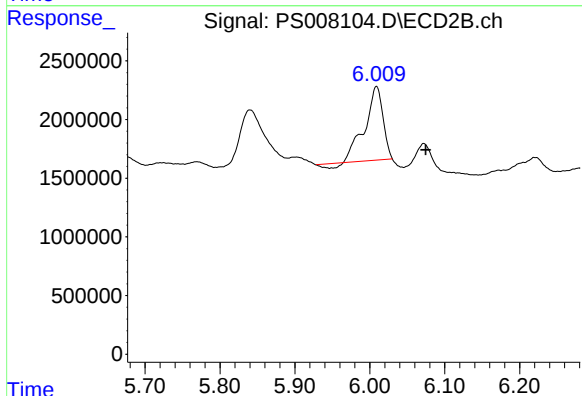


#9 2,4-D

R.T.: 6.009 min
Delta R.T.: -0.066 min
Response: 10386334
Conc: 12.77 ng/ml

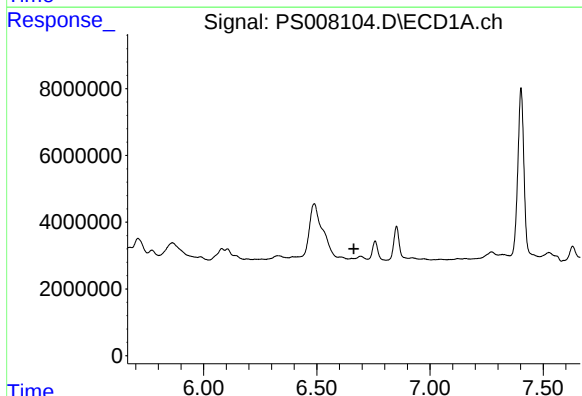


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.663 min
Response: 0
Conc: N.D.

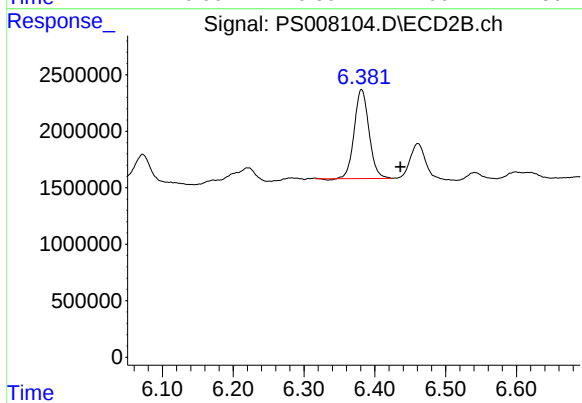

#10 Pentachlorophenol


R.T.: 6.381 min
Delta R.T.: -0.055 min
Response: 11400366
Conc: 1.12 ng/ml

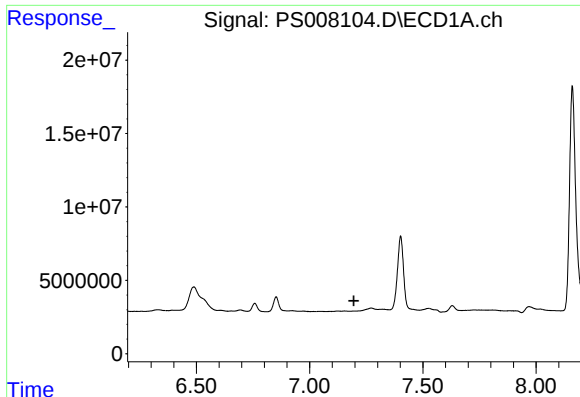

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.195 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

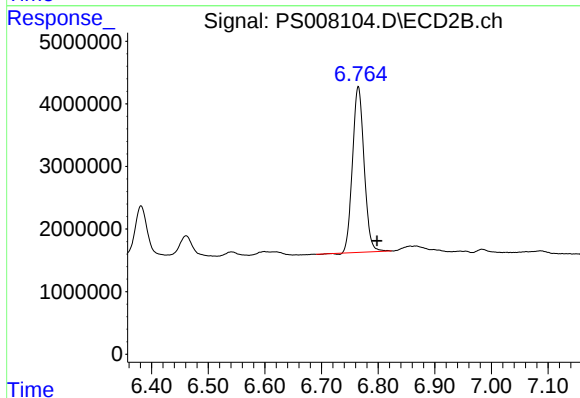


#11 2,4,5-TP (SILVEX)

R.T.: 6.765 min
Delta R.T.: -0.033 min
Response: 37715910
Conc: 9.32 ng/ml

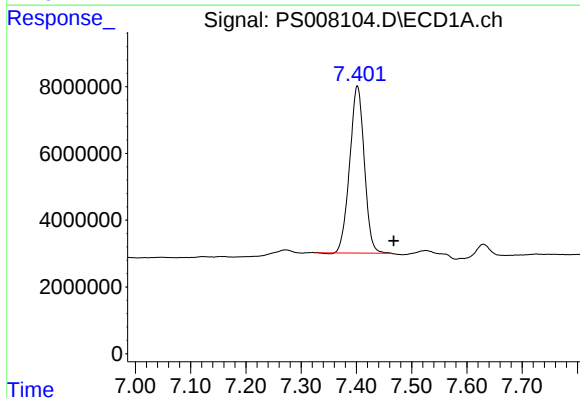


#12 2,4,5-T

R.T.: 7.402 min
Delta R.T.: -0.066 min
Response: 91912075
Conc: 10.77 ng/ml

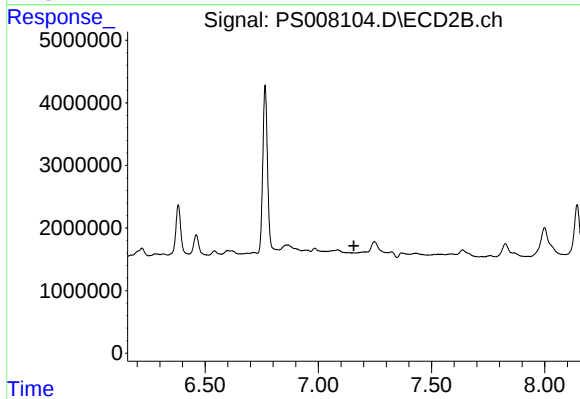

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.157 min
Response: 0
Conc: N.D.

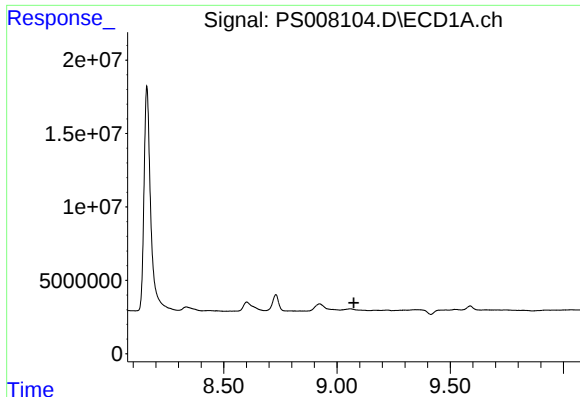

#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 9.075 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

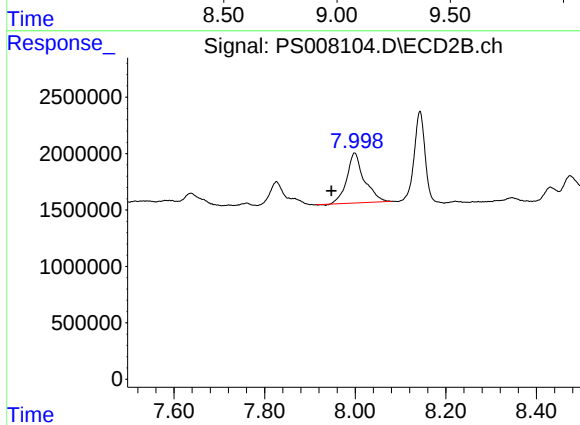

#14 DINOSEB

R.T.: 7.999 min
Delta R.T.: 0.051 min
Response: 11818463
Conc: 4.65 ng/ml