

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121919\
 Data File : PS008109.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2019 18:30
 Operator : SM\AJ
 Sample : K6299-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 05:36:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121819.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 18 11:09:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.428	5.159	344.1E6	165.8E6	229.677	225.857
Target Compounds							
2) T	3,5-DICHL...	0.000	4.491	0	61587814	N.D.	65.313
5) T	DICAMBA	5.518	0.000	61667719	0	11.141	N.D. #
7) T	MCPA	5.892	5.526	26545613	23609907	4.651	7.906 #
8) T	DICHLORPROP	0.000	5.825	0	3419694	N.D.	4.986
10) T	Pentachlo...	0.000	6.370	0	25788256	N.D.	2.535
11) T	2,4,5-TP ...	0.000	6.756	0	28814343	N.D.	7.123
14) T	DINOSEB	0.000	7.946	0	17542212	N.D.	6.906
15) T	Picloram	0.000	8.921	0	18351085	N.D.	3.049



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121919\
Data File : PS008109.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2019 18:30
Operator : SM\AJ
Sample : K6299-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 05:36:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121819.M
Quant Title : 8080.M
QLast Update : Wed Dec 18 11:09:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

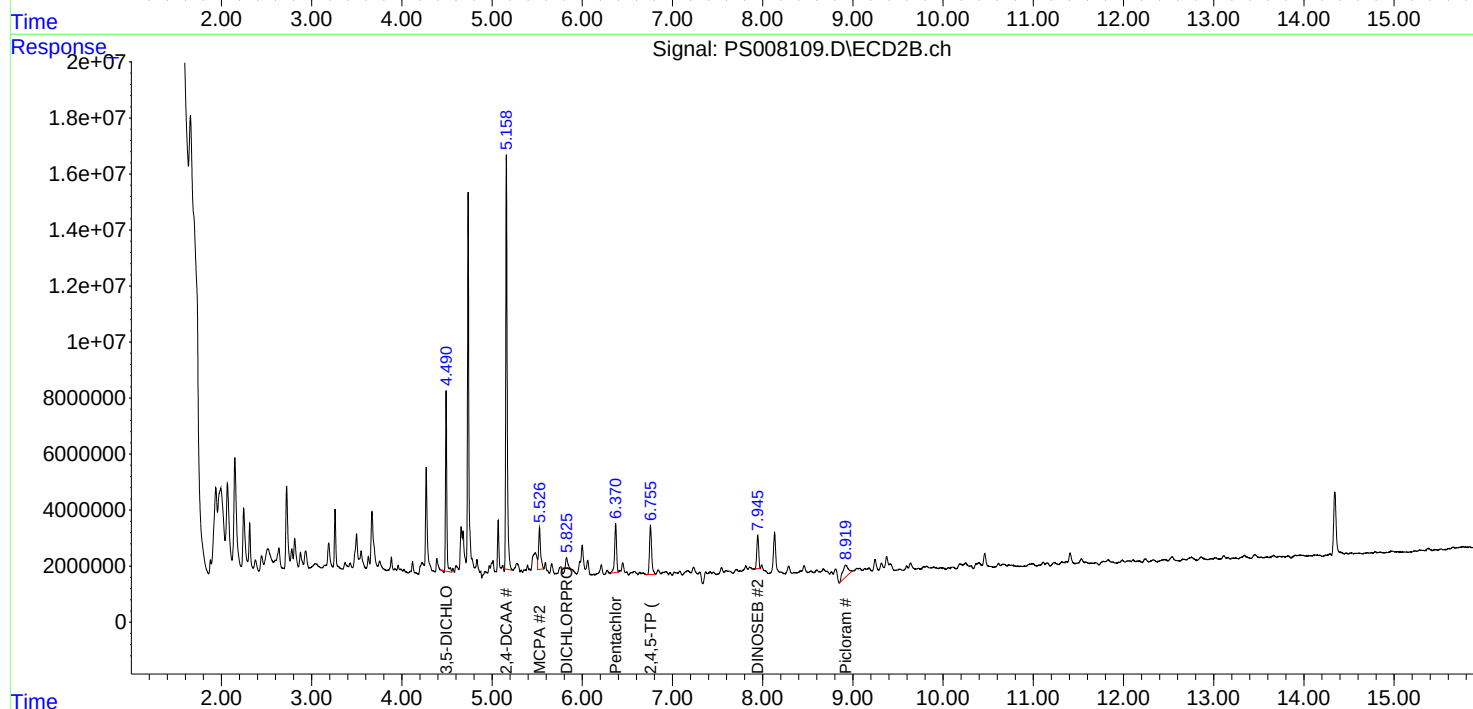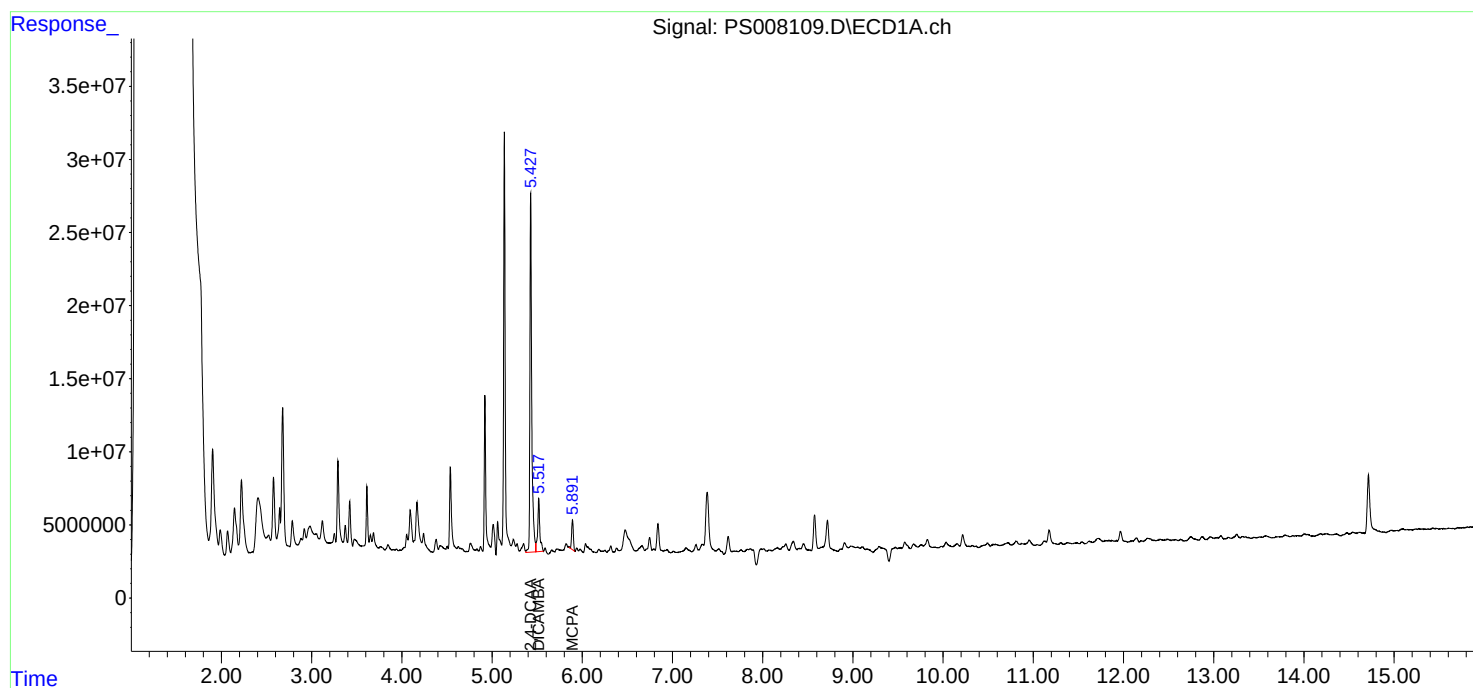


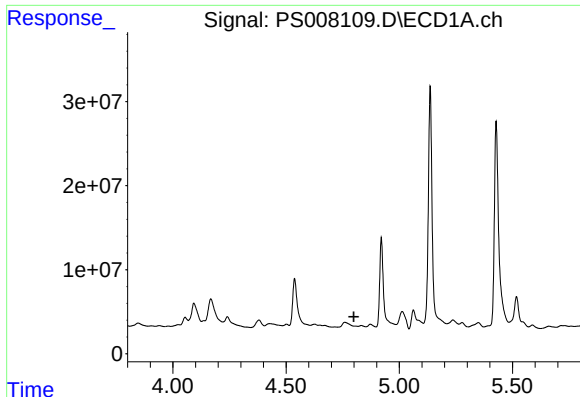

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.800 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

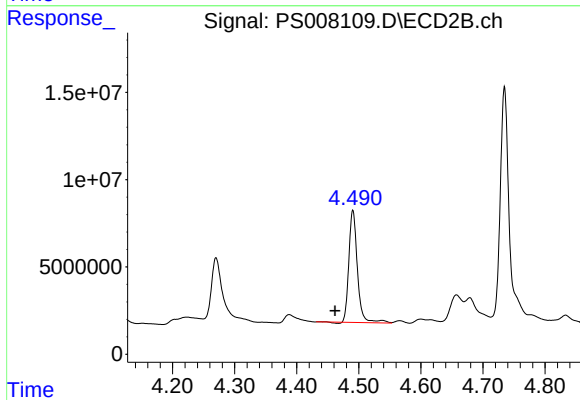


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.491 min
Delta R.T.: 0.029 min
Response: 61587814
Conc: 65.31 ng/ml

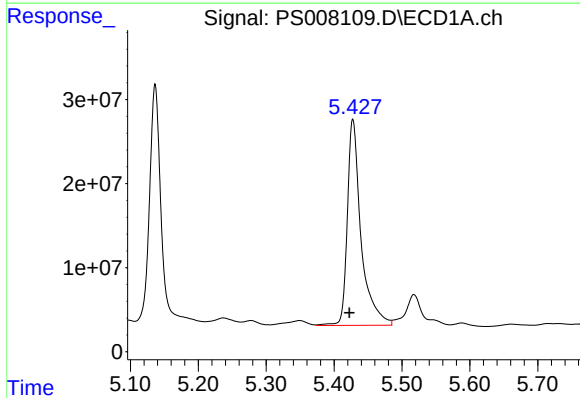


#4 2,4-DCAA

R.T.: 5.428 min
Delta R.T.: 0.005 min
Response: 344080411
Conc: 229.68 ng/ml

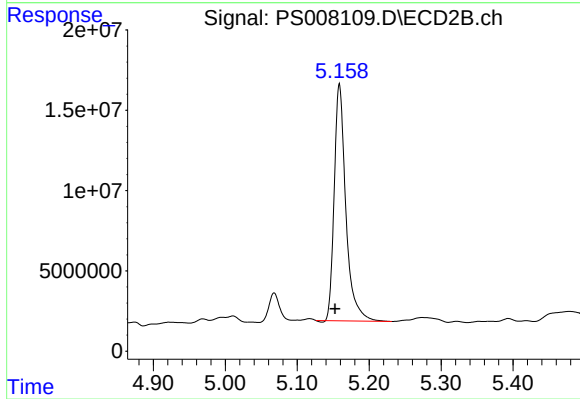

#4 2,4-DCAA


R.T.: 5.159 min
Delta R.T.: 0.006 min
Response: 165764370
Conc: 225.86 ng/ml

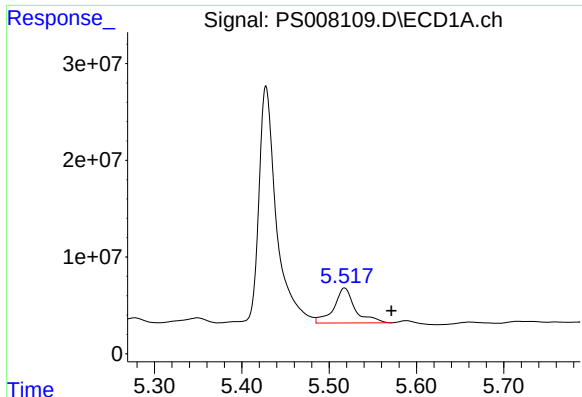

#5 DICAMBA


R.T.: 5.518 min
Delta R.T.: -0.054 min
Response: 61667719
Conc: 11.14 ng/ml

Instrument :
ECD_S
ClientSampleId :

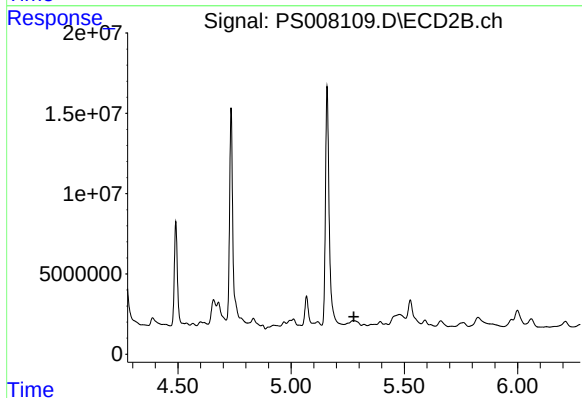


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.277 min
Response: 0
Conc: N.D.

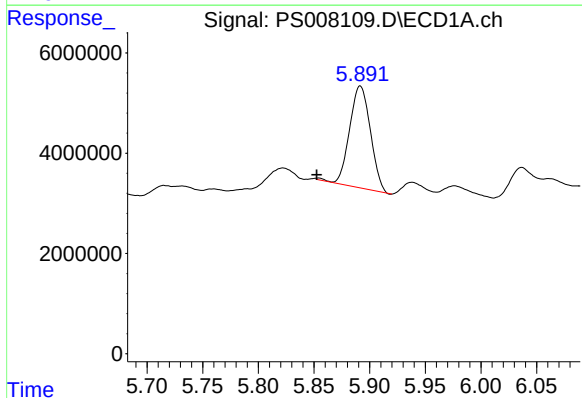


#7 MCPA

R.T.: 5.892 min
Delta R.T.: 0.039 min
Response: 26545613
Conc: 4.65 ug/ml

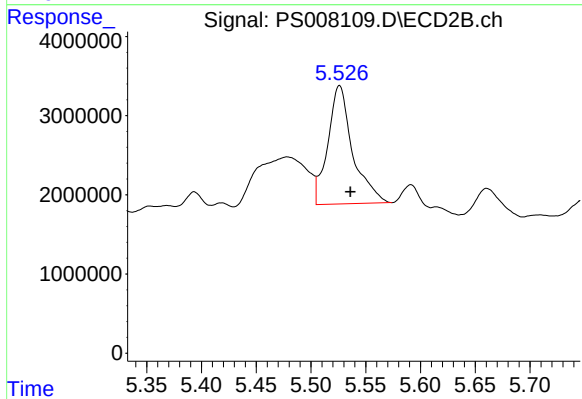

#7 MCPA


R.T.: 5.526 min
Delta R.T.: -0.010 min
Response: 23609907
Conc: 7.91 ug/ml

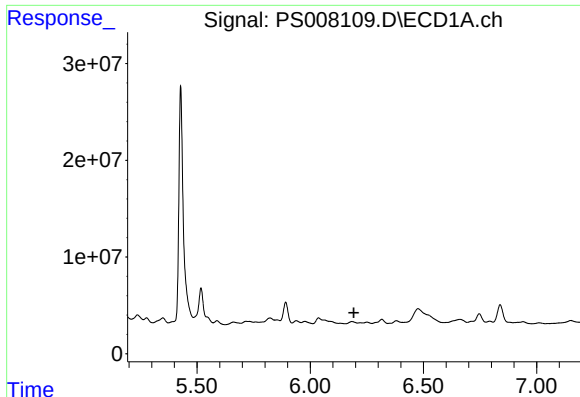

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.193 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

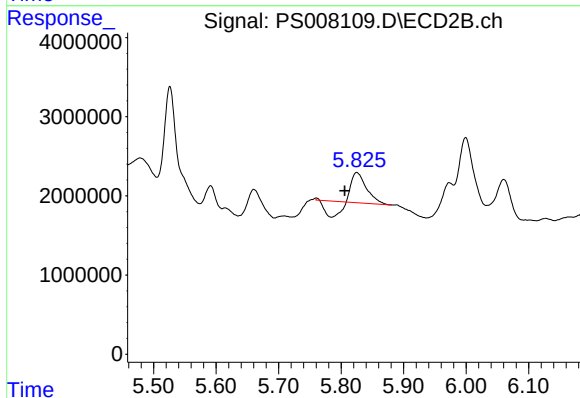


#8 DICHLORPROP

R.T.: 5.825 min
Delta R.T.: 0.020 min
Response: 3419694
Conc: 4.99 ng/ml

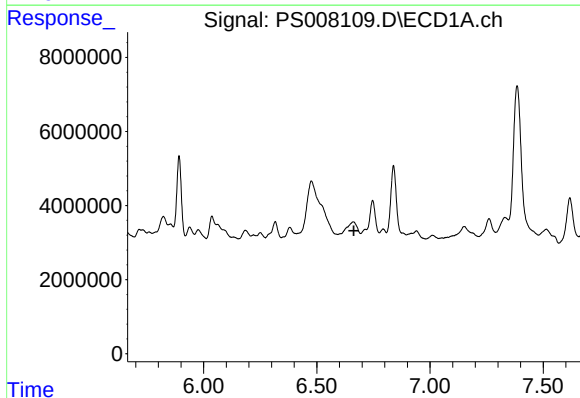


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.663 min
Response: 0
Conc: N.D.

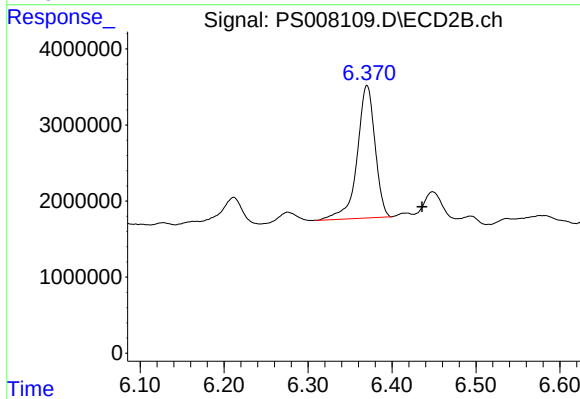

#10 Pentachlorophenol


R.T.: 6.370 min
Delta R.T.: -0.066 min
Response: 25788256
Conc: 2.54 ng/ml

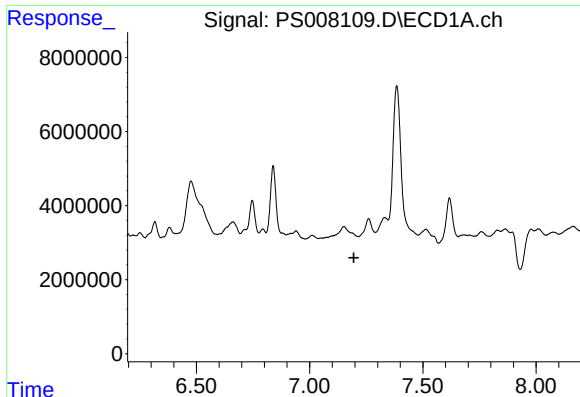

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.195 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

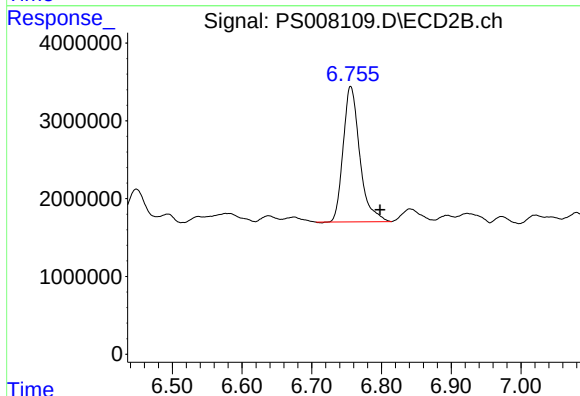


#11 2,4,5-TP (SILVEX)

R.T.: 6.756 min
Delta R.T.: -0.042 min
Response: 28814343
Conc: 7.12 ng/ml

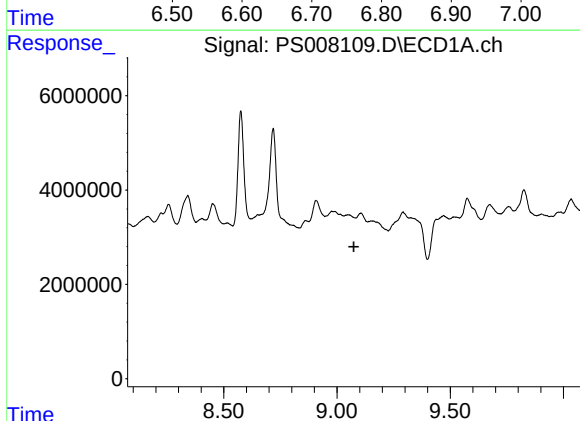


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 9.075 min
Response: 0
Conc: N.D.

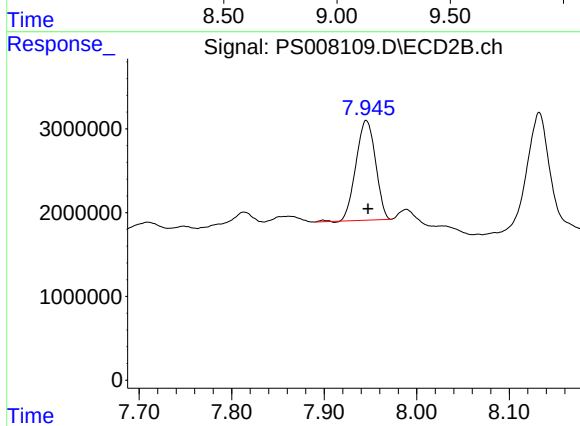

#14 DINOSEB


R.T.: 7.946 min
Delta R.T.: -0.002 min
Response: 17542212
Conc: 6.91 ng/ml

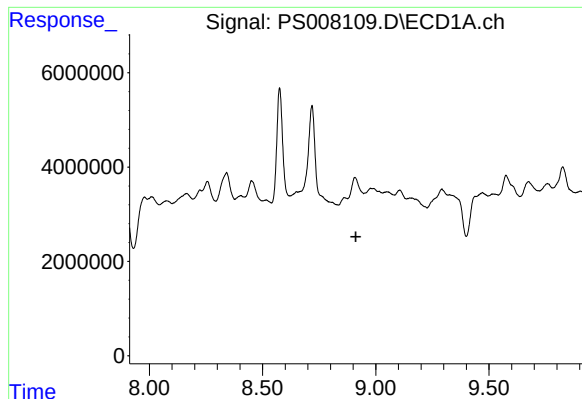

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.912 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

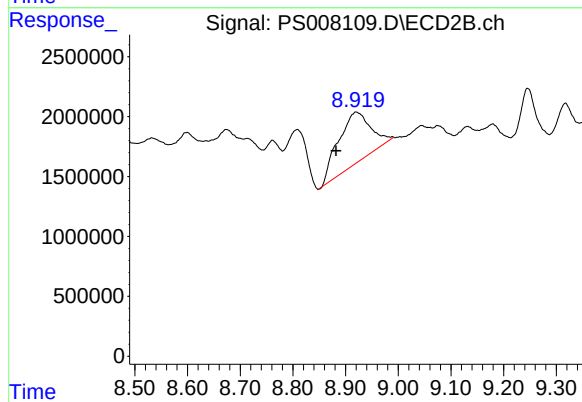

#15 Picloram

R.T.: 8.921 min
Delta R.T.: 0.039 min
Response: 18351085
Conc: 3.05 ng/ml