

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121919\
 Data File : PS008110.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2019 18:52
 Operator : SM\AJ
 Sample : K6299-06
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 05:37:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121819.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 18 11:09:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.425	5.157	485.1E6	210.3E6	323.825	286.561
Target Compounds							
1) T	Dalapon	1.985	0.000	64763020	0	34.594	N.D. #
2) T	3,5-DICHL...	0.000	4.490	0	54733118	N.D.	58.044
5) T	DICAMBA	5.518	5.276	83643242	11233586	15.112	4.065 #
6) T	MCP	0.000	5.392	0	8393540	N.D.	4.296
7) T	MCPA	5.891	5.525	35434395	36660498	6.208	12.276 #
8) T	DICHLORPROP	0.000	5.821	0	6387726	N.D.	9.313
10) T	Pentachlo...	0.000	6.448	0	11962693	N.D.	1.176
11) T	2,4,5-TP ...	0.000	6.757	0	27268571	N.D.	6.741
13) T	2,4-DB	0.000	7.590	0	13284256	N.D.	27.070
14) T	DINOSEB	0.000	7.944	0	25467145	N.D.	10.025
15) T	Picloram	0.000	8.913	0	29512182	N.D.	4.904



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121919\
Data File : PS008110.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2019 18:52
Operator : SM\AJ
Sample : K6299-06
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 05:37:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121819.M
Quant Title : 8080.M
QLast Update : Wed Dec 18 11:09:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

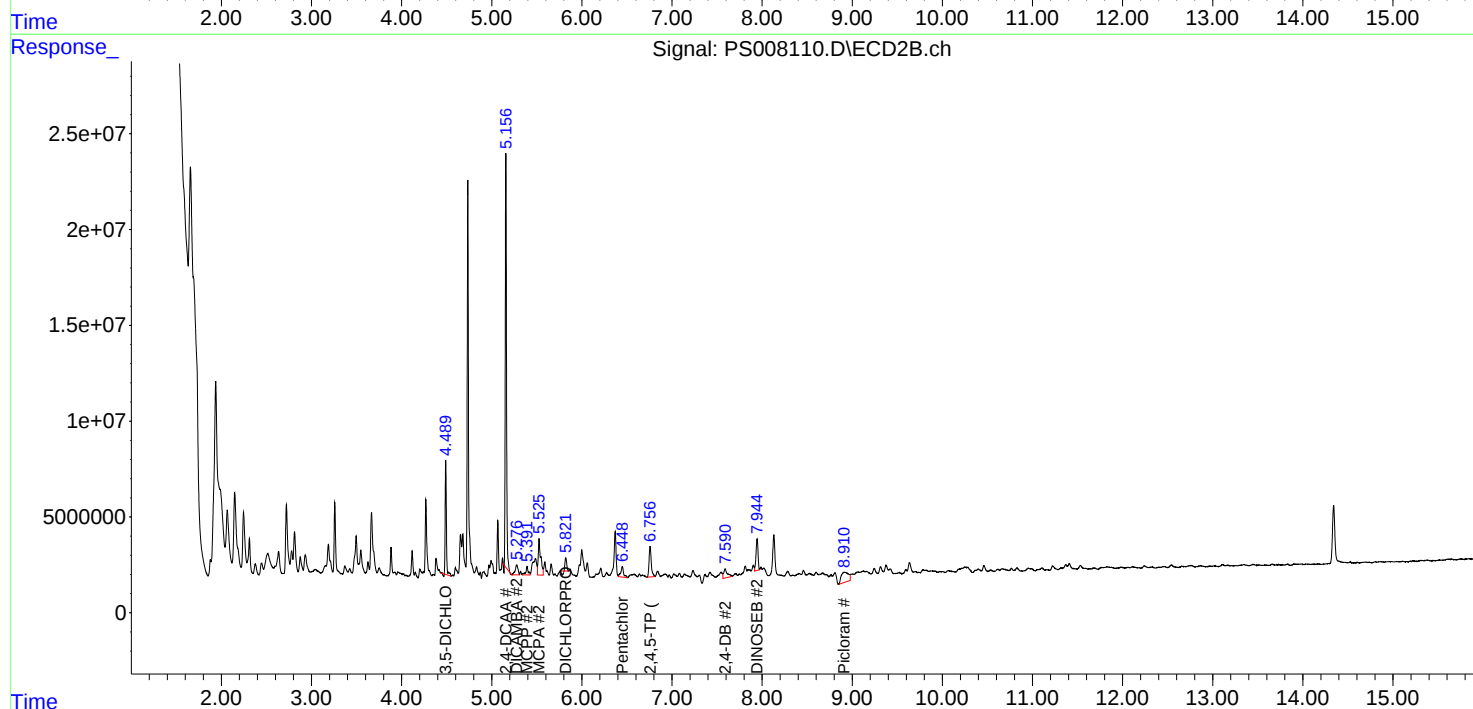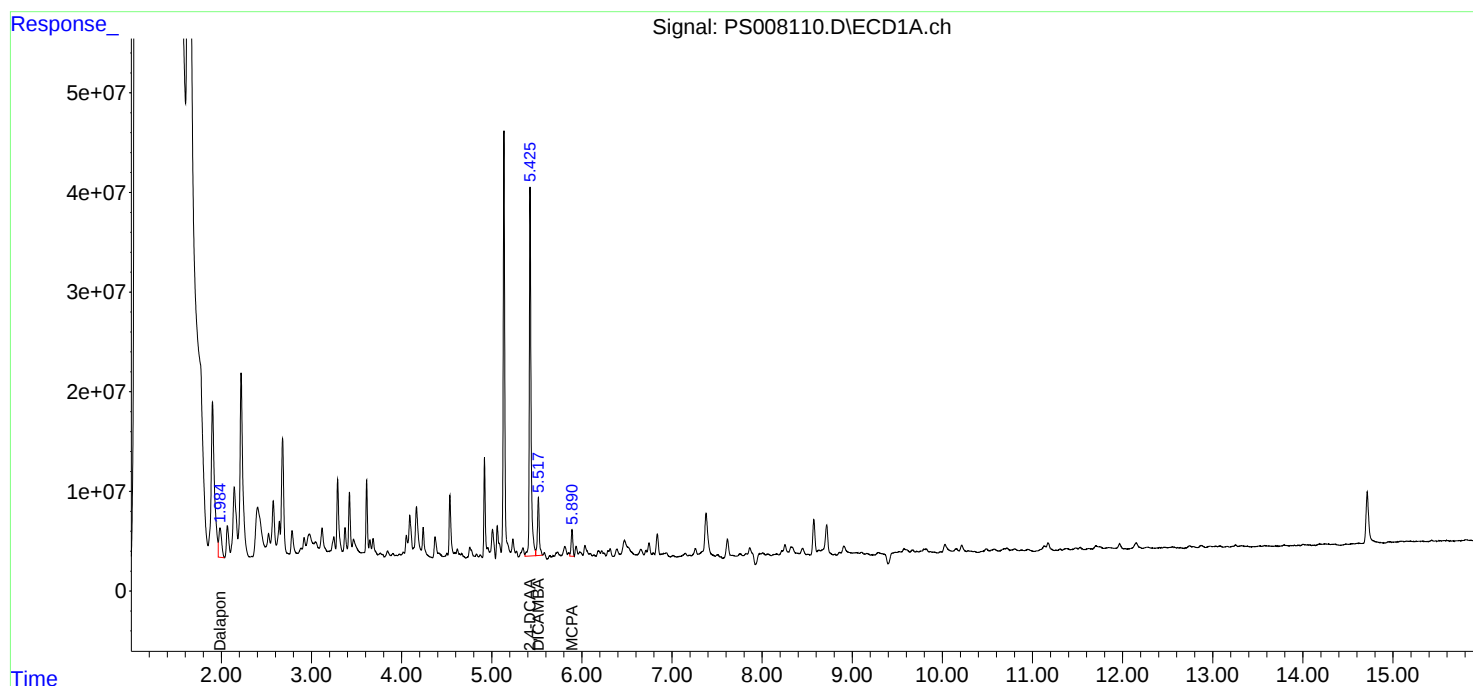


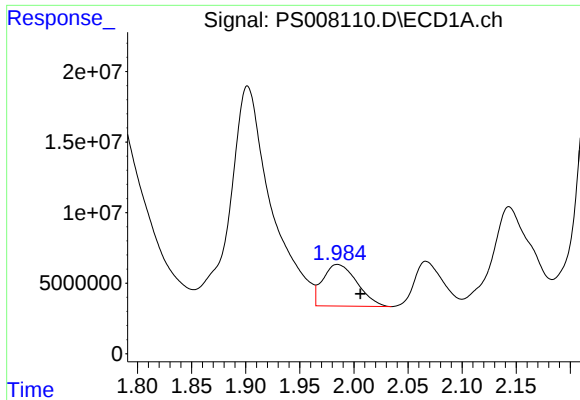

#1 Dalapon


R.T.: 1.985 min
Delta R.T.: -0.021 min
Response: 64763020
Conc: 34.59 ng/ml

Instrument :
ECD_S
ClientSampleId :

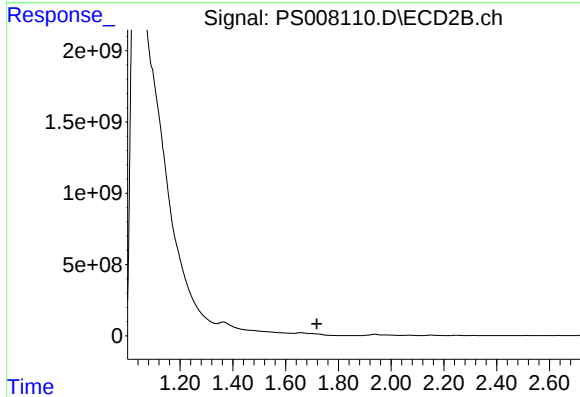


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.717 min
Response: 0
Conc: N.D.

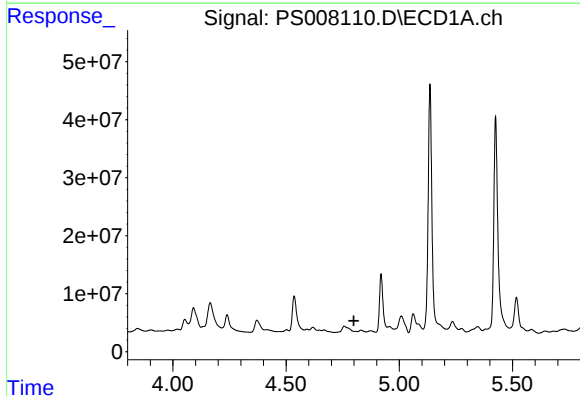


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.800 min
Response: 0
Conc: N.D.

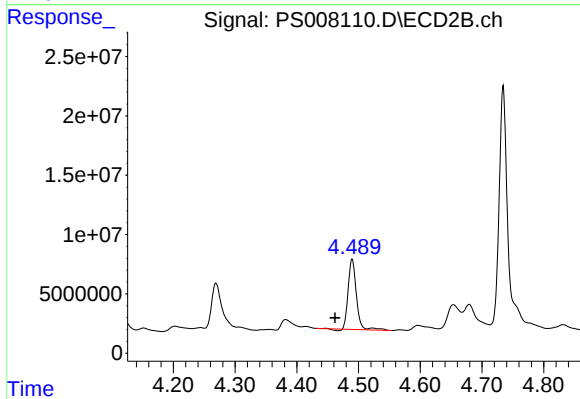

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.490 min
Delta R.T.: 0.028 min
Response: 54733118
Conc: 58.04 ng/ml

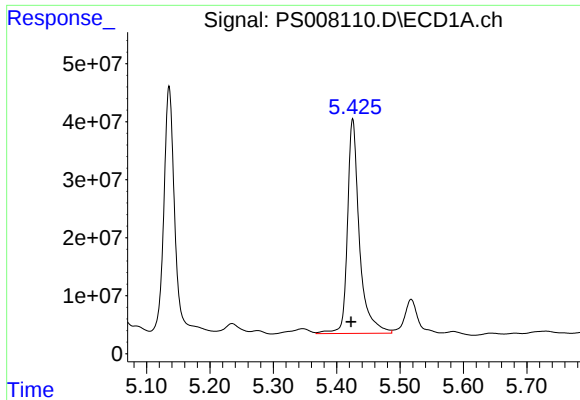

#4 2,4-DCAA


R.T.: 5.425 min
Delta R.T.: 0.003 min
Response: 485123999
Conc: 323.82 ng/ml

Instrument :
ECD_S
ClientSampleId :

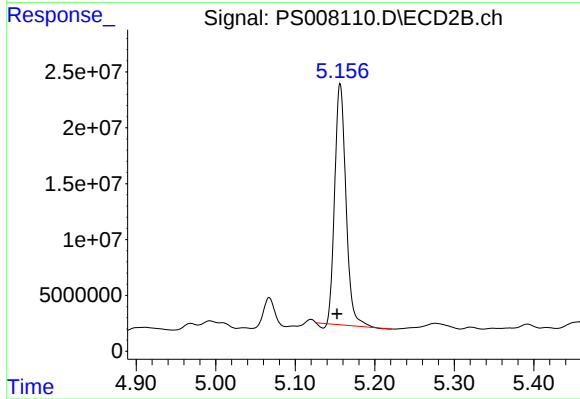


#4 2,4-DCAA

R.T.: 5.157 min
Delta R.T.: 0.004 min
Response: 210316796
Conc: 286.56 ng/ml

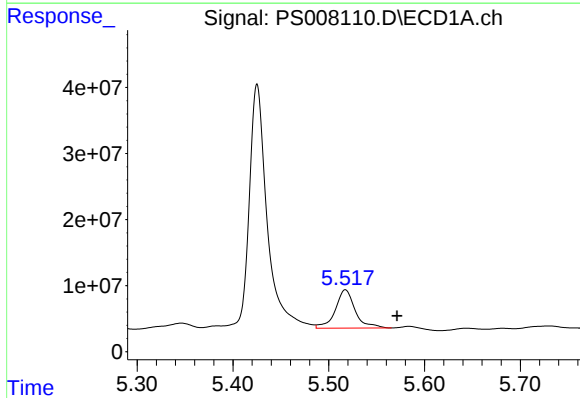


#5 DICAMBA

R.T.: 5.518 min
Delta R.T.: -0.054 min
Response: 83643242
Conc: 15.11 ng/ml

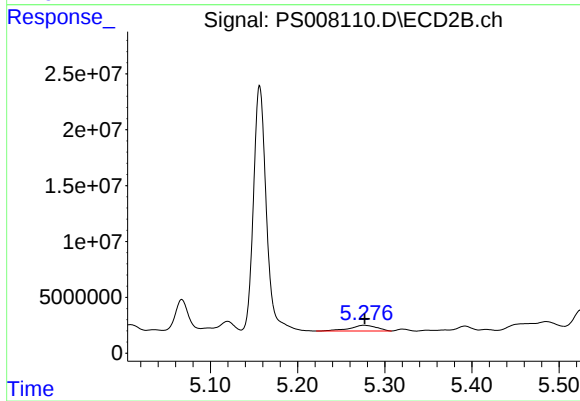

#5 DICAMBA


R.T.: 5.276 min
Delta R.T.: 0.000 min
Response: 11233586
Conc: 4.07 ng/ml

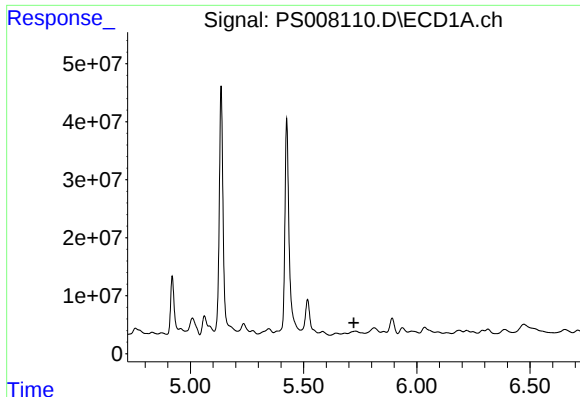

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 5.722 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

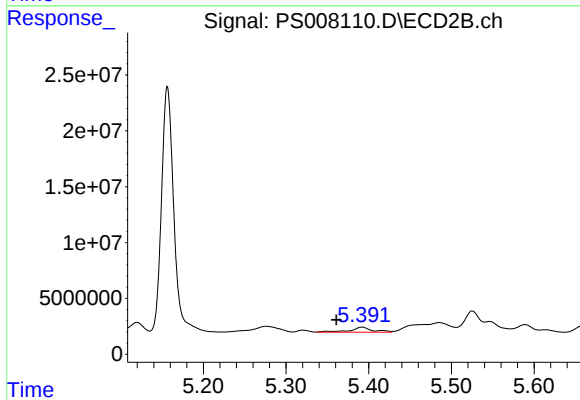


#6 MCPP

R.T.: 5.392 min
Delta R.T.: 0.031 min
Response: 8393540
Conc: 4.30 ug/ml

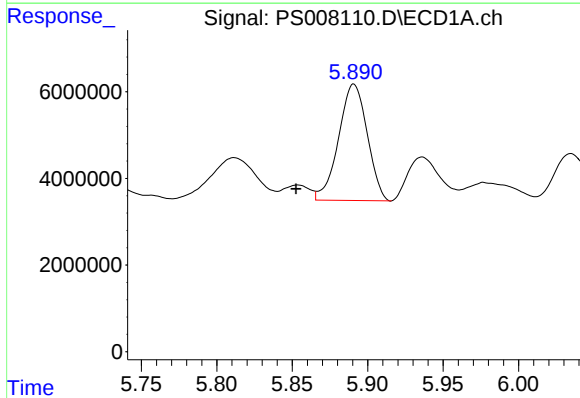


#7 MCPA

R.T.: 5.891 min
Delta R.T.: 0.038 min
Response: 35434395
Conc: 6.21 ug/ml

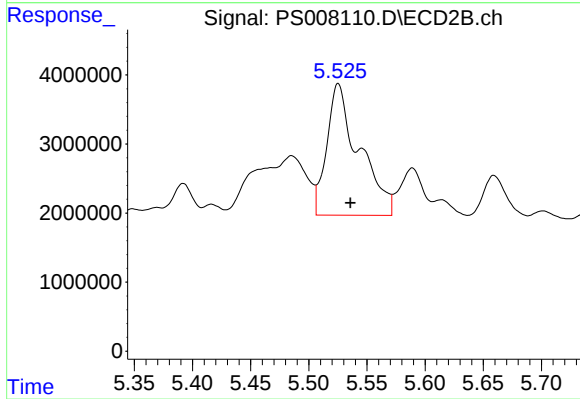

#7 MCPA


R.T.: 5.525 min
Delta R.T.: -0.010 min
Response: 36660498
Conc: 12.28 ug/ml

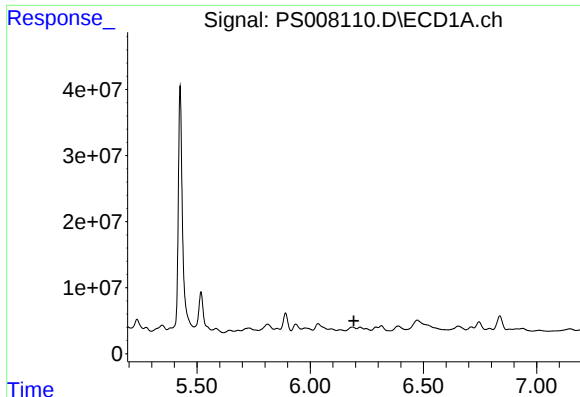

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 6.193 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

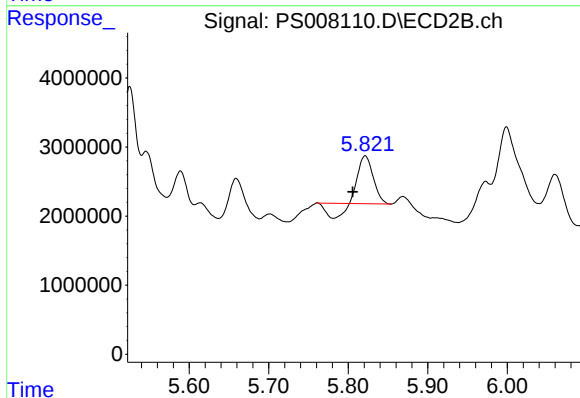


#8 DICHLORPROP

R.T.: 5.821 min
Delta R.T.: 0.016 min
Response: 6387726
Conc: 9.31 ng/ml

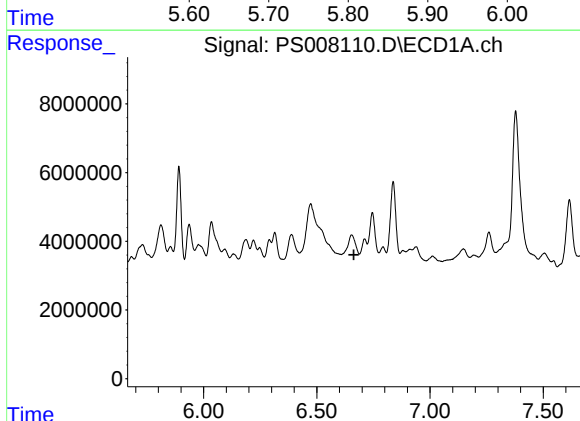


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.663 min
Response: 0
Conc: N.D.

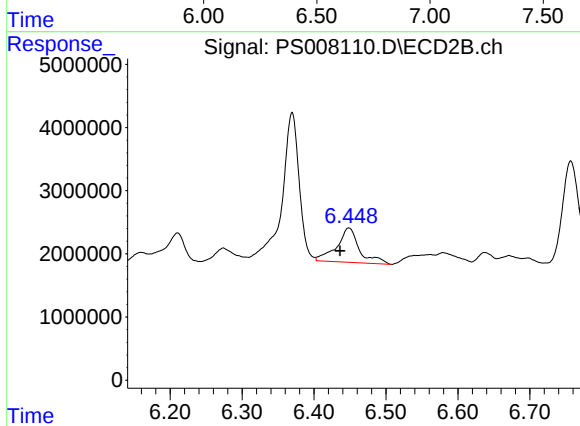

#10 Pentachlorophenol


R.T.: 6.448 min
Delta R.T.: 0.012 min
Response: 11962693
Conc: 1.18 ng/ml

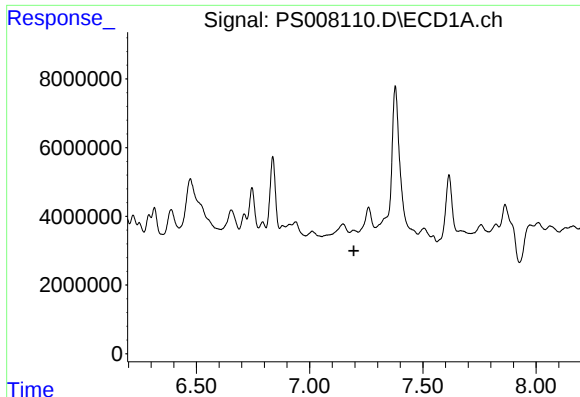

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.195 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

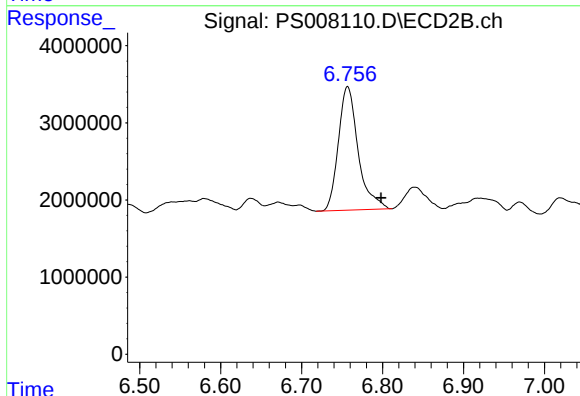


#11 2,4,5-TP (SILVEX)

R.T.: 6.757 min
Delta R.T.: -0.041 min
Response: 27268571
Conc: 6.74 ng/ml

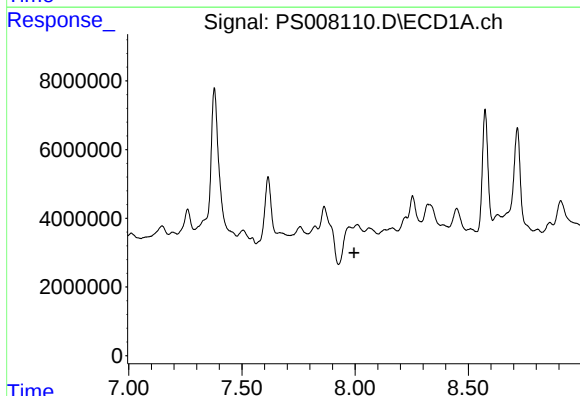


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 7.995 min
Response: 0
Conc: N.D.

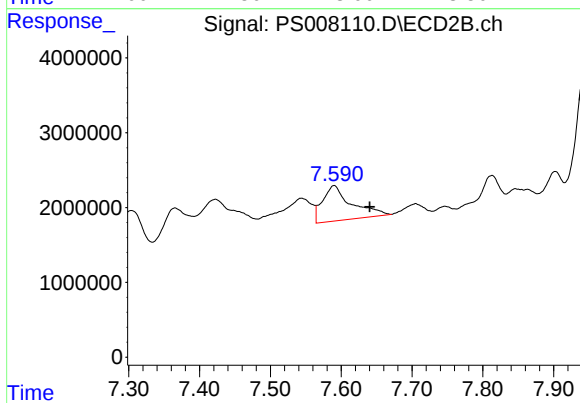

#13 2,4-DB


R.T.: 7.590 min
Delta R.T.: -0.050 min
Response: 13284256
Conc: 27.07 ng/ml

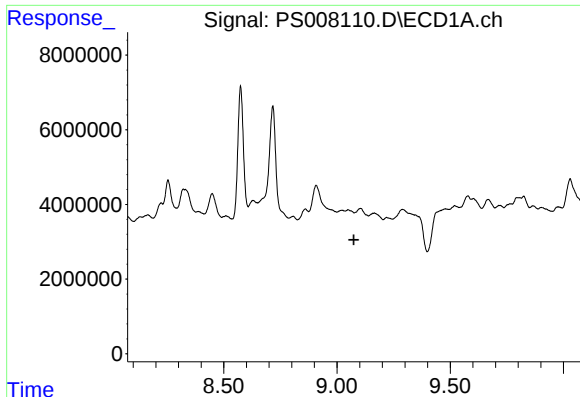

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.075 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

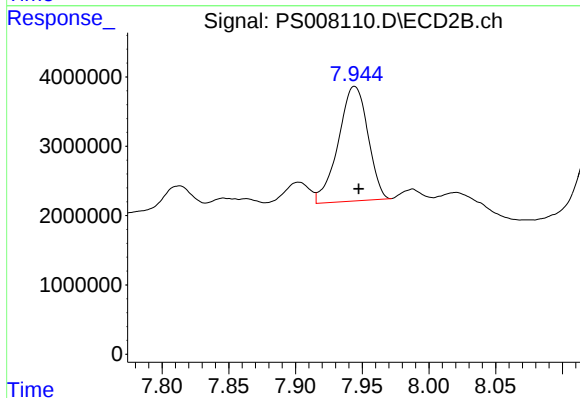


#14 DINOSEB

R.T.: 7.944 min
Delta R.T.: -0.003 min
Response: 25467145
Conc: 10.03 ng/ml

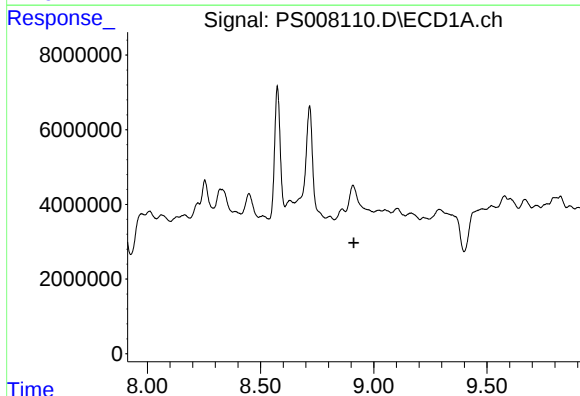

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.912 min
Response: 0
Conc: N.D.

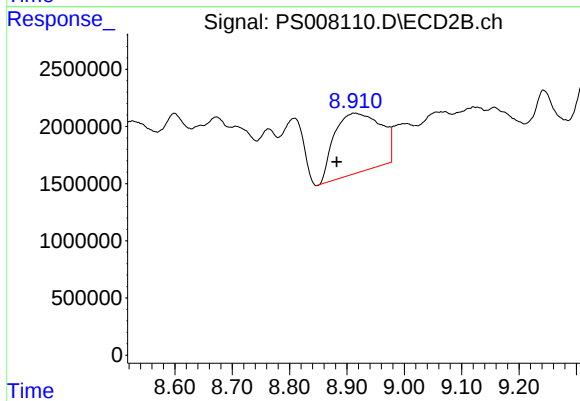

#15 Picloram

R.T.: 8.913 min
Delta R.T.: 0.032 min
Response: 29512182
Conc: 4.90 ng/ml