

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121919\
 Data File : PS008120.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2019 22:31
 Operator : SM\AJ
 Sample : K6318-08
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 05:40:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121819.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 18 11:09:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.421	5.137	574.7E6	161.2E6	383.622	219.646 #
Target Compounds							
1) T	Dalapon	1.981	0.000	74284800	0	39.681	N.D. #
2) T	3,5-DICHL...	0.000	4.471	0	91081510	N.D.	96.590
3) T	4-Nitroph...	0.000	4.813	0	15086727	N.D.	38.619
5) T	DICAMBA	5.513	0.000	81356000	0	14.698	N.D. #
7) T	MCPA	5.886	5.506	37380390	32441392	6.549	10.863 #
8) T	DICHLORPROP	0.000	5.800	0	15062326	N.D.	21.959
10) T	Pentachlo...	0.000	6.430	0	10567984	N.D.	1.039
11) T	2,4,5-TP ...	0.000	6.820	0	6706301	N.D.	1.658
13) T	2,4-DB	8.058	0.000	170.1E6	0	150.561	N.D. #
14) T	DINOSEB	0.000	7.927	0	40930915	N.D.	16.113
15) T	Picloram	0.000	8.918	0	18284442	N.D.	3.038
16) T	DCPA	0.000	8.786	0	16151499	N.D.	3.050



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121919\
Data File : PS008120.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2019 22:31
Operator : SM\AJ
Sample : K6318-08
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 05:40:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121819.M
Quant Title : 8080.M
QLast Update : Wed Dec 18 11:09:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

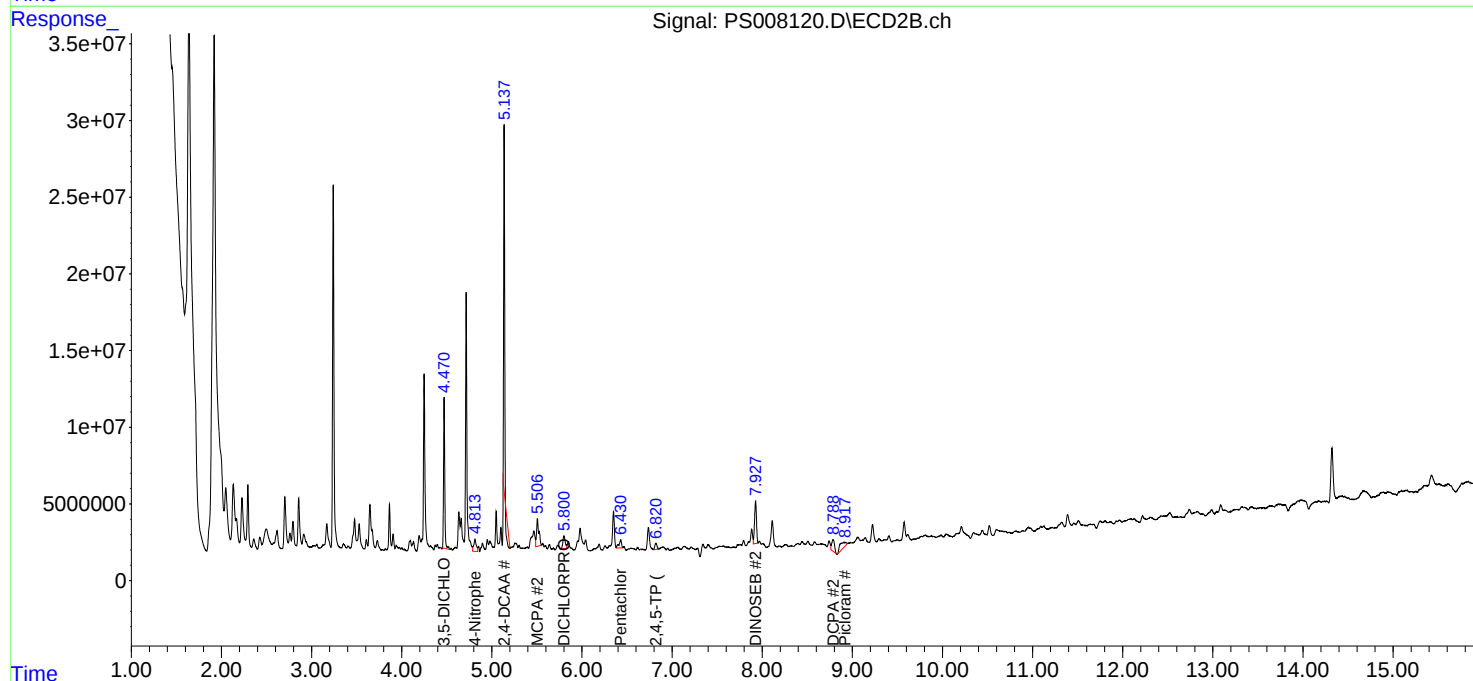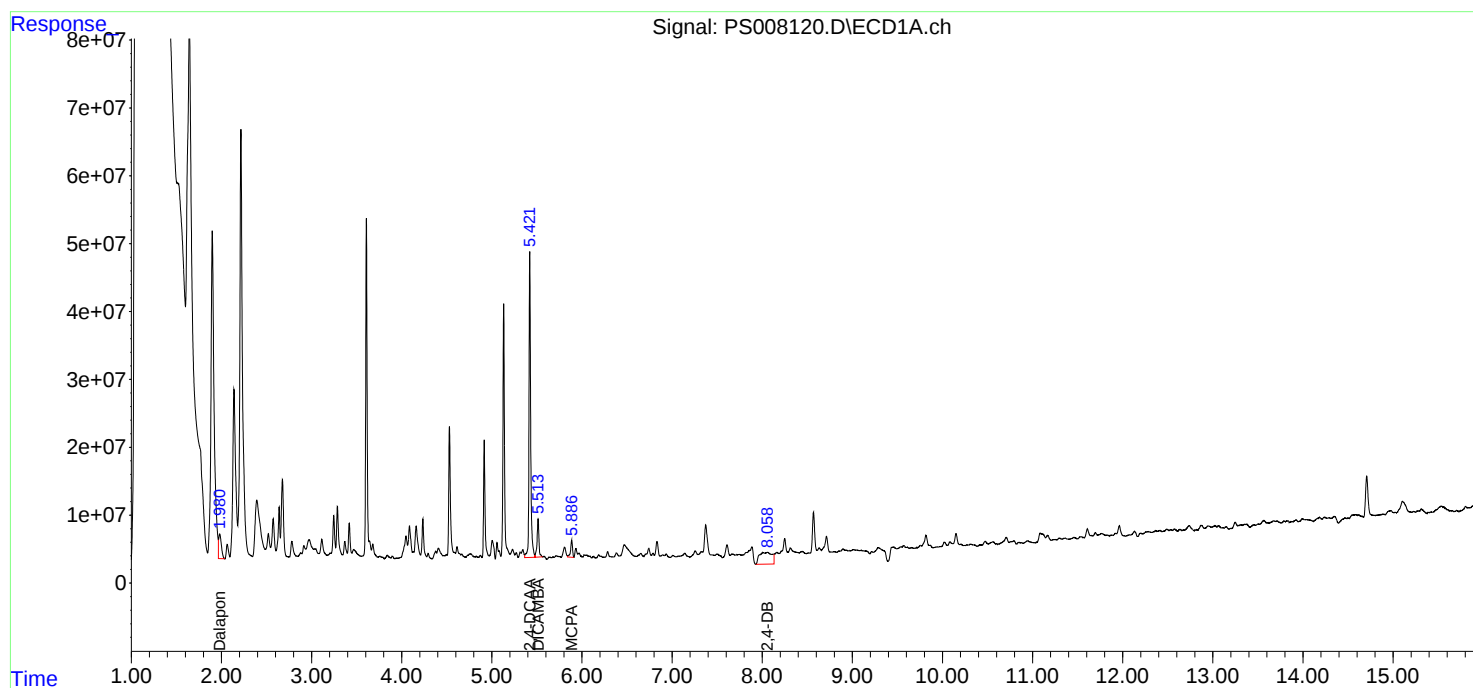


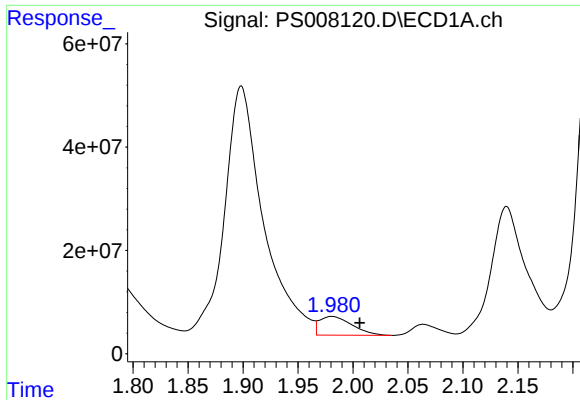

#1 Dalapon


R.T.: 1.981 min
Delta R.T.: -0.025 min
Response: 74284800
Conc: 39.68 ng/ml

Instrument :
ECD_S
ClientSampleId :

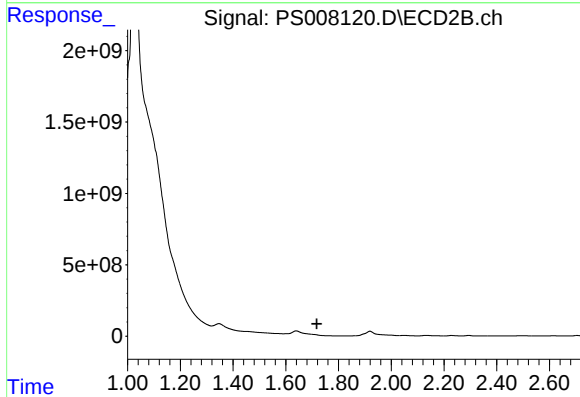


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.717 min
Response: 0
Conc: N.D.

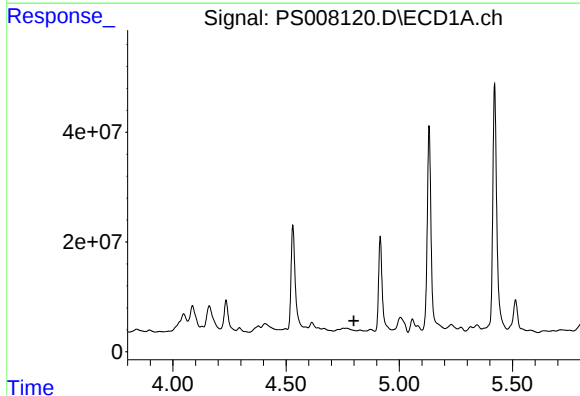


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.800 min
Response: 0
Conc: N.D.

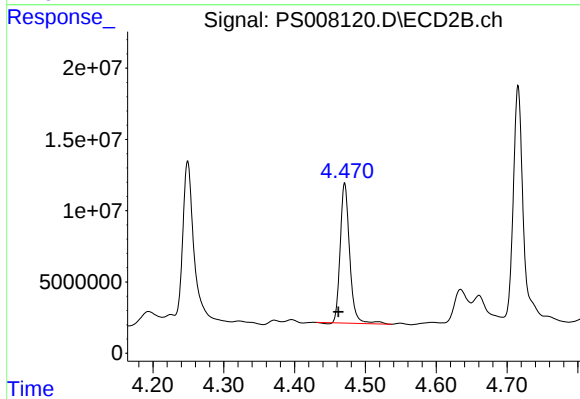

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.471 min
Delta R.T.: 0.009 min
Response: 91081510
Conc: 96.59 ng/ml

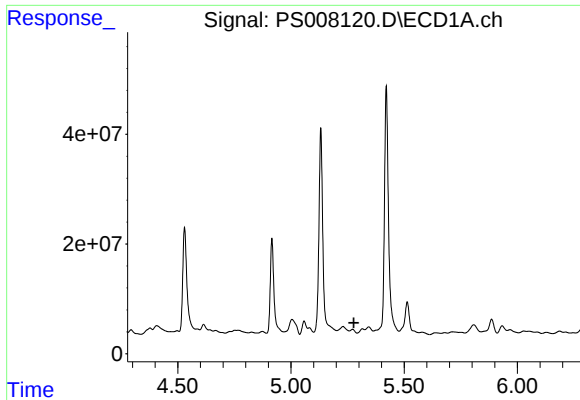

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 5.278 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

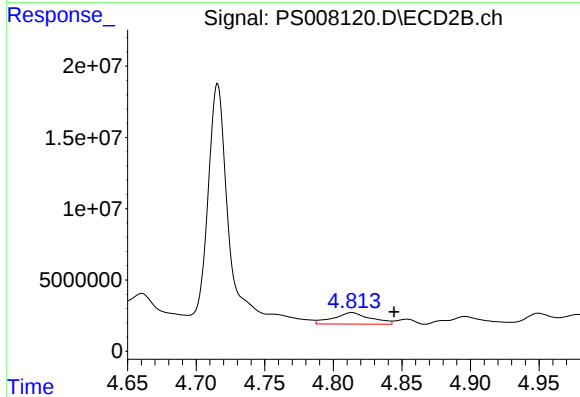


#3 4-Nitrophenol

R.T.: 4.813 min
Delta R.T.: -0.031 min
Response: 15086727
Conc: 38.62 ng/ml

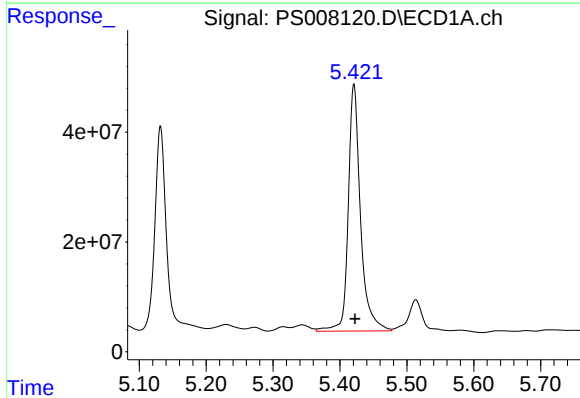


#4 2,4-DCAA

R.T.: 5.421 min
Delta R.T.: -0.002 min
Response: 574706408
Conc: 383.62 ng/ml

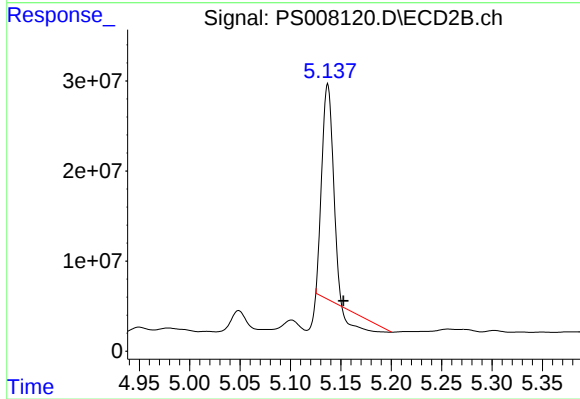

#4 2,4-DCAA


R.T.: 5.137 min
Delta R.T.: -0.015 min
Response: 161205650
Conc: 219.65 ng/ml

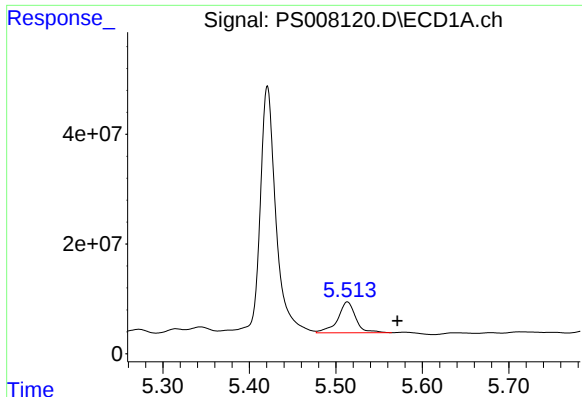

#5 DICAMBA


R.T.: 5.513 min
Delta R.T.: -0.058 min
Response: 81356000
Conc: 14.70 ng/ml

Instrument :
ECD_S
ClientSampleId :

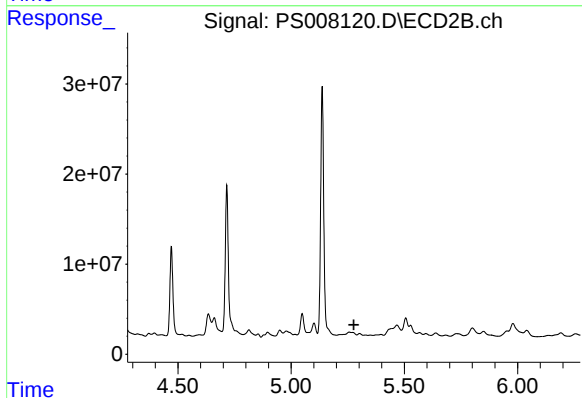


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 5.277 min
Response: 0
Conc: N.D.

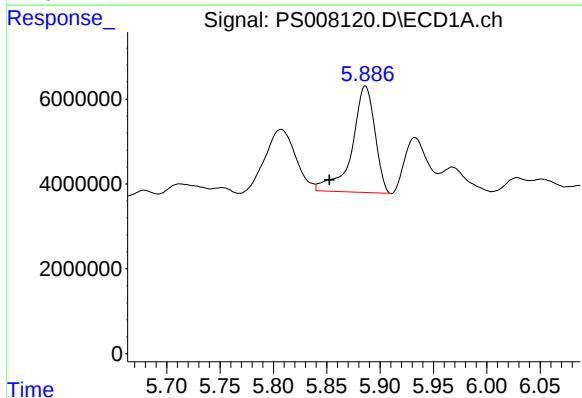


#7 MCPA

R.T.: 5.886 min
Delta R.T.: 0.034 min
Response: 37380390
Conc: 6.55 ug/ml

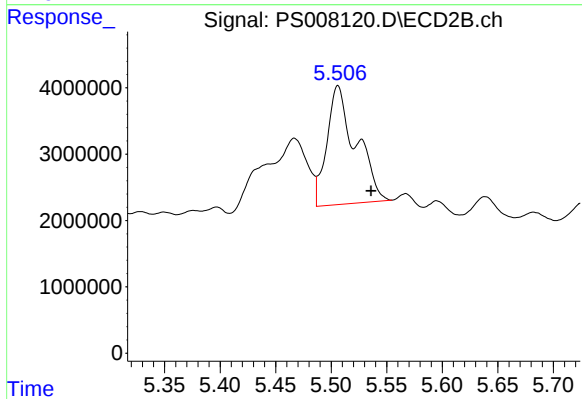

#7 MCPA


R.T.: 5.506 min
Delta R.T.: -0.030 min
Response: 32441392
Conc: 10.86 ug/ml

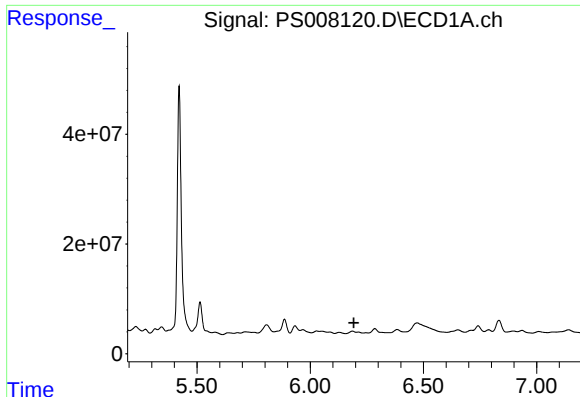

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.193 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

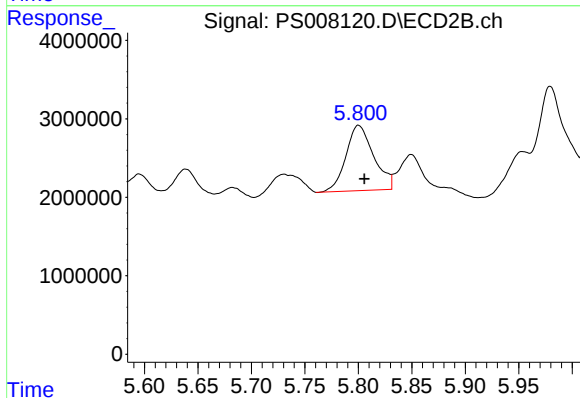


#8 DICHLORPROP

R.T.: 5.800 min
Delta R.T.: -0.005 min
Response: 15062326
Conc: 21.96 ng/ml

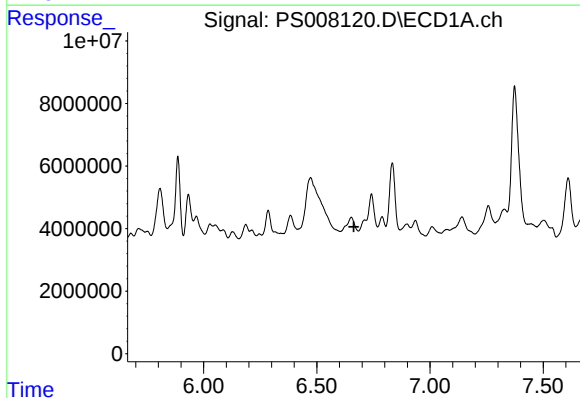


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.663 min
Response: 0
Conc: N.D.

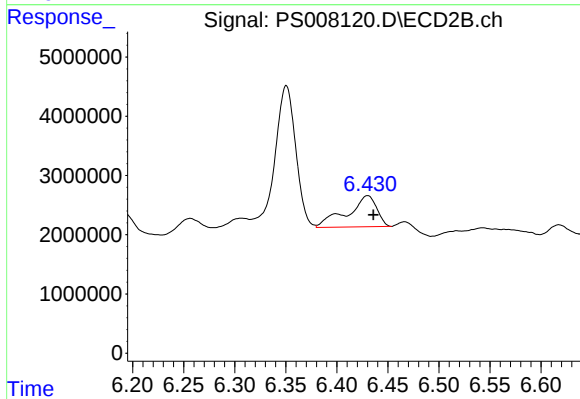

#10 Pentachlorophenol


R.T.: 6.430 min
Delta R.T.: -0.006 min
Response: 10567984
Conc: 1.04 ng/ml

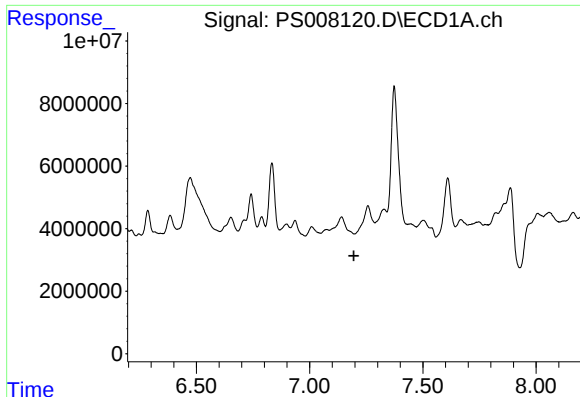

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.195 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

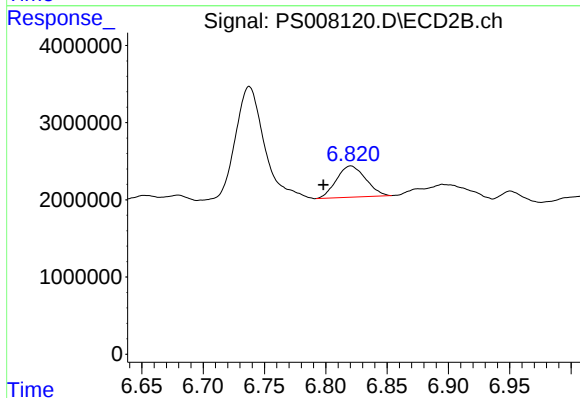


#11 2,4,5-TP (SILVEX)

R.T.: 6.820 min
Delta R.T.: 0.022 min
Response: 6706301
Conc: 1.66 ng/ml

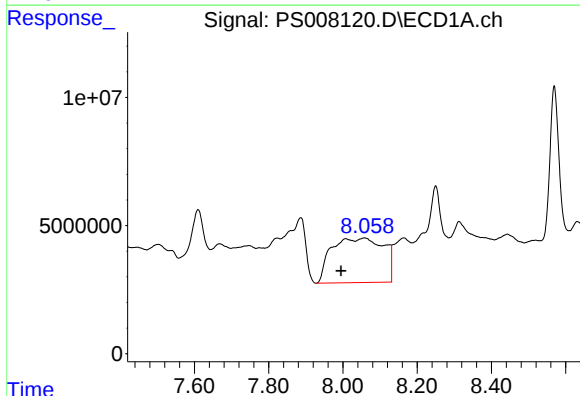


#13 2,4-DB

R.T.: 8.058 min
Delta R.T.: 0.063 min
Response: 170118509
Conc: 150.56 ng/ml

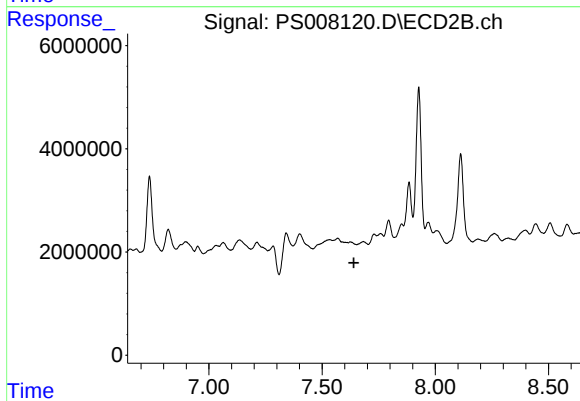

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 7.640 min
Response: 0
Conc: N.D.

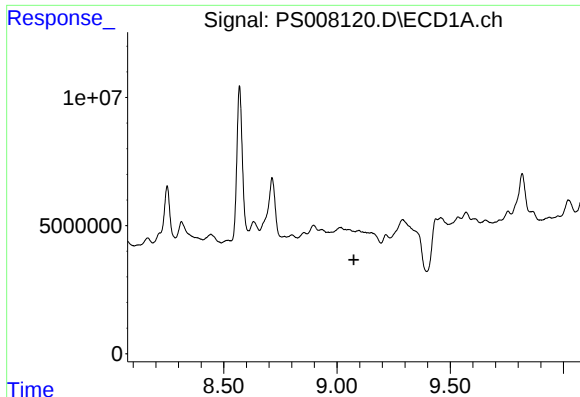

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.075 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

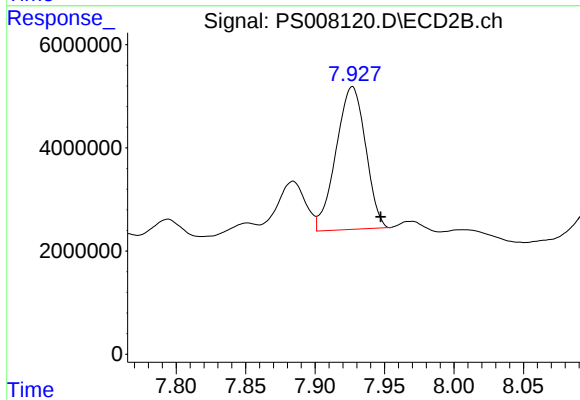


#14 DINOSEB

R.T.: 7.927 min
Delta R.T.: -0.021 min
Response: 40930915
Conc: 16.11 ng/ml

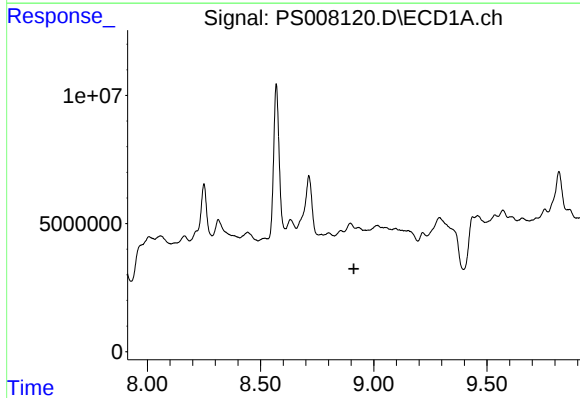


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.912 min
Response: 0
Conc: N.D.

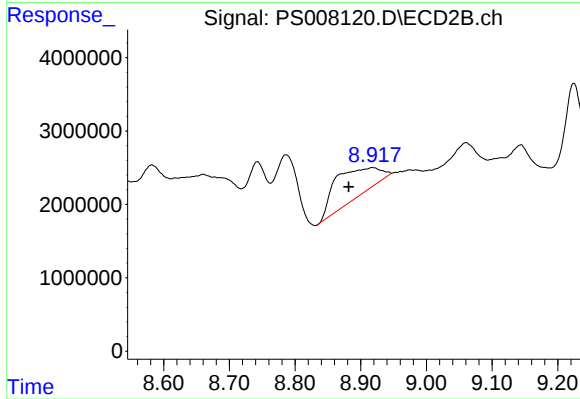

#15 Picloram


R.T.: 8.918 min
Delta R.T.: 0.036 min
Response: 18284442
Conc: 3.04 ng/ml

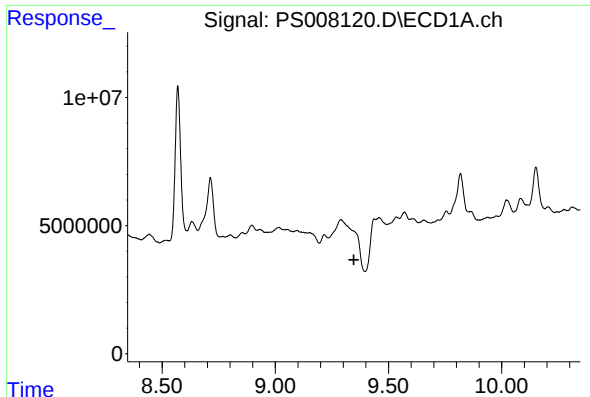

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.347 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

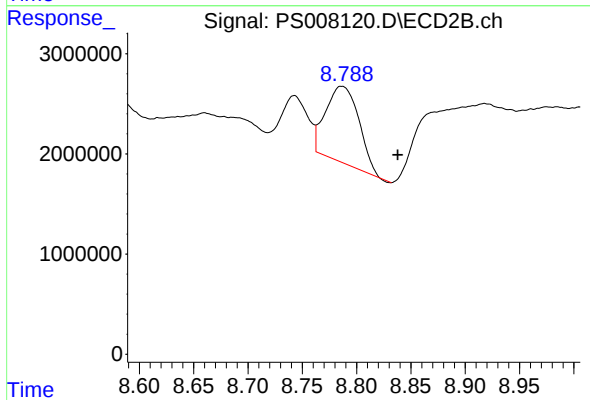

#16 DCPA

R.T.: 8.786 min
Delta R.T.: -0.052 min
Response: 16151499
Conc: 3.05 ng/ml