

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122319\
 Data File : PS008140.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2019 15:11
 Operator : SM\AJ
 Sample : PB125666BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 24 01:21:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121819.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 18 11:09:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.429	5.152	661.3E6	356.2E6	441.420	485.348
Target Compounds							
1) T	Dalapon	1.978	1.686	88086117	29376148	47.053	33.164 #
2) T	3,5-DICHL...	0.000	4.485	0	33863981	N.D.	35.912
5) T	DICAMBA	5.520	5.277	54645151	19107937	9.873	6.915 #
7) T	MCPA	5.836	5.521	28166560	16854485	4.935	5.644
8) T	DICHLORPROP	0.000	5.742	0	10692150	N.D.	15.588
9) T	2,4-D	0.000	6.057	0	6469900	N.D.	7.952
10) T	Pentachlo...	0.000	6.440	0	12018218	N.D.	1.182
11) T	2,4,5-TP ...	0.000	6.755	0	12701504	N.D.	3.140
12) T	2,4,5-T	0.000	7.214	0	49298374	N.D.	13.102
14) T	DINOSEB	0.000	7.944	0	5546470	N.D.	2.183
15) T	Picloram	8.959	8.901	209.3E6	130.2E6	17.666	21.630
16) T	DCPA	0.000	8.901	0	130.2E6	N.D.	24.587



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122319\
Data File : PS008140.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2019 15:11
Operator : SM\AJ
Sample : PB125666BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 01:21:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121819.M
Quant Title : 8080.M
QLast Update : Wed Dec 18 11:09:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

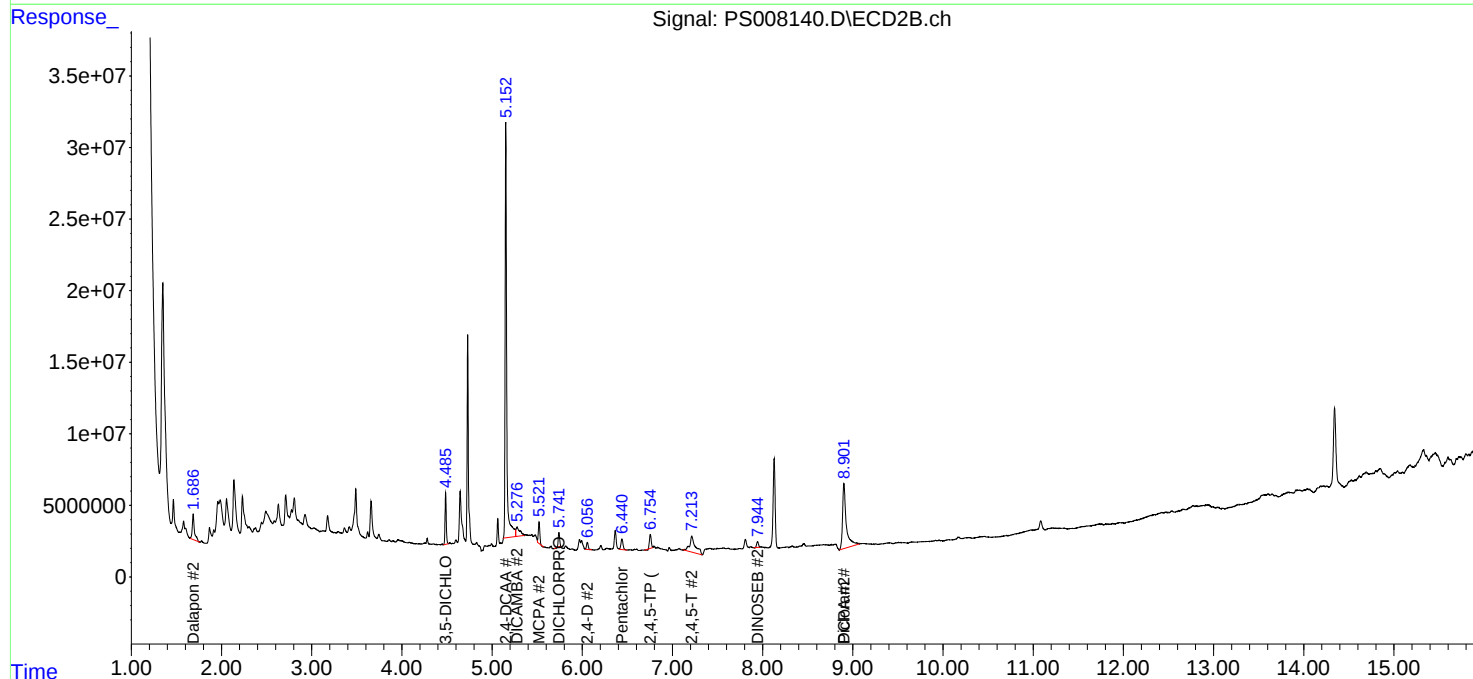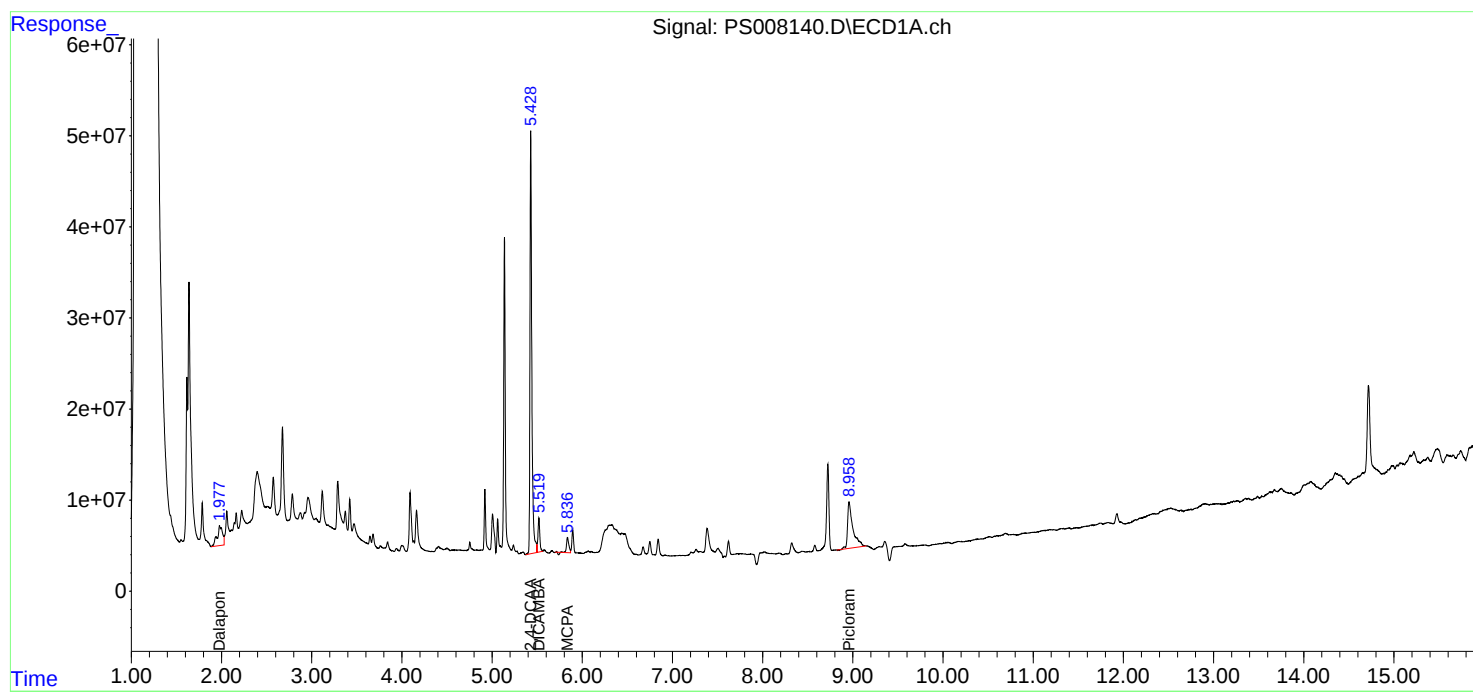


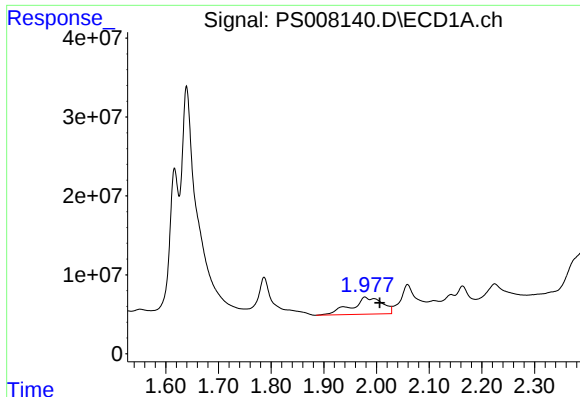

#1 Dalapon


R.T.: 1.978 min
Delta R.T.: -0.028 min
Response: 88086117
Conc: 47.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

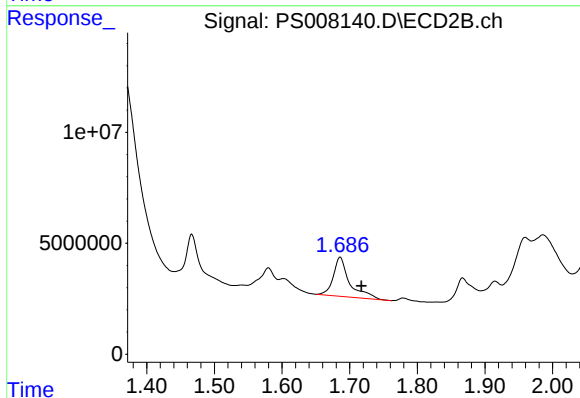


#1 Dalapon

R.T.: 1.686 min
Delta R.T.: -0.032 min
Response: 29376148
Conc: 33.16 ng/ml

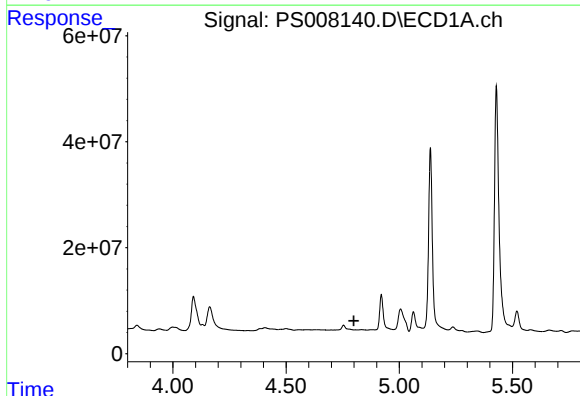


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.800 min
Response: 0
Conc: N.D.

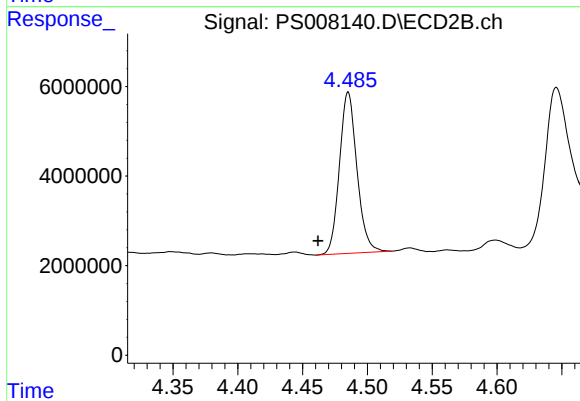

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.485 min
Delta R.T.: 0.023 min
Response: 33863981
Conc: 35.91 ng/ml

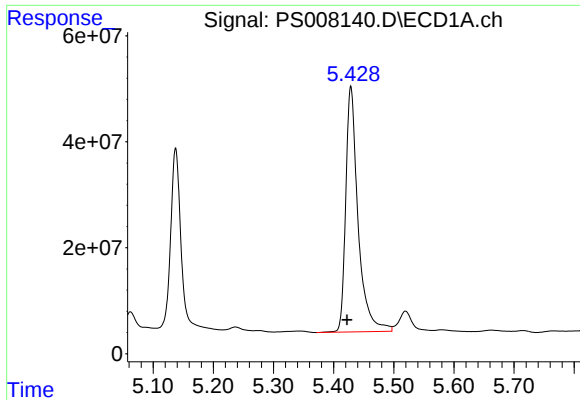

#4 2,4-DCAA


R.T.: 5.429 min
Delta R.T.: 0.006 min
Response: 661294764
Conc: 441.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

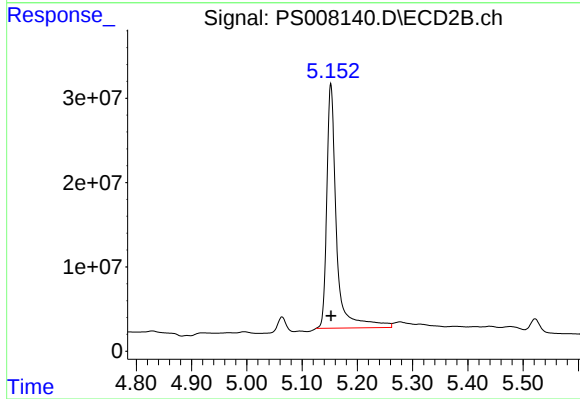


#4 2,4-DCAA

R.T.: 5.152 min
Delta R.T.: 0.000 min
Response: 356213346
Conc: 485.35 ng/ml

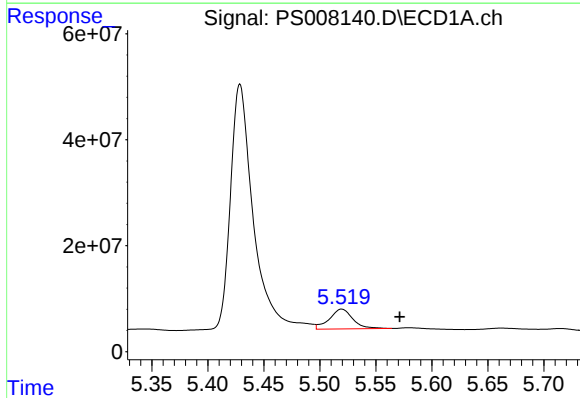


#5 DICAMBA

R.T.: 5.520 min
Delta R.T.: -0.052 min
Response: 54645151
Conc: 9.87 ng/ml

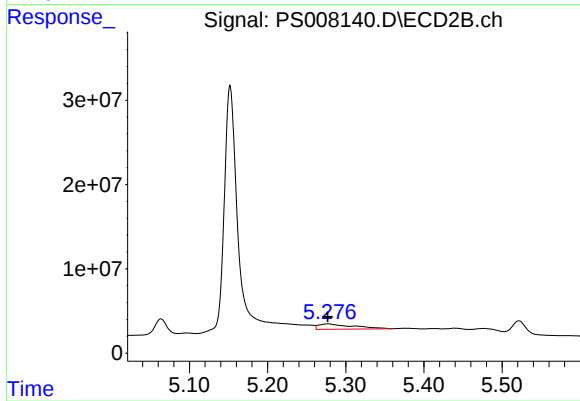

#5 DICAMBA


R.T.: 5.277 min
Delta R.T.: 0.000 min
Response: 19107937
Conc: 6.91 ng/ml

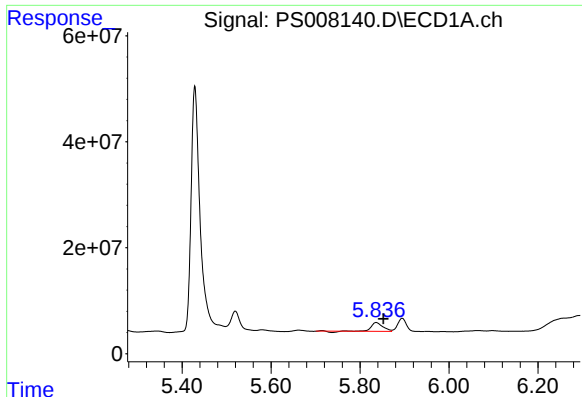

#7 MCPA


R.T.: 5.836 min
Delta R.T.: -0.016 min
Response: 28166560
Conc: 4.93 ug/ml

Instrument :
ECD_S
ClientSampleId :

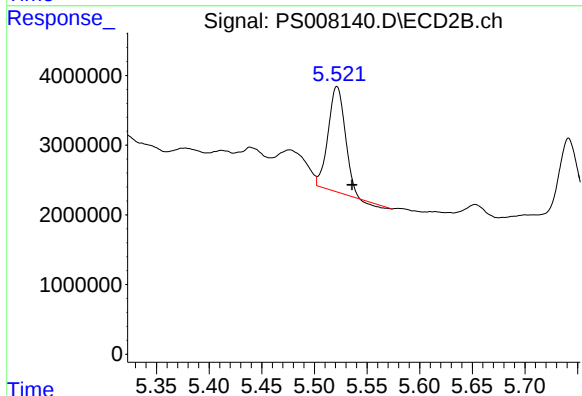


#7 MCPA

R.T.: 5.521 min
Delta R.T.: -0.014 min
Response: 16854485
Conc: 5.64 ug/ml

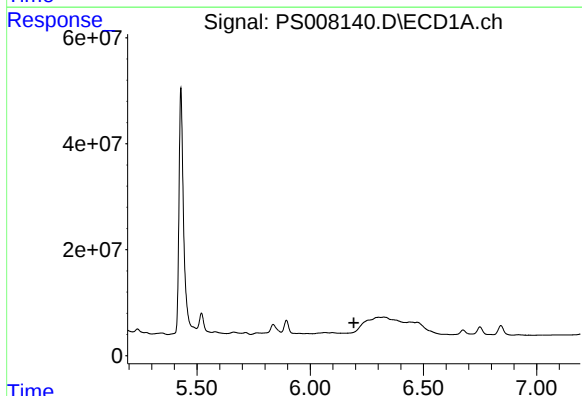


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.193 min
Response: 0
Conc: N.D.

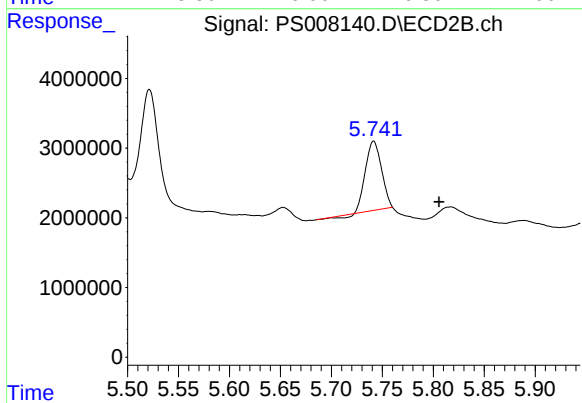

#8 DICHLORPROP


R.T.: 5.742 min
Delta R.T.: -0.064 min
Response: 10692150
Conc: 15.59 ng/ml

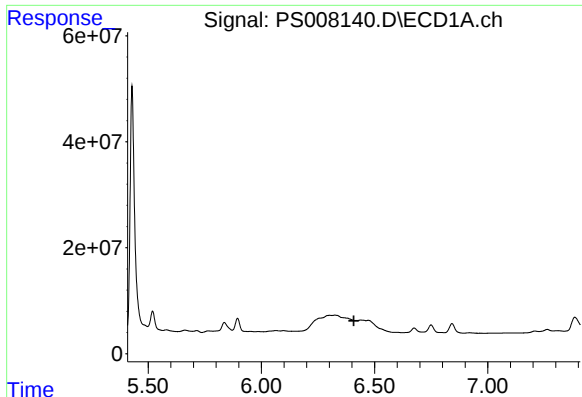

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.409 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

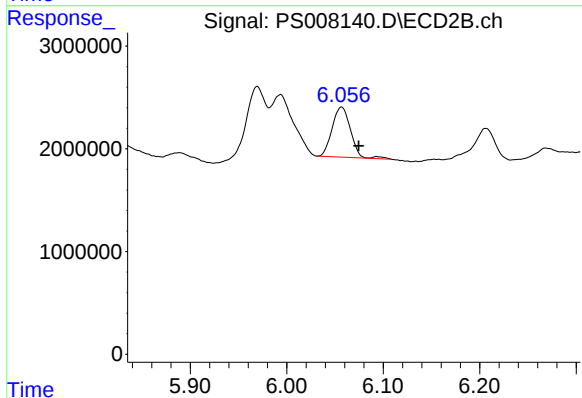


#9 2,4-D

R.T.: 6.057 min
Delta R.T.: -0.018 min
Response: 6469900
Conc: 7.95 ng/ml

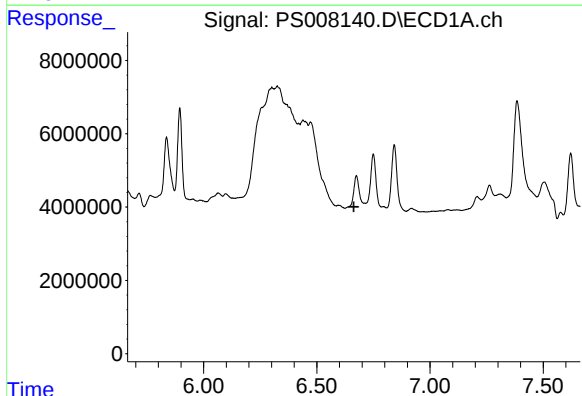


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.663 min
Response: 0
Conc: N.D.

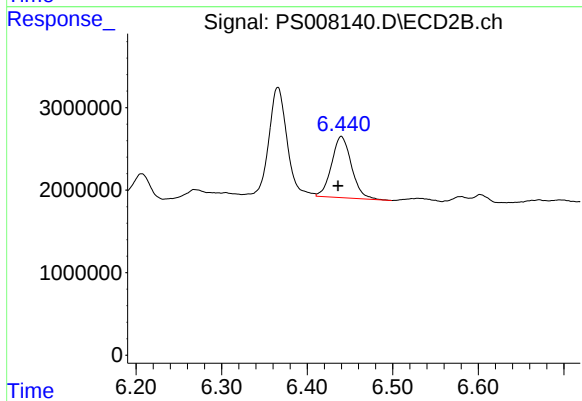

#10 Pentachlorophenol


R.T.: 6.440 min
Delta R.T.: 0.004 min
Response: 12018218
Conc: 1.18 ng/ml

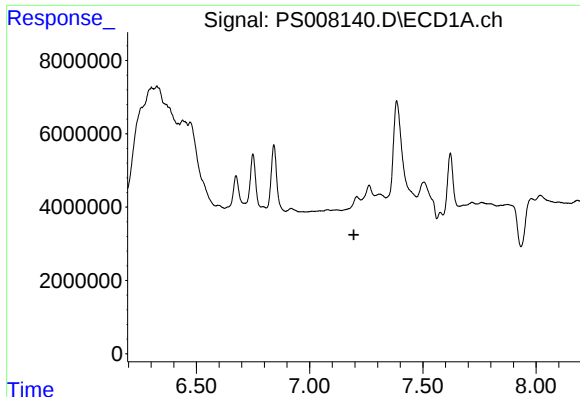

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.195 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

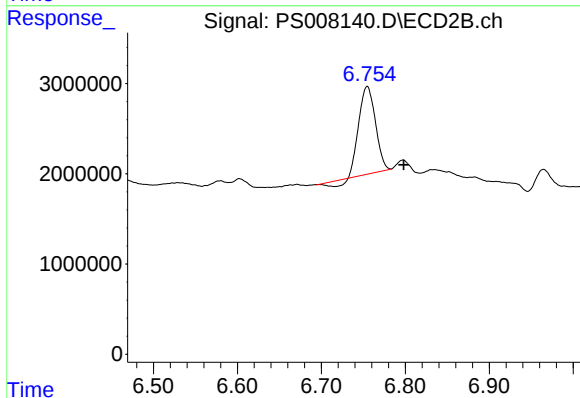


#11 2,4,5-TP (SILVEX)

R.T.: 6.755 min
Delta R.T.: -0.043 min
Response: 12701504
Conc: 3.14 ng/ml

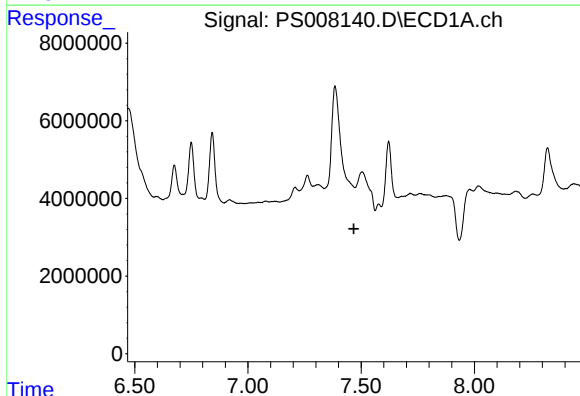


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 7.468 min
Response: 0
Conc: N.D.

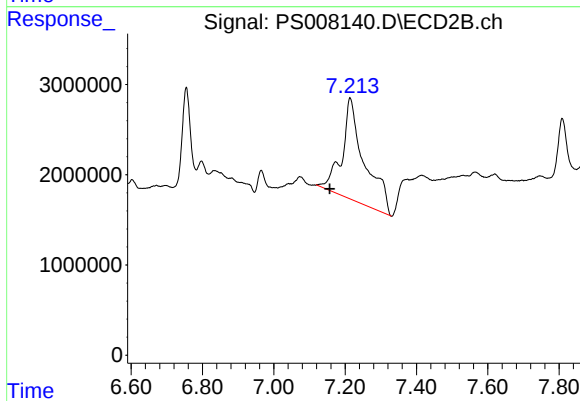

#12 2,4,5-T


R.T.: 7.214 min
Delta R.T.: 0.057 min
Response: 49298374
Conc: 13.10 ng/ml

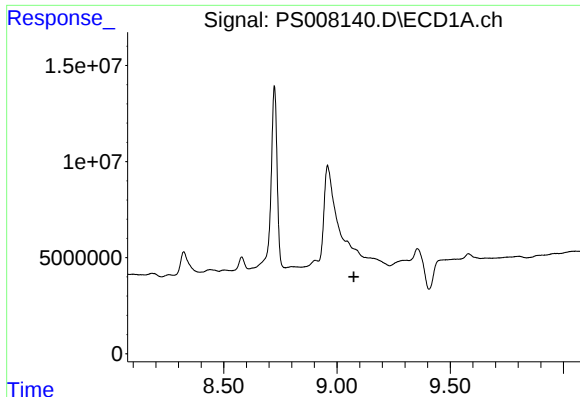

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.075 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

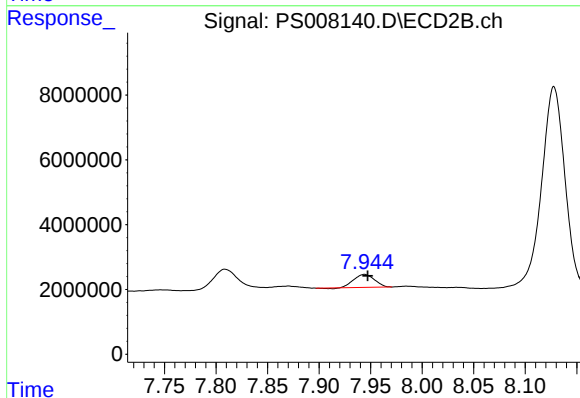


#14 DINOSEB

R.T.: 7.944 min
Delta R.T.: -0.003 min
Response: 5546470
Conc: 2.18 ng/ml

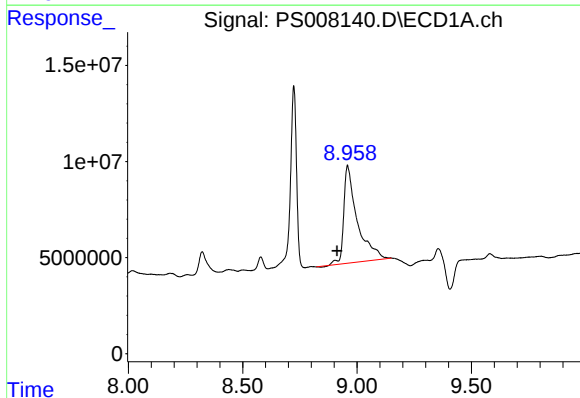


#15 Picloram

R.T.: 8.959 min
Delta R.T.: 0.047 min
Response: 209250232
Conc: 17.67 ng/ml

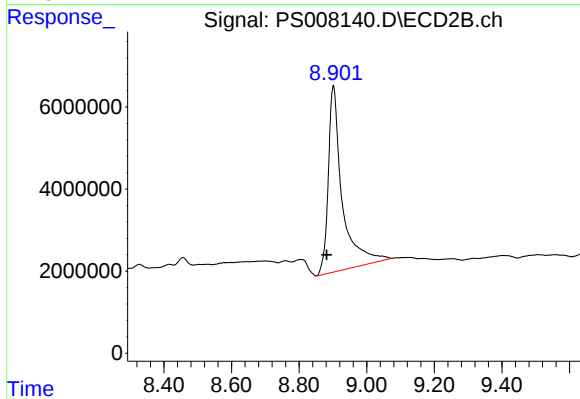

#15 Picloram


R.T.: 8.901 min
Delta R.T.: 0.020 min
Response: 130182170
Conc: 21.63 ng/ml

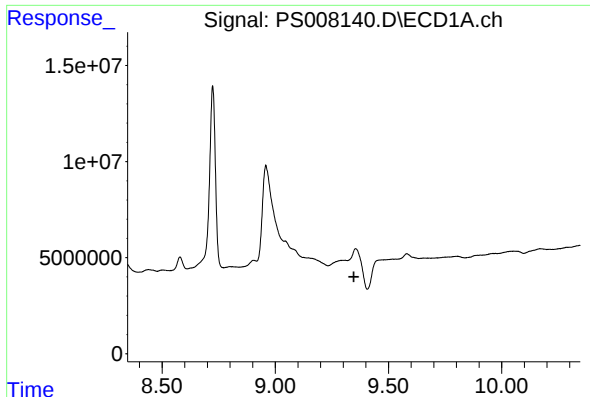

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.347 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

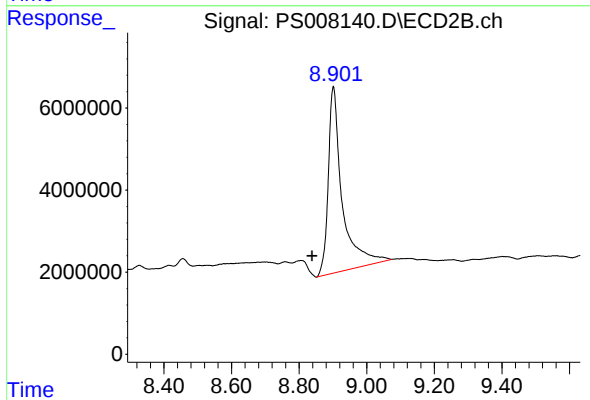

#16 DCPA

R.T.: 8.901 min
Delta R.T.: 0.063 min
Response: 130182170
Conc: 24.59 ng/ml