

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122319\
 Data File : PS008142.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2019 15:55
 Operator : SM\AJ
 Sample : PB125666TB
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 24 01:22:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121819.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 18 11:09:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.428	5.156	648.6E6	326.3E6	432.972	444.535
Target Compounds							
1) T	Dalapon	1.978	1.690	61653500	29982734	32.933	33.849
2) T	3,5-DICHL...	0.000	4.490	0	34261730	N.D.	36.334
5) T	DICAMBA	5.516	0.000	66140984	0	11.950	N.D. #
7) T	MCPA	5.890	5.524	35959851	27801659	6.300	9.310 #
8) T	DICHLORPROP	0.000	5.747	0	4183524	N.D.	6.099
9) T	2,4-D	6.476	6.059	91930580	7885445	61.015	9.692 #
10) T	Pentachlo...	0.000	6.444	0	16064439	N.D.	1.579
11) T	2,4,5-TP ...	0.000	6.761	0	11537301	N.D.	2.852
14) T	DINOSEB	0.000	7.948	0	6342620	N.D.	2.497
15) T	Picloram	0.000	8.927	0	20673274	N.D.	3.435



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122319\
Data File : PS008142.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2019 15:55
Operator : SM\AJ
Sample : PB125666TB
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 01:22:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121819.M
Quant Title : 8080.M
QLast Update : Wed Dec 18 11:09:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

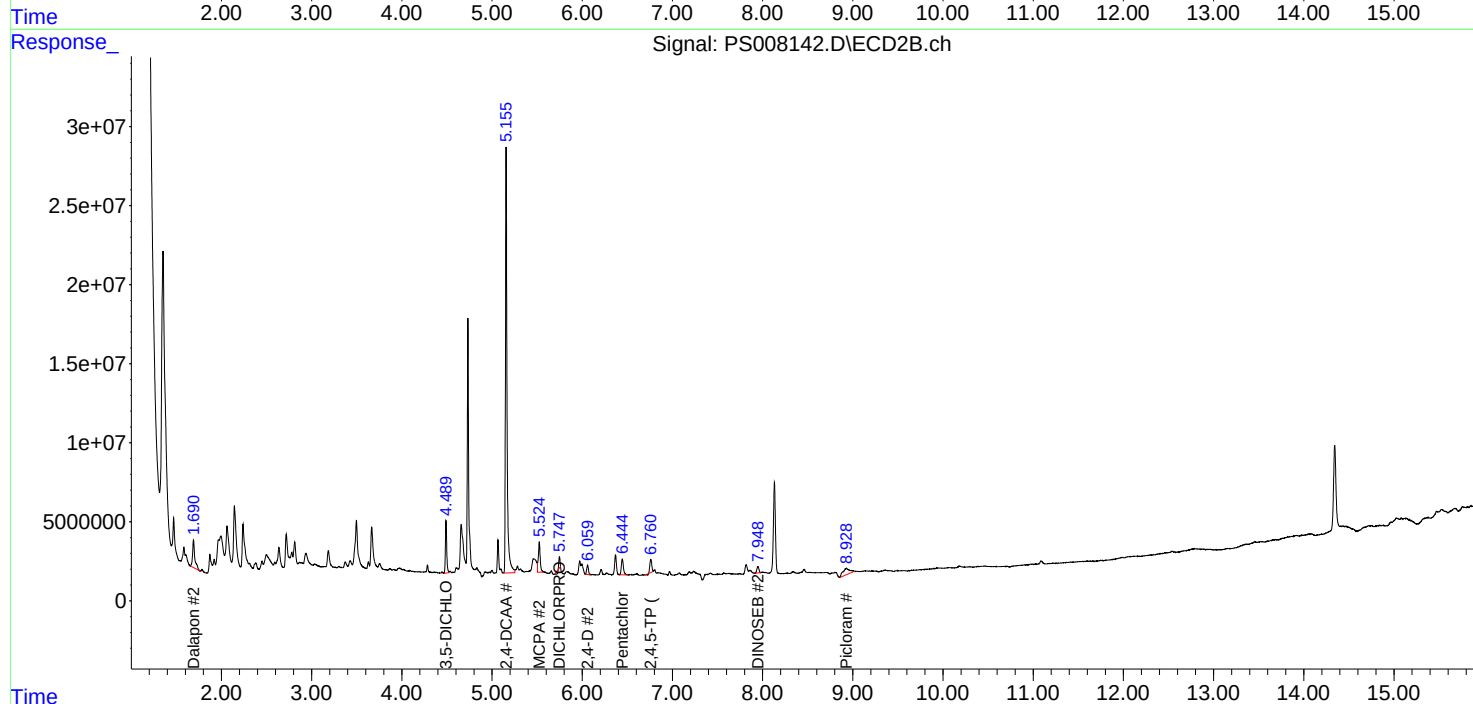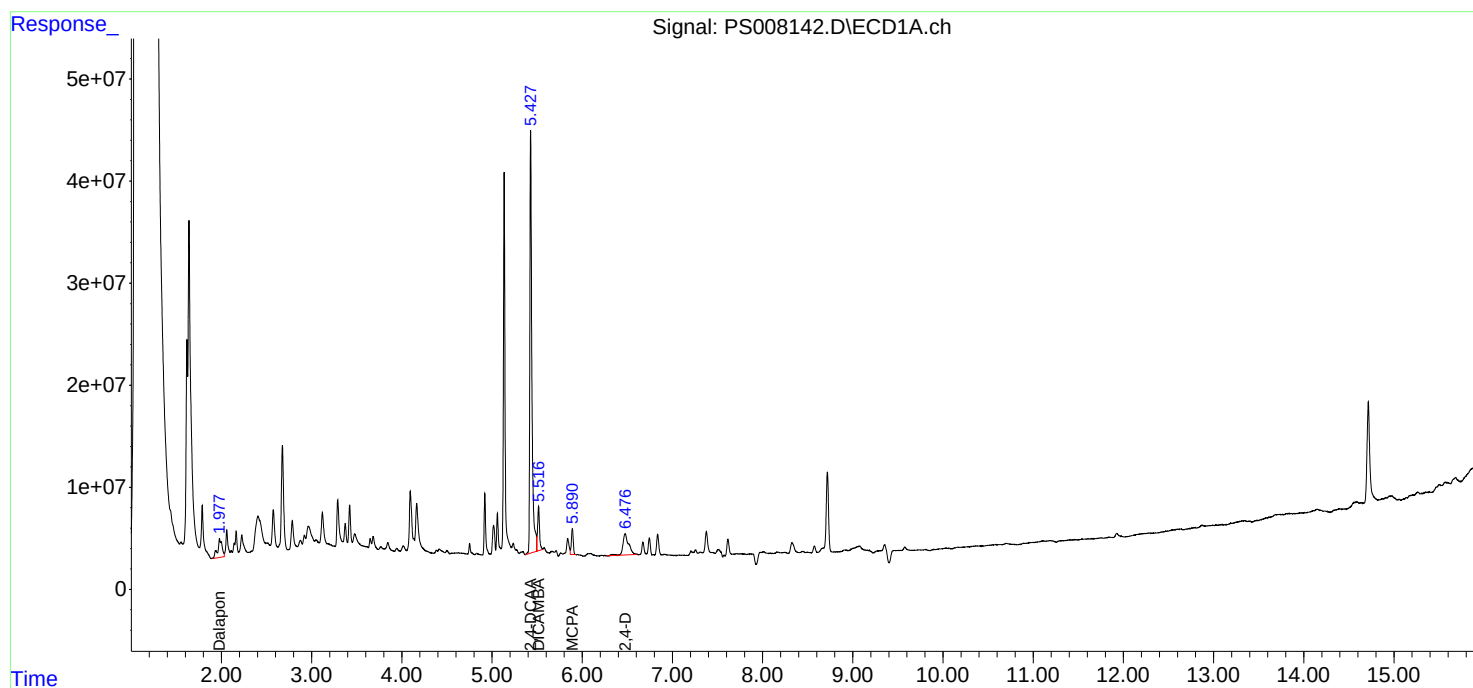


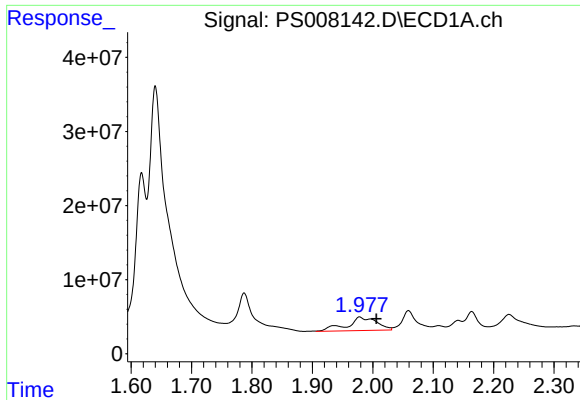

#1 Dalapon


R.T.: 1.978 min
Delta R.T.: -0.028 min
Response: 61653500
Conc: 32.93 ng/ml

Instrument :
ECD_S
ClientSampleId :

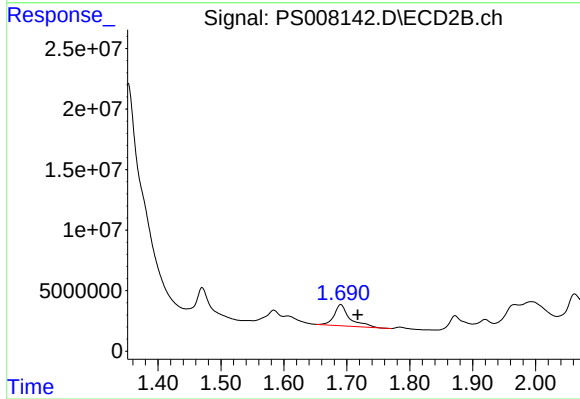


#1 Dalapon

R.T.: 1.690 min
Delta R.T.: -0.027 min
Response: 29982734
Conc: 33.85 ng/ml

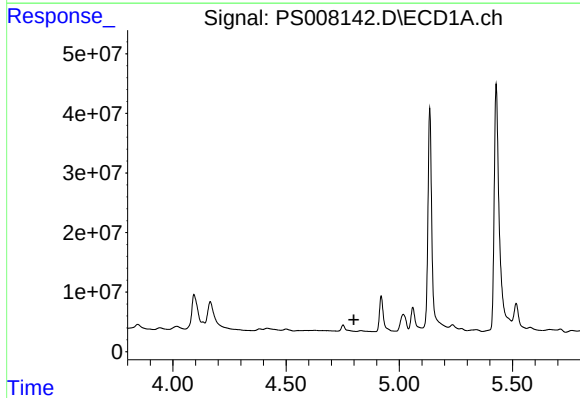


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.800 min
Response: 0
Conc: N.D.

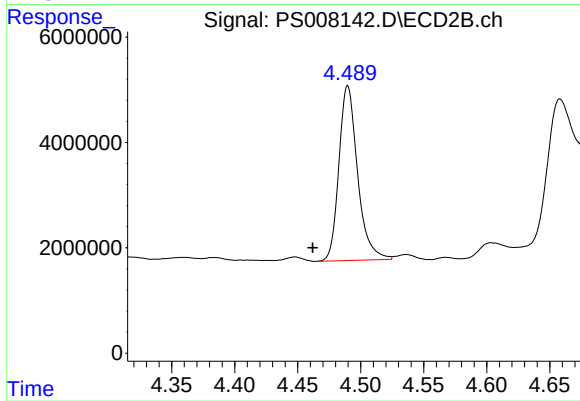

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.490 min
Delta R.T.: 0.028 min
Response: 34261730
Conc: 36.33 ng/ml

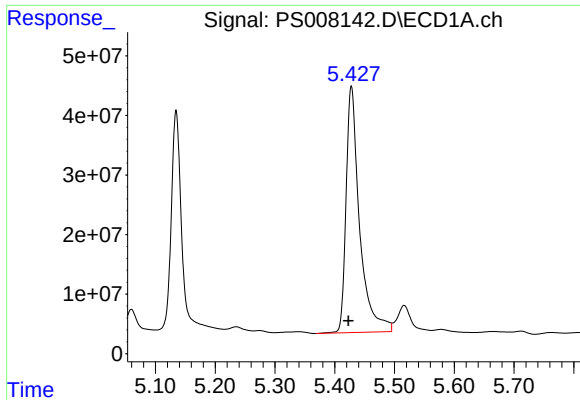

#4 2,4-DCAA


R.T.: 5.428 min
Delta R.T.: 0.006 min
Response: 648638119
Conc: 432.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

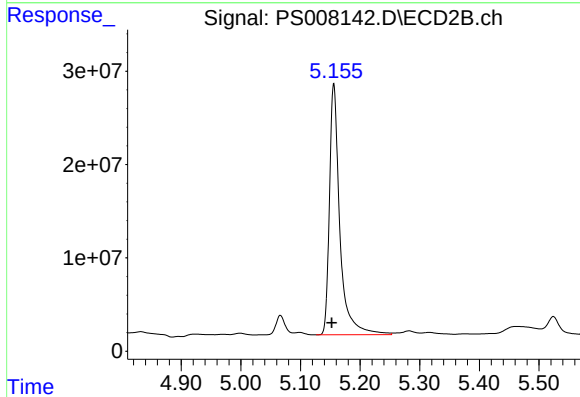


#4 2,4-DCAA

R.T.: 5.156 min
Delta R.T.: 0.004 min
Response: 326259175
Conc: 444.53 ng/ml

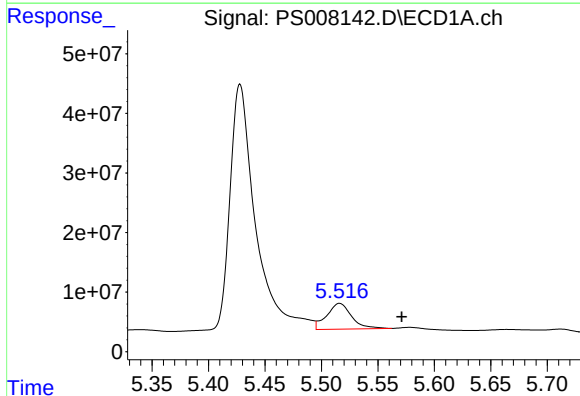


#5 DICAMBA

R.T.: 5.516 min
Delta R.T.: -0.055 min
Response: 66140984
Conc: 11.95 ng/ml

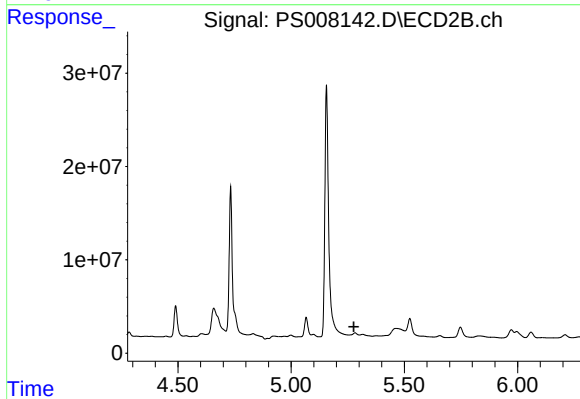

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.277 min
Response: 0
Conc: N.D.

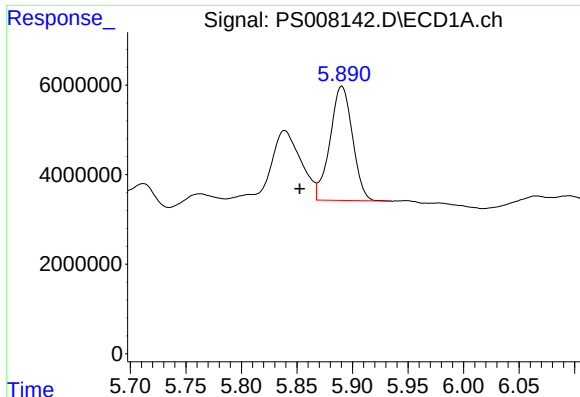

#7 MCPA


R.T.: 5.890 min
Delta R.T.: 0.038 min
Response: 35959851
Conc: 6.30 ug/ml

Instrument :
ECD_S
ClientSampleId :

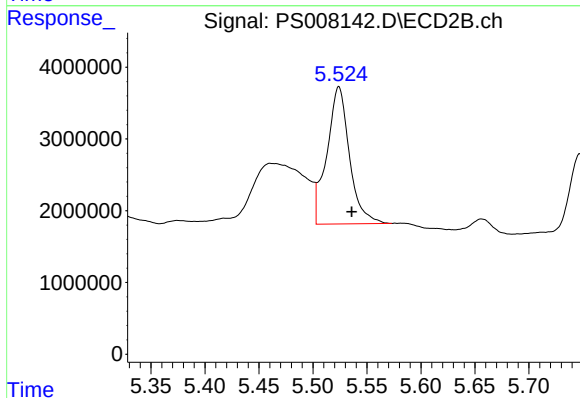


#7 MCPA

R.T.: 5.524 min
Delta R.T.: -0.012 min
Response: 27801659
Conc: 9.31 ug/ml

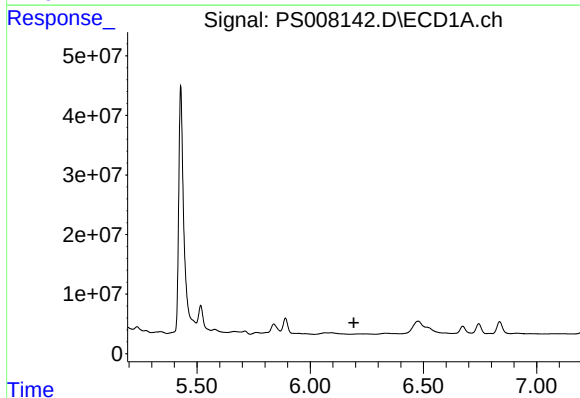


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.193 min
Response: 0
Conc: N.D.

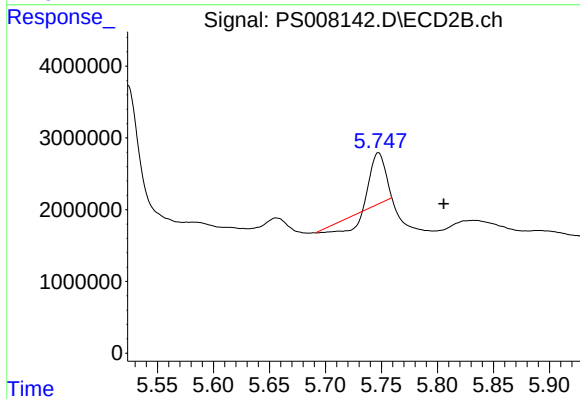

#8 DICHLORPROP


R.T.: 5.747 min
Delta R.T.: -0.058 min
Response: 4183524
Conc: 6.10 ng/ml

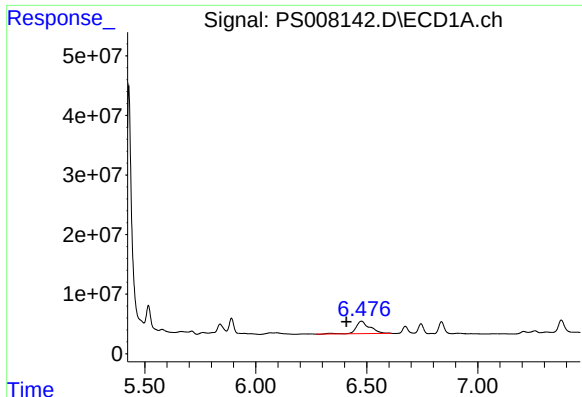

#9 2,4-D


R.T.: 6.476 min
Delta R.T.: 0.067 min
Response: 91930580
Conc: 61.02 ng/ml

Instrument :
ECD_S
ClientSampleId :

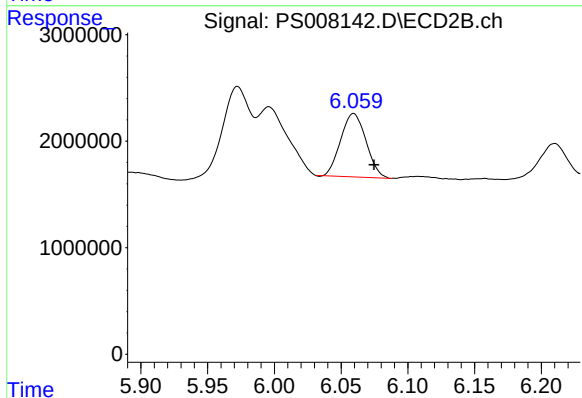


#9 2,4-D

R.T.: 6.059 min
Delta R.T.: -0.015 min
Response: 7885445
Conc: 9.69 ng/ml

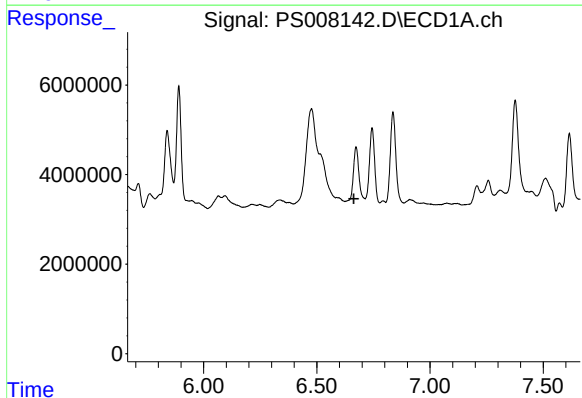


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.663 min
Response: 0
Conc: N.D.

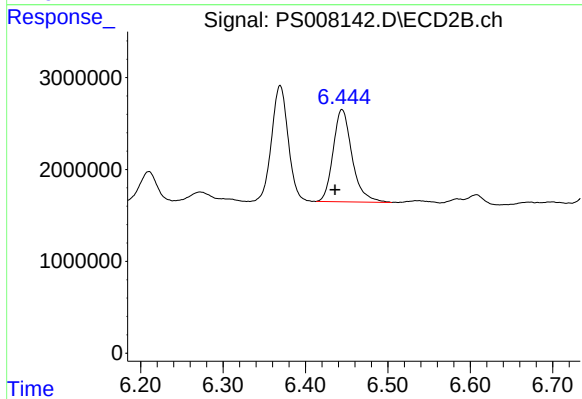

#10 Pentachlorophenol


R.T.: 6.444 min
Delta R.T.: 0.008 min
Response: 16064439
Conc: 1.58 ng/ml

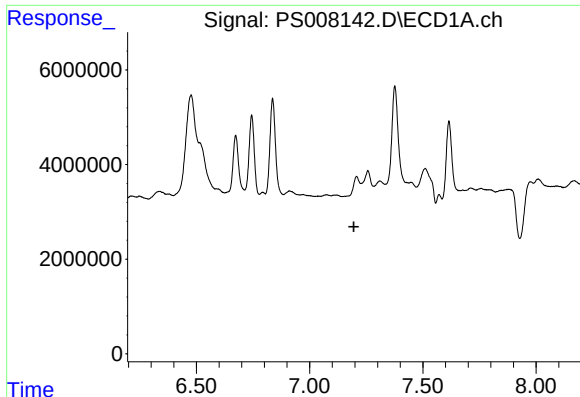

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.195 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

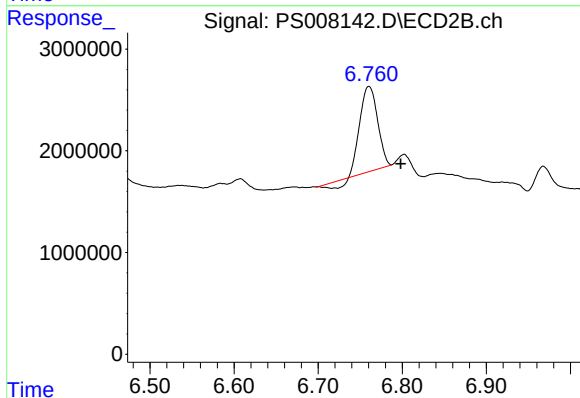


#11 2,4,5-TP (SILVEX)

R.T.: 6.761 min
Delta R.T.: -0.038 min
Response: 11537301
Conc: 2.85 ng/ml

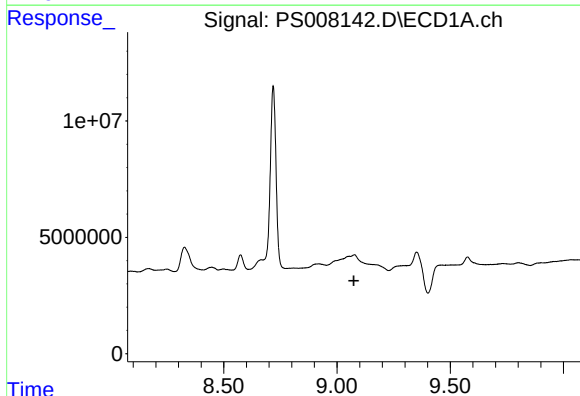


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 9.075 min
Response: 0
Conc: N.D.

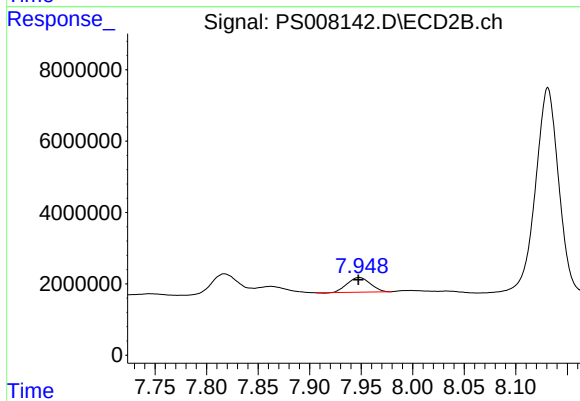

#14 DINOSEB


R.T.: 7.948 min
Delta R.T.: 0.000 min
Response: 6342620
Conc: 2.50 ng/ml

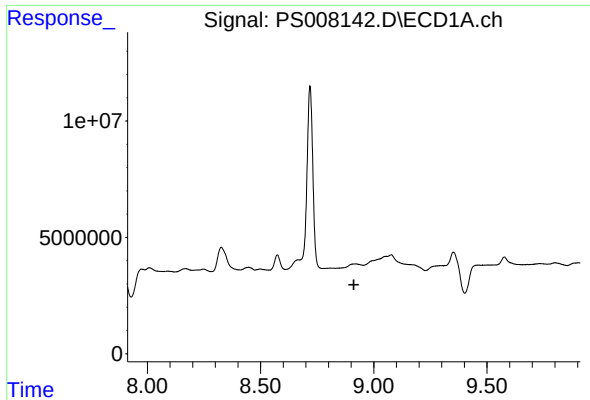

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.912 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

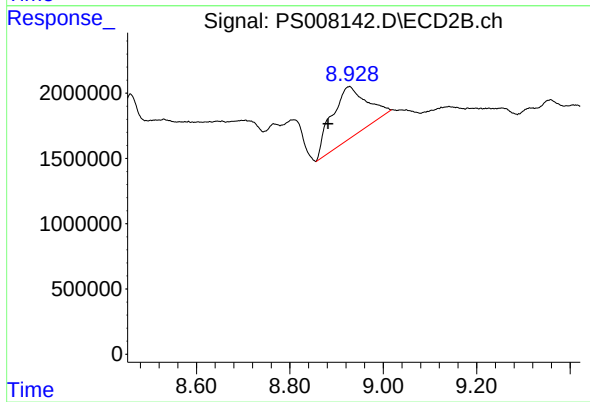

#15 Picloram

R.T.: 8.927 min
Delta R.T.: 0.045 min
Response: 20673274
Conc: 3.43 ng/ml