

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122319\
 Data File : PS008140.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2019 15:11
 Operator : SM\AJ
 Sample : PB125666BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB125666BL

Manual Integrations
 APPROVED

Ankita
 12/24/2019 9:15:28 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 24 01:21:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121819.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 18 11:09:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	5.429	5.152	661.3E6	351.2E6	441.420	478.520m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS122319\
Data File : PS008140.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2019 15:11
Operator : SM\AJ
Sample : PB125666BL
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
PB125666BL


Manual Integrations
APPROVED

Ankita
12/24/2019 9:15:28 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 01:21:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121819.M
Quant Title : 8080.M
QLast Update : Wed Dec 18 11:09:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

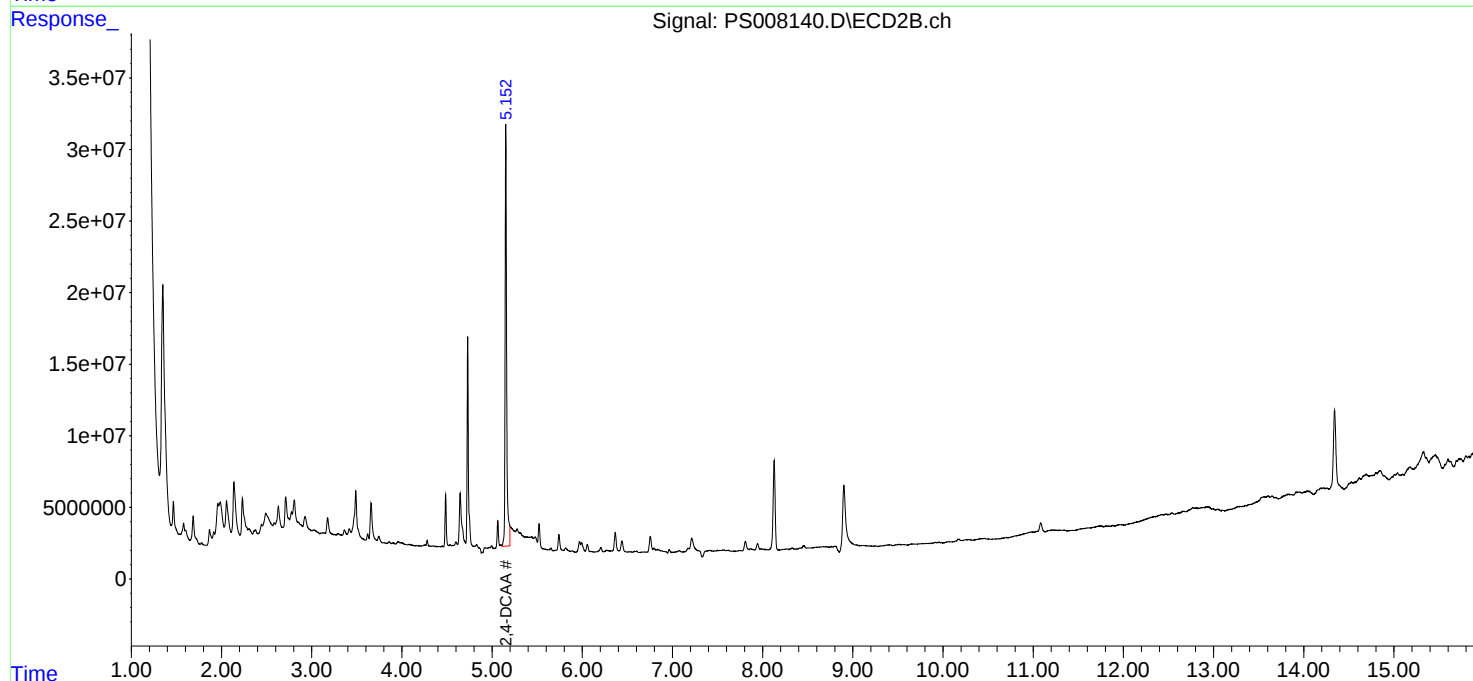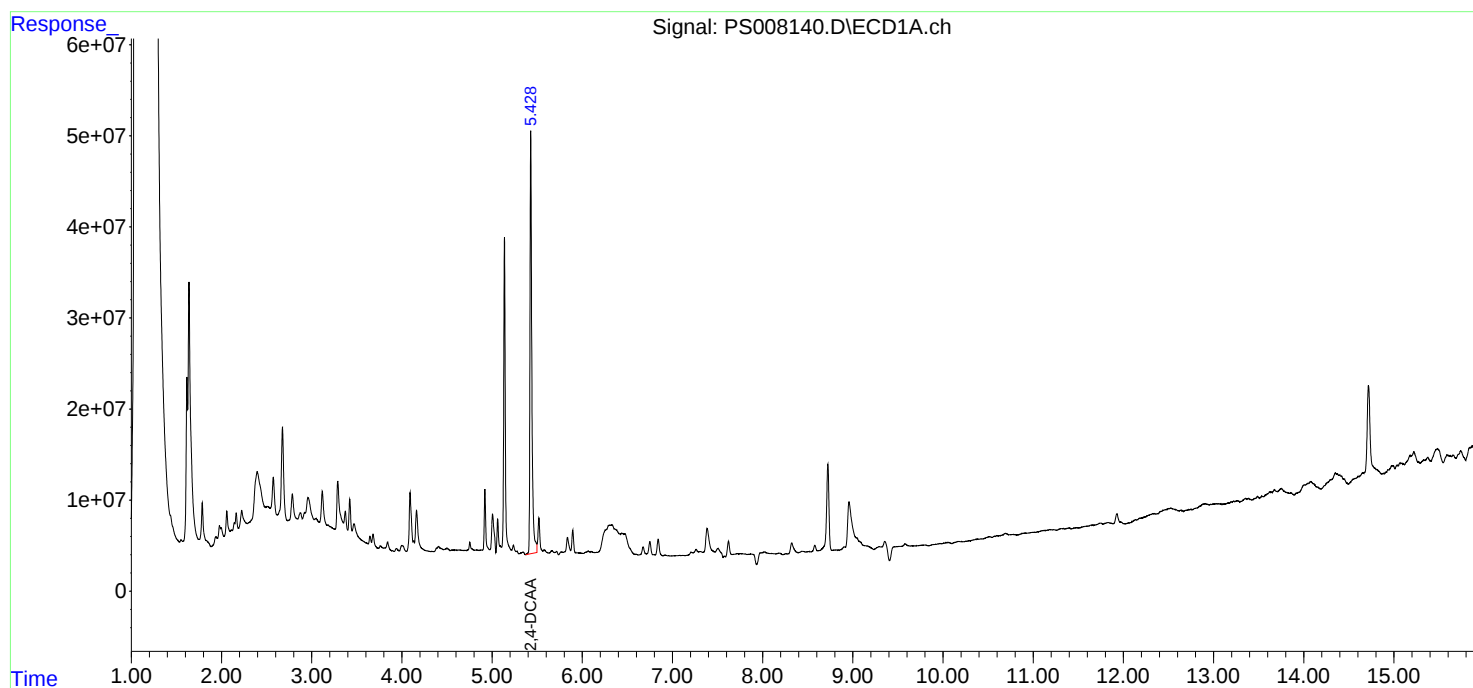

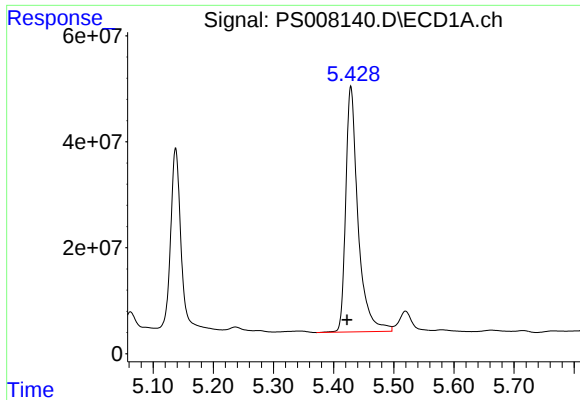


#4 2,4-DCAA

R.T.: 5.429 min
Delta R.T.: 0.006 min
Response: 661294764
Conc: 441.42 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB125666BL

Manual Integrations
APPROVED

Ankita
12/24/2019 9:15:28 AM

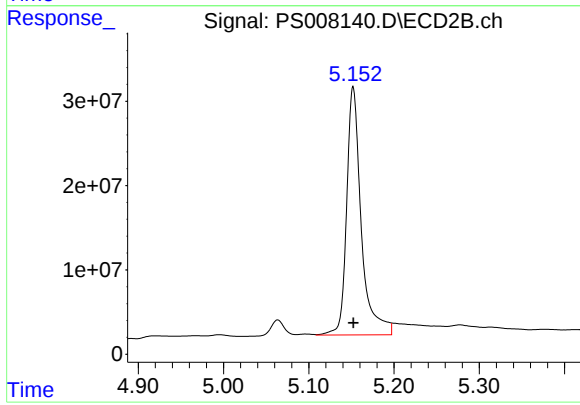

#4 2,4-DCAA

R.T.: 5.152 min
Delta R.T.: 0.000 min
Response: 351202288
Conc: 478.52 ng/ml m