

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010219\
Data File : FF003121.D
Signal(s) : FID2B.ch
Acq On : 02 Jan 2019 12:41
Operator : AJ\SJ
Sample : PB116086BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 02 23:50:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.628	185031	1.425 ug/ml
Target Compounds				
10)	N-TETRACOSANE	14.807	163899	1.134 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010219\
Data File : FF003121.D
Signal(s) : FID2B.ch
Acq On : 02 Jan 2019 12:41
Operator : AJ\SJ
Sample : PB116086BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 02 23:50:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

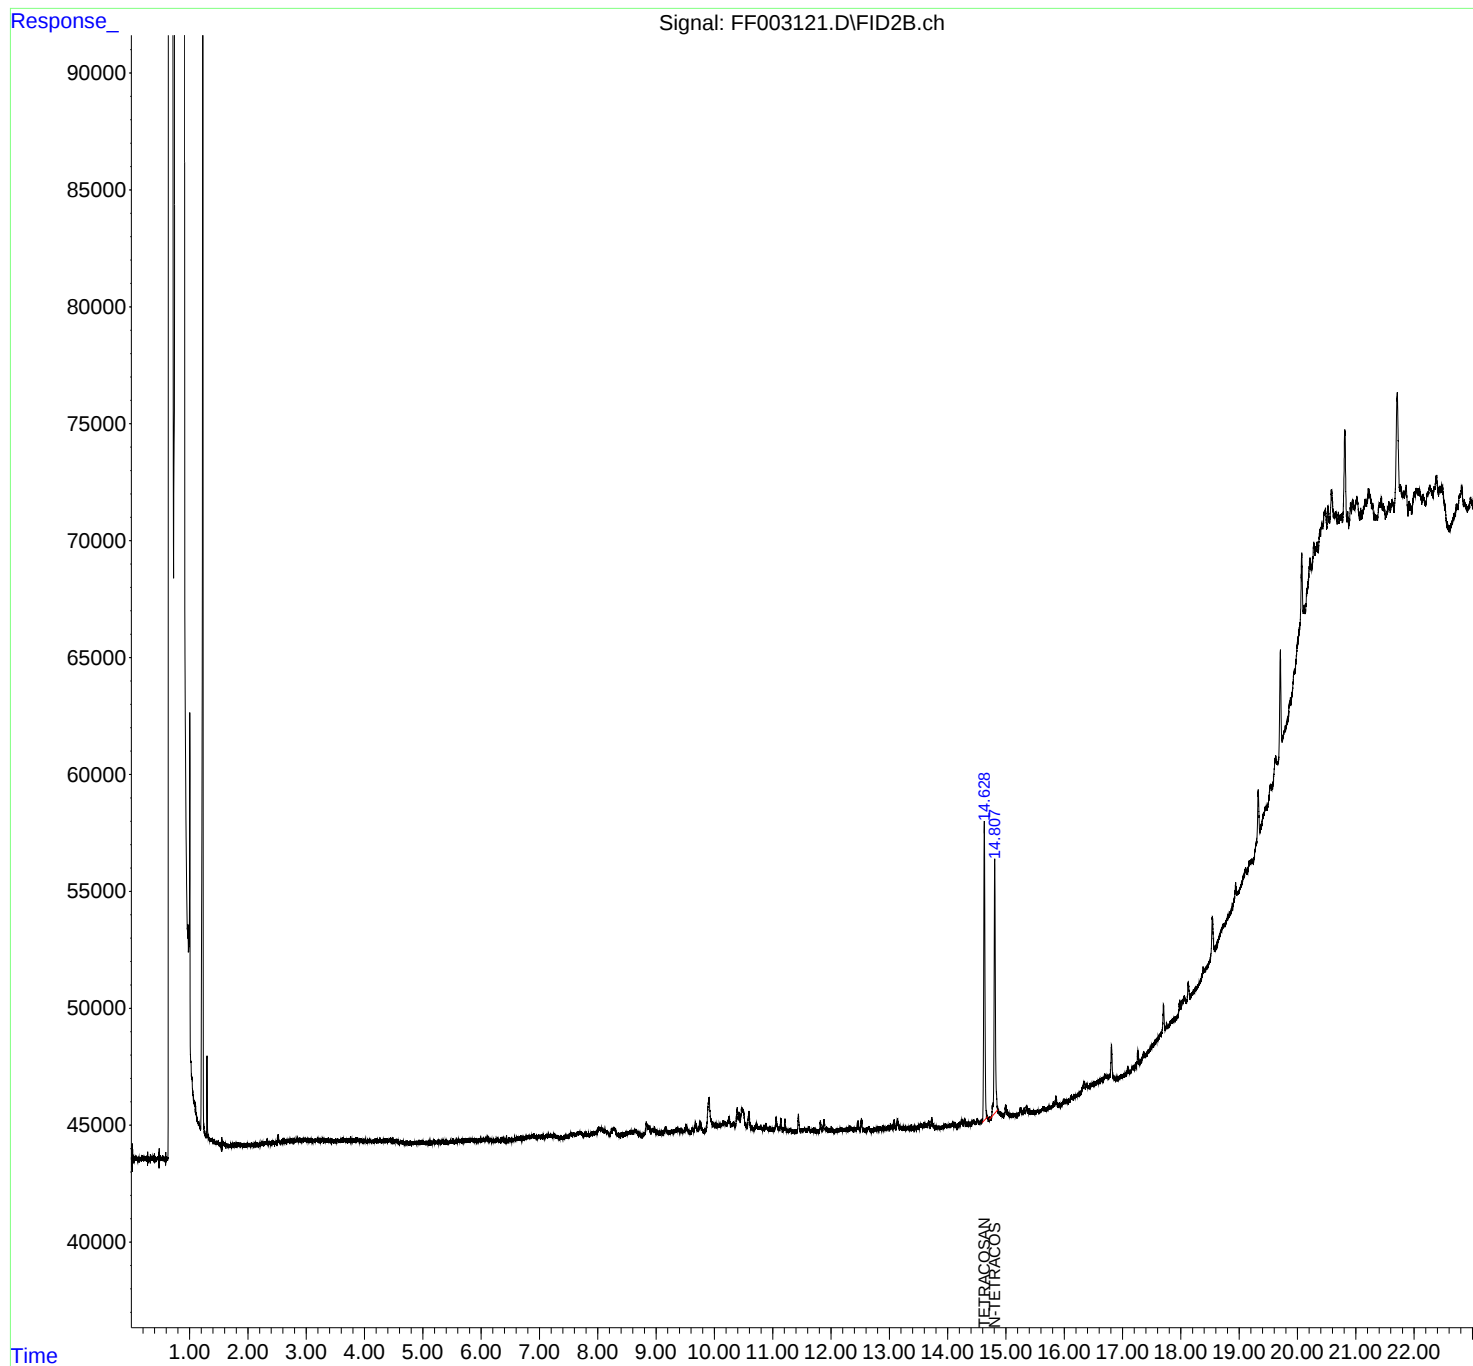


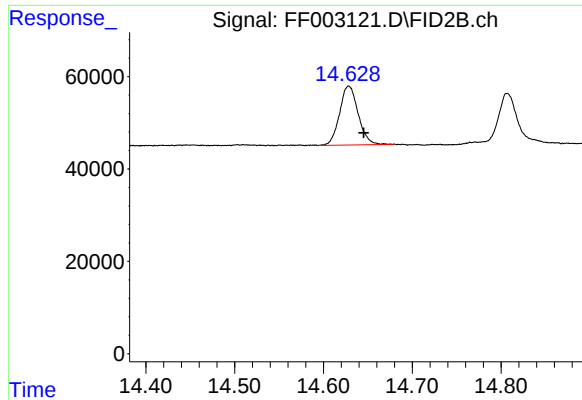

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.628 min
Delta R.T.: -0.017 min
Response: 185031
Conc: 1.43 ug/ml

Instrument :
FID_F
ClientSampleId :

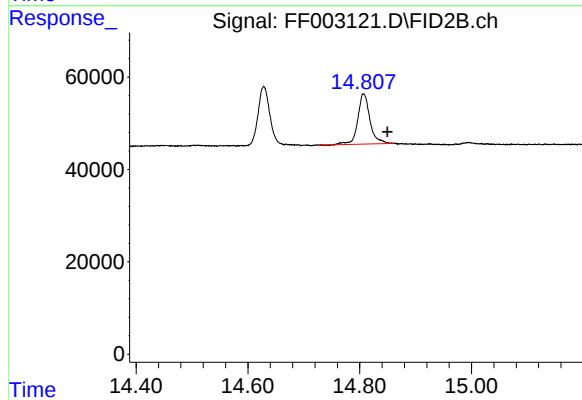

#10 N-TETRACOSANE

R.T.: 14.807 min
Delta R.T.: -0.043 min
Response: 163899
Conc: 1.13 ug/ml