

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010219\
Data File : FF003124.D
Signal(s) : FID2B.ch
Acq On : 02 Jan 2019 14:31
Operator : AJ\SJ
Sample : J6587-05 100X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 02 23:51:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
4) N-TETRADECANE	8.247f	106309	0.663 ug/ml
5) N-HEXADECANE	9.794	311967	1.948 ug/ml
6) N-OCTADECANE	11.192	576839	3.641 ug/ml
10) N-TETRACOSANE	14.809	192591	1.333 ug/ml
17) N-OCTATRIACONTANE	20.751f	321696	3.170 ug/ml
18) N-TETRACONTANE	21.677	190518	1.813 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010219\
Data File : FF003124.D
Signal(s) : FID2B.ch
Acq On : 02 Jan 2019 14:31
Operator : AJ\SJ
Sample : J6587-05 100X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Jan 02 23:51:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

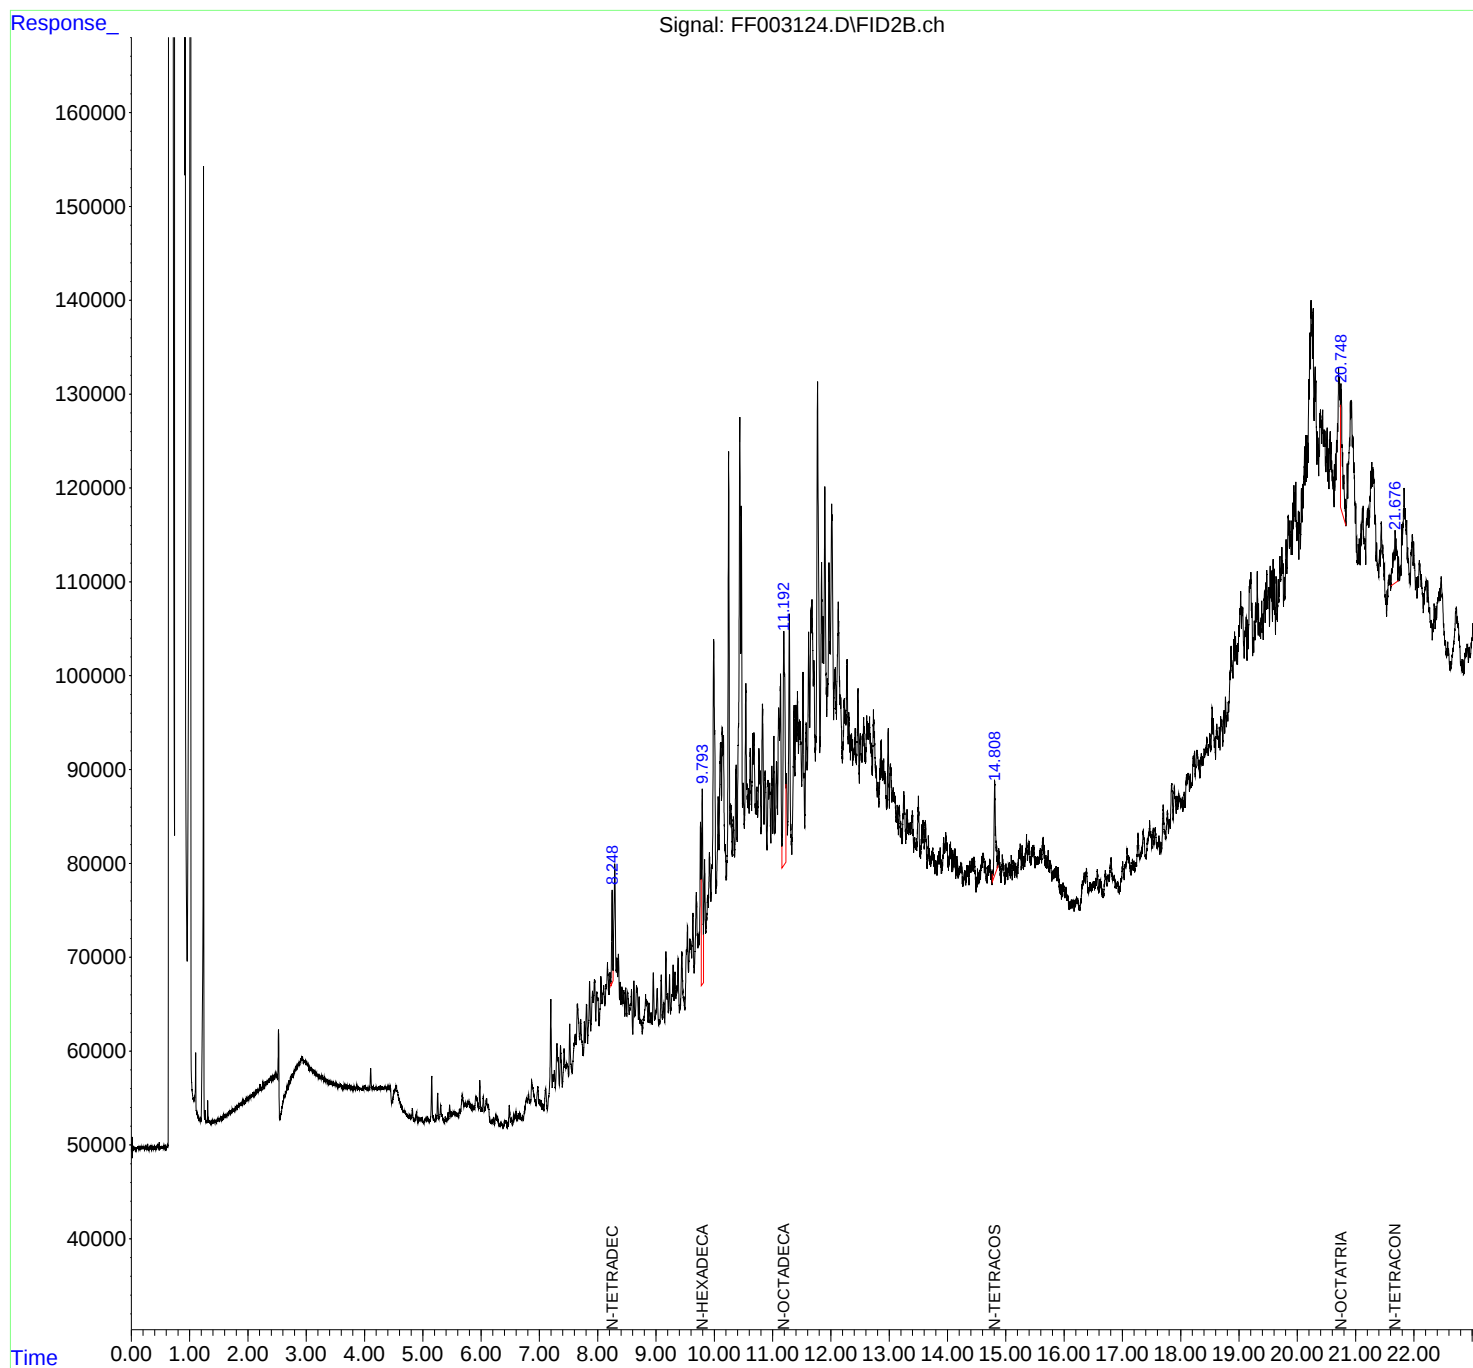


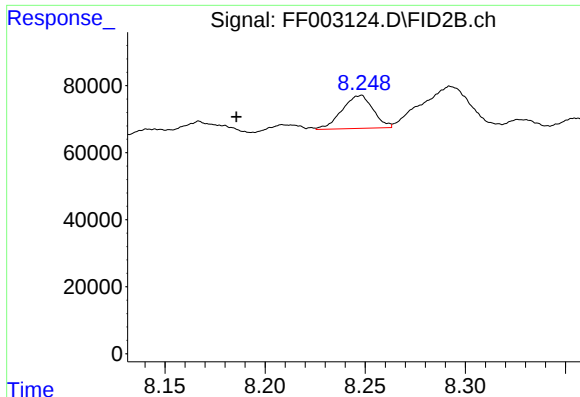

#4 N-TETRADECANE


R.T.: 8.247 min
Delta R.T.: 0.062 min
Response: 106309
Conc: 0.66 ug/ml

Instrument :
FID_F
ClientSampleId :

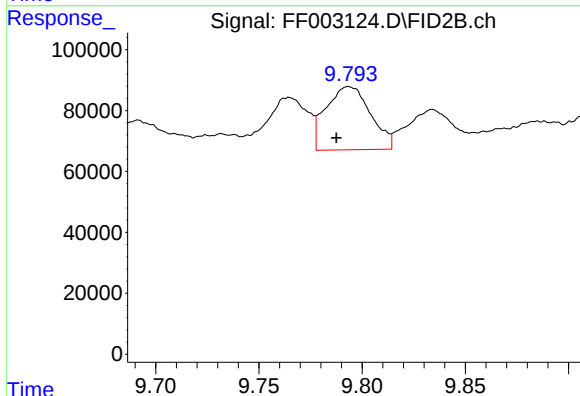


#5 N-HEXADECANE

R.T.: 9.794 min
Delta R.T.: 0.006 min
Response: 311967
Conc: 1.95 ug/ml

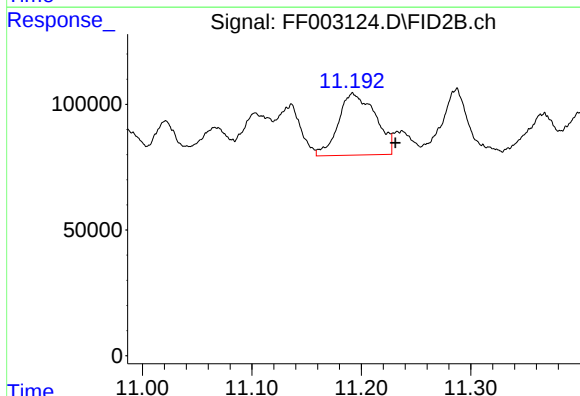


#6 N-OCTADECANE

R.T.: 11.192 min
Delta R.T.: -0.039 min
Response: 576839
Conc: 3.64 ug/ml

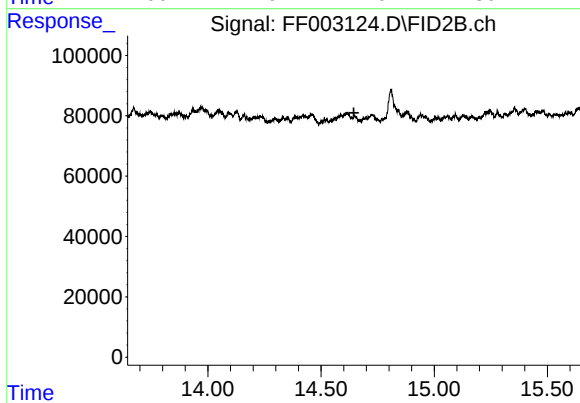

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.645 min
Response: 0
Conc: N.D.

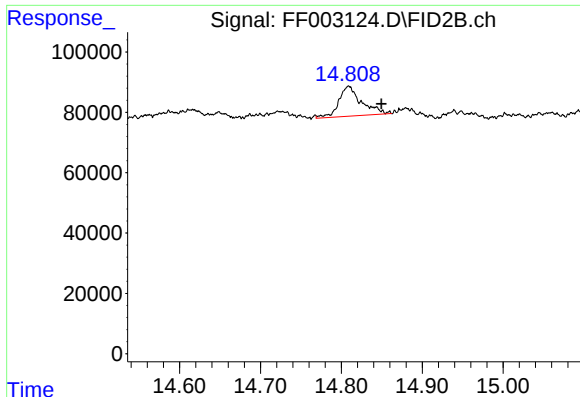

#10 N-TETRACOSANE


R.T.: 14.809 min
Delta R.T.: -0.041 min
Response: 192591
Conc: 1.33 ug/ml

Instrument :
FID_F
ClientSampleId :

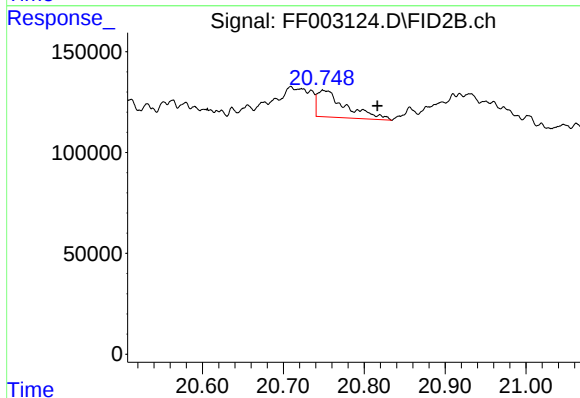

#17 N-OCTATRIACONTANE

R.T.: 20.751 min
Delta R.T.: -0.066 min
Response: 321696
Conc: 3.17 ug/ml

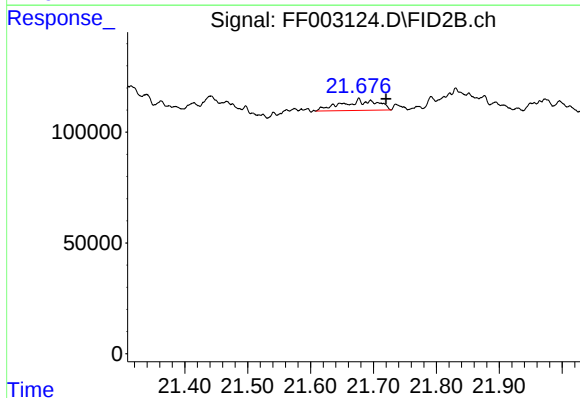

#18 N-TETRACONTANE

R.T.: 21.677 min
Delta R.T.: -0.043 min
Response: 190518
Conc: 1.81 ug/ml