

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010219\
Data File : FF003125.D
Signal(s) : FID2B.ch
Acq On : 02 Jan 2019 15:01
Operator : AJ\SJ
Sample : PB116089BL
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB116089BL

Integration File: autoint1.e
Quant Time: Jan 02 23:51:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.631	2163587	16.665 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010219\
Data File : FF003125.D
Signal(s) : FID2B.ch
Acq On : 02 Jan 2019 15:01
Operator : AJ\SJ
Sample : PB116089BL
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB116089BL

Integration File: autoint1.e
Quant Time: Jan 02 23:51:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

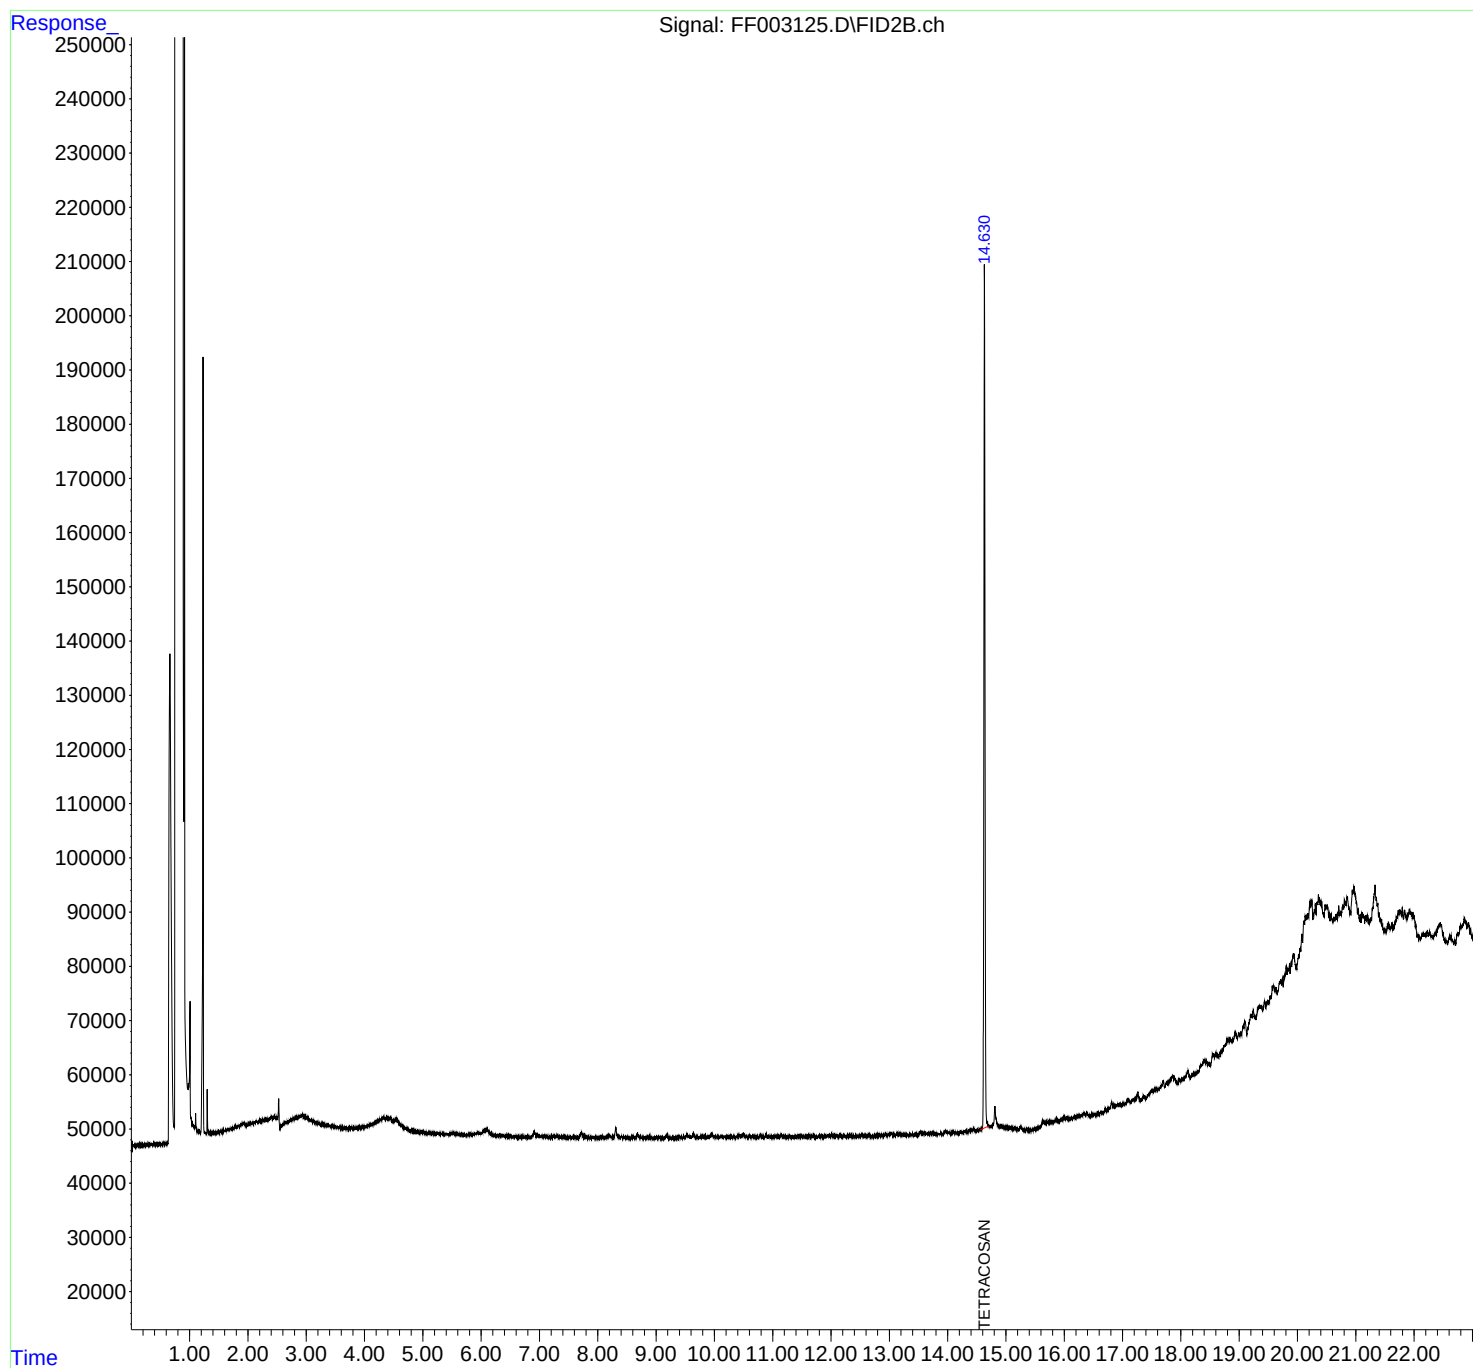

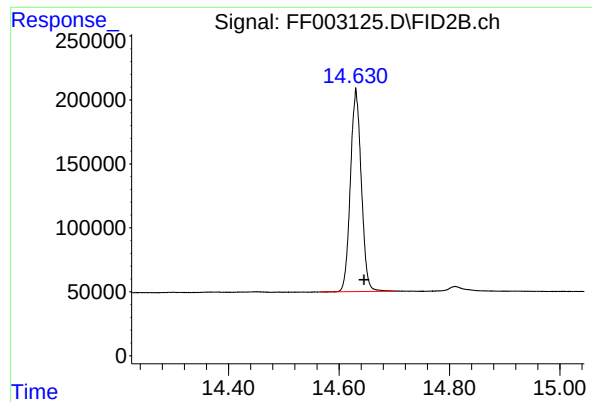

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.631 min
Delta R.T.: -0.015 min
Response: 2163587
Conc: 16.67 ug/ml

Instrument :
FID_F
ClientSampleId :
PB116089BL