

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010224\
Data File : FF013900.D
Signal(s) : FID2B.ch
Acq On : 02 Jan 2024 09:25
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 03 03:19:44 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010224.M
Quant Title :
QLast Update : Wed Jan 03 03:19:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) N-DOTRIACONTANE	18.875	87461	0.681 ug/ml
16) N-HEXATRIACONTANE	20.430	71300	0.882 ug/ml
18) N-TETRACONTANE	22.046	472365	5.808 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010224\
Data File : FF013900.D
Signal(s) : FID2B.ch
Acq On : 02 Jan 2024 09:25
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 03 03:19:44 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010224.M
Quant Title :
QLast Update : Wed Jan 03 03:19:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

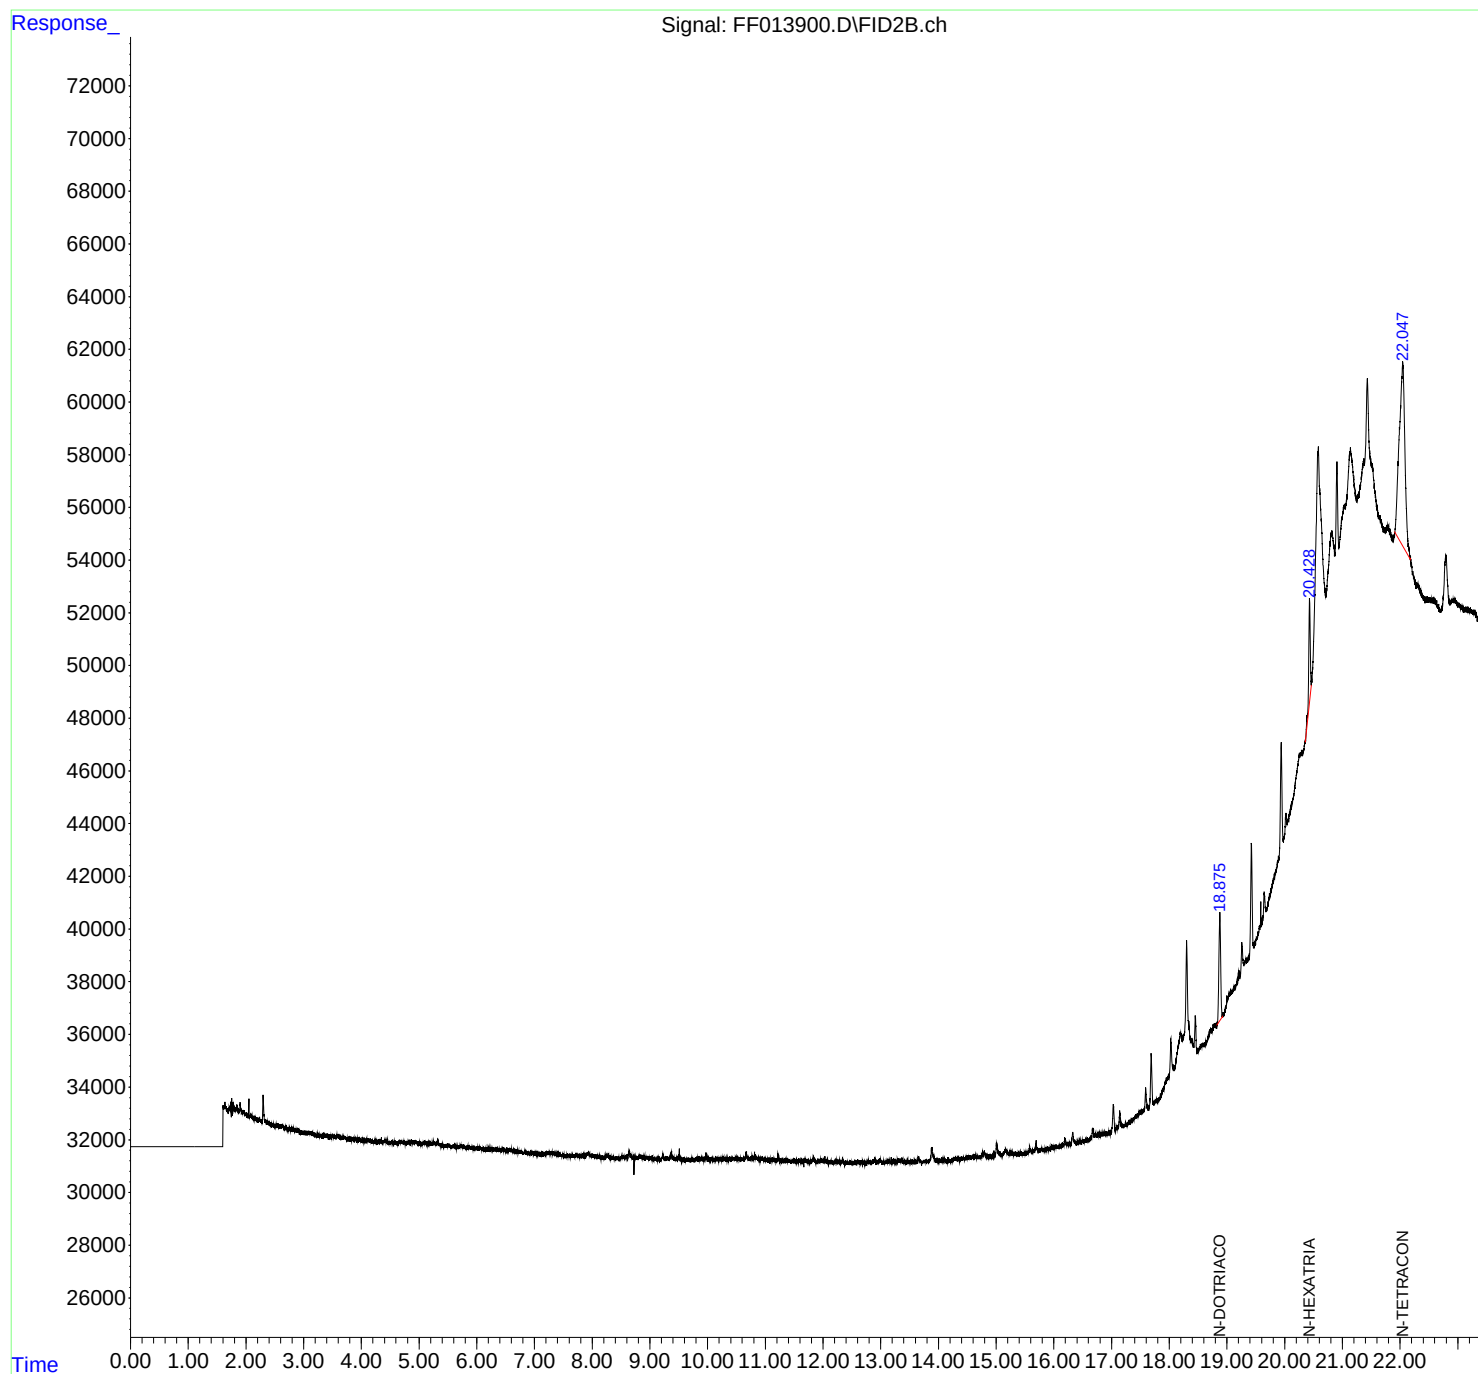


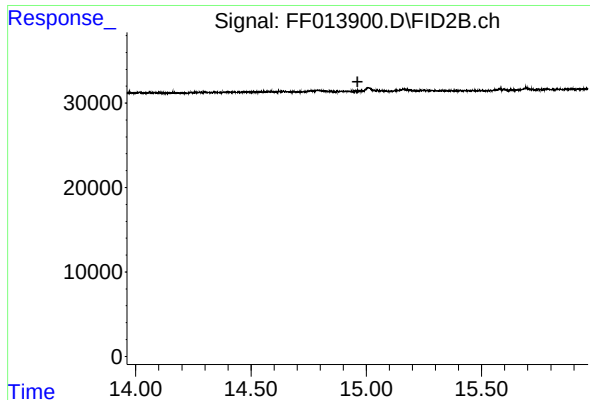

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.962 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

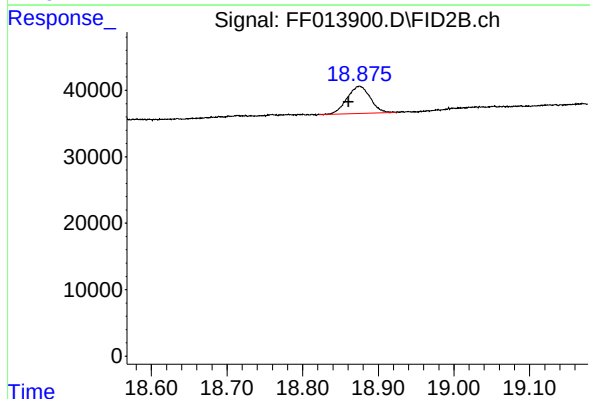


#14 N-DOTRIACONTANE

R.T.: 18.875 min
Delta R.T.: 0.015 min
Response: 87461
Conc: 0.68 ug/ml

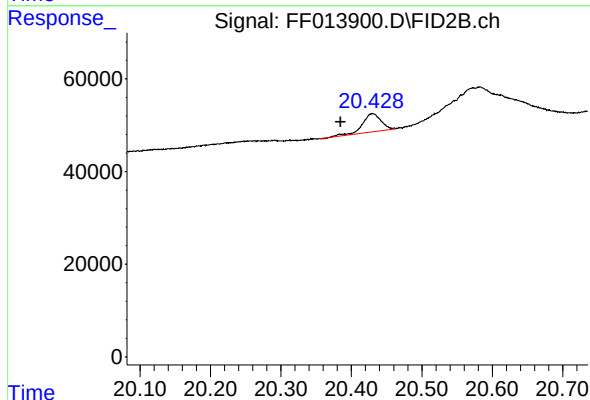

#16 N-HEXATRIACONTANE

R.T.: 20.430 min
Delta R.T.: 0.046 min
Response: 71300
Conc: 0.88 ug/ml

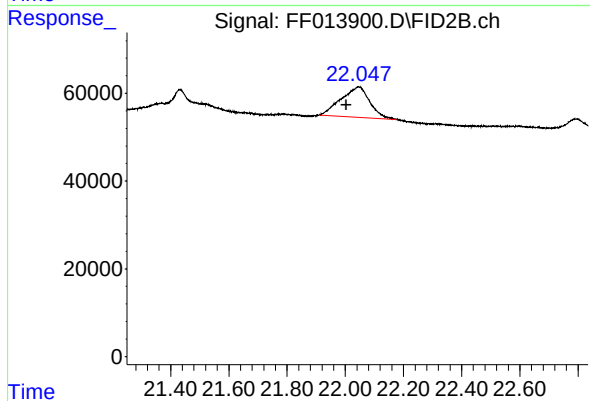

#18 N-TETRACONTANE

R.T.: 22.046 min
Delta R.T.: 0.042 min
Response: 472365
Conc: 5.81 ug/ml