

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_F\Data\FF010319\
Data File : FF003134.D
Signal(s) : FID2B.ch
Acq On : 03 Jan 2019 10:47
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 03 15:27:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.371	2745742	17.291 ug/ml
10) N-TETRACOSANE	14.804	143217	0.991 ug/ml
12) N-OCTACOSANE	16.809	2475150	18.473 ug/ml
13) N-TRIACONTANE	17.700	112437	0.877 ug/ml
14) N-DOTRIACONTANE	18.536	130409	1.092 ug/ml
15) N-TETRATRIACONTANE	19.324	127190	1.122 ug/ml
16) N-HEXATRIACONTANE	20.068	140796	1.305 ug/ml
17) N-OCTATRIACONTANE	20.807	187959	1.852 ug/ml
18) N-TETRACONTANE	21.706	297847	2.834 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_F\Data\FF010319\
Data File : FF003134.D
Signal(s) : FID2B.ch
Acq On : 03 Jan 2019 10:47
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 03 15:27:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

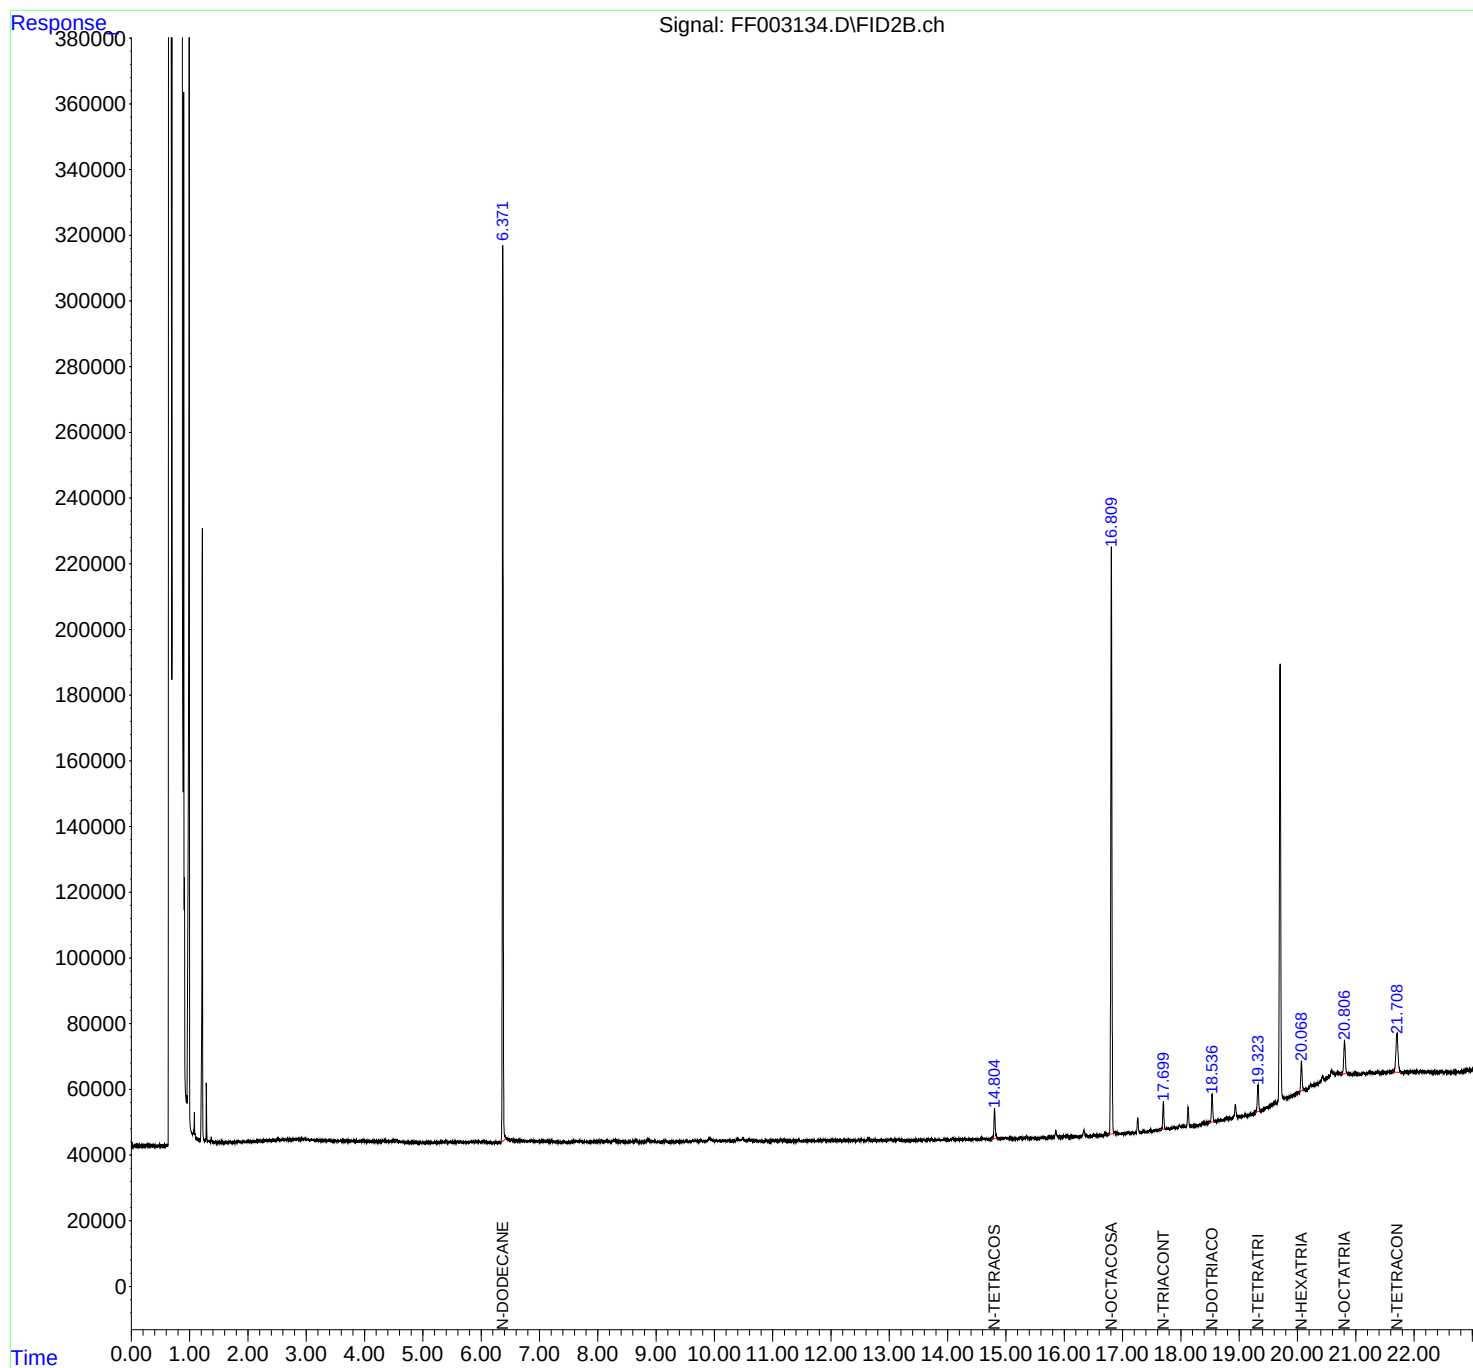


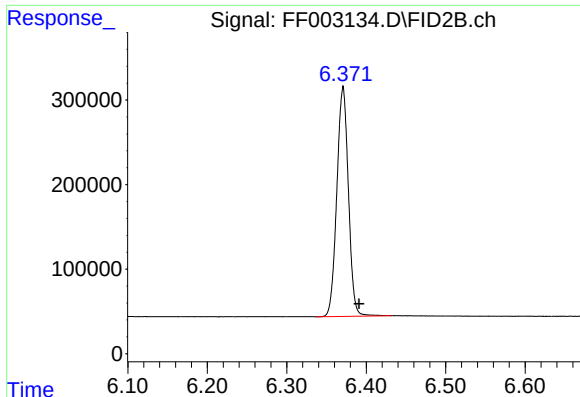

#3 N-DODECANE


R.T.: 6.371 min
Delta R.T.: -0.020 min
Response: 2745742
Conc: 17.29 ug/ml

Instrument :
FID_F
ClientSampleId :

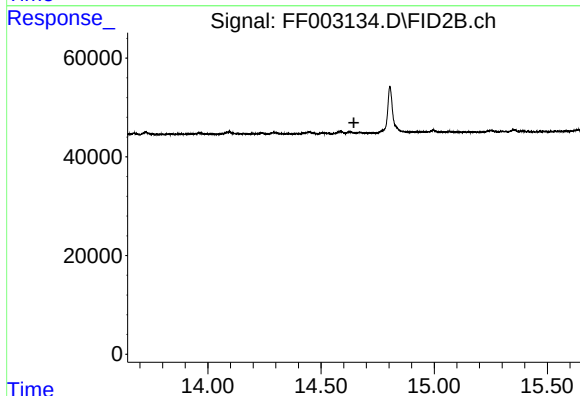


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.645 min
Response: 0
Conc: N.D.

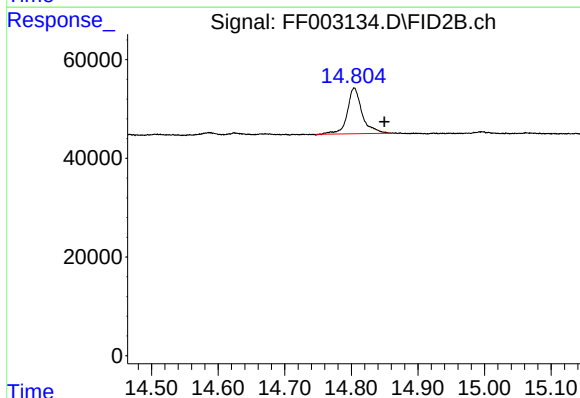


#10 N-TETRACOSANE

R.T.: 14.804 min
Delta R.T.: -0.045 min
Response: 143217
Conc: 0.99 ug/ml

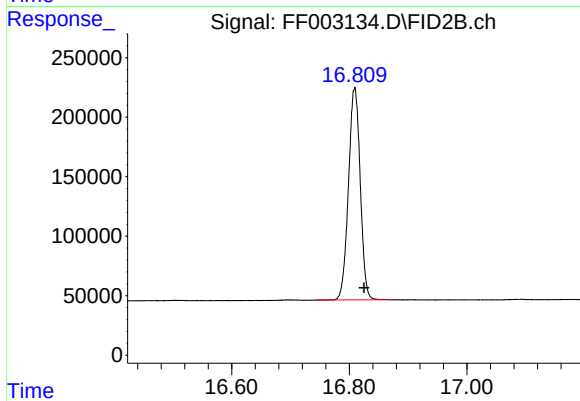

#12 N-OCTACOSANE


R.T.: 16.809 min
Delta R.T.: -0.016 min
Response: 2475150
Conc: 18.47 ug/ml

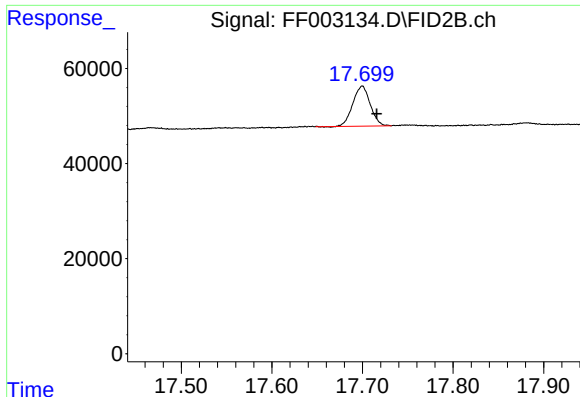

#13 N-TRIACONTANE


R.T.: 17.700 min
Delta R.T.: -0.016 min
Response: 112437
Conc: 0.88 ug/ml

Instrument :
FID_F
ClientSampleId :

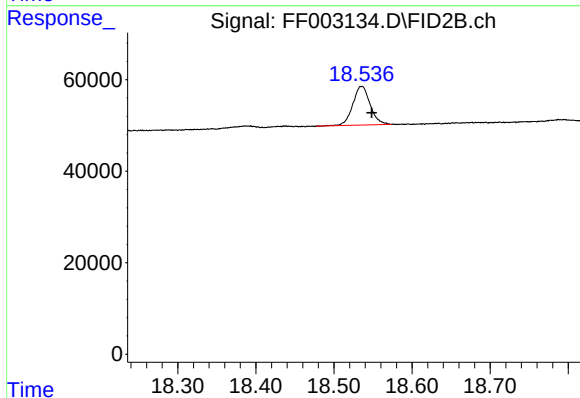


#14 N-DOTRIACONTANE

R.T.: 18.536 min
Delta R.T.: -0.013 min
Response: 130409
Conc: 1.09 ug/ml

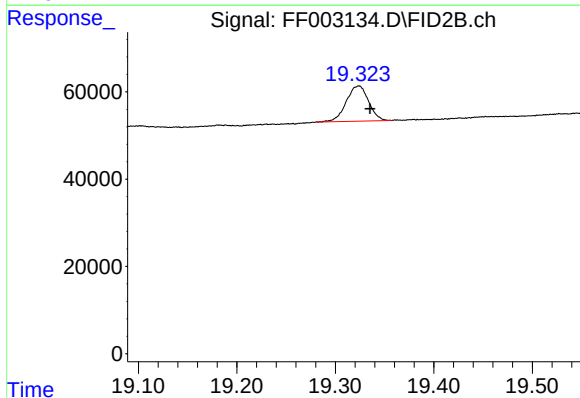


#15 N-TETRATRIACONTANE

R.T.: 19.324 min
Delta R.T.: -0.012 min
Response: 127190
Conc: 1.12 ug/ml

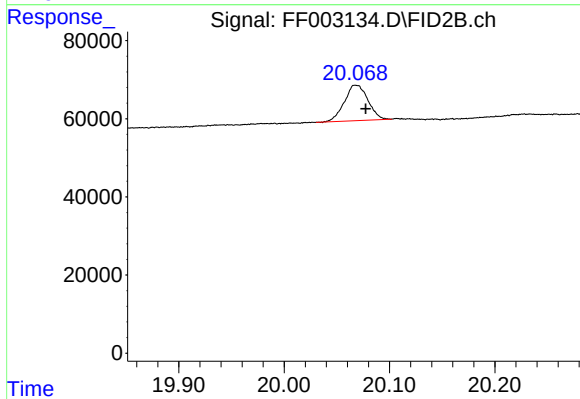

#16 N-HEXATRIACONTANE


R.T.: 20.068 min
Delta R.T.: -0.010 min
Response: 140796
Conc: 1.30 ug/ml

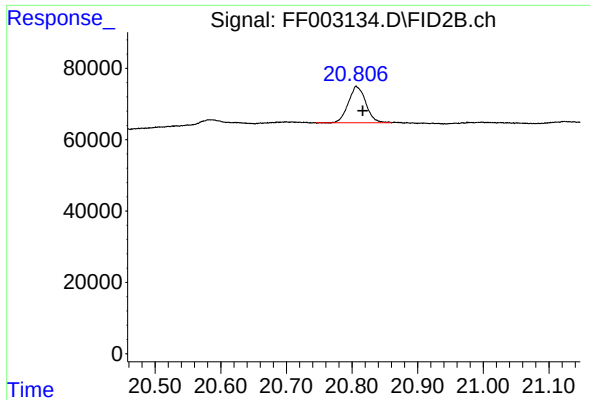

#17 N-OCTATRIACONTANE

R.T.: 20.807 min
Delta R.T.: -0.010 min
Response: 187959
Conc: 1.85 ug/ml

Instrument :
FID_F
ClientSampleId :

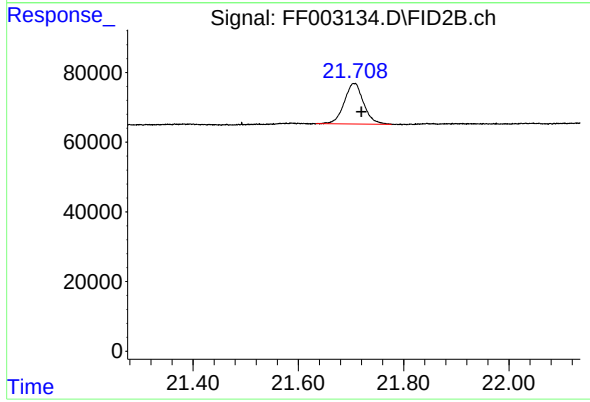

#18 N-TETRACONTANE

R.T.: 21.706 min
Delta R.T.: -0.014 min
Response: 297847
Conc: 2.83 ug/ml