

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010322\
 Data File : FF009610.D
 Signal(s) : FID2B.ch
 Acq On : 03 Jan 2022 14:09
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 04 00:12:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
 Quant Title :
 QLast Update : Thu Dec 16 03:33:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.460	2599871	22.444 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.625	135703	1.140 ug/ml
13) N-TRIACONTANE	17.509	284023	2.480 ug/ml
14) N-DOTRIACONTANE	18.337	183286	1.677 ug/ml
16) N-HEXATRIACONTANE	19.858	231013	2.306 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010322\
Data File : FF009610.D
Signal(s) : FID2B.ch
Acq On : 03 Jan 2022 14:09
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 04 00:12:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

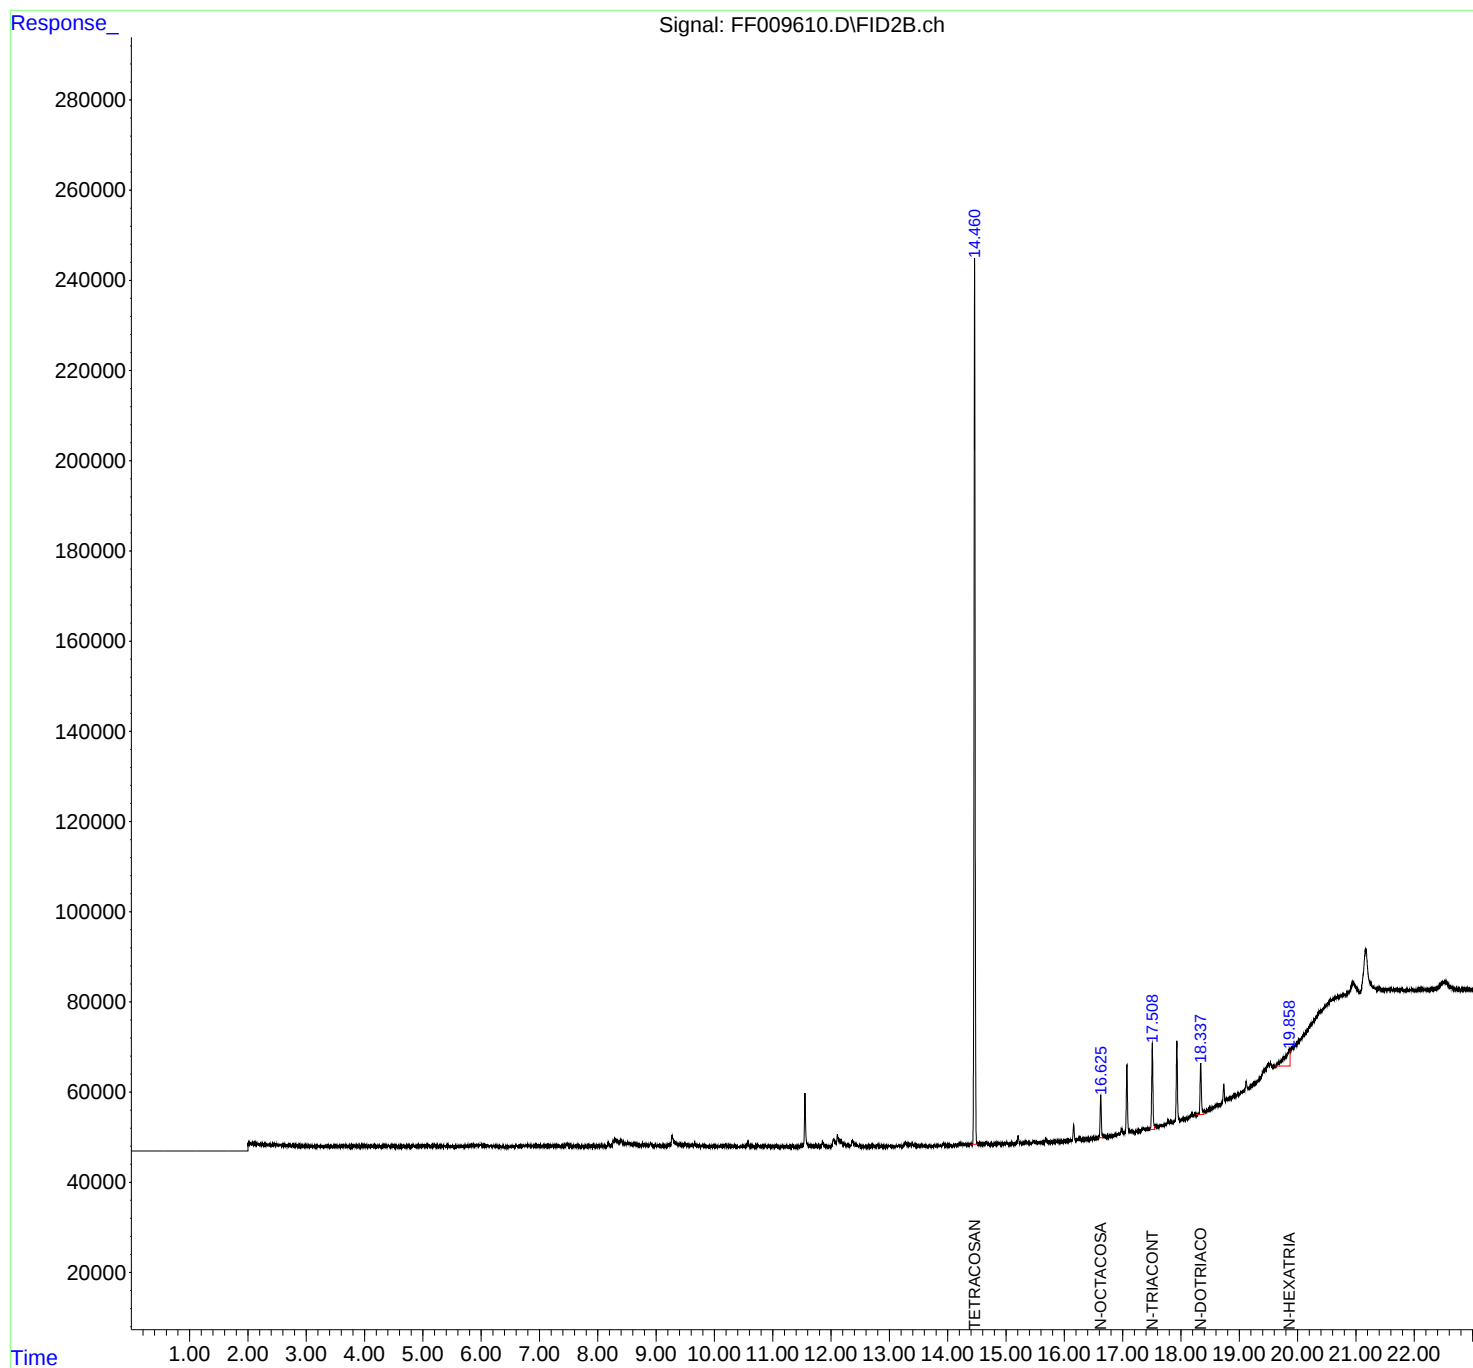


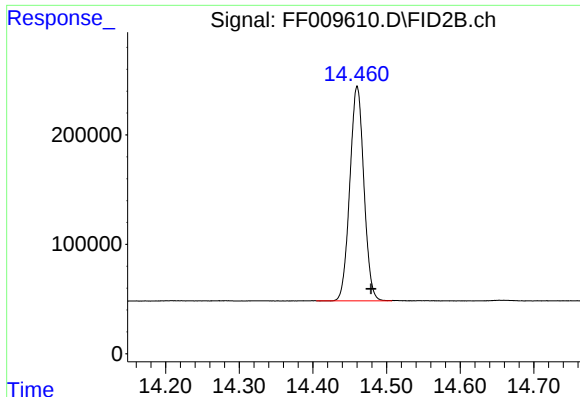

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.460 min
Delta R.T.: -0.019 min
Response: 2599871
Conc: 22.44 ug/ml

Instrument :
FID_F
ClientSampleId :

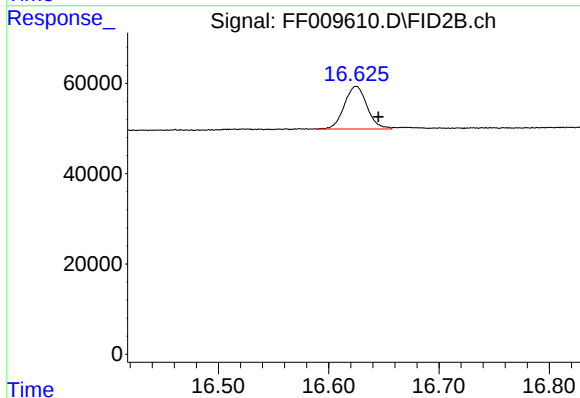


#12 N-OCTACOSANE

R.T.: 16.625 min
Delta R.T.: -0.020 min
Response: 135703
Conc: 1.14 ug/ml

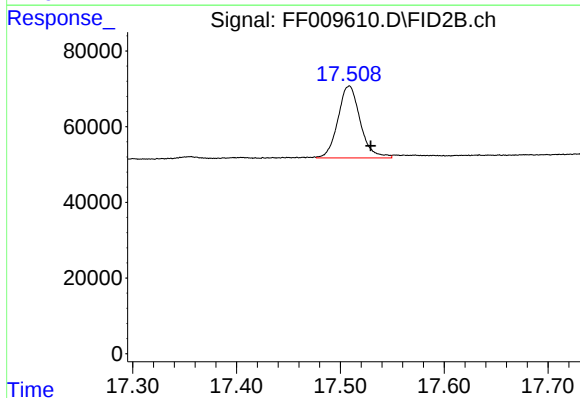


#13 N-TRIACONTANE

R.T.: 17.509 min
Delta R.T.: -0.020 min
Response: 284023
Conc: 2.48 ug/ml

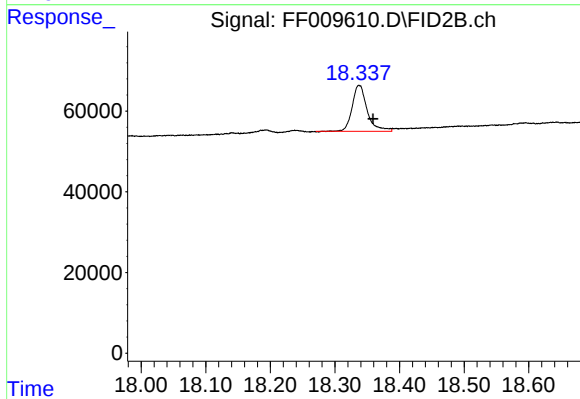

#14 N-DOTRIACONTANE

R.T.: 18.337 min
Delta R.T.: -0.022 min
Response: 183286
Conc: 1.68 ug/ml

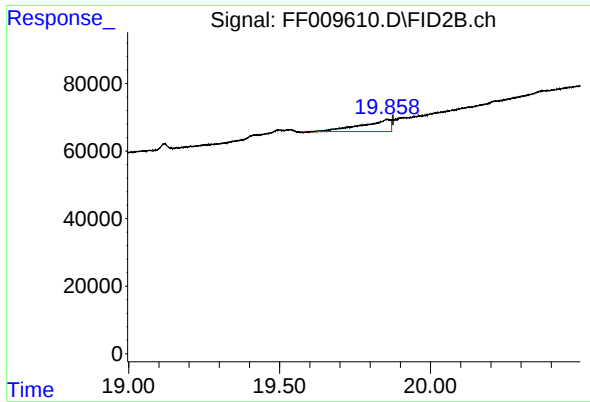

#16 N-HEXATRIACONTANE

R.T.: 19.858 min
Delta R.T.: -0.018 min
Response: 231013
Conc: 2.31 ug/ml

Instrument :
FID_F
ClientSampleId :