

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010322\
 Data File : FF009613.D
 Signal(s) : FID2B.ch
 Acq On : 03 Jan 2022 16:12
 Operator : AJ\MA
 Sample : PB141799BL
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 04 00:13:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
 Quant Title :
 QLast Update : Thu Dec 16 03:33:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.459	2562764	22.123 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.624	69587	0.584 ug/ml
13) N-TRIACONTANE	17.508	145301	1.268 ug/ml
14) N-DOTRIACONTANE	18.338	138855	1.271 ug/ml
15) N-TETRATRIACONTANE	19.116	56880	0.537 ug/ml
16) N-HEXATRIACONTANE	19.856	117135	1.169 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010322\
Data File : FF009613.D
Signal(s) : FID2B.ch
Acq On : 03 Jan 2022 16:12
Operator : AJ\MA
Sample : PB141799BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 04 00:13:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

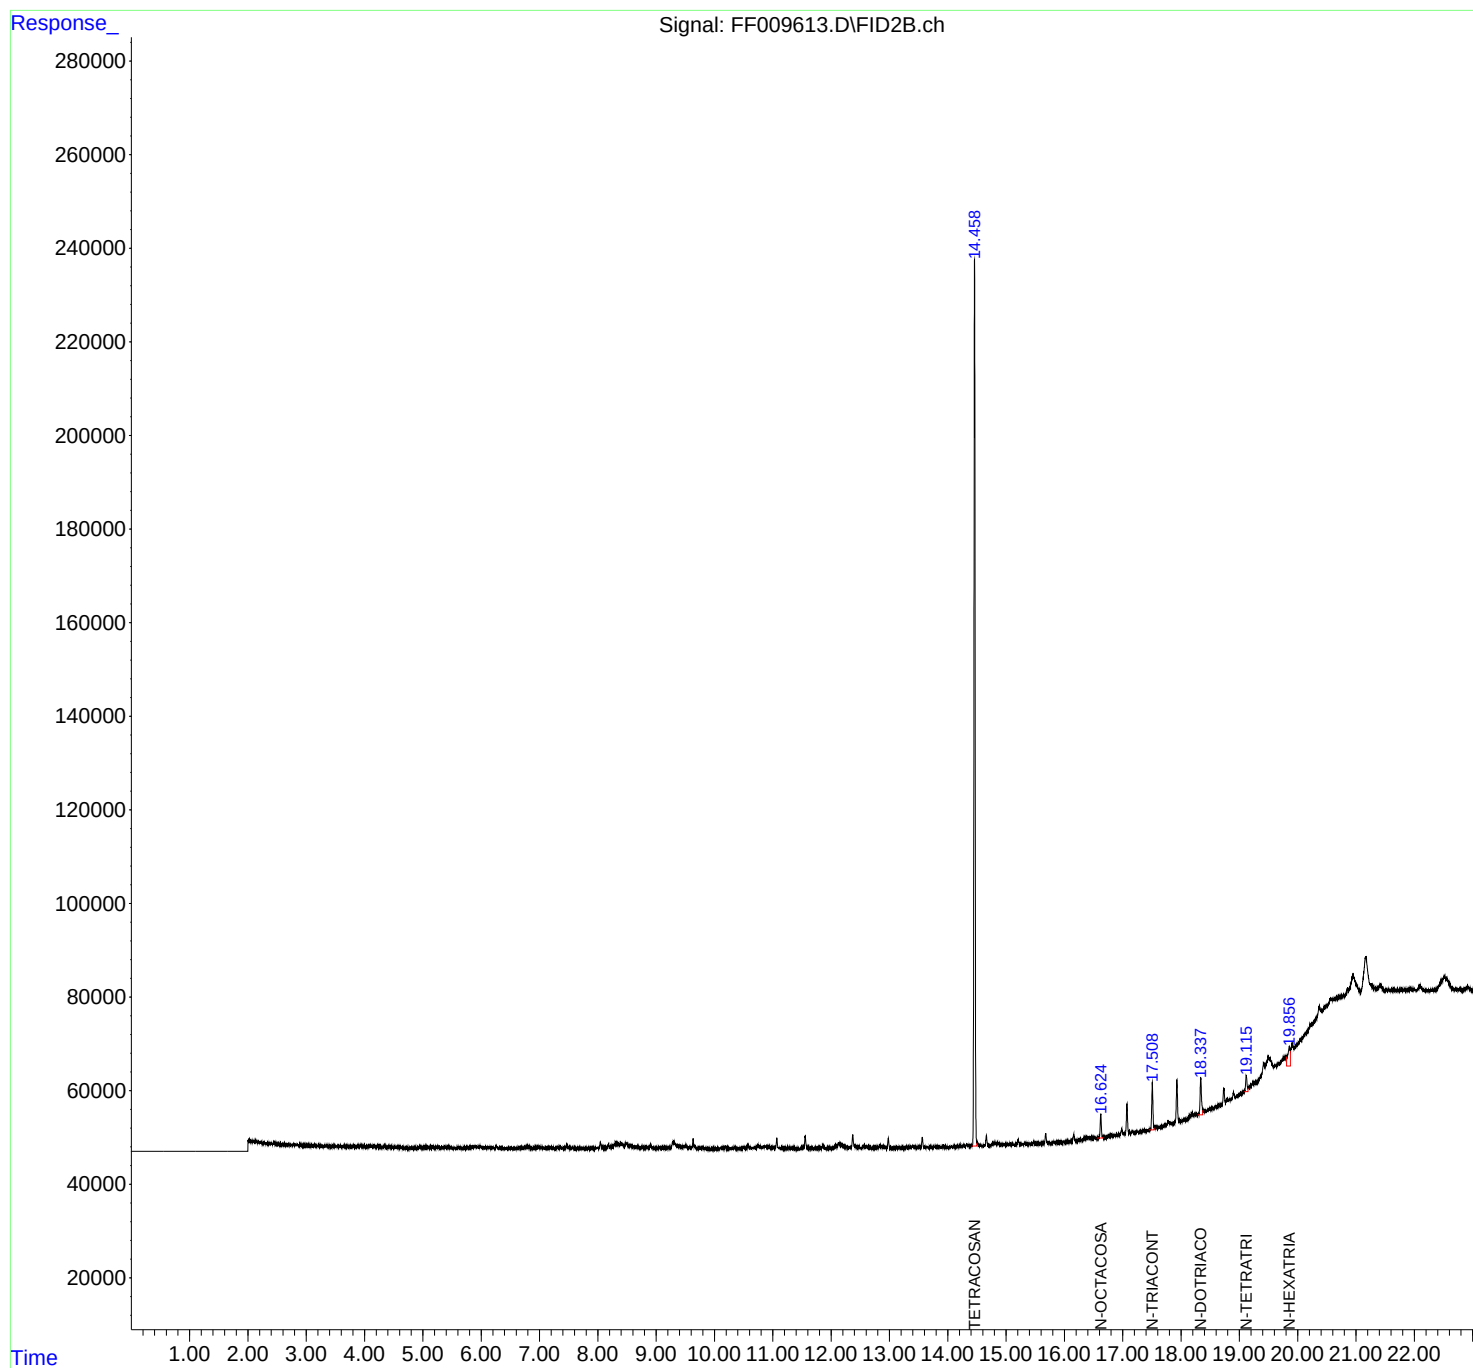


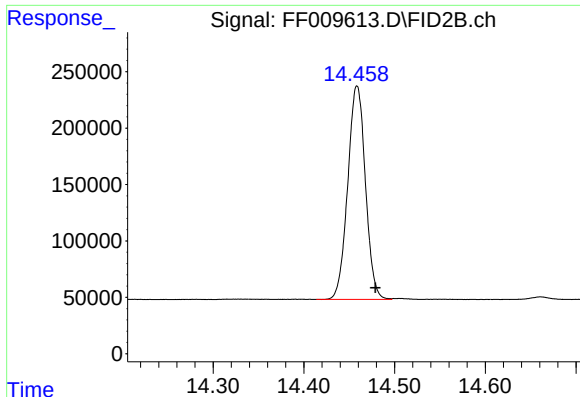

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.459 min
Delta R.T.: -0.020 min
Response: 2562764
Conc: 22.12 ug/ml

Instrument :
FID_F
ClientSampleId :

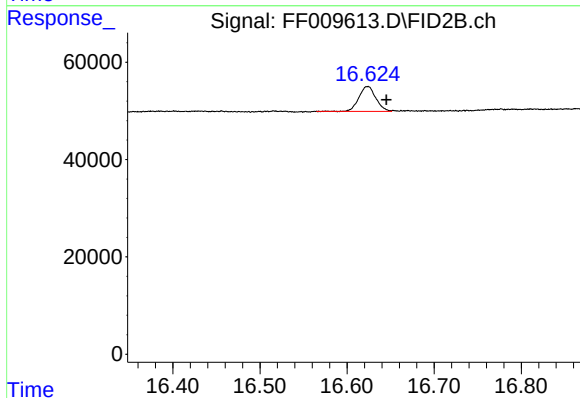


#12 N-OCTACOSANE

R.T.: 16.624 min
Delta R.T.: -0.021 min
Response: 69587
Conc: 0.58 ug/ml

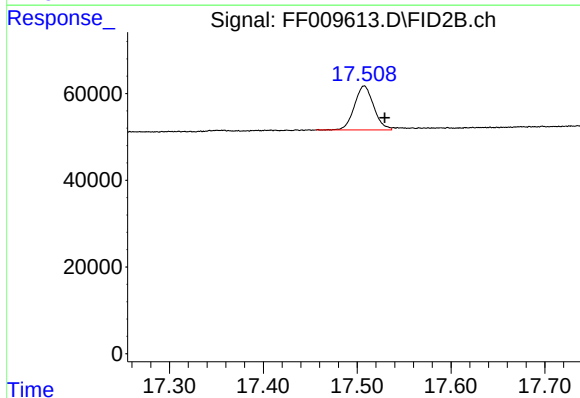


#13 N-TRIACONTANE

R.T.: 17.508 min
Delta R.T.: -0.021 min
Response: 145301
Conc: 1.27 ug/ml

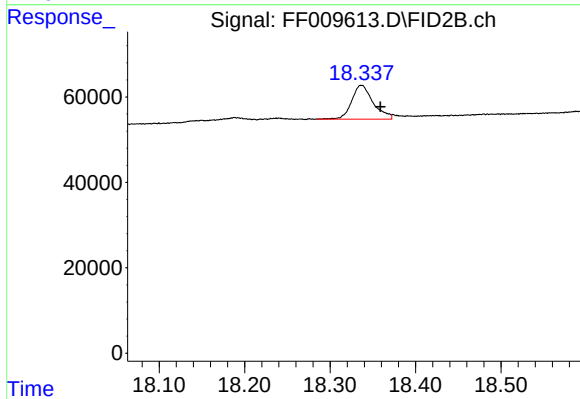

#14 N-DOTRIACONTANE


R.T.: 18.338 min
Delta R.T.: -0.021 min
Response: 138855
Conc: 1.27 ug/ml

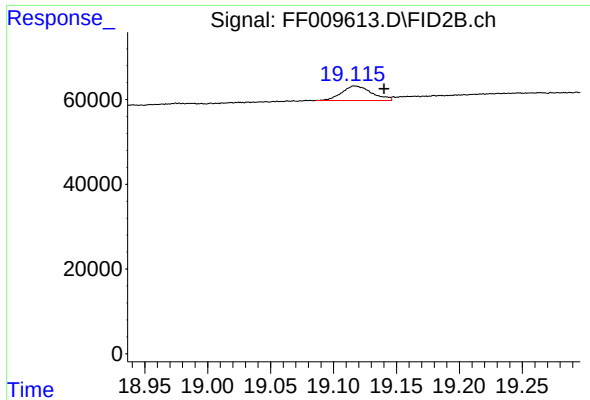

#15 N-TETRATRIACONTANE

R.T.: 19.116 min
Delta R.T.: -0.024 min
Response: 56880
Conc: 0.54 ug/ml

Instrument :
FID_F
ClientSampleId :

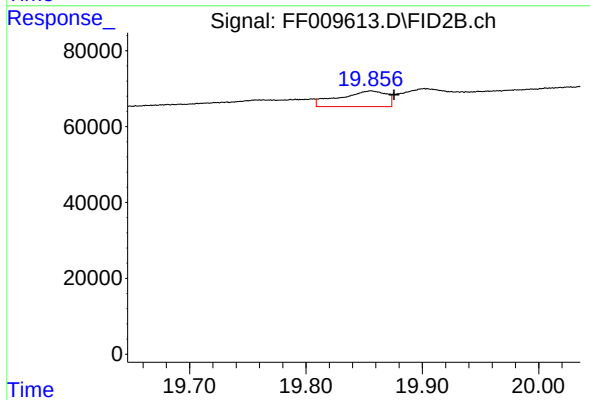

#16 N-HEXATRIACONTANE

R.T.: 19.856 min
Delta R.T.: -0.020 min
Response: 117135
Conc: 1.17 ug/ml