

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010322\
 Data File : FF009615.D
 Signal(s) : FID2B.ch
 Acq On : 03 Jan 2022 17:13
 Operator : AJ\MA
 Sample : M5330-02
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 04 00:13:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
 Quant Title :
 QLast Update : Thu Dec 16 03:33:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.458	2287873	19.750 ug/ml
Target Compounds			
4) N-TETRADECANE	8.093	59315	0.408 ug/ml
6) N-OCTADECANE	11.148f	42095	0.292 ug/ml
10) N-TETRACOSANE	14.660	54741	0.416 ug/ml
11) N-HEXACOSANE	15.678	104409	0.835 ug/ml
12) N-OCTACOSANE	16.623	126219	1.060 ug/ml
13) N-TRIACONTANE	17.506	171957	1.501 ug/ml
14) N-DOTRIACONTANE	18.335	161405	1.477 ug/ml
15) N-TETRATRIACONTANE	19.116	67462	0.637 ug/ml
16) N-HEXATRIACONTANE	19.853	136234	1.360 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010322\
Data File : FF009615.D
Signal(s) : FID2B.ch
Acq On : 03 Jan 2022 17:13
Operator : AJ\MA
Sample : M5330-02
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 04 00:13:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

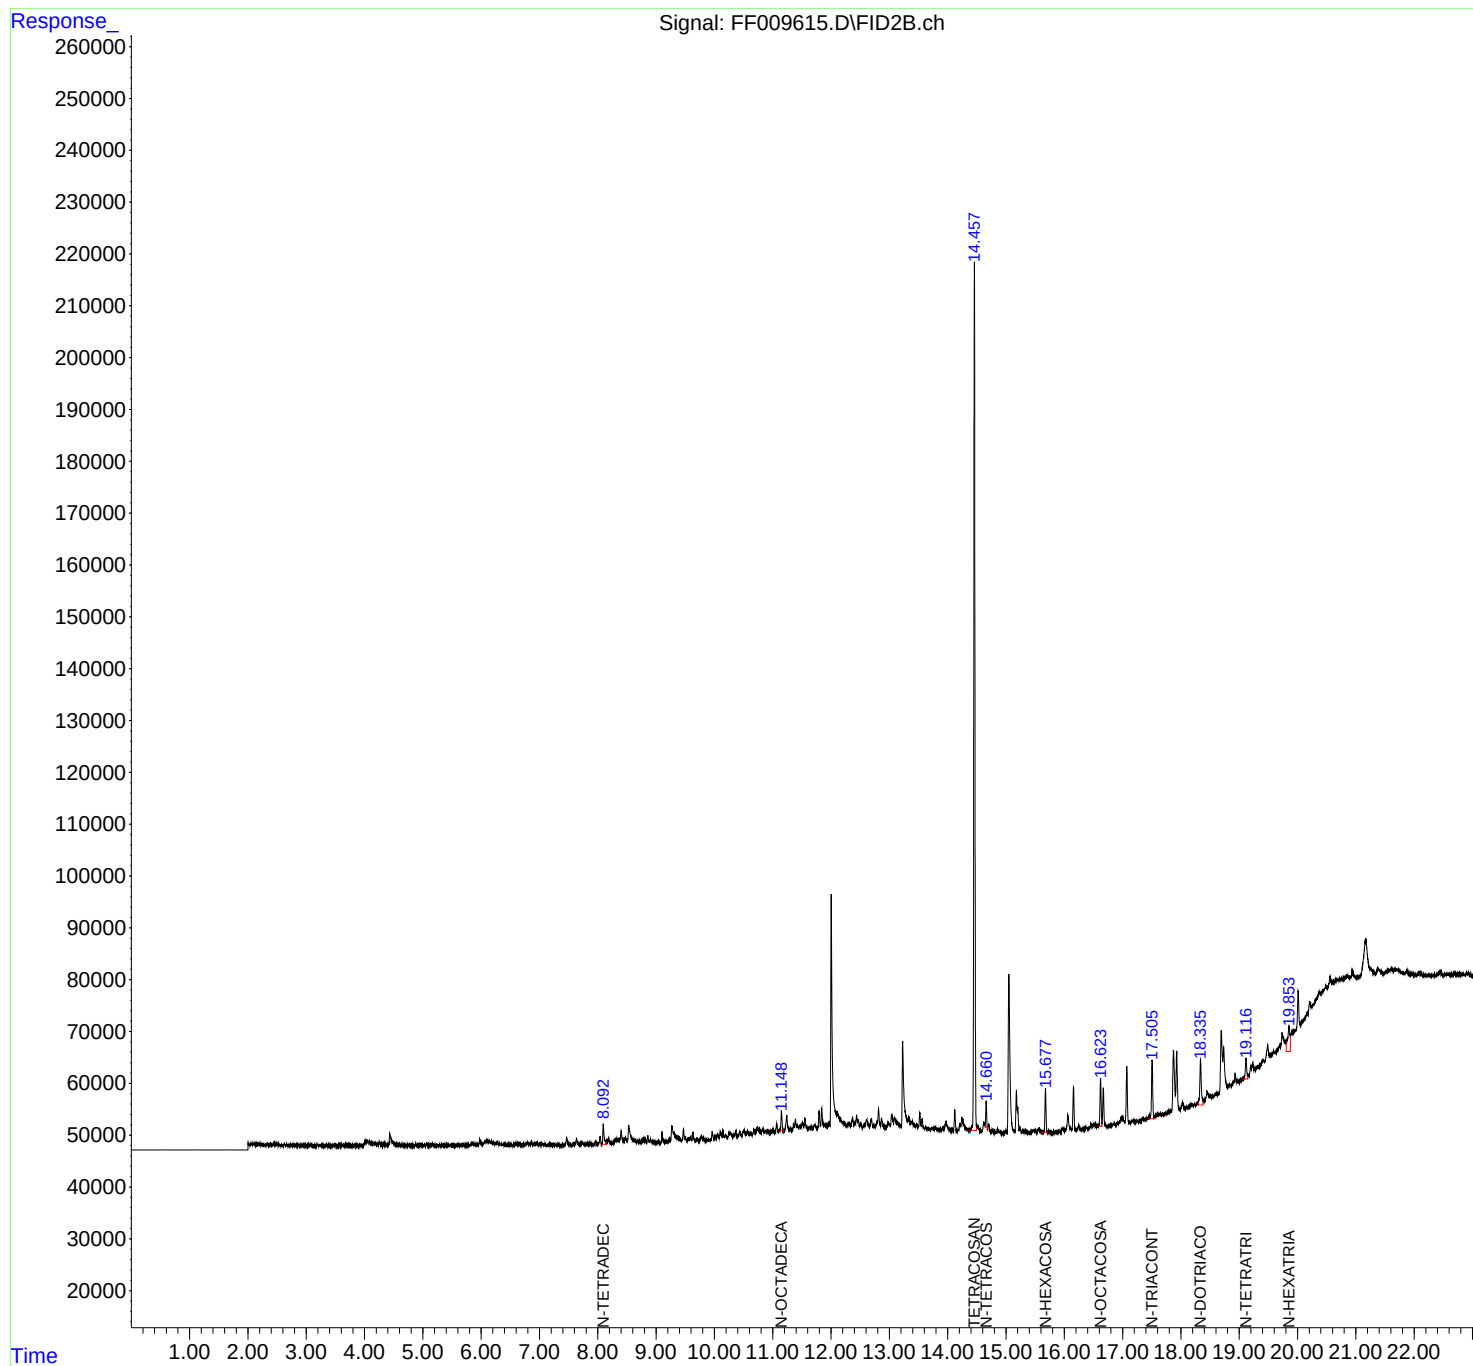


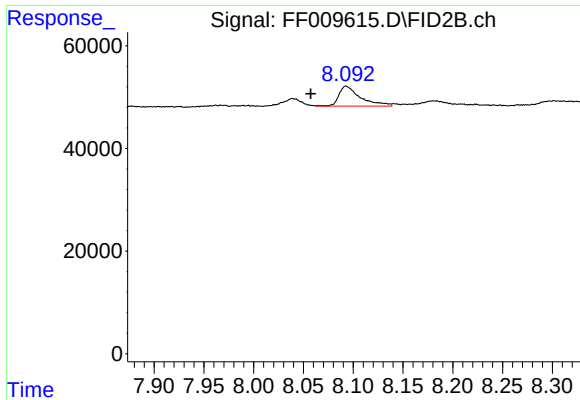

#4 N-TETRADECANE


R.T.: 8.093 min
Delta R.T.: 0.035 min
Response: 59315
Conc: 0.41 ug/ml

Instrument :
FID_F
ClientSampleId :

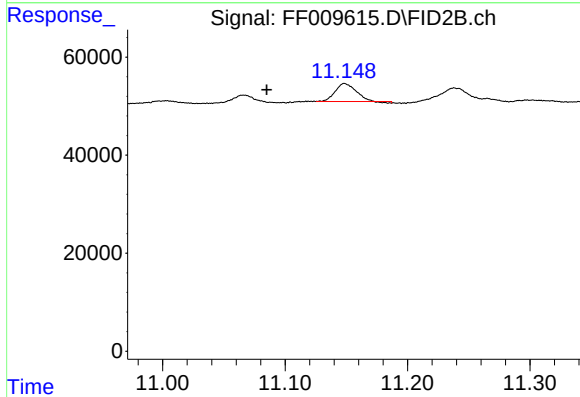


#6 N-OCTADECANE

R.T.: 11.148 min
Delta R.T.: 0.063 min
Response: 42095
Conc: 0.29 ug/ml

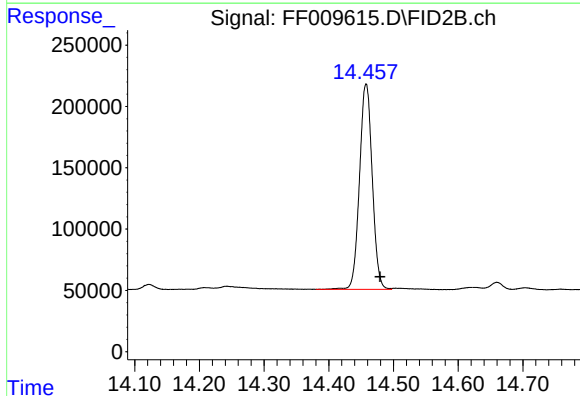


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.458 min
Delta R.T.: -0.021 min
Response: 2287873
Conc: 19.75 ug/ml

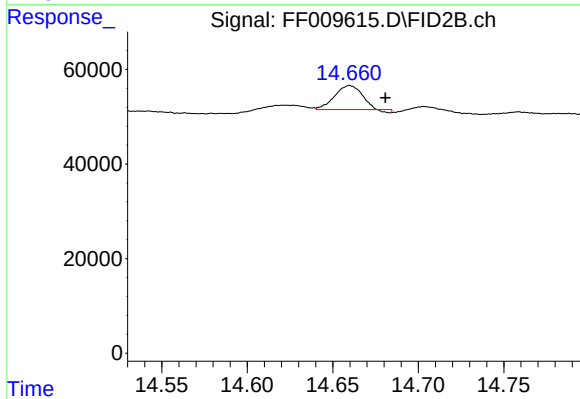

#10 N-TETRACOSANE


R.T.: 14.660 min
Delta R.T.: -0.021 min
Response: 54741
Conc: 0.42 ug/ml

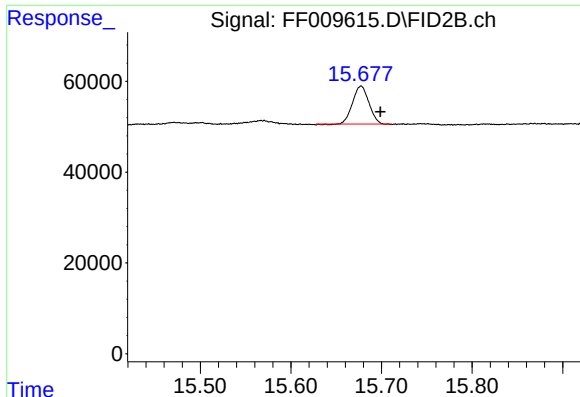

#11 N-HEXACOSANE


R.T.: 15.678 min
Delta R.T.: -0.021 min
Response: 104409
Conc: 0.84 ug/ml

Instrument :
FID_F
ClientSampleId :

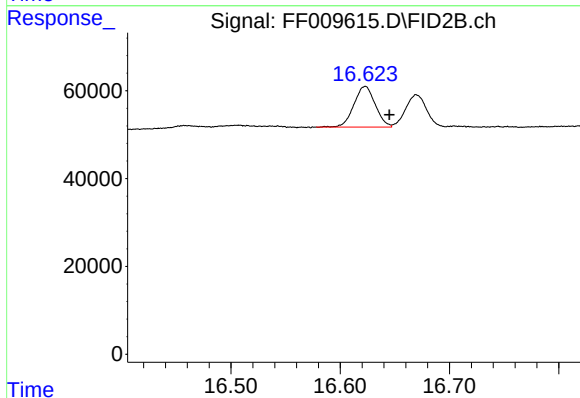


#12 N-OCTACOSANE

R.T.: 16.623 min
Delta R.T.: -0.022 min
Response: 126219
Conc: 1.06 ug/ml

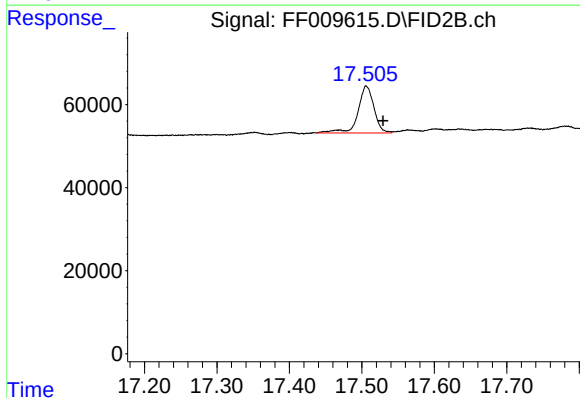


#13 N-TRIACONTANE

R.T.: 17.506 min
Delta R.T.: -0.024 min
Response: 171957
Conc: 1.50 ug/ml

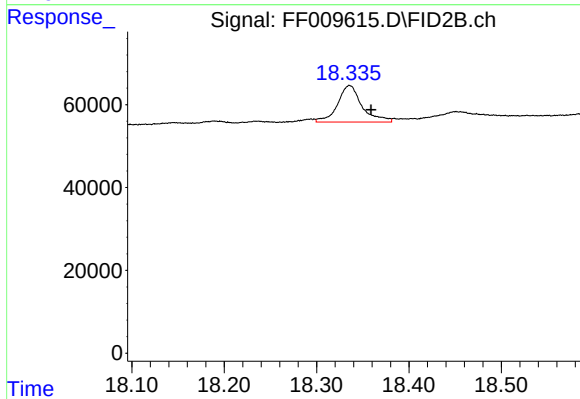

#14 N-DOTRIACONTANE


R.T.: 18.335 min
Delta R.T.: -0.024 min
Response: 161405
Conc: 1.48 ug/ml

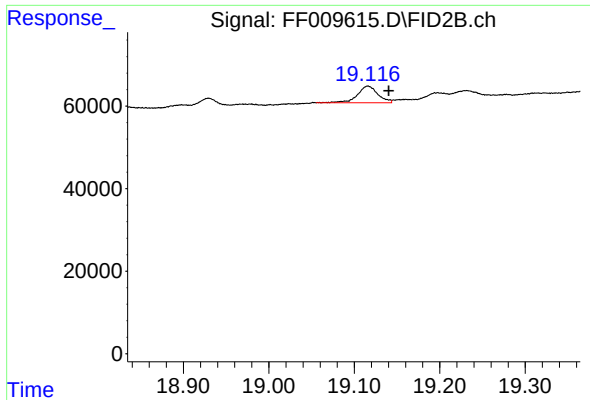

#15 N-TETRATRIACONTANE

R.T.: 19.116 min
Delta R.T.: -0.024 min
Response: 67462
Conc: 0.64 ug/ml

Instrument :
FID_F
ClientSampleId :

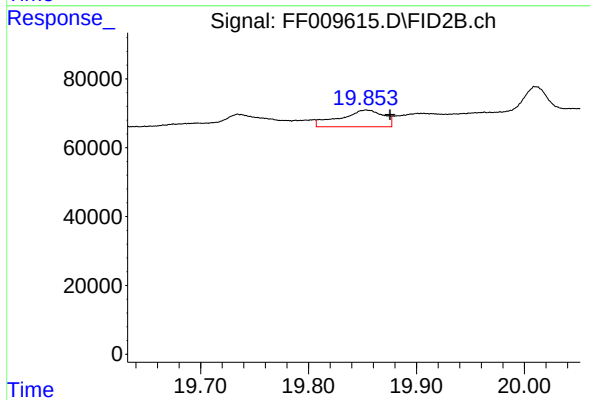

#16 N-HEXATRIACONTANE

R.T.: 19.853 min
Delta R.T.: -0.022 min
Response: 136234
Conc: 1.36 ug/ml