

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010322\
 Data File : FF009616.D
 Signal(s) : FID2B.ch
 Acq On : 03 Jan 2022 17:43
 Operator : AJ\MA
 Sample : M5330-03
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 04 00:14:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
 Quant Title :
 QLast Update : Thu Dec 16 03:33:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.457	2222878	19.189 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.622	77622	0.652 ug/ml
13) N-TRIACONTANE	17.505	134090	1.171 ug/ml
14) N-DOTRIACONTANE	18.336	179127	1.639 ug/ml
15) N-TETRATRIACONTANE	19.116	78748	0.743 ug/ml
16) N-HEXATRIACONTANE	19.853	122481	1.223 ug/ml
18) N-TETRACONTANE	21.420	350187	3.467 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010322\
Data File : FF009616.D
Signal(s) : FID2B.ch
Acq On : 03 Jan 2022 17:43
Operator : AJ\MA
Sample : M5330-03
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 04 00:14:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

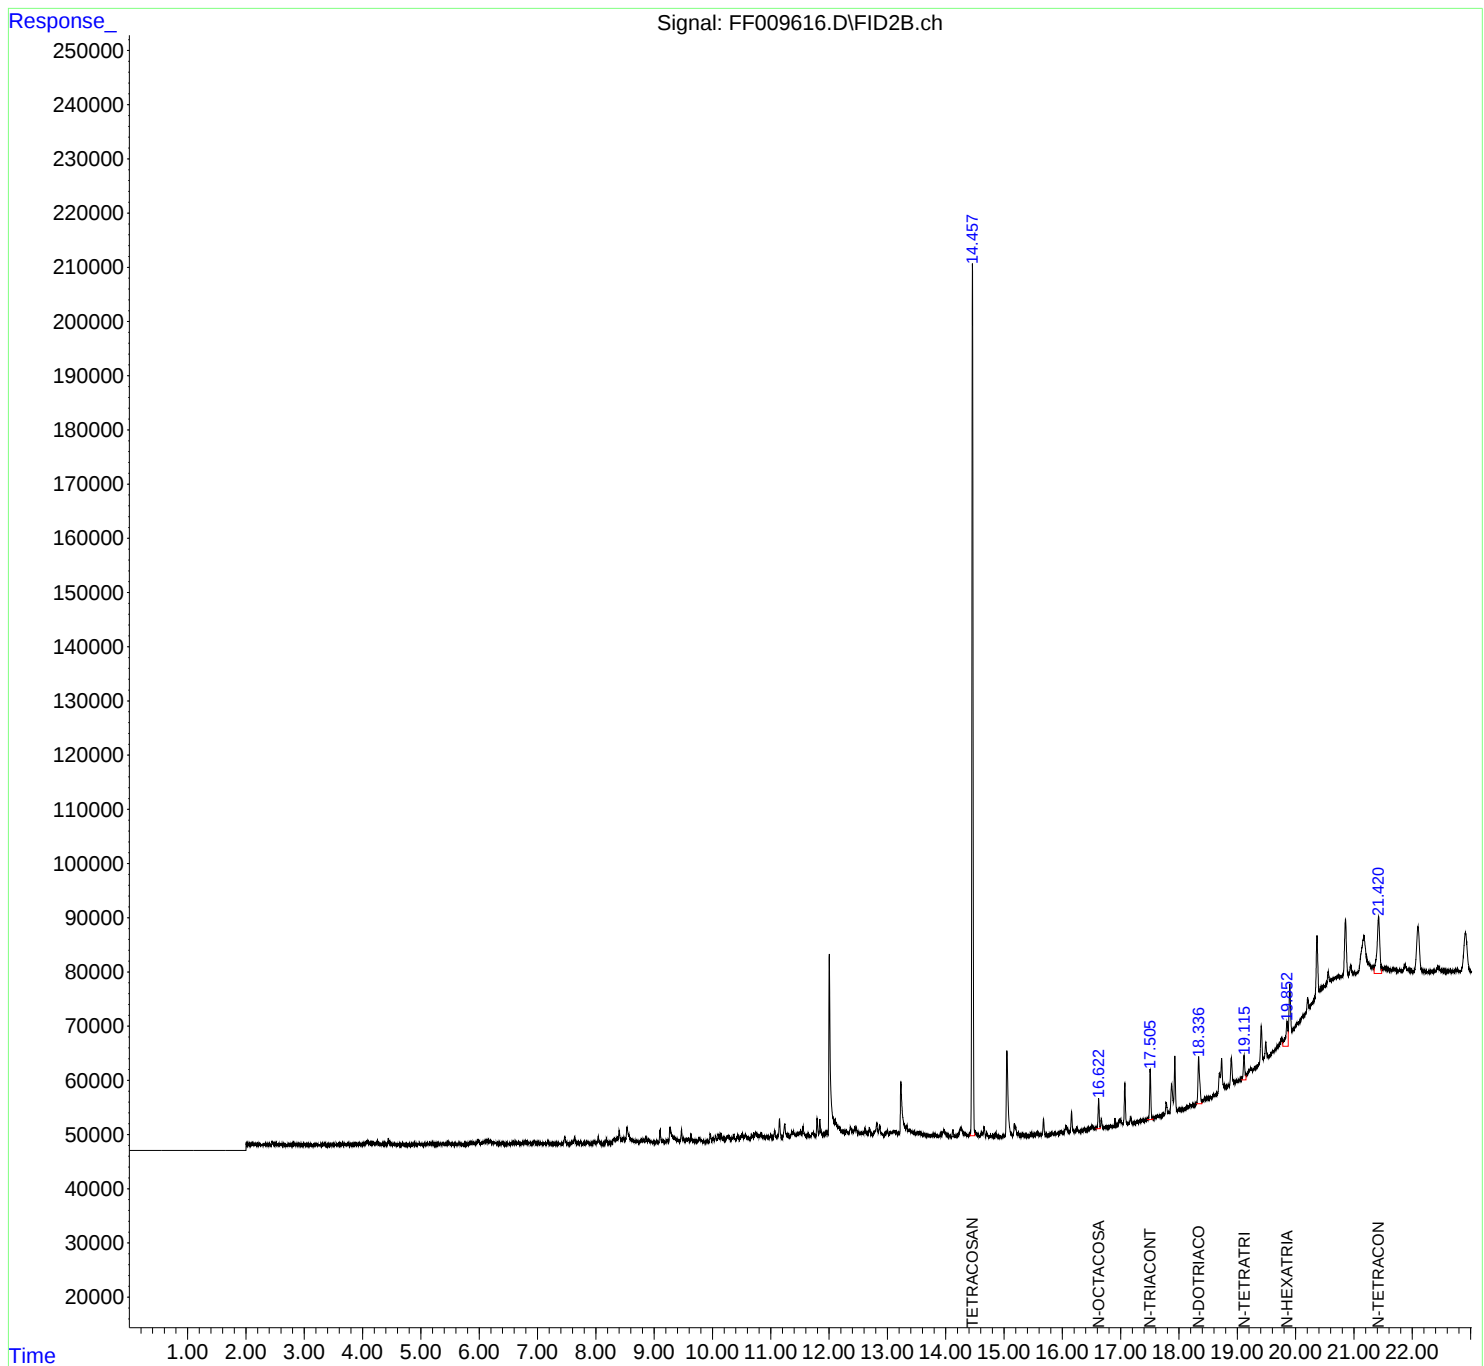


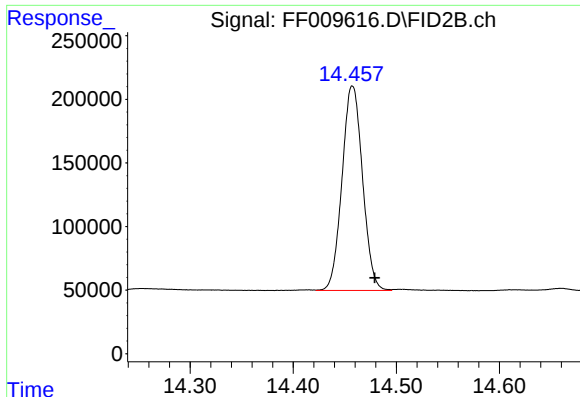

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.457 min
Delta R.T.: -0.022 min
Response: 2222878
Conc: 19.19 ug/ml

Instrument :
FID_F
ClientSampleId :

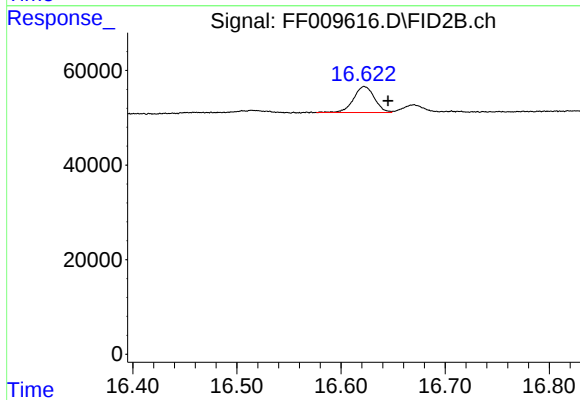


#12 N-OCTACOSANE

R.T.: 16.622 min
Delta R.T.: -0.023 min
Response: 77622
Conc: 0.65 ug/ml

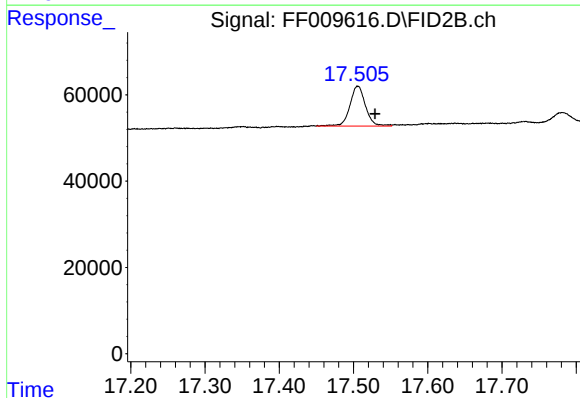


#13 N-TRIACONTANE

R.T.: 17.505 min
Delta R.T.: -0.024 min
Response: 134090
Conc: 1.17 ug/ml

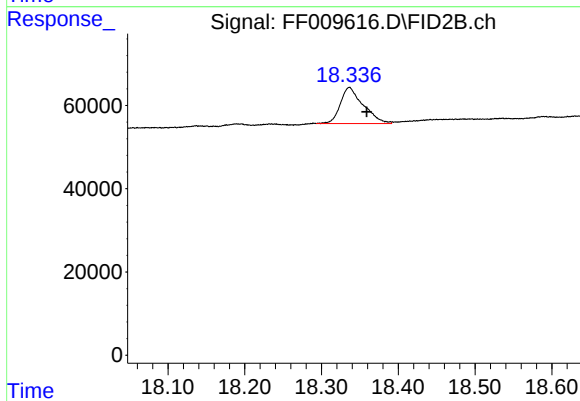

#14 N-DOTRIACONTANE


R.T.: 18.336 min
Delta R.T.: -0.022 min
Response: 179127
Conc: 1.64 ug/ml

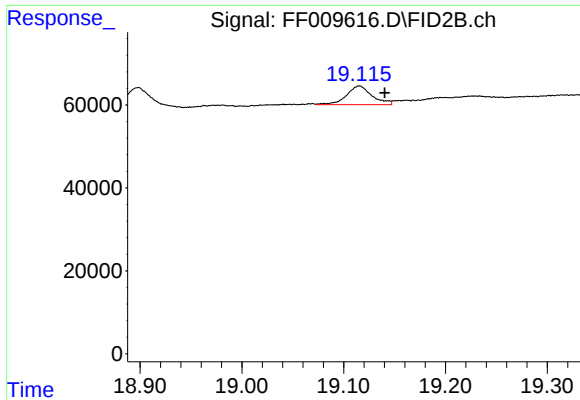

#15 N-TETRATRIACONTANE


R.T.: 19.116 min
Delta R.T.: -0.025 min
Response: 78748
Conc: 0.74 ug/ml

Instrument :
FID_F
ClientSampleId :

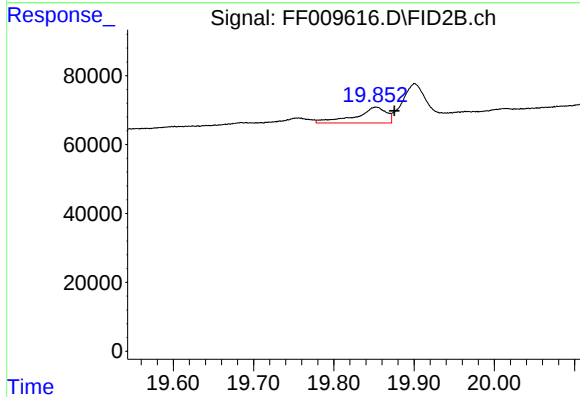

#16 N-HEXATRIACONTANE

R.T.: 19.853 min
Delta R.T.: -0.023 min
Response: 122481
Conc: 1.22 ug/ml

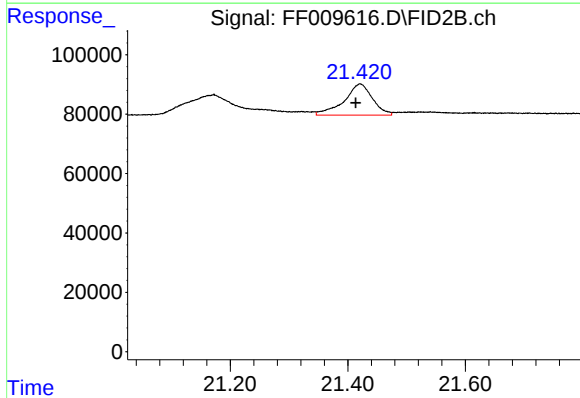

#18 N-TETRACONTANE

R.T.: 21.420 min
Delta R.T.: 0.007 min
Response: 350187
Conc: 3.47 ug/ml