

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010322\
 Data File : FF009617.D
 Signal(s) : FID2B.ch
 Acq On : 03 Jan 2022 18:14
 Operator : AJ\MA
 Sample : M5330-04
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 04 00:14:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
 Quant Title :
 QLast Update : Thu Dec 16 03:33:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.459	2885884	24.913 ug/ml
Target Compounds			
6) N-OCTADECANE	11.149f	37131	0.257 ug/ml
10) N-TETRACOSANE	14.660	65782	0.500 ug/ml
11) N-HEXACOSANE	15.678	104907	0.839 ug/ml
12) N-OCTACOSANE	16.622	116254	0.976 ug/ml
13) N-TRIACONTANE	17.507	155076	1.354 ug/ml
14) N-DOTRIACONTANE	18.335	164581	1.506 ug/ml
15) N-TETRATRIACONTANE	19.116	82743	0.781 ug/ml
16) N-HEXATRIACONTANE	19.853	133394	1.332 ug/ml
17) N-OCTATRIACONTANE	20.559	463846	4.724 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010322\
Data File : FF009617.D
Signal(s) : FID2B.ch
Acq On : 03 Jan 2022 18:14
Operator : AJ\MA
Sample : M5330-04
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 04 00:14:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

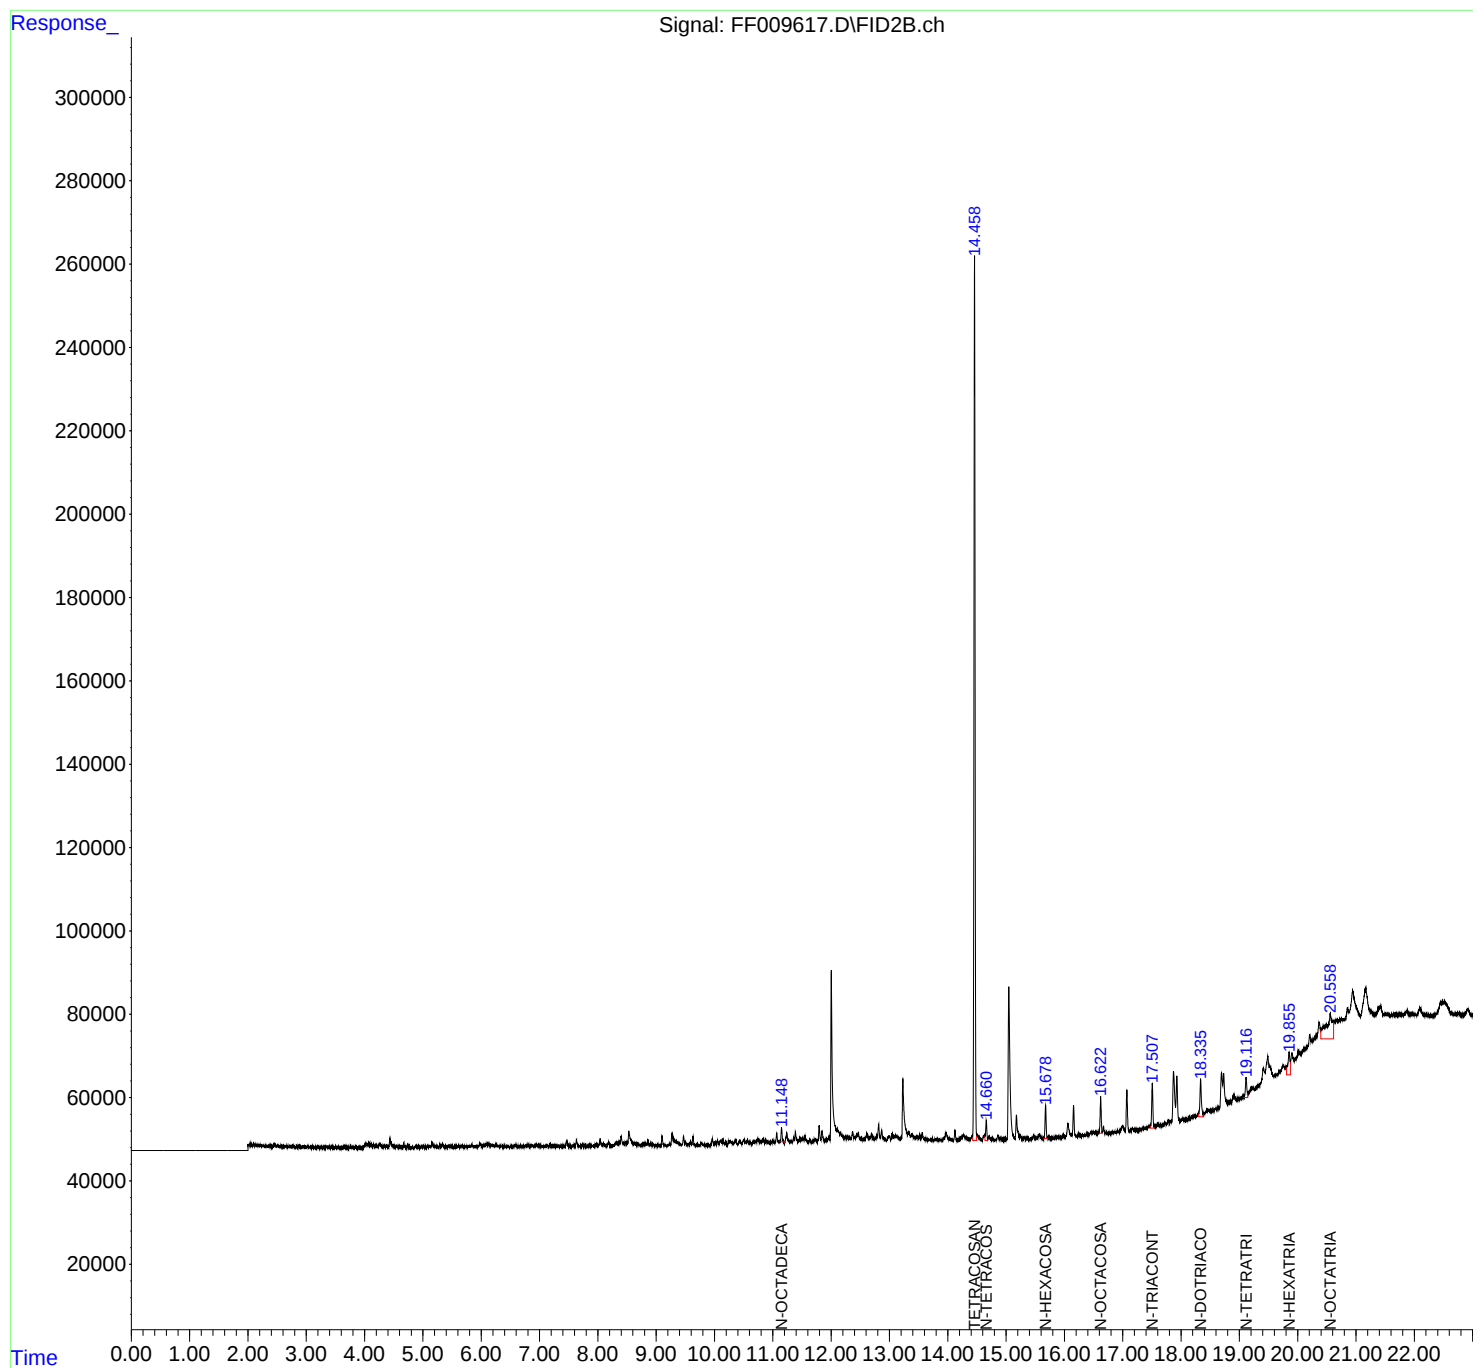


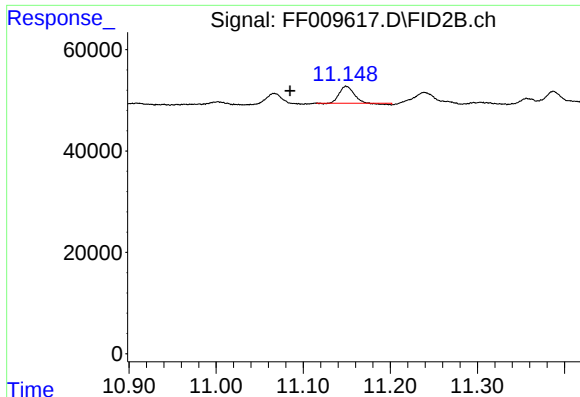

#6 N-OCTADECANE


R.T.: 11.149 min
Delta R.T.: 0.064 min
Response: 37131
Conc: 0.26 ug/ml

Instrument :
FID_F
ClientSampleId :

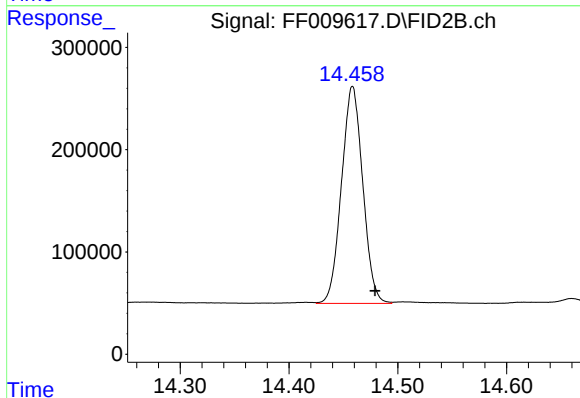


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.459 min
Delta R.T.: -0.021 min
Response: 2885884
Conc: 24.91 ug/ml

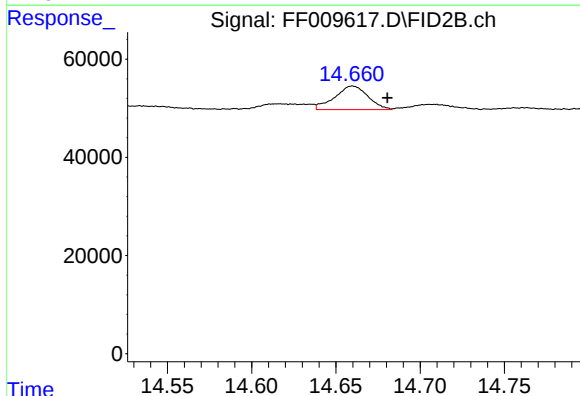


#10 N-TETRACOSANE

R.T.: 14.660 min
Delta R.T.: -0.021 min
Response: 65782
Conc: 0.50 ug/ml

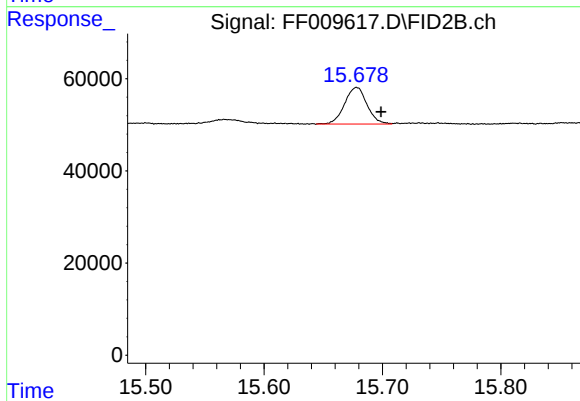

#11 N-HEXACOSANE


R.T.: 15.678 min
Delta R.T.: -0.021 min
Response: 104907
Conc: 0.84 ug/ml

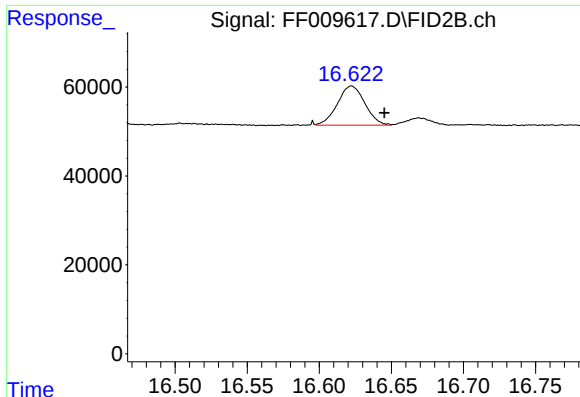

#12 N-OCTACOSANE


R.T.: 16.622 min
Delta R.T.: -0.023 min
Response: 116254
Conc: 0.98 ug/ml

Instrument :
FID_F
ClientSampleId :

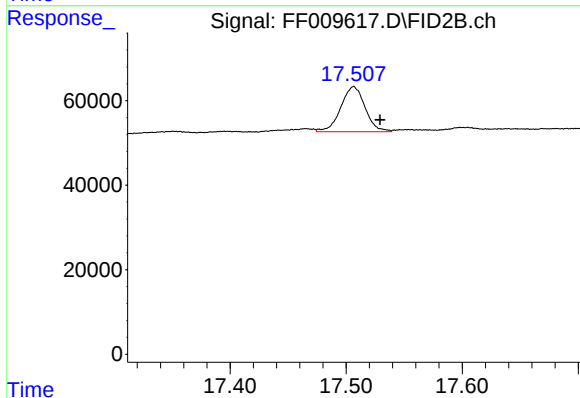


#13 N-TRIACONTANE

R.T.: 17.507 min
Delta R.T.: -0.022 min
Response: 155076
Conc: 1.35 ug/ml

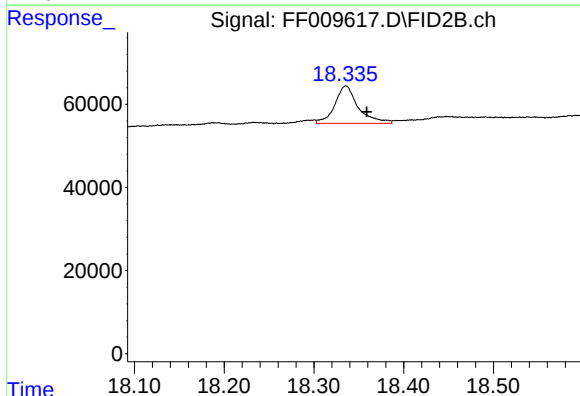


#14 N-DOTRIACONTANE

R.T.: 18.335 min
Delta R.T.: -0.024 min
Response: 164581
Conc: 1.51 ug/ml

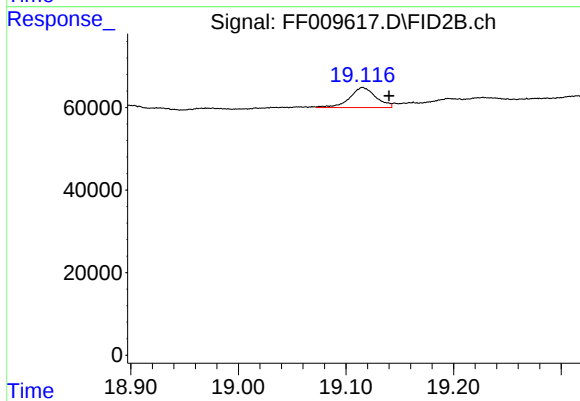

#15 N-TETRATRIACONTANE


R.T.: 19.116 min
Delta R.T.: -0.024 min
Response: 82743
Conc: 0.78 ug/ml

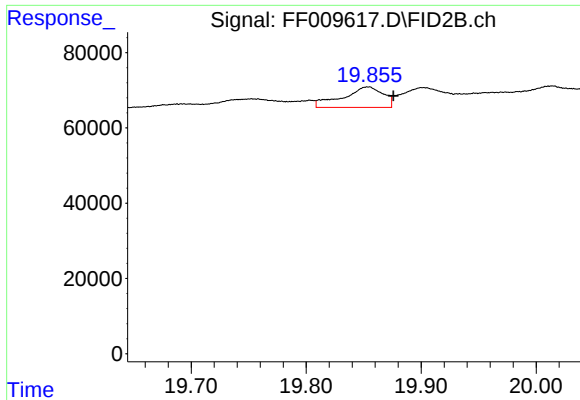

#16 N-HEXATRIACONTANE

R.T.: 19.853 min
Delta R.T.: -0.022 min
Response: 133394
Conc: 1.33 ug/ml

Instrument :
FID_F
ClientSampleId :

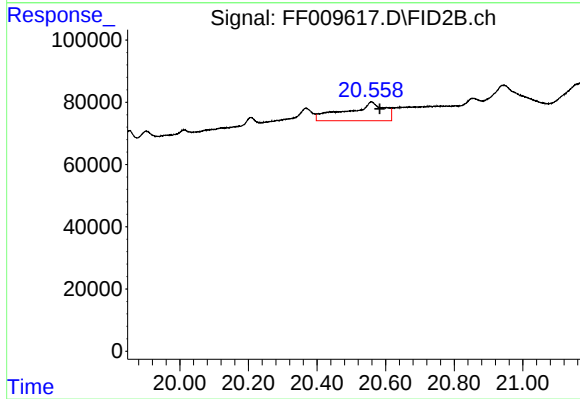

#17 N-OCTATRIACONTANE

R.T.: 20.559 min
Delta R.T.: -0.024 min
Response: 463846
Conc: 4.72 ug/ml