

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010322\
 Data File : FF009626.D
 Signal(s) : FID2B.ch
 Acq On : 03 Jan 2022 22:47
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 04 00:17:09 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
 Quant Title :
 QLast Update : Thu Dec 16 03:33:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.463	1983207	17.120 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.627	151799	1.275 ug/ml
13) N-TRIACONTANE	17.512	249335	2.177 ug/ml
14) N-DOTRIACONTANE	18.355	1073854	9.826 ug/ml
15) N-TETRATRIACONTANE	19.137	451300	4.260 ug/ml
16) N-HEXATRIACONTANE	19.877	3343431	33.380 ug/ml
17) N-OCTATRIACONTANE	20.554	2667063	27.161 ug/ml
18) N-TETRACONTANE	21.406	573696	5.680 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010322\
Data File : FF009626.D
Signal(s) : FID2B.ch
Acq On : 03 Jan 2022 22:47
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 04 00:17:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

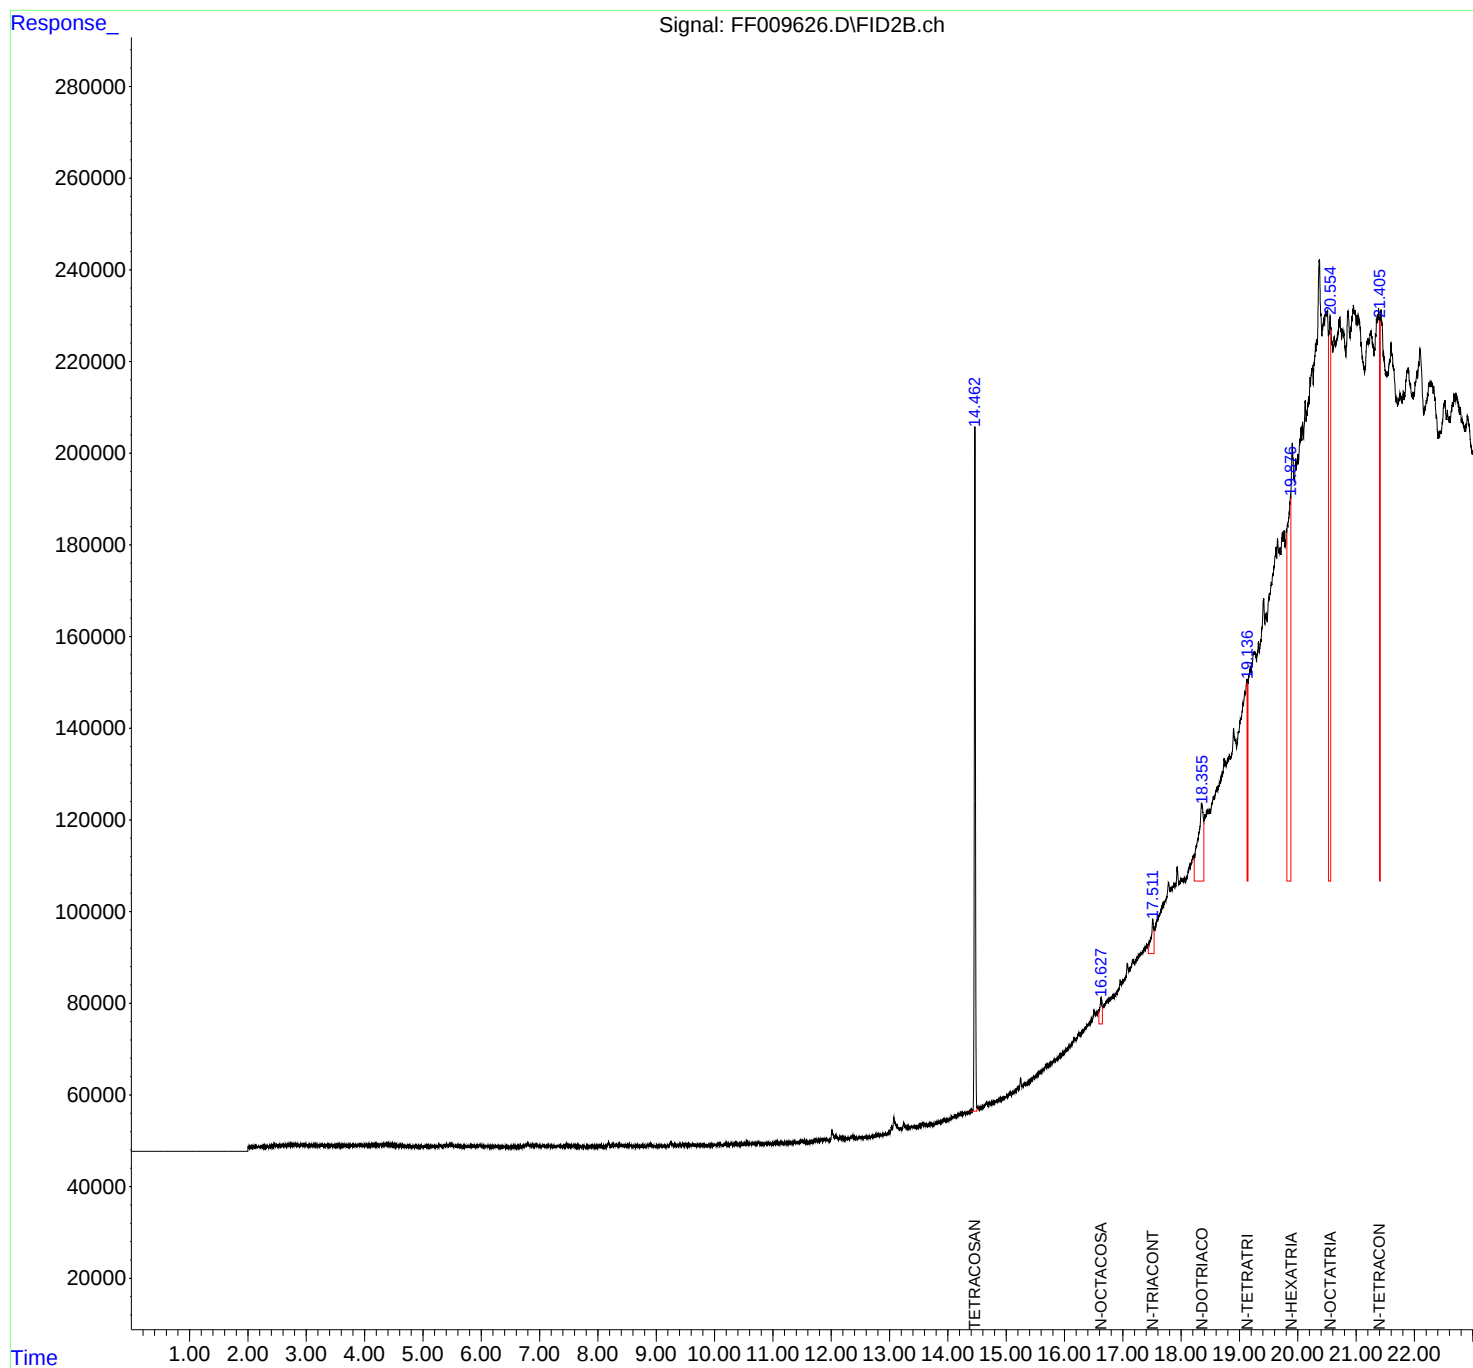


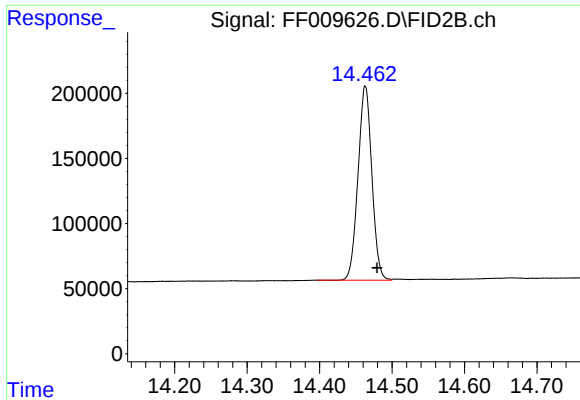

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.463 min
Delta R.T.: -0.016 min
Response: 1983207
Conc: 17.12 ug/ml

Instrument :
FID_F
ClientSampleId :

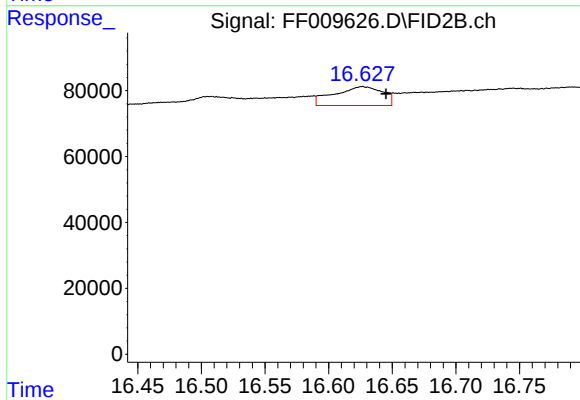


#12 N-OCTACOSANE

R.T.: 16.627 min
Delta R.T.: -0.018 min
Response: 151799
Conc: 1.27 ug/ml

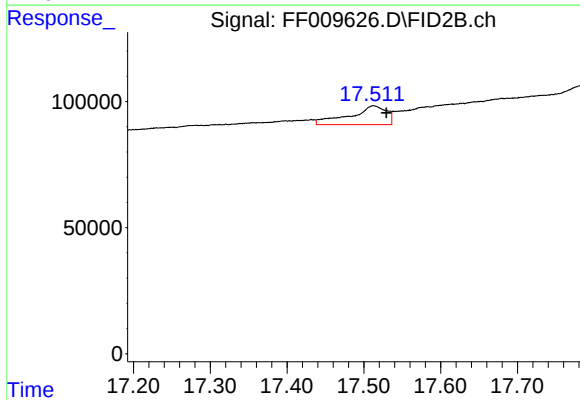


#13 N-TRIACONTANE

R.T.: 17.512 min
Delta R.T.: -0.017 min
Response: 249335
Conc: 2.18 ug/ml

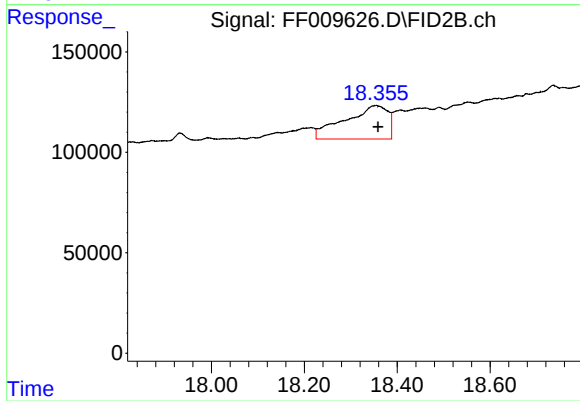

#14 N-DOTRIACONTANE


R.T.: 18.355 min
Delta R.T.: -0.004 min
Response: 1073854
Conc: 9.83 ug/ml

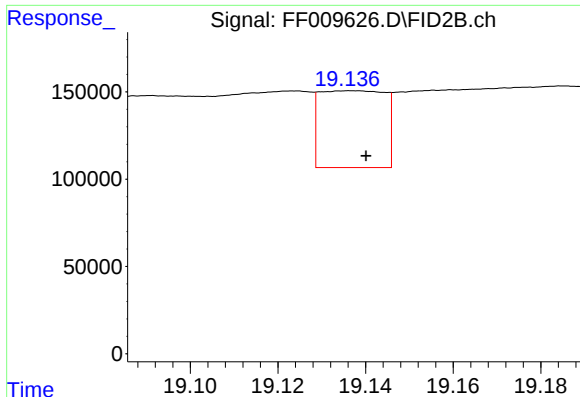

#15 N-TETRATRIACONTANE


R.T.: 19.137 min
Delta R.T.: -0.003 min
Response: 451300
Conc: 4.26 ug/ml

Instrument :
FID_F
ClientSampleId :

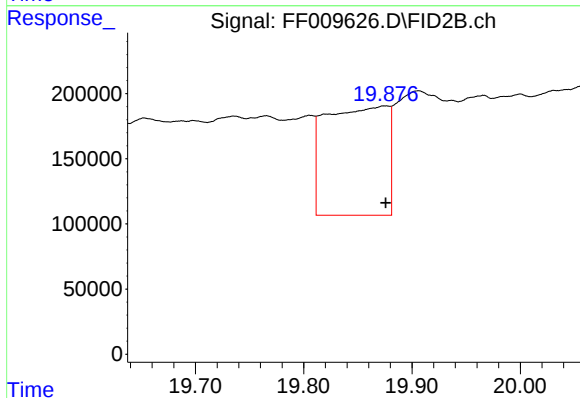


#16 N-HEXATRIACONTANE

R.T.: 19.877 min
Delta R.T.: 0.000 min
Response: 3343431
Conc: 33.38 ug/ml

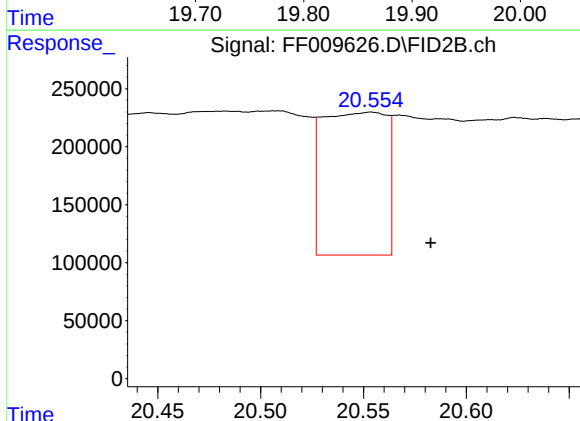

#17 N-OCTATRIACONTANE

R.T.: 20.554 min
Delta R.T.: -0.029 min
Response: 2667063
Conc: 27.16 ug/ml

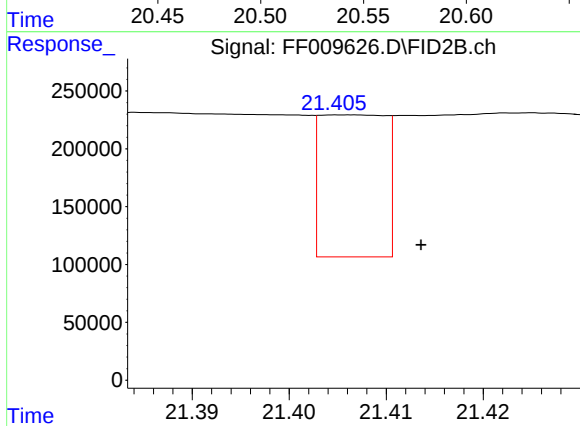

#18 N-TETRACONTANE

R.T.: 21.406 min
Delta R.T.: -0.007 min
Response: 573696
Conc: 5.68 ug/ml