

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF010322\  
 Data File : FF009620.D  
 Signal(s) : FID2B.ch  
 Acq On : 03 Jan 2022 19:45  
 Operator : AJ\MA  
 Sample : M5256-01  
 Misc :  
 ALS Vial : 62 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :  
 BU-03-122921

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 01/04/2022  
 Supervised By :Ankita Jodhani 01/04/2022

Integration File: Sample.e  
 Quant Time: Jan 04 00:15:17 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF121521.M  
 Quant Title :  
 QLast Update : Thu Dec 16 03:33:07 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units    |
|-------------------------------|--------|----------|---------------|
| -----                         |        |          |               |
| System Monitoring Compounds   |        |          |               |
| 9) S TETRACOSANE-d50 (SURR... | 14.460 | 2331492  | 20.127 ug/mlm |

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF010322\  
Data File : FF009620.D  
Signal(s) : FID2B.ch  
Acq On : 03 Jan 2022 19:45  
Operator : AJ\MA  
Sample : M5256-01  
Misc :  
ALS Vial : 62 Sample Multiplier: 1


Instrument :  
FID\_F  
ClientSampleId :  
BU-03-122921


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 01/04/2022  
Supervised By :Ankita Jodhani 01/04/2022

Integration File: Sample.e  
Quant Time: Jan 04 00:15:17 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF121521.M  
Quant Title :  
QLast Update : Thu Dec 16 03:33:07 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

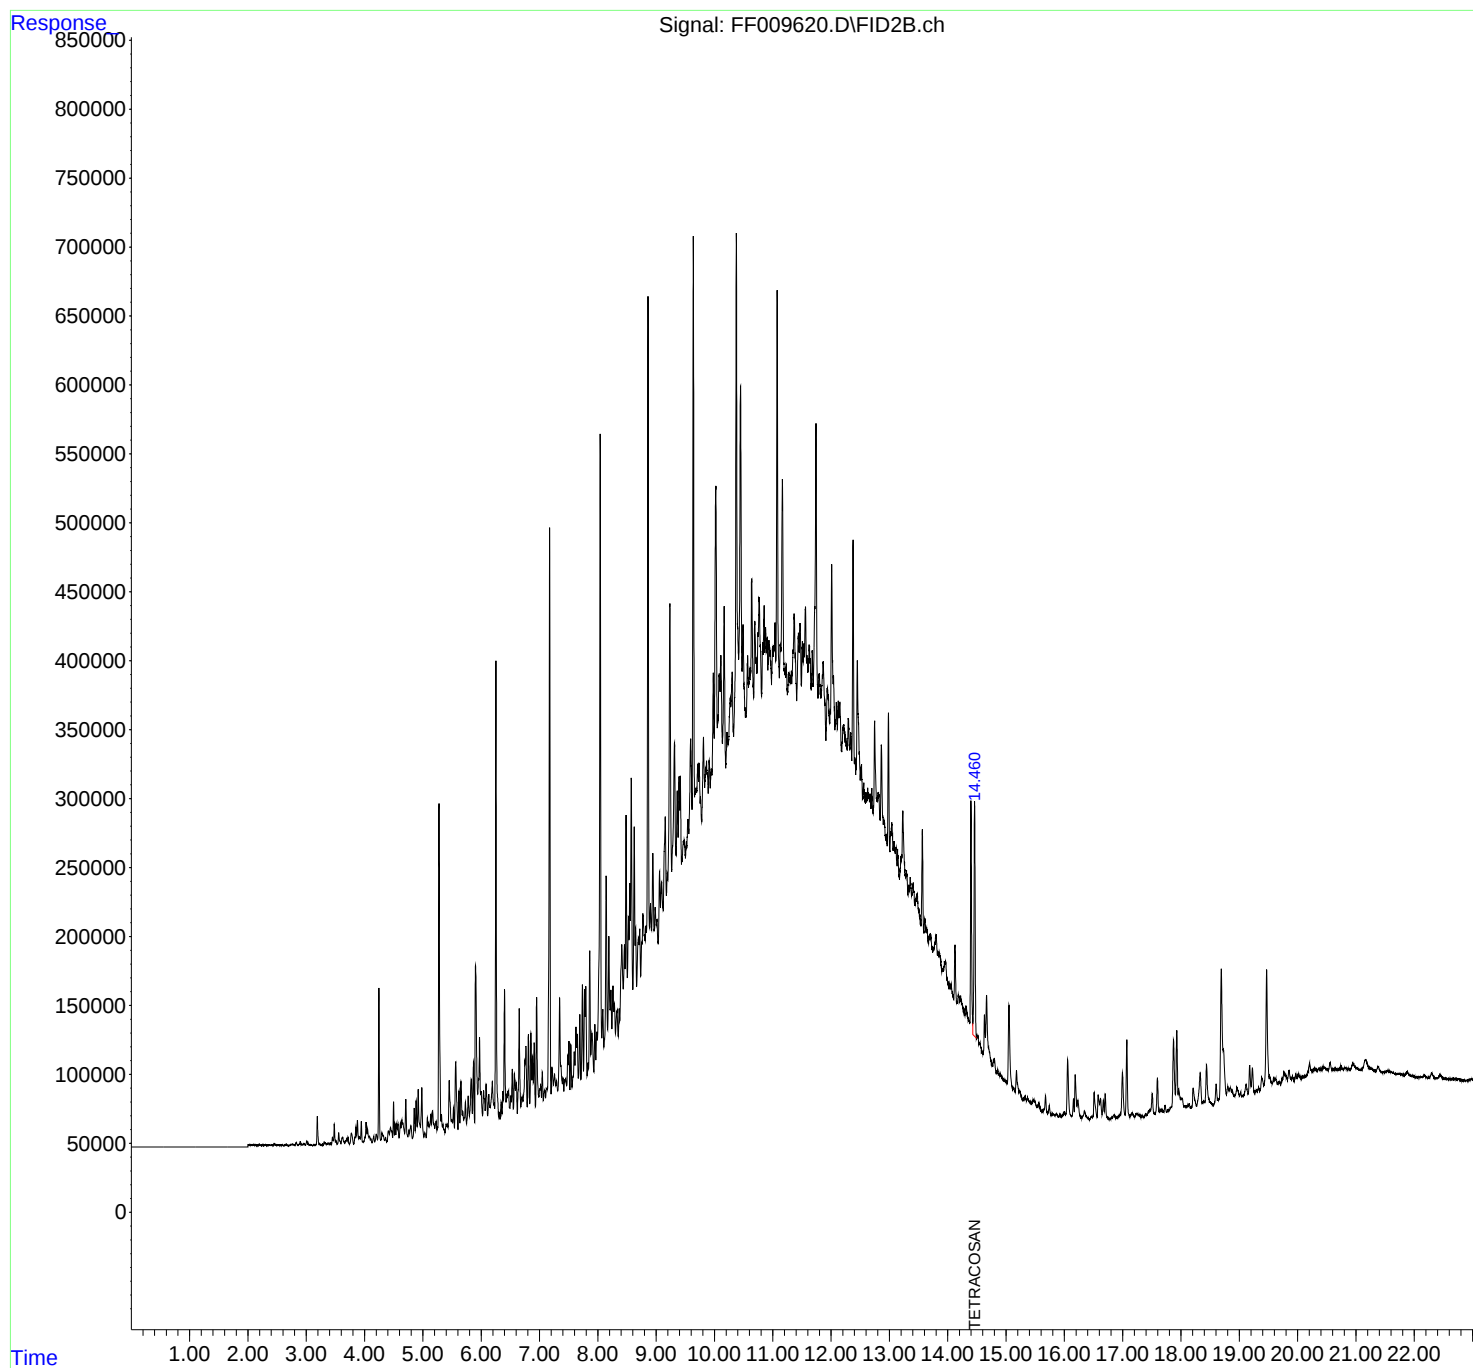

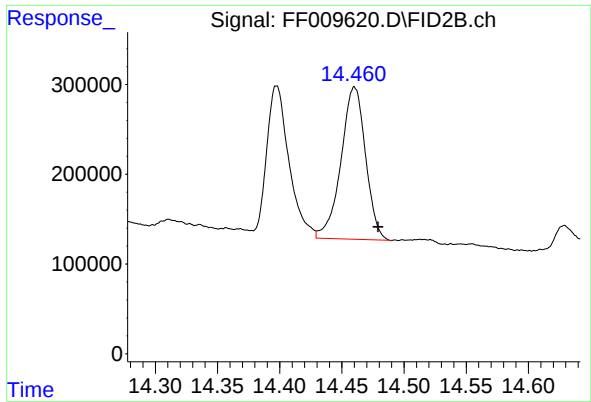

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.460 min  
Delta R.T.: -0.020 min  
Response: 2331492  
Conc: 20.13 ug/ml

Instrument :  
FID\_F  
ClientSampleId :  
BU-03-122921

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 01/04/2022  
Supervised By :Ankita Jodhani 01/04/2022