

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010322\
 Data File : FF009623.D
 Signal(s) : FID2B.ch
 Acq On : 03 Jan 2022 21:16
 Operator : AJ\MA
 Sample : M5330-01 10X
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 DB-24-(10-15)-12-29-21

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/04/2022
 Supervised By :Ankita Jodhani 01/04/2022

Integration File: Sample.e
 Quant Time: Jan 04 00:16:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
 Quant Title :
 QLast Update : Thu Dec 16 03:33:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.460	292242	2.523 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010322\
Data File : FF009623.D
Signal(s) : FID2B.ch
Acq On : 03 Jan 2022 21:16
Operator : AJ\MA
Sample : M5330-01 10X
Misc :
ALS Vial : 65 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
DB-24-(10-15)-12-29-21


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/04/2022
Supervised By :Ankita Jodhani 01/04/2022

Integration File: Sample.e
Quant Time: Jan 04 00:16:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

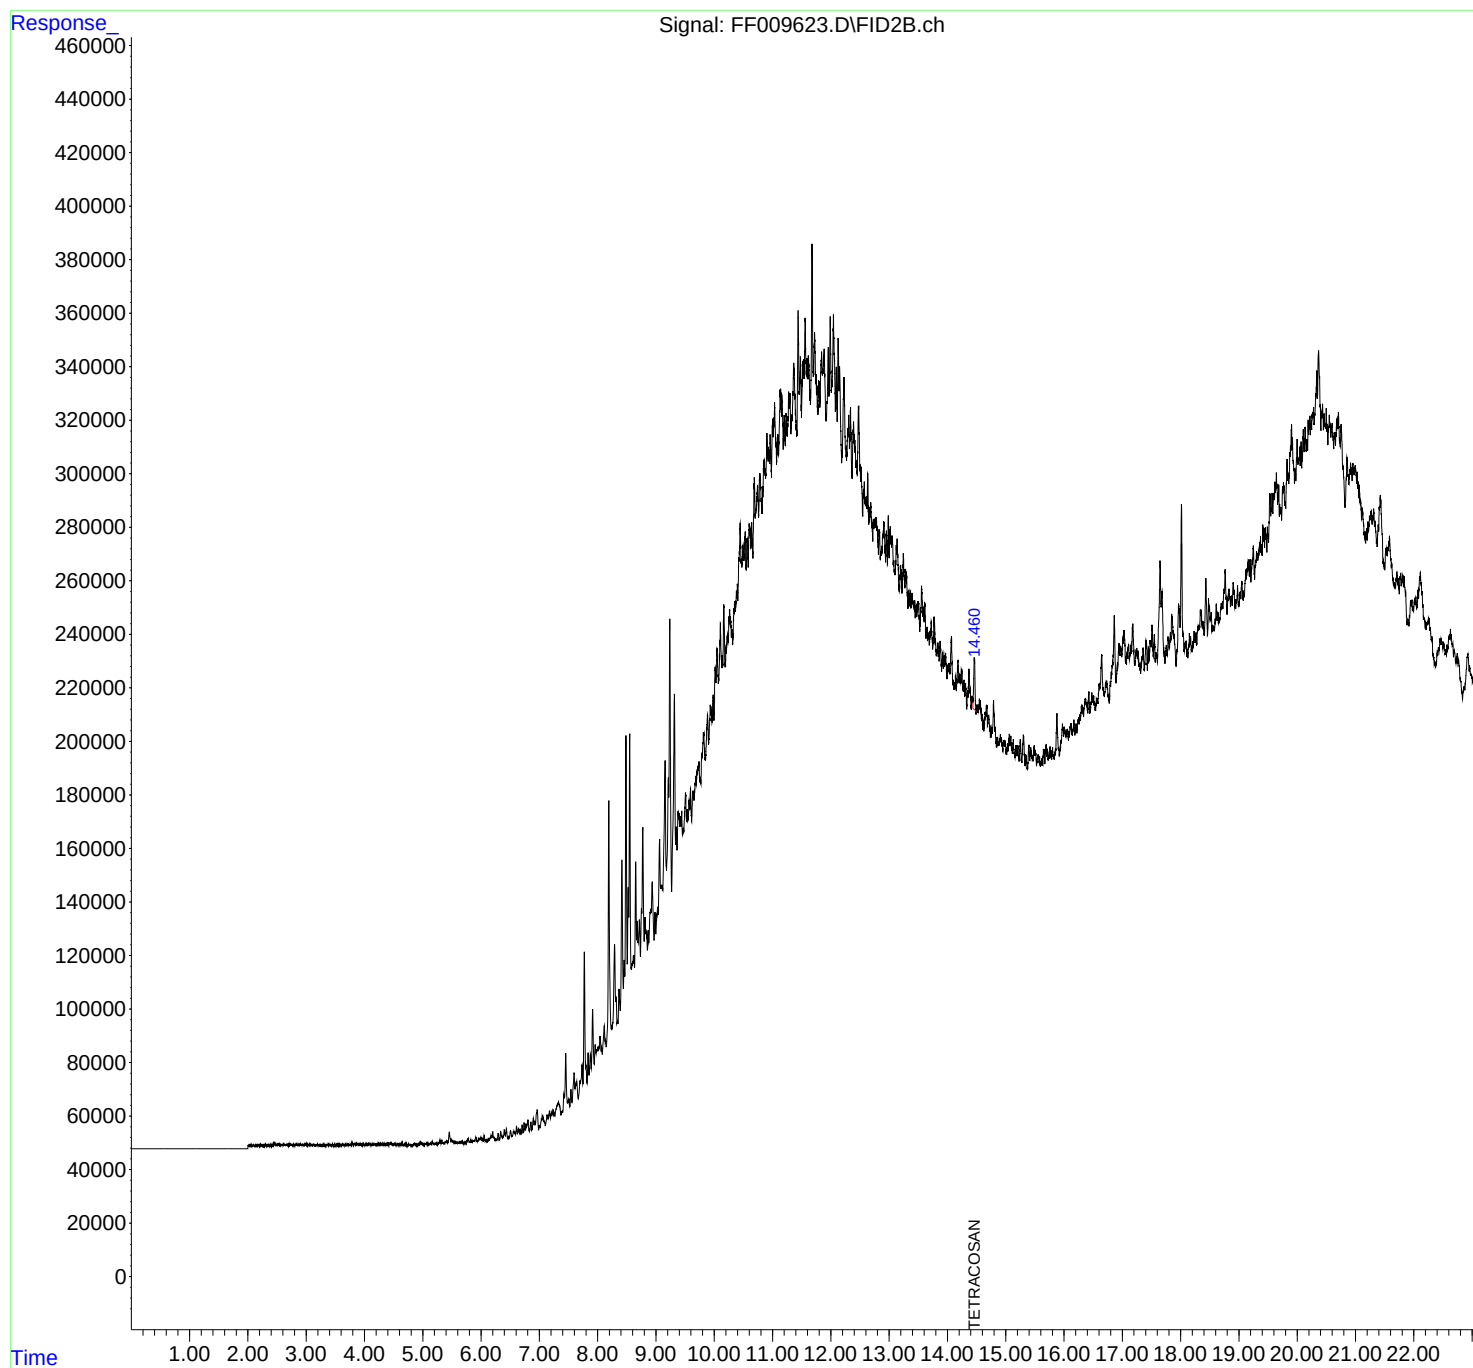

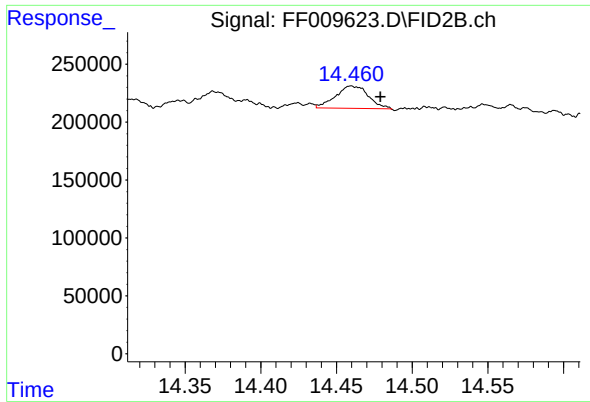

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.460 min
Delta R.T.: -0.019 min
Response: 292242
Conc: 2.52 ug/ml

Instrument :
FID_F
ClientSampleId :
DB-24-(10-15)-12-29-21

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/04/2022
Supervised By :Ankita Jodhani 01/04/2022