

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010419\
 Data File : FF003141.D
 Signal(s) : FID2B.ch
 Acq On : 04 Jan 2019 14:18
 Operator : AJ\SJ
 Sample : 50 TRPH STD
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 50 TRPH STD

Integration File: autoint1.e
 Quant Time: Jan 04 14:46:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Fri Jan 04 14:45:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.630	6647268	50.000 ug/ml
Target Compounds			
1) N-OCTANE	2.260	7442735	50.000 ug/ml
2) N-DECANE	4.358	7508370	50.000 ug/ml
3) N-DODECANE	6.380	7566868	50.000 ug/ml
4) N-TETRADECANE	8.174	7622601	50.000 ug/ml
5) N-HEXADECANE	9.774	7665151	50.000 ug/ml
6) N-OCTADECANE	11.216	7690430	50.000 ug/ml
7) N-EICOSANE	12.528	7613637	50.000 ug/ml
8) N-DOCOSANE	13.729	7537919	50.000 ug/ml
10) N-TETRACOSANE	14.835	7450165	50.000 ug/ml
11) N-HEXACOSANE	15.857	7356470	50.000 ug/ml
12) N-OCTACOSANE	16.812	7276904	50.000 ug/ml
13) N-TRIACONTANE	17.701	7140943	50.000 ug/ml
14) N-DOTRIACONTANE	18.535	6661807	50.000 ug/ml
15) N-TETRATRIACONTANE	19.321	6197386	50.000 ug/ml
16) N-HEXATRIACONTANE	20.066	5640198	50.000 ug/ml
17) N-OCTATRIACONTANE	20.804	5010160	50.000 ug/ml
18) N-TETRACONTANE	21.701	5040606	50.000 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010419\
Data File : FF003141.D
Signal(s) : FID2B.ch
Acq On : 04 Jan 2019 14:18
Operator : AJ\SJ
Sample : 50 TRPH STD
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
50 TRPH STD

Integration File: autoint1.e
Quant Time: Jan 04 14:46:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Fri Jan 04 14:45:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

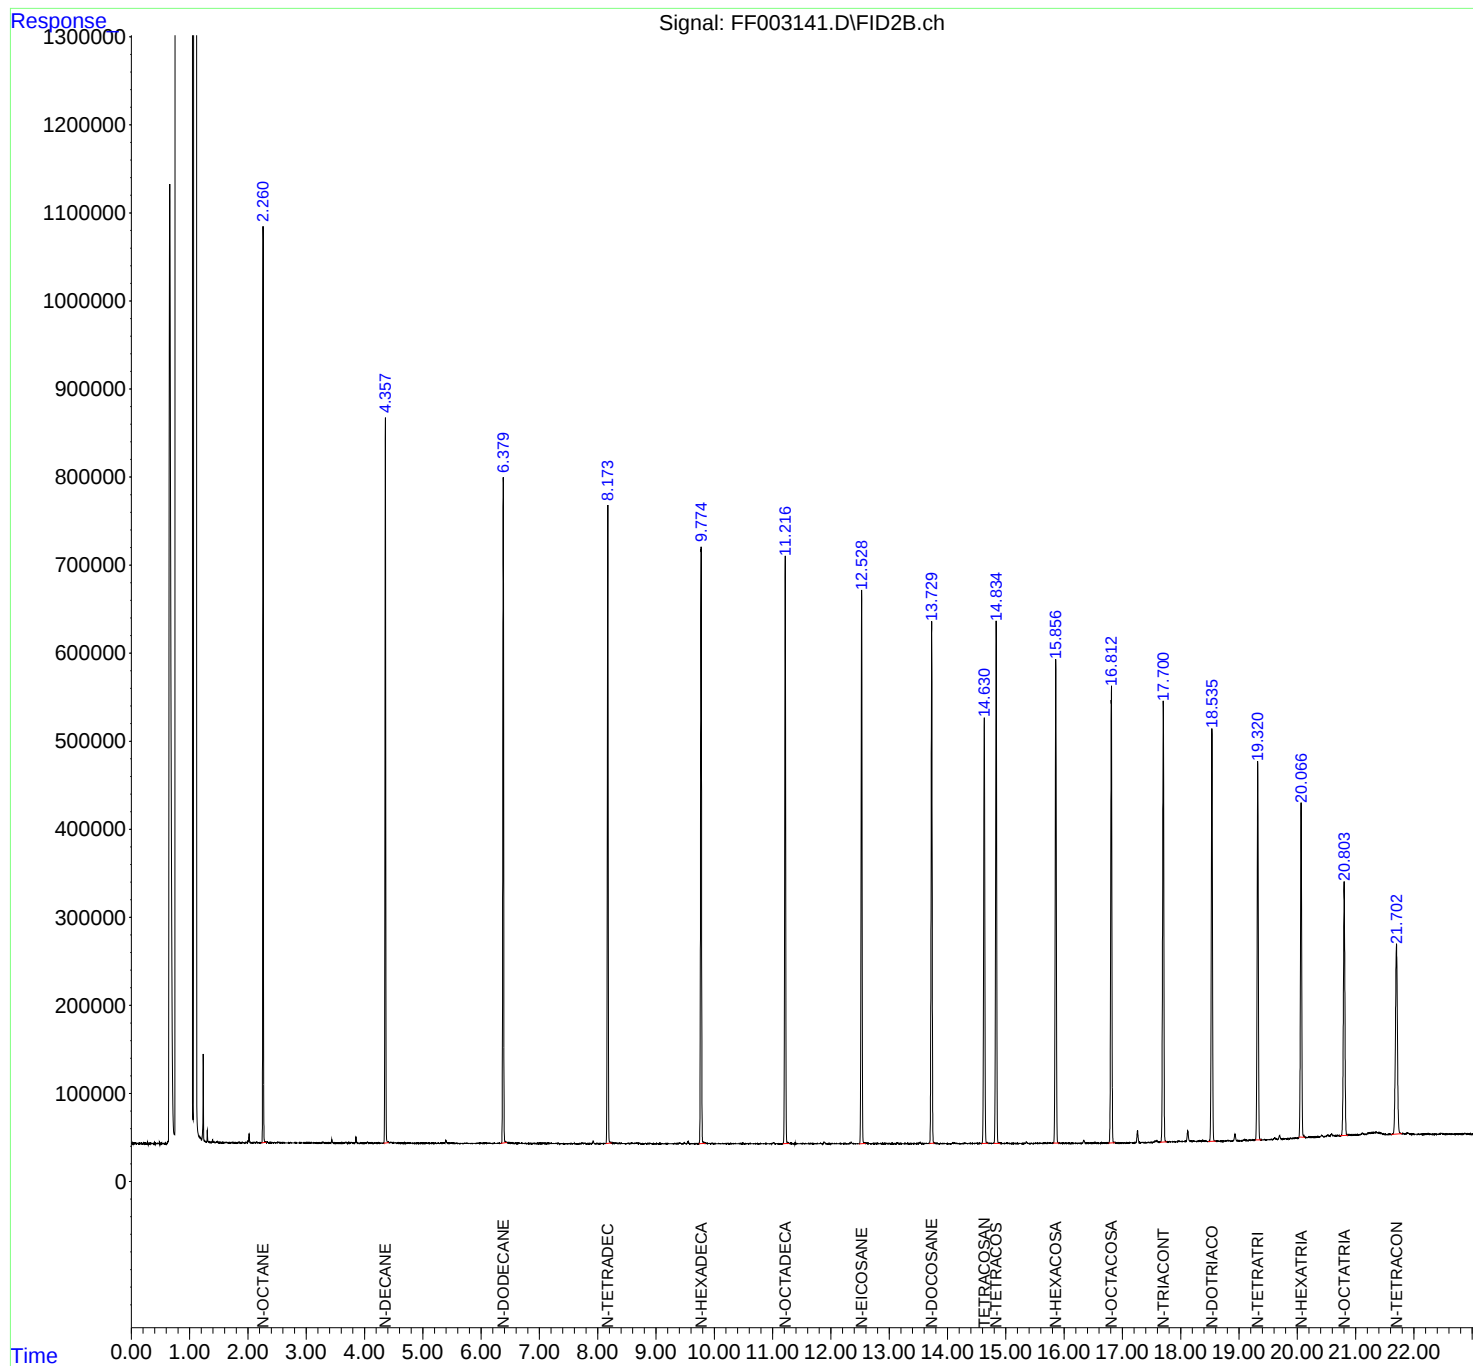


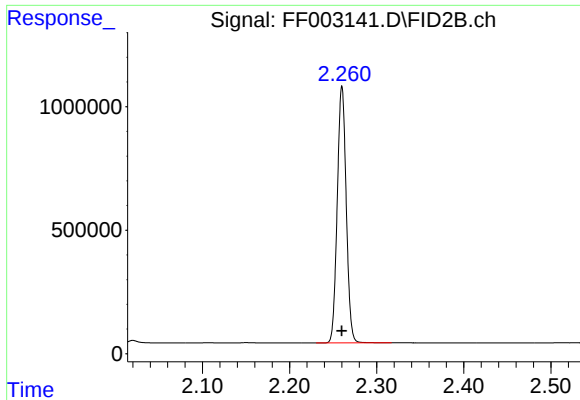

#1 N-OCTANE


R.T.: 2.260 min
Delta R.T.: 0.000 min
Response: 7442735
Conc: 50.00 ug/ml

Instrument :
FID_F
ClientSampleId :
50 TRPH STD

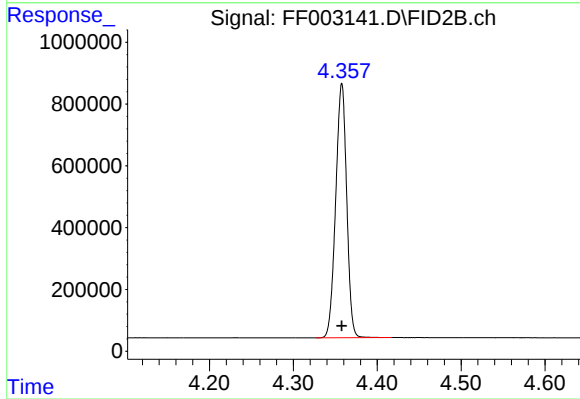


#2 N-DECANE

R.T.: 4.358 min
Delta R.T.: 0.000 min
Response: 7508370
Conc: 50.00 ug/ml

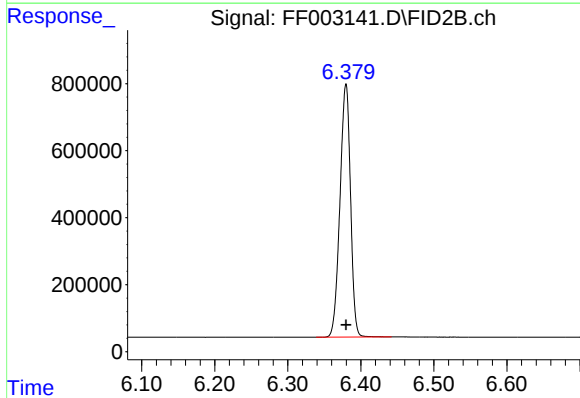


#3 N-DODECANE

R.T.: 6.380 min
Delta R.T.: 0.000 min
Response: 7566868
Conc: 50.00 ug/ml

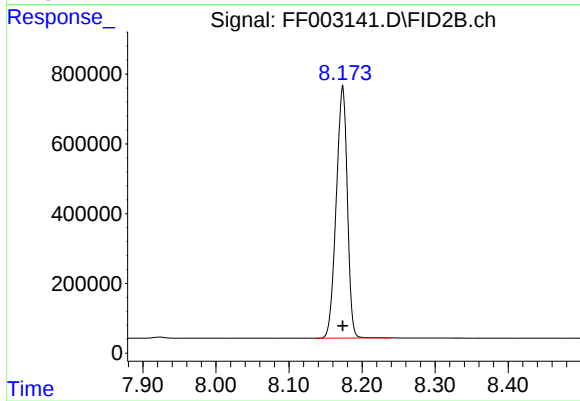

#4 N-TETRADECANE


R.T.: 8.174 min
Delta R.T.: 0.000 min
Response: 7622601
Conc: 50.00 ug/ml

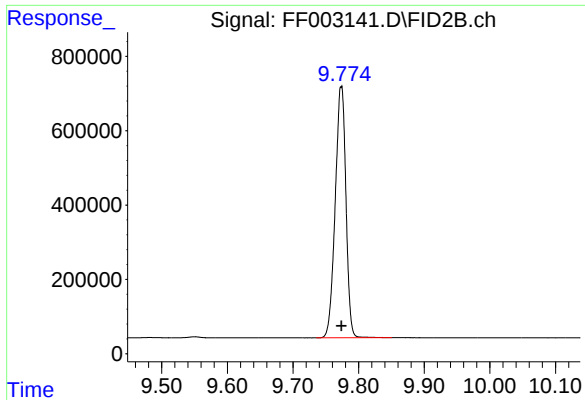

#5 N-HEXADECANE


R.T.: 9.774 min
Delta R.T.: 0.000 min
Response: 7665151
Conc: 50.00 ug/ml

Instrument :
FID_F
ClientSampleId :
50 TRPH STD

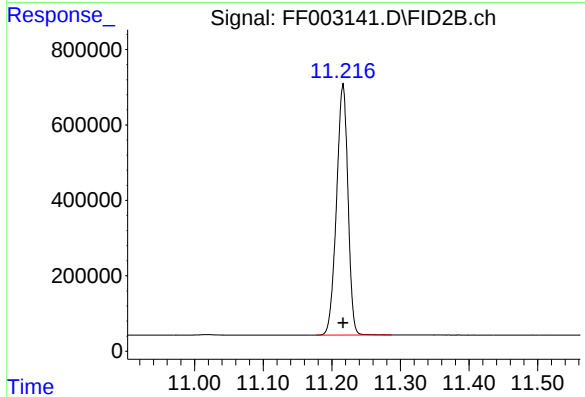


#6 N-OCTADECANE

R.T.: 11.216 min
Delta R.T.: 0.000 min
Response: 7690430
Conc: 50.00 ug/ml

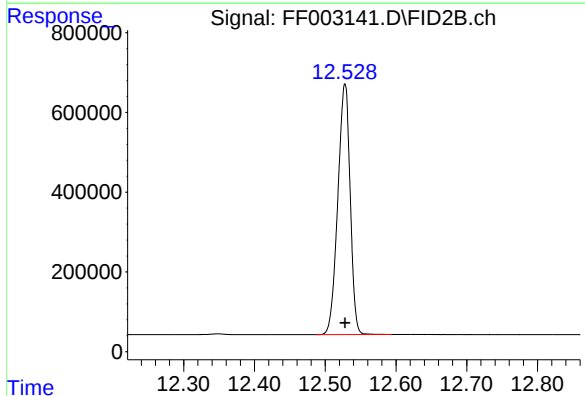


#7 N-EICOSANE

R.T.: 12.528 min
Delta R.T.: 0.000 min
Response: 7613637
Conc: 50.00 ug/ml

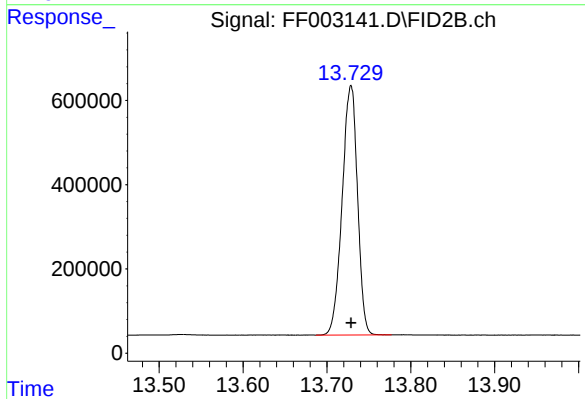

#8 N-DOCOSANE


R.T.: 13.729 min
Delta R.T.: 0.000 min
Response: 7537919
Conc: 50.00 ug/ml

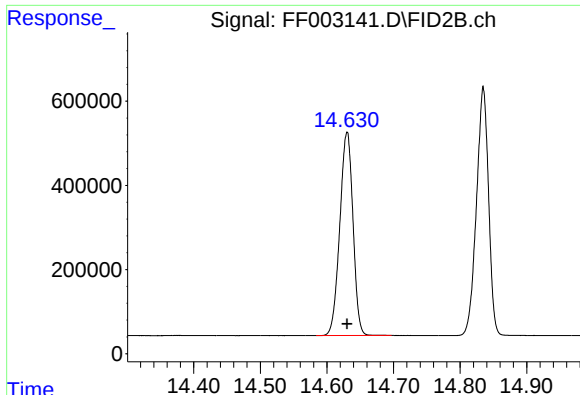

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.630 min
Delta R.T.: 0.000 min
Response: 6647268
Conc: 50.00 ug/ml

Instrument :
FID_F
ClientSampleId :
50 TRPH STD

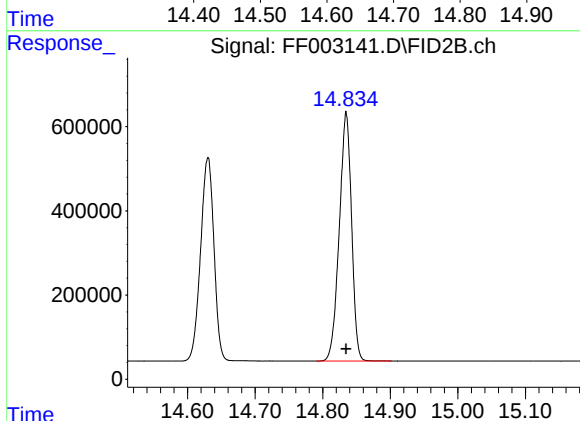


#10 N-TETRACOSANE

R.T.: 14.835 min
Delta R.T.: 0.000 min
Response: 7450165
Conc: 50.00 ug/ml

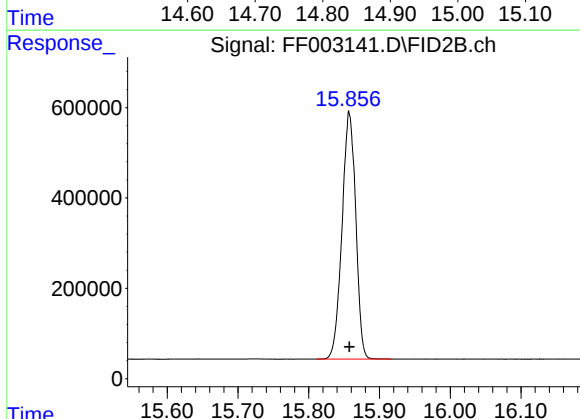


#11 N-HEXACOSANE

R.T.: 15.857 min
Delta R.T.: 0.000 min
Response: 7356470
Conc: 50.00 ug/ml

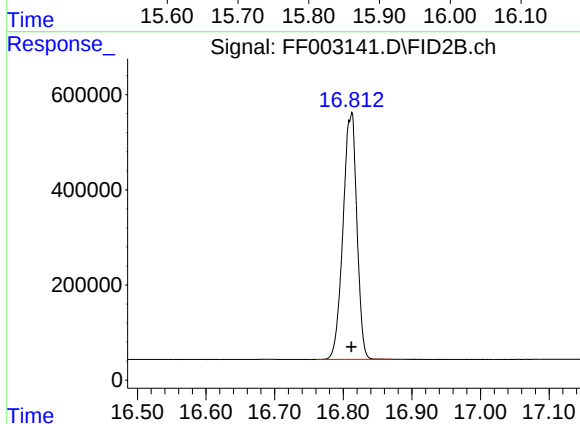

#12 N-OCTACOSANE


R.T.: 16.812 min
Delta R.T.: 0.000 min
Response: 7276904
Conc: 50.00 ug/ml

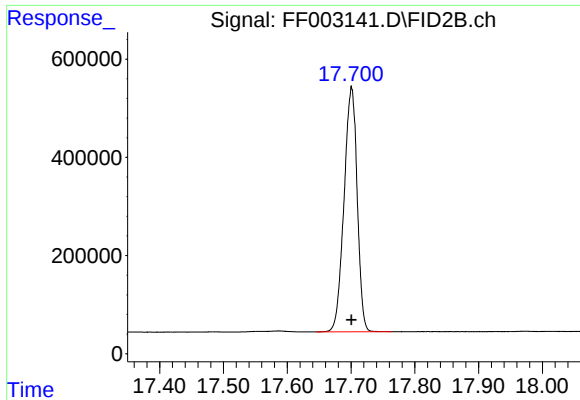

#13 N-TRIACONTANE


R.T.: 17.701 min
Delta R.T.: 0.000 min
Response: 7140943
Conc: 50.00 ug/ml

Instrument :
FID_F
ClientSampleId :
50 TRPH STD

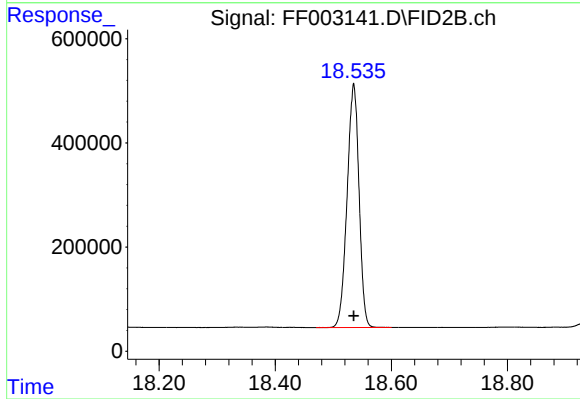


#14 N-DOTRIACONTANE

R.T.: 18.535 min
Delta R.T.: 0.000 min
Response: 6661807
Conc: 50.00 ug/ml

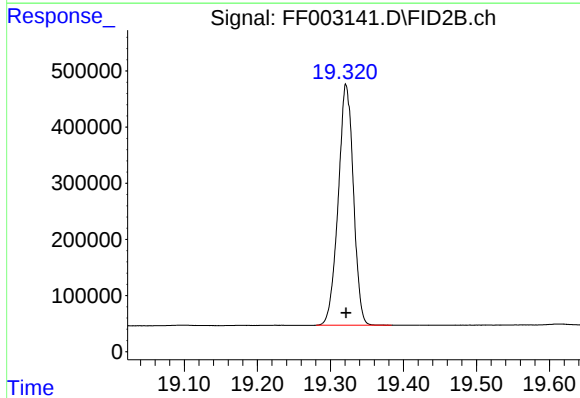


#15 N-TETRATRIACONTANE

R.T.: 19.321 min
Delta R.T.: 0.000 min
Response: 6197386
Conc: 50.00 ug/ml

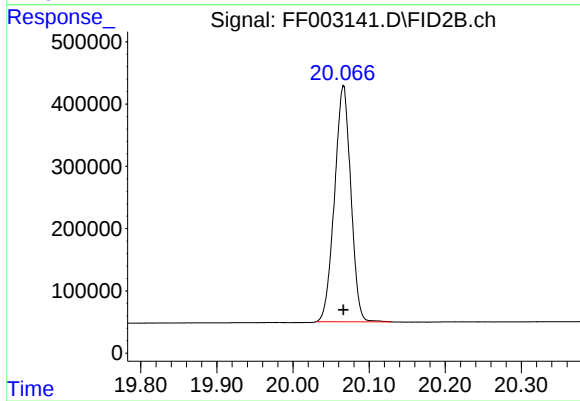

#16 N-HEXATRIACONTANE


R.T.: 20.066 min
Delta R.T.: 0.000 min
Response: 5640198
Conc: 50.00 ug/ml

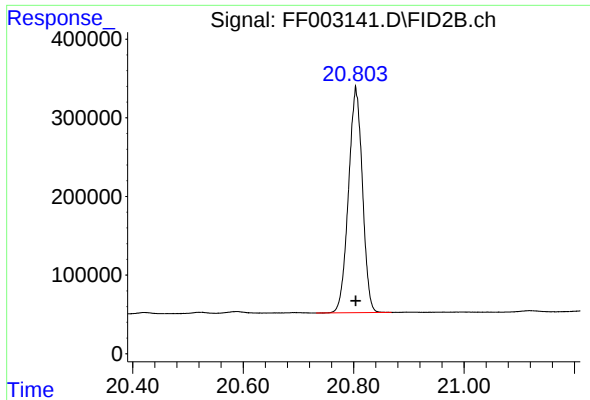

#17 N-OCTATRIACONTANE

R.T.: 20.804 min
Delta R.T.: 0.000 min
Response: 5010160
Conc: 50.00 ug/ml

Instrument :
FID_F
ClientSampleId :
50 TRPH STD

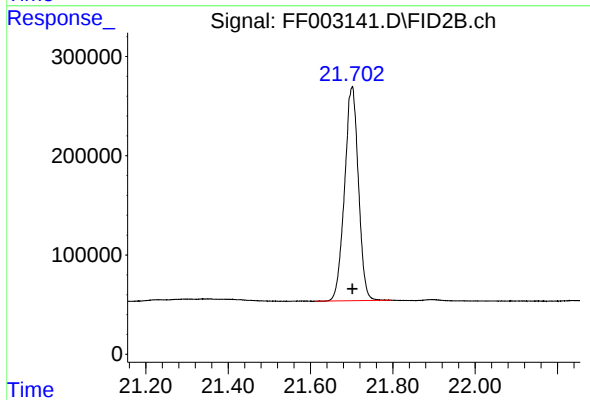

#18 N-TETRACONTANE

R.T.: 21.701 min
Delta R.T.: 0.000 min
Response: 5040606
Conc: 50.00 ug/ml