

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010421\
 Data File : FF008058.D
 Signal(s) : FID2B.ch
 Acq On : 05 Jan 2021 08:14
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jan 05 12:15:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010421.M
 Quant Title :
 QLast Update : Tue Jan 05 12:03:34 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.678	6164318	49.784 ug/ml
Target Compounds			
2) N-DECANE	4.403	6465924	52.328 ug/ml
3) N-DODECANE	6.425	6668516	51.872 ug/ml
4) N-TETRADECANE	8.221	6862610	50.763 ug/ml
5) N-HEXADECANE	9.822	6953280	50.111 ug/ml
6) N-OCTADECANE	11.266	7142775	49.870 ug/ml
7) N-EICOSANE	12.577	7190444	49.821 ug/ml
8) N-DOCOSANE	13.777	7093776	49.784 ug/ml
10) N-TETRACOSANE	14.883	7095586	49.726 ug/ml
11) N-HEXACOSANE	15.905	6937067	49.606 ug/ml
12) N-OCTACOSANE	16.856	6747262	49.356 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010421\
Data File : FF008058.D
Signal(s) : FID2B.ch
Acq On : 05 Jan 2021 08:14
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 58 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jan 05 12:15:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010421.M
Quant Title :
QLast Update : Tue Jan 05 12:03:34 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

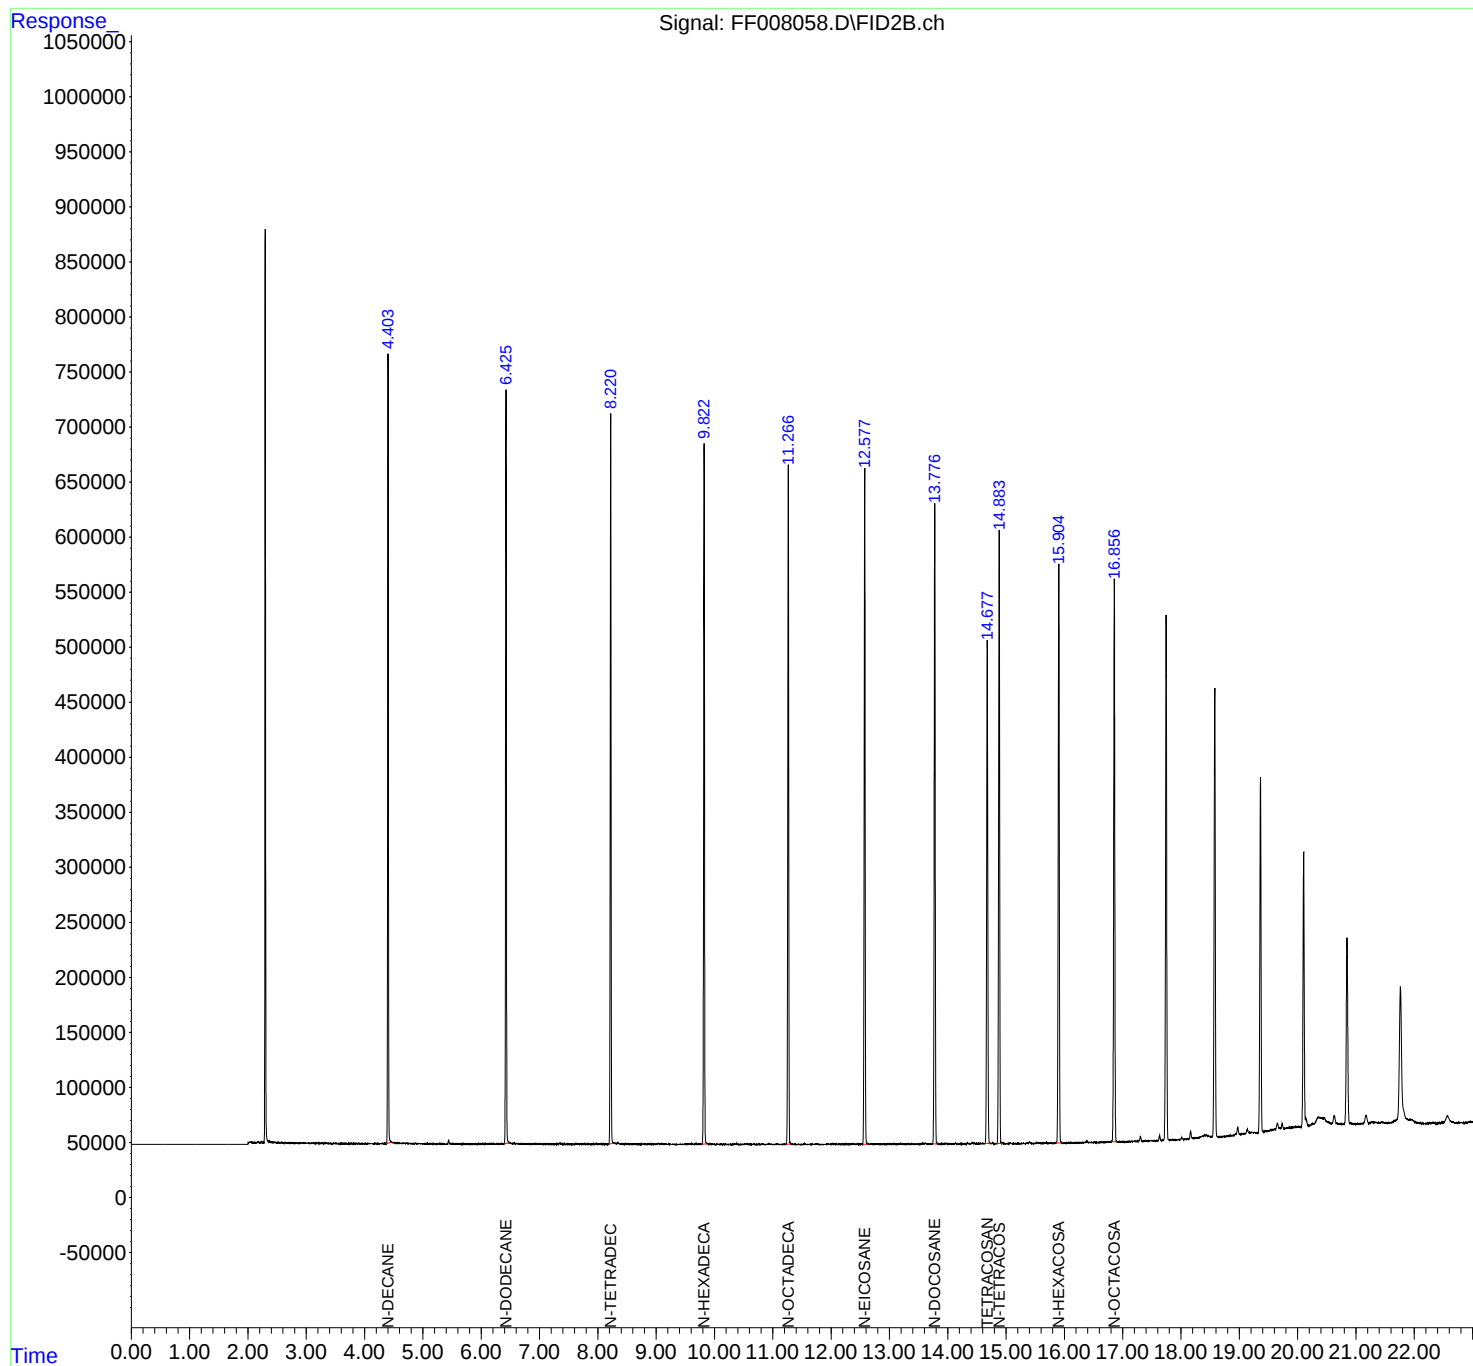

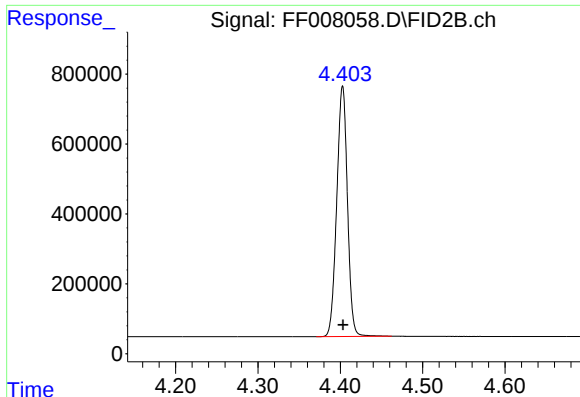


#2 N-DECANE

R.T.: 4.403 min
Delta R.T.: 0.000 min
Response: 6465924
Conc: 52.33 ug/ml

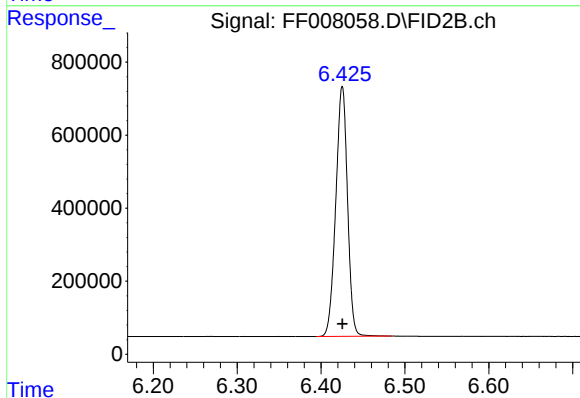


#3 N-DODECANE

R.T.: 6.425 min
Delta R.T.: 0.000 min
Response: 6668516
Conc: 51.87 ug/ml

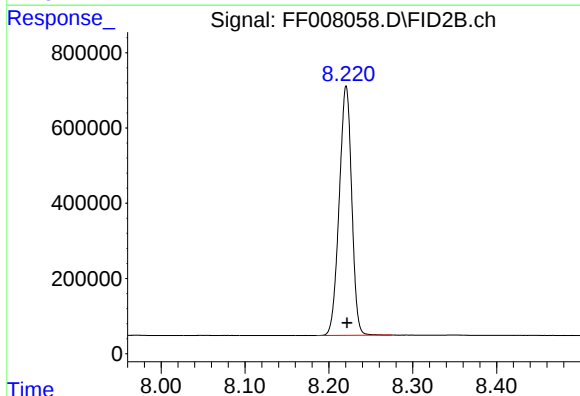


#4 N-TETRADECANE

R.T.: 8.221 min
Delta R.T.: -0.001 min
Response: 6862610
Conc: 50.76 ug/ml

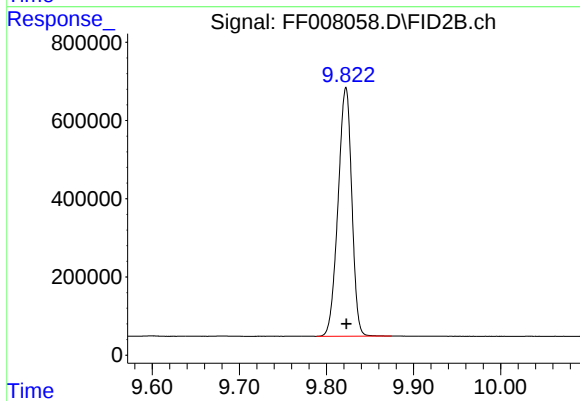


#5 N-HEXADECANE

R.T.: 9.822 min
Delta R.T.: 0.000 min
Response: 6953280
Conc: 50.11 ug/ml

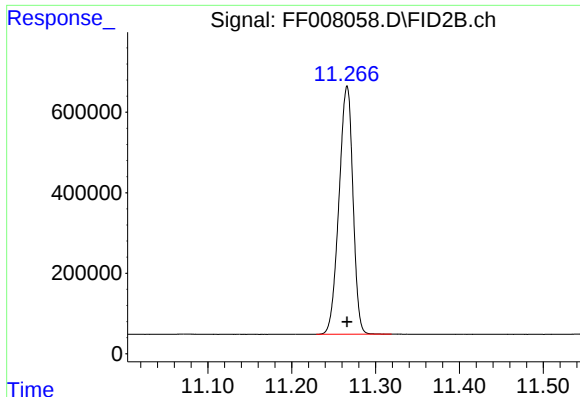


#6 N-OCTADECANE

R.T.: 11.266 min
Delta R.T.: 0.000 min
Response: 7142775
Conc: 49.87 ug/ml

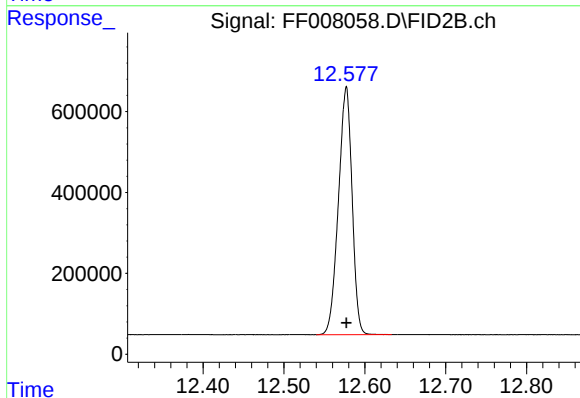


#7 N-EICOSANE

R.T.: 12.577 min
Delta R.T.: 0.000 min
Response: 7190444
Conc: 49.82 ug/ml

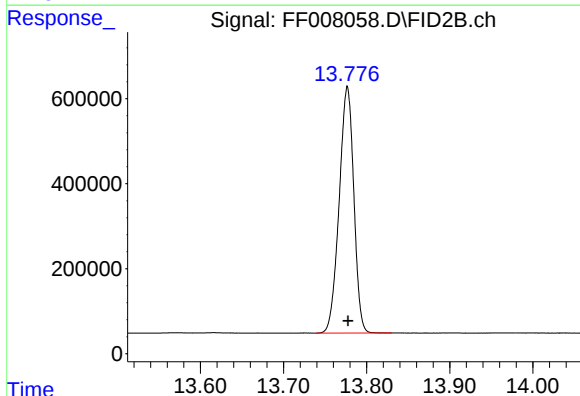


#8 N-DOCOSANE

R.T.: 13.777 min
Delta R.T.: 0.000 min
Response: 7093776
Conc: 49.78 ug/ml

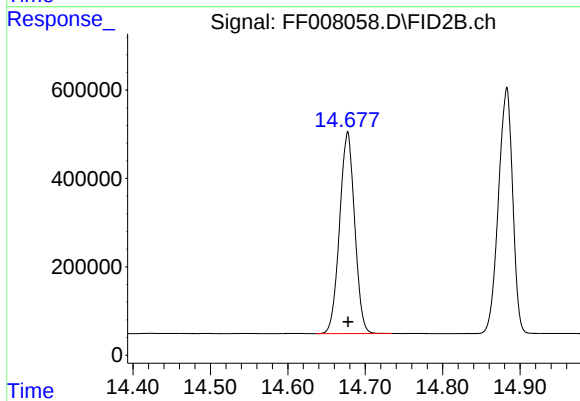


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.678 min
Delta R.T.: 0.000 min
Response: 6164318
Conc: 49.78 ug/ml

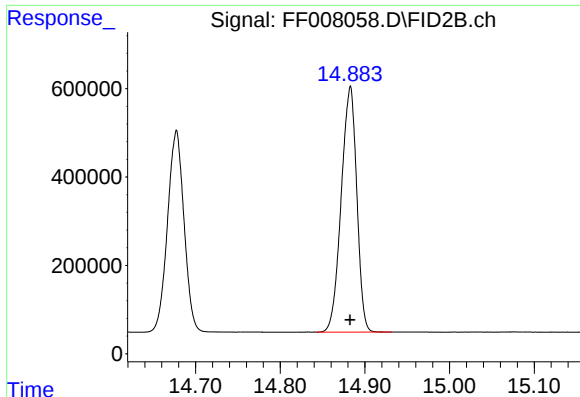


#10 N-TETRACOSANE

R.T.: 14.883 min
Delta R.T.: 0.000 min
Response: 7095586
Conc: 49.73 ug/ml

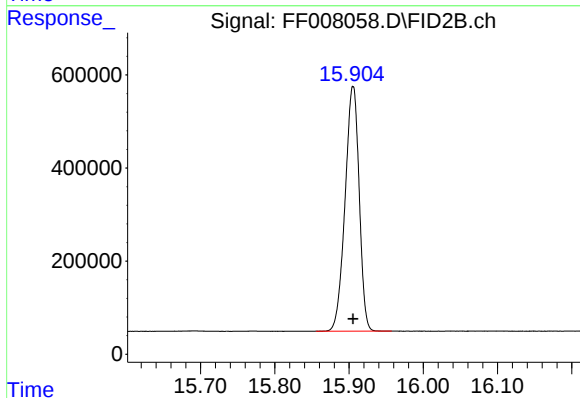

#11 N-HEXACOSANE

R.T.: 15.905 min
Delta R.T.: 0.000 min
Response: 6937067
Conc: 49.61 ug/ml

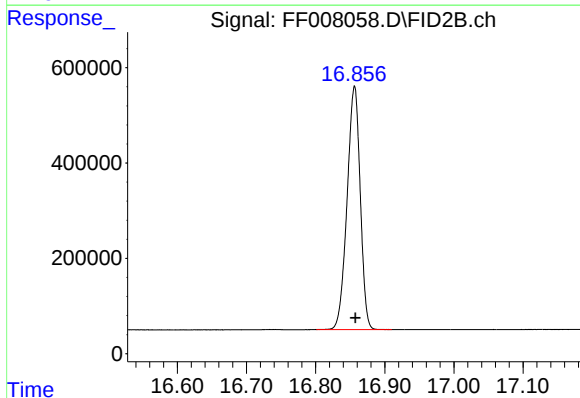

#12 N-OCTACOSANE

R.T.: 16.856 min
Delta R.T.: -0.001 min
Response: 6747262
Conc: 49.36 ug/ml