

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010422\
 Data File : FF009628.D
 Signal(s) : FID2B.ch
 Acq On : 04 Jan 2022 09:49
 Operator : AJ\MA
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 04 14:24:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
 Quant Title :
 QLast Update : Thu Dec 16 03:33:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds				
7) N-EICOSANE	12.358	213333	1.505	ug/ml
8) N-DOCOSANE	13.558	389867	2.861	ug/ml
10) N-TETRACOSANE	14.659	427097	3.244	ug/ml
11) N-HEXACOSANE	15.675	268410	2.148	ug/ml
12) N-OCTACOSANE	16.626	1855479	15.582	ug/ml
13) N-TRIACONTANE	17.509	3213302	28.053	ug/ml
14) N-DOTRIACONTANE	18.342	389353	3.563	ug/ml
15) N-TETRATRIACONTANE	19.121	366762	3.462	ug/ml
16) N-HEXATRIACONTANE	19.858	660208	6.591	ug/ml
18) N-TETRACONTANE	21.420	5213484	51.621	ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010422\
Data File : FF009628.D
Signal(s) : FID2B.ch
Acq On : 04 Jan 2022 09:49
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 04 14:24:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

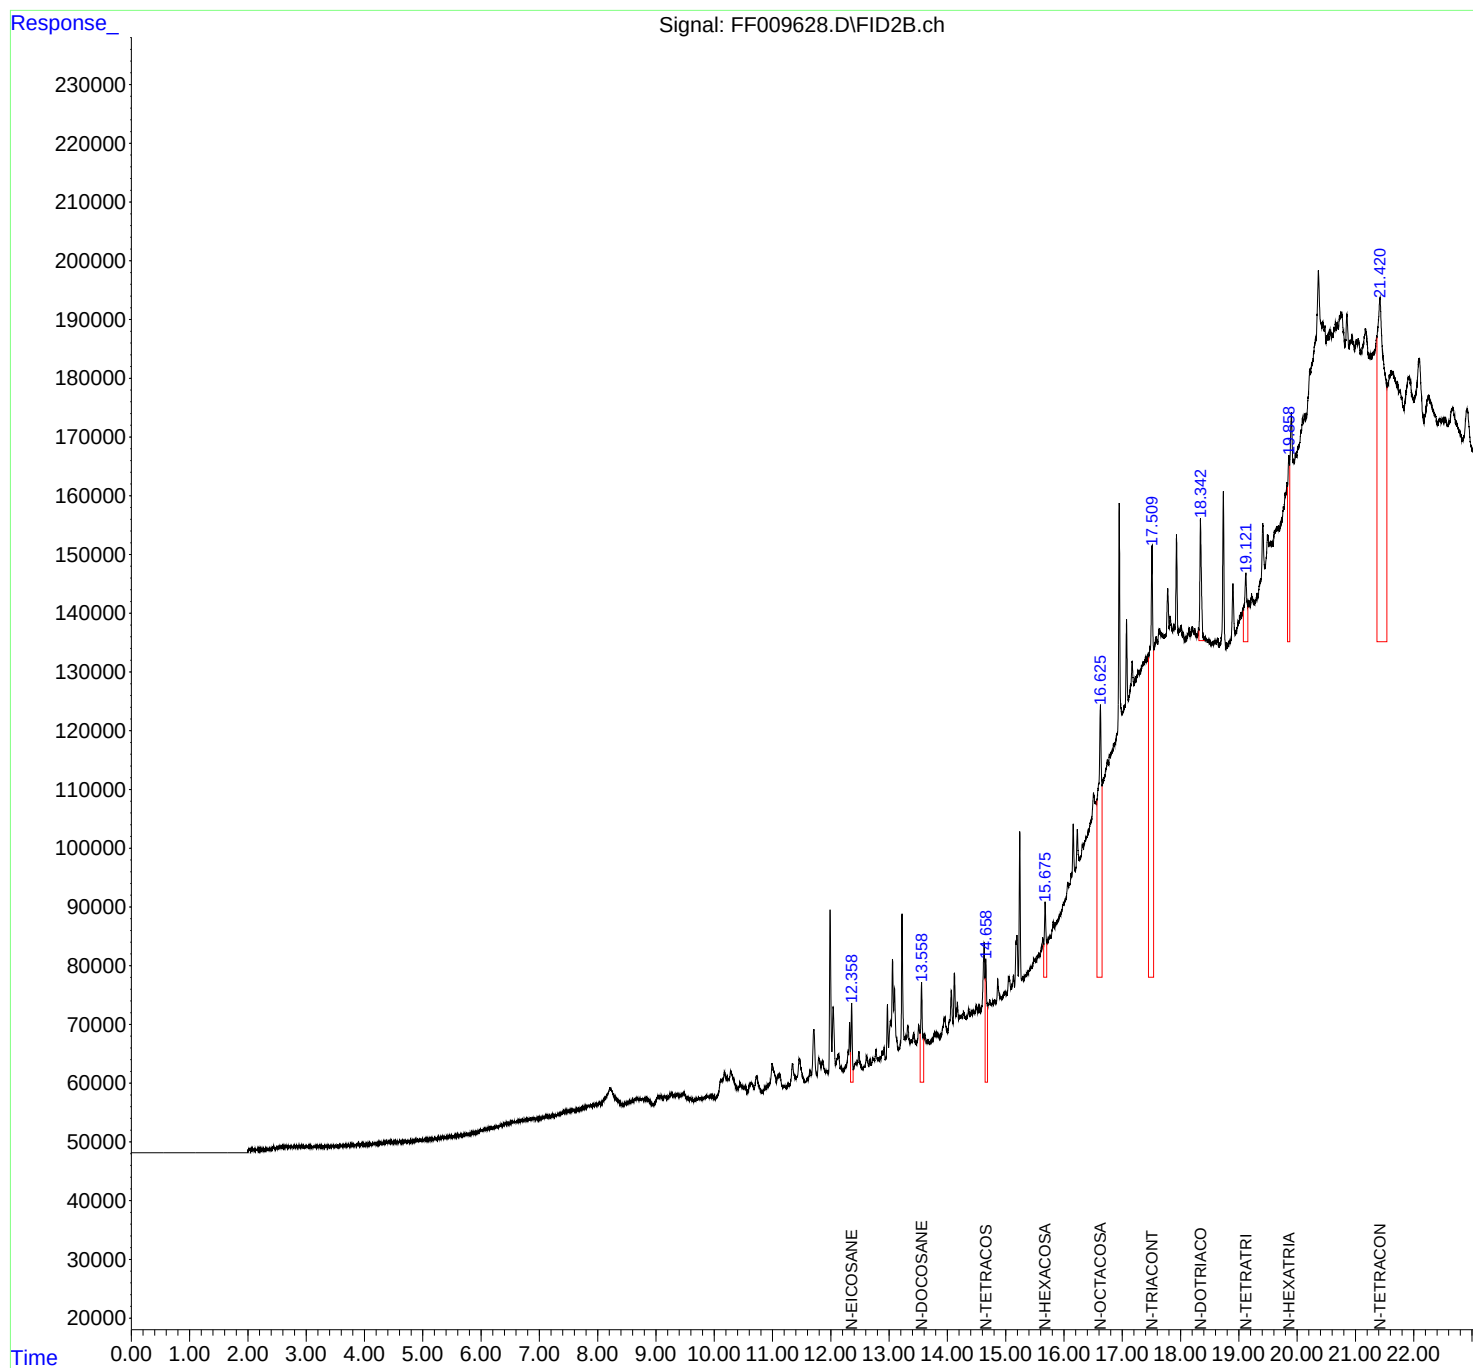


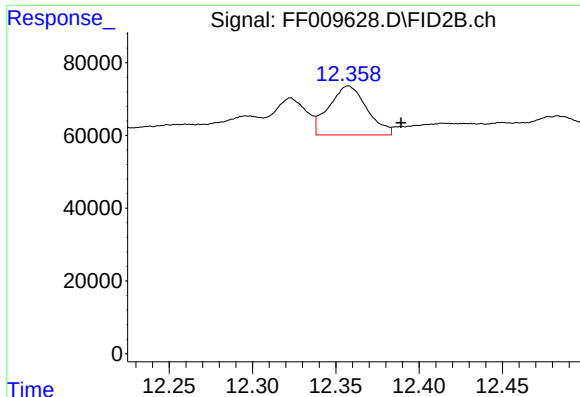

#7 N-EICOSANE


R.T.: 12.358 min
Delta R.T.: -0.031 min
Response: 213333
Conc: 1.51 ug/ml

Instrument :
FID_F
ClientSampleId :

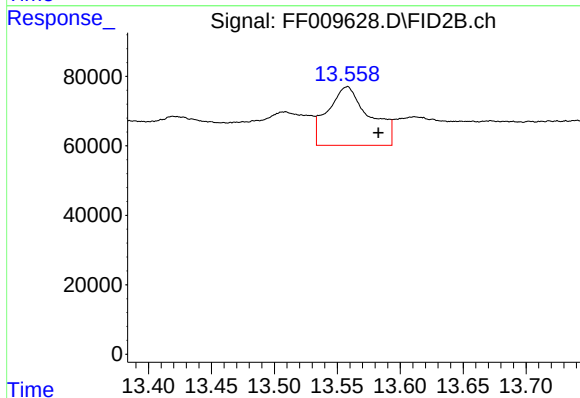


#8 N-DOCOSANE

R.T.: 13.558 min
Delta R.T.: -0.024 min
Response: 389867
Conc: 2.86 ug/ml

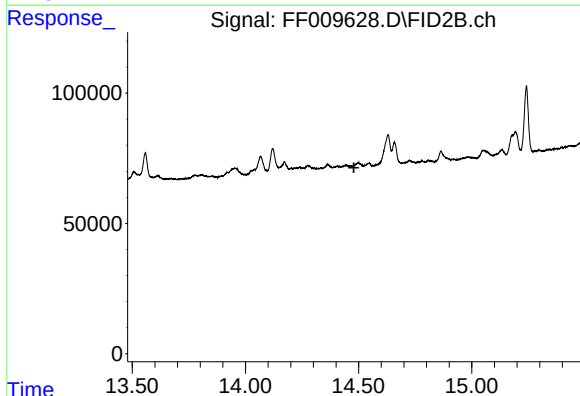


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.479 min
Response: 0
Conc: N.D.

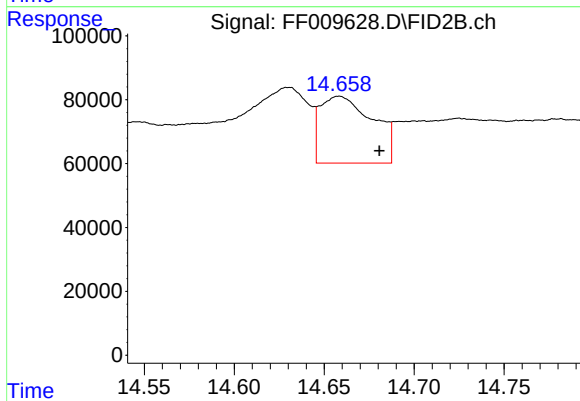

#10 N-TETRACOSANE


R.T.: 14.659 min
Delta R.T.: -0.022 min
Response: 427097
Conc: 3.24 ug/ml

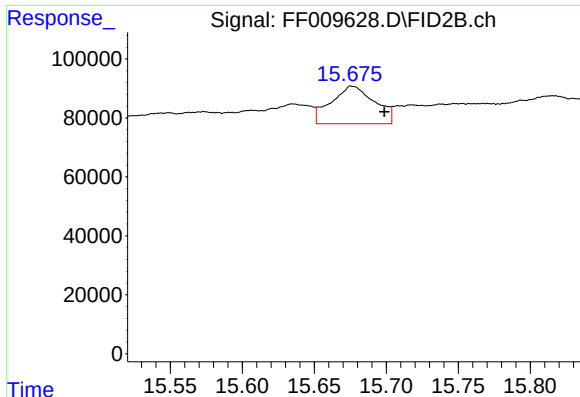

#11 N-HEXACOSANE


R.T.: 15.675 min
Delta R.T.: -0.023 min
Response: 268410
Conc: 2.15 ug/ml

Instrument :
FID_F
ClientSampleId :

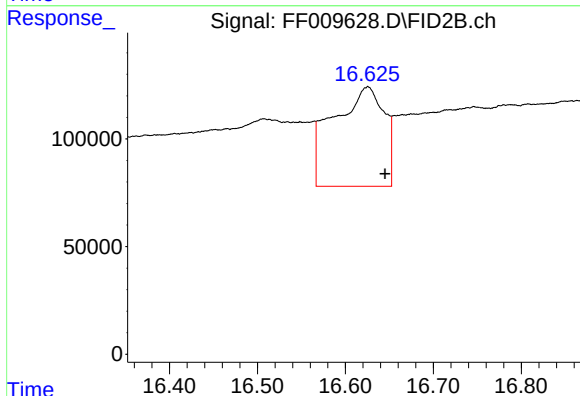


#12 N-OCTACOSANE

R.T.: 16.626 min
Delta R.T.: -0.020 min
Response: 1855479
Conc: 15.58 ug/ml

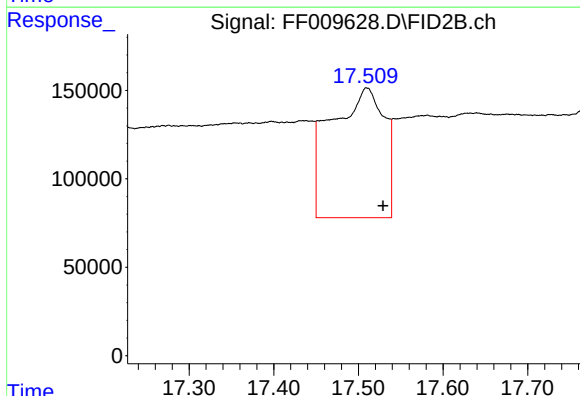


#13 N-TRIACONTANE

R.T.: 17.509 min
Delta R.T.: -0.020 min
Response: 3213302
Conc: 28.05 ug/ml

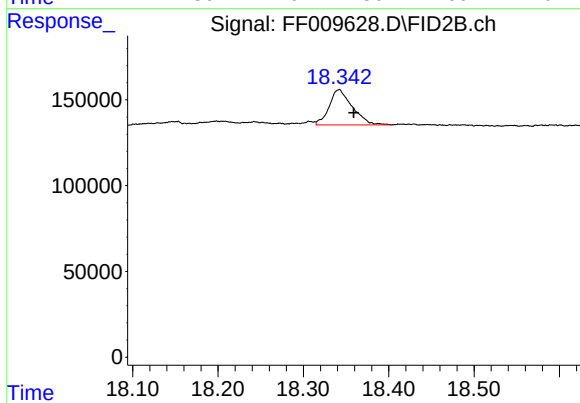

#14 N-DOTRIACONTANE


R.T.: 18.342 min
Delta R.T.: -0.017 min
Response: 389353
Conc: 3.56 ug/ml

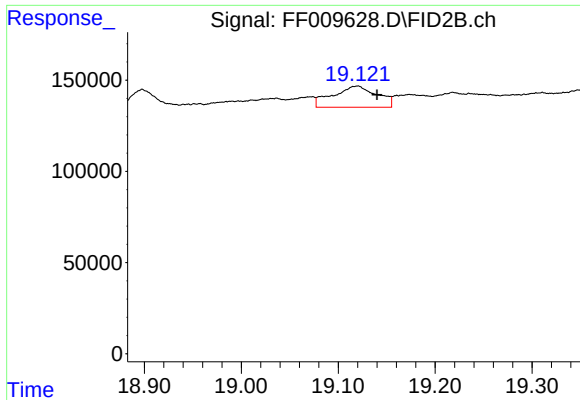

#15 N-TETRATRIACONTANE


R.T.: 19.121 min
Delta R.T.: -0.020 min
Response: 366762
Conc: 3.46 ug/ml

Instrument :
FID_F
ClientSampleId :

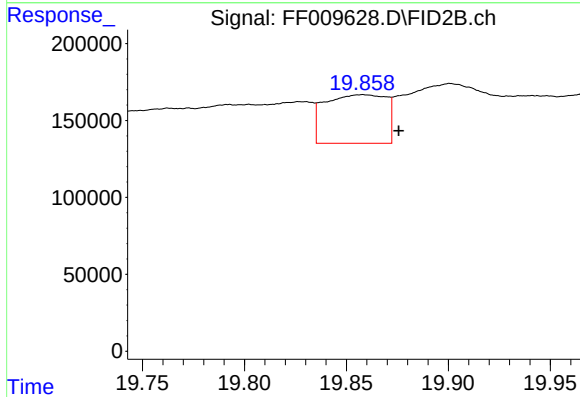

#16 N-HEXATRIACONTANE

R.T.: 19.858 min
Delta R.T.: -0.018 min
Response: 660208
Conc: 6.59 ug/ml

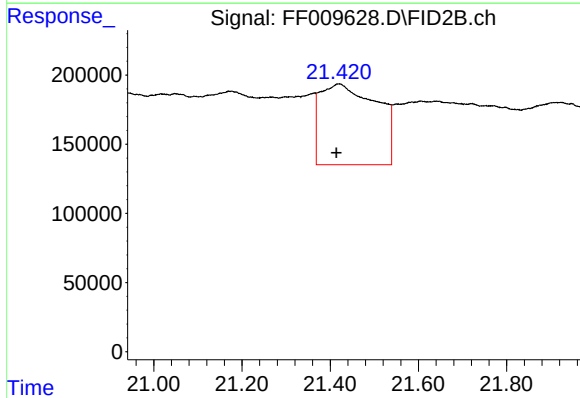

#18 N-TETRACONTANE

R.T.: 21.420 min
Delta R.T.: 0.007 min
Response: 5213484
Conc: 51.62 ug/ml