

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010422\
Data File : FF009631.D
Signal(s) : FID2B.ch
Acq On : 04 Jan 2022 11:20
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 04 14:24:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.255	2942826	20.349 ug/ml
12)	N-OCTACOSANE	16.630	2516308	21.132 ug/ml
13)	N-TRIACONTANE	17.511	84545	0.738 ug/ml
14)	N-DOTRIACONTANE	18.346	210749	1.928 ug/ml
15)	N-TETRATRIACONTANE	19.122	742367	7.008 ug/ml
16)	N-HEXATRIACONTANE	19.862	3968222	39.618 ug/ml
18)	N-TETRACONTANE	21.423	487680	4.829 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010422\
Data File : FF009631.D
Signal(s) : FID2B.ch
Acq On : 04 Jan 2022 11:20
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 04 14:24:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

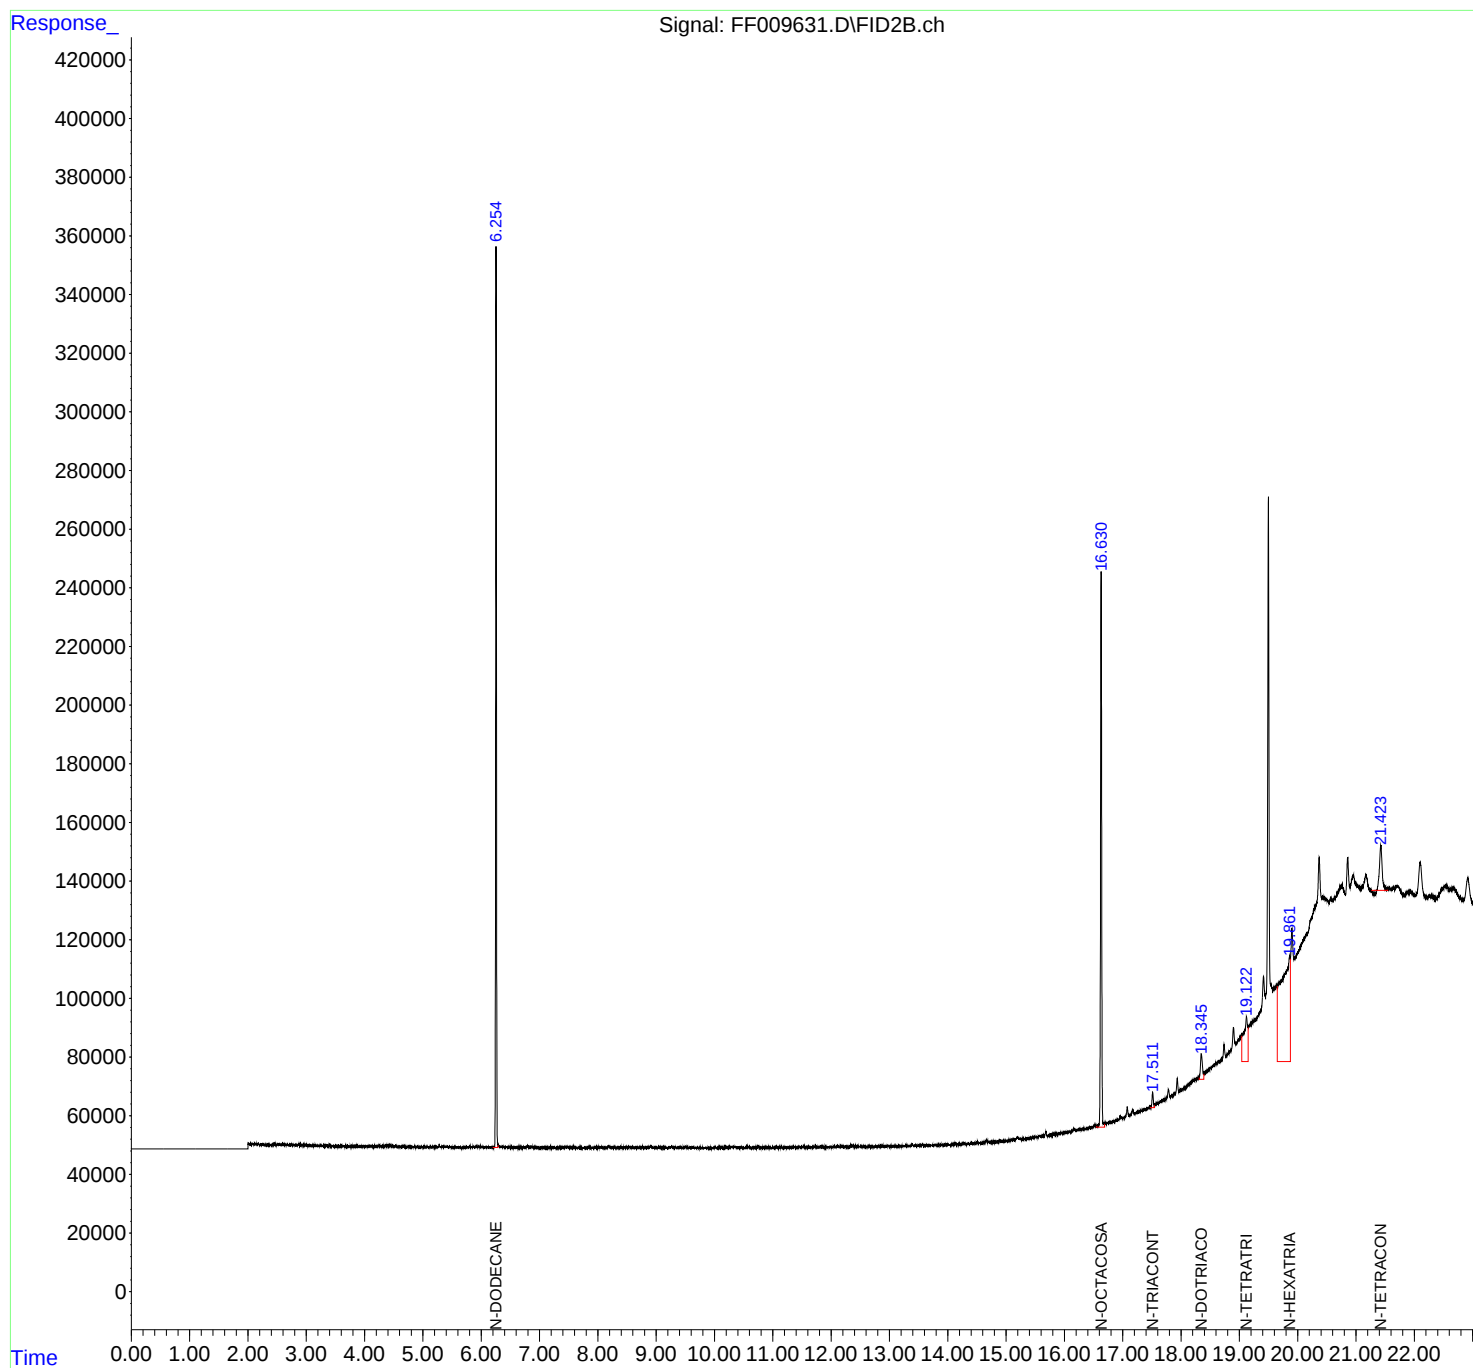


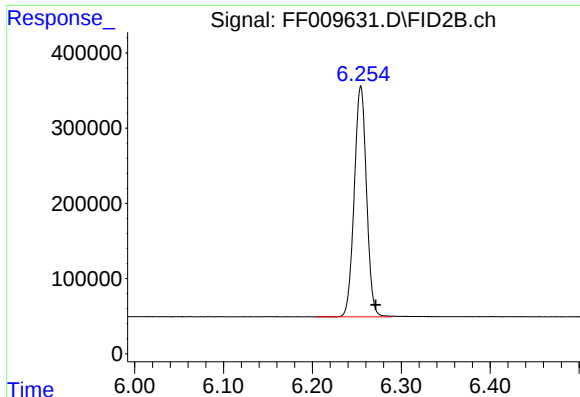

#3 N-DODECANE


R.T.: 6.255 min
Delta R.T.: -0.017 min
Response: 2942826
Conc: 20.35 ug/ml

Instrument :
FID_F
ClientSampleId :

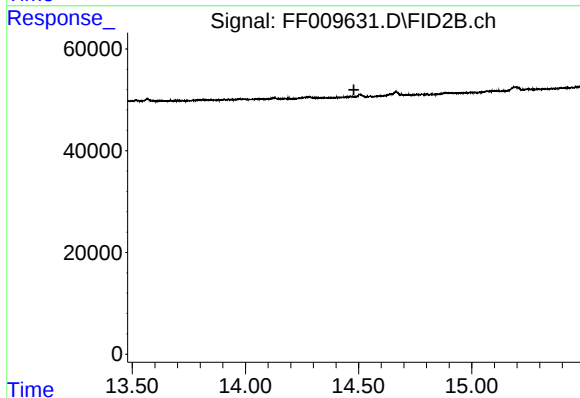


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.479 min
Response: 0
Conc: N.D.

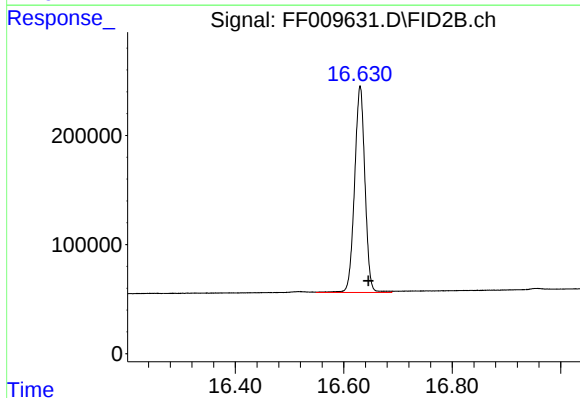


#12 N-OCTACOSANE

R.T.: 16.630 min
Delta R.T.: -0.015 min
Response: 2516308
Conc: 21.13 ug/ml

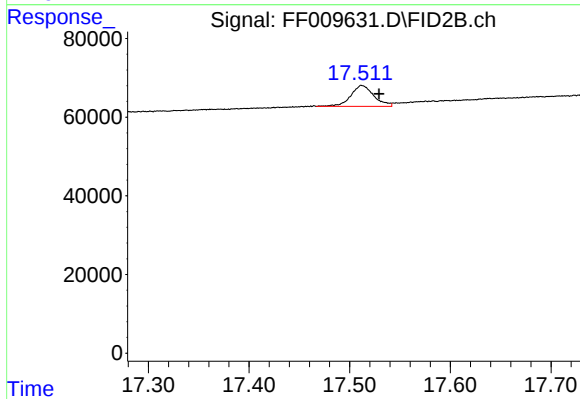

#13 N-TRIACONTANE


R.T.: 17.511 min
Delta R.T.: -0.018 min
Response: 84545
Conc: 0.74 ug/ml

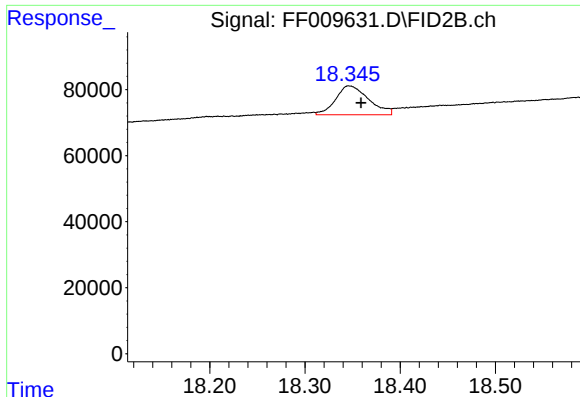

#14 N-DOTRIACONTANE


R.T.: 18.346 min
Delta R.T.: -0.013 min
Response: 210749
Conc: 1.93 ug/ml

Instrument :
FID_F
ClientSampleId :

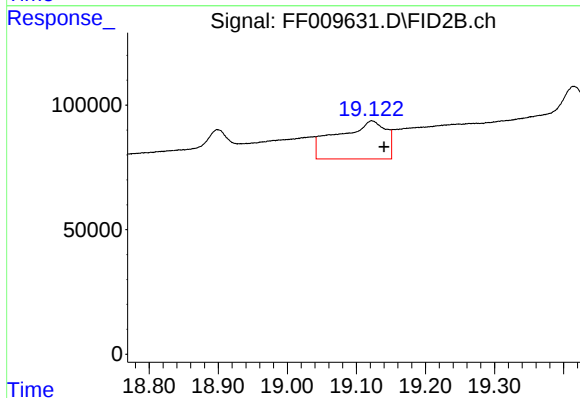


#15 N-TETRATRIACONTANE

R.T.: 19.122 min
Delta R.T.: -0.018 min
Response: 742367
Conc: 7.01 ug/ml

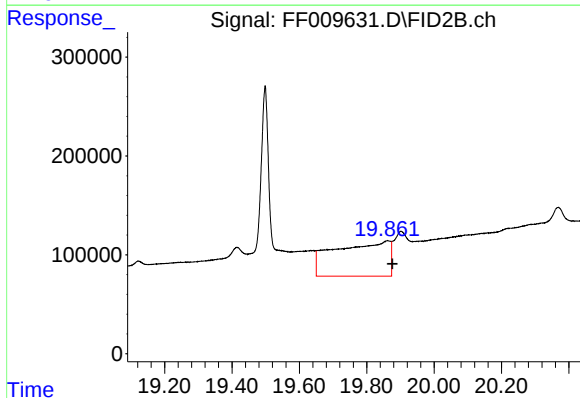

#16 N-HEXATRIACONTANE

R.T.: 19.862 min
Delta R.T.: -0.014 min
Response: 3968222
Conc: 39.62 ug/ml

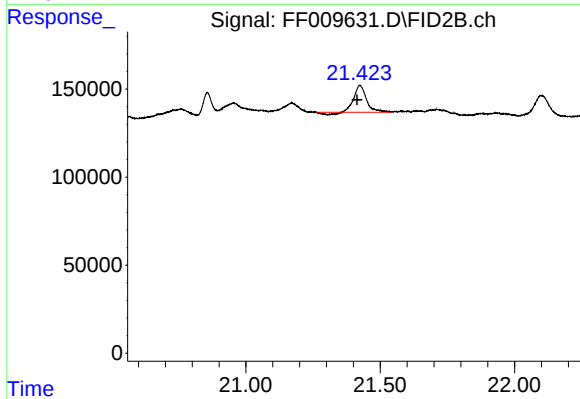

#18 N-TETRACONTANE

R.T.: 21.423 min
Delta R.T.: 0.010 min
Response: 487680
Conc: 4.83 ug/ml