

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010422\
Data File : FF009634.D
Signal(s) : FID2B.ch
Acq On : 04 Jan 2022 13:15
Operator : AJ\MA
Sample : M5331-01 50X
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 04 14:25:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

13)	N-TRIACONTANE	17.511	93875	0.820 ug/ml
14)	N-DOTRIACONTANE	18.341	526717	4.820 ug/ml
15)	N-TETRATRIACONTANE	19.151	95386	0.900 ug/ml
16)	N-HEXATRIACONTANE	19.862	1811083	18.081 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010422\
Data File : FF009634.D
Signal(s) : FID2B.ch
Acq On : 04 Jan 2022 13:15
Operator : AJ\MA
Sample : M5331-01 50X
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 04 14:25:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

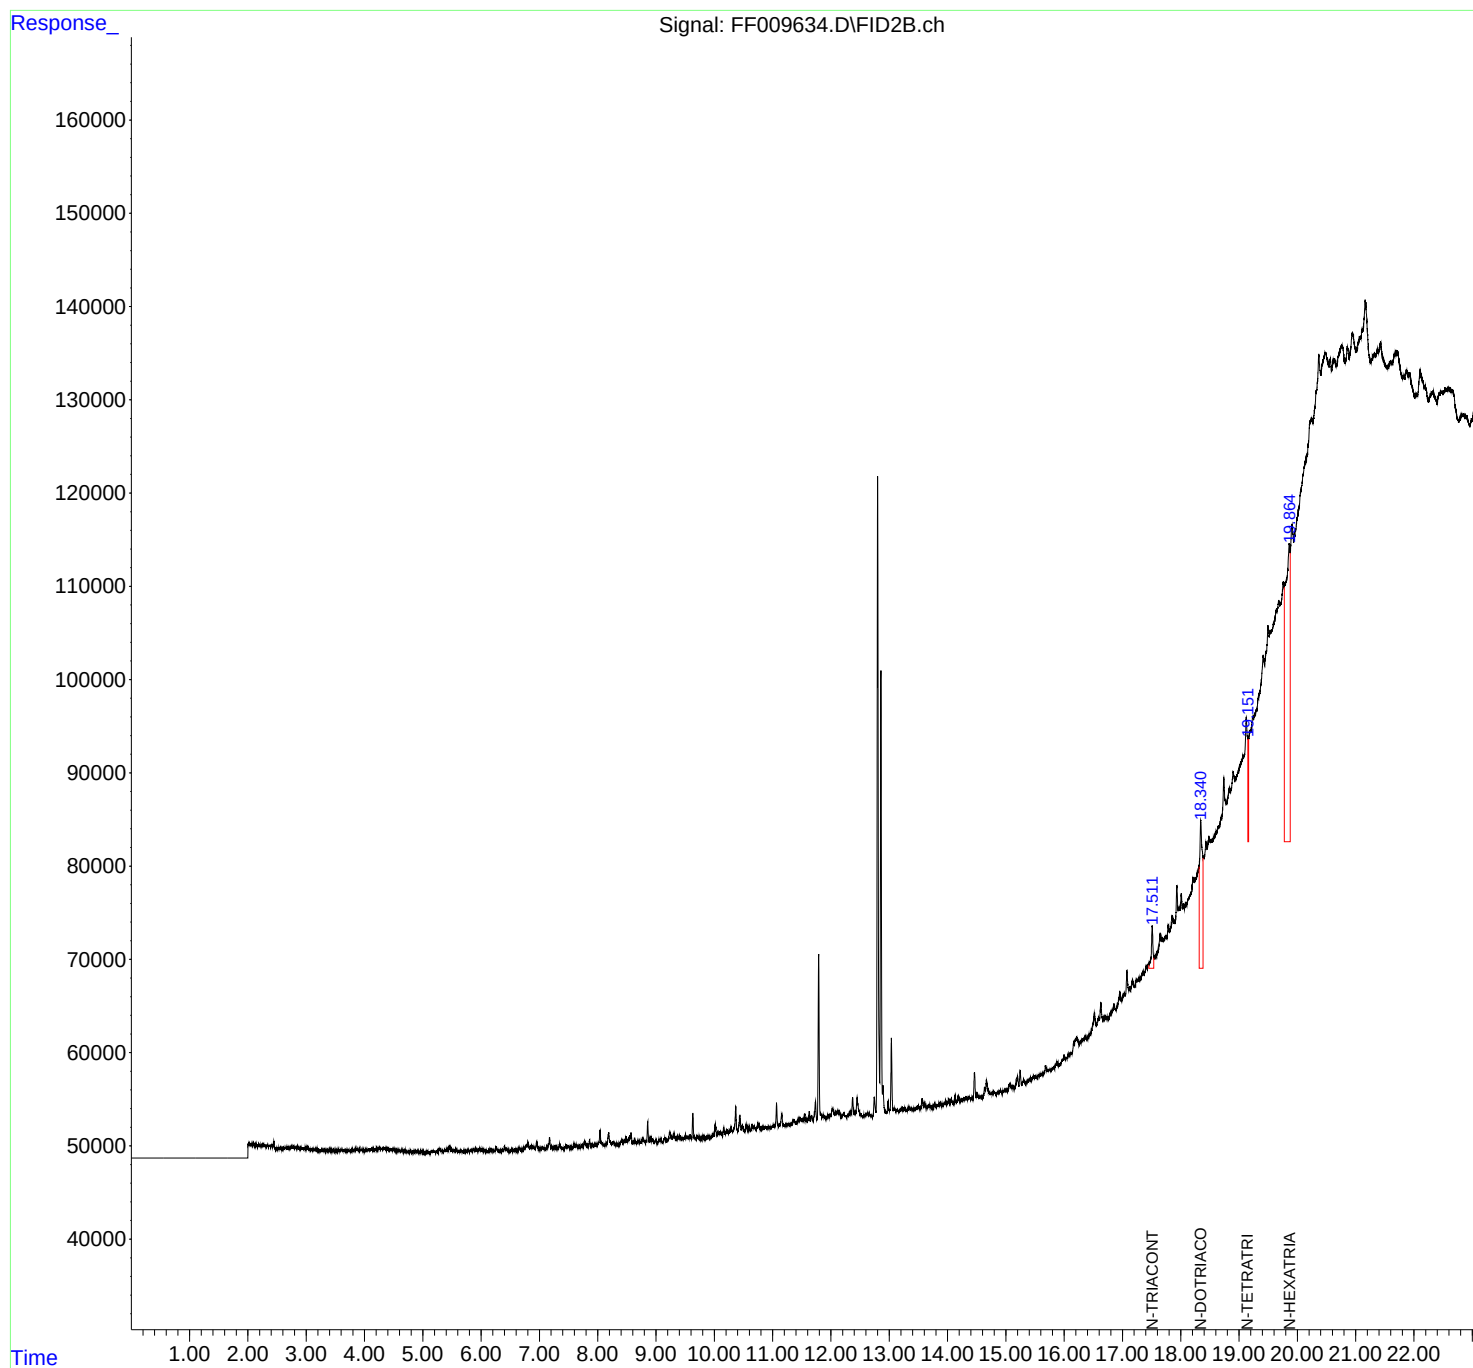


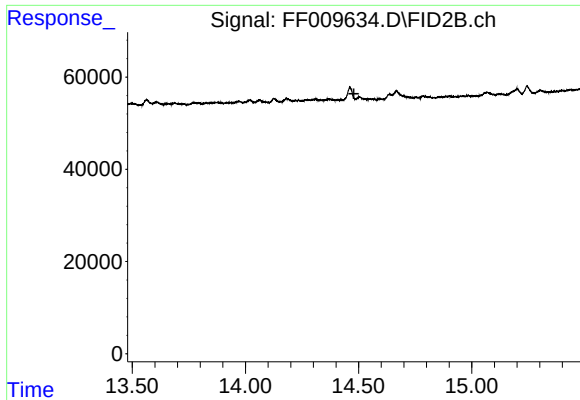

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.479 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

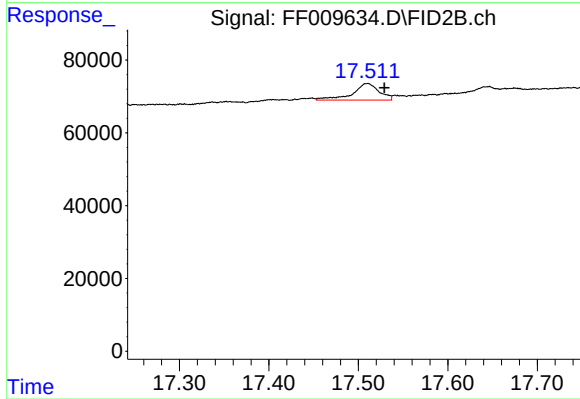


#13 N-TRIACONTANE

R.T.: 17.511 min
Delta R.T.: -0.018 min
Response: 93875
Conc: 0.82 ug/ml

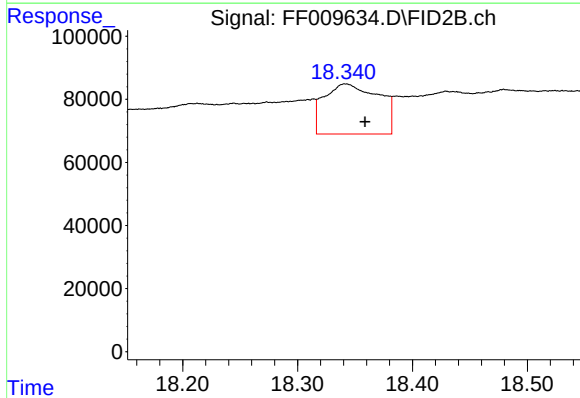


#14 N-DOTRIACONTANE

R.T.: 18.341 min
Delta R.T.: -0.018 min
Response: 526717
Conc: 4.82 ug/ml

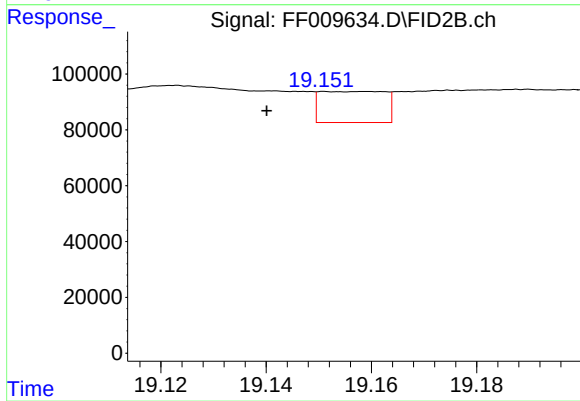

#15 N-TETRATRIACONTANE

R.T.: 19.151 min
Delta R.T.: 0.011 min
Response: 95386
Conc: 0.90 ug/ml

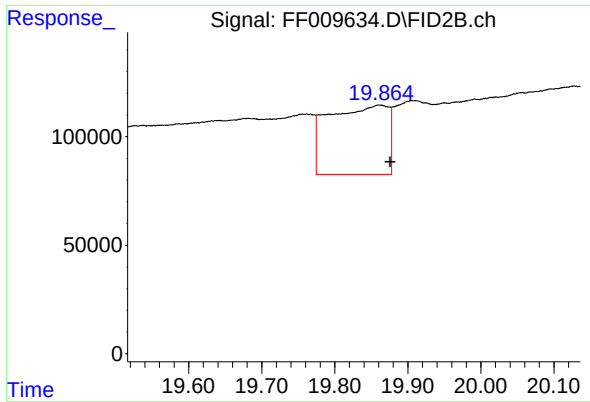

#16 N-HEXATRIACONTANE

R.T.: 19.862 min
Delta R.T.: -0.014 min
Response: 1811083
Conc: 18.08 ug/ml

Instrument :
FID_F
ClientSampleId :