

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010422\
Data File : FF009635.D
Signal(s) : FID2B.ch
Acq On : 04 Jan 2022 13:45
Operator : AJ\MA
Sample : M5330-01 100X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 04 14:25:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

13)	N-TRIACONTANE	17.509	236519	2.065 ug/ml
14)	N-DOTRIACONTANE	18.350	894938	8.189 ug/ml
15)	N-TETRATRIACONTANE	19.123	286676	2.706 ug/ml
16)	N-HEXATRIACONTANE	19.861	1367419	13.652 ug/ml
18)	N-TETRACONTANE	21.420	265576	2.630 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010422\
Data File : FF009635.D
Signal(s) : FID2B.ch
Acq On : 04 Jan 2022 13:45
Operator : AJ\MA
Sample : M5330-01 100X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 04 14:25:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

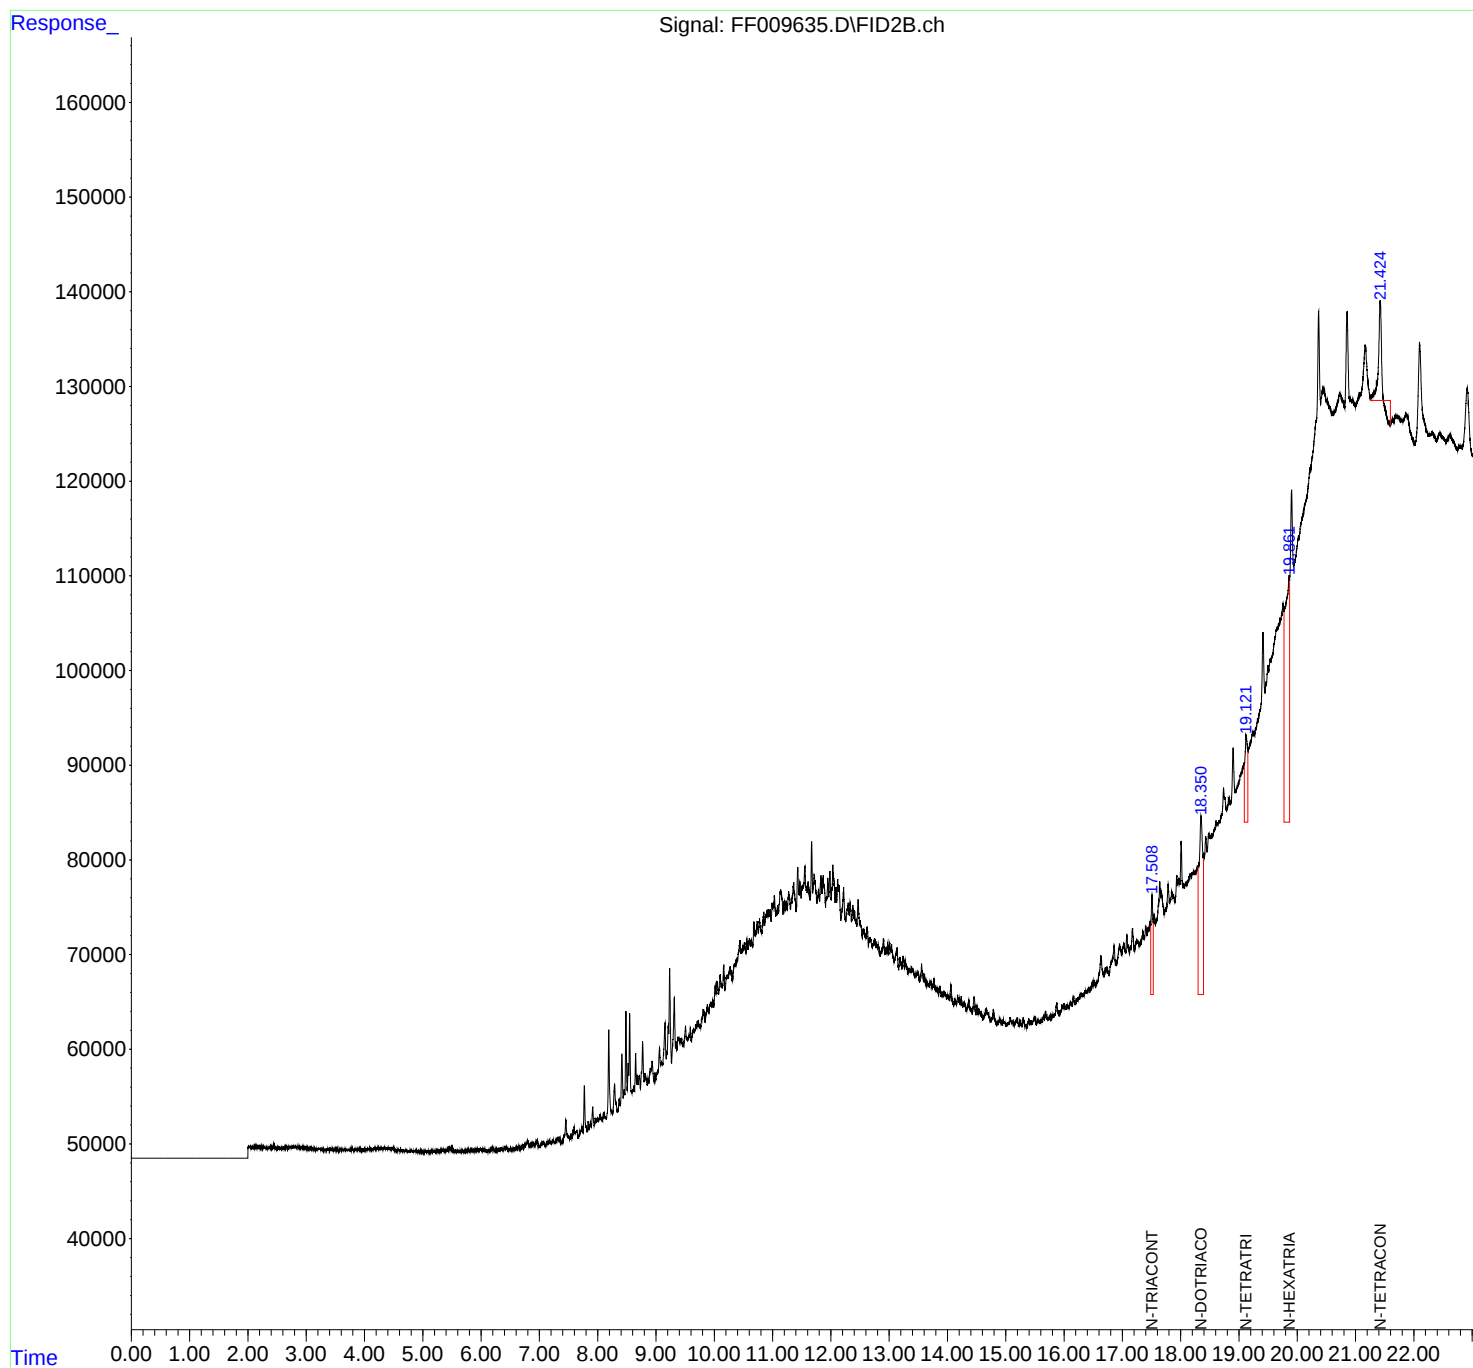


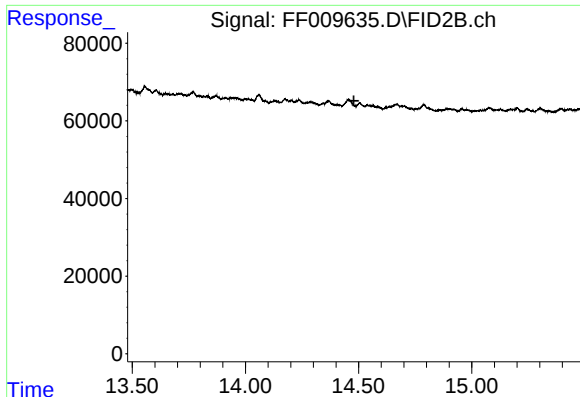

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.479 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

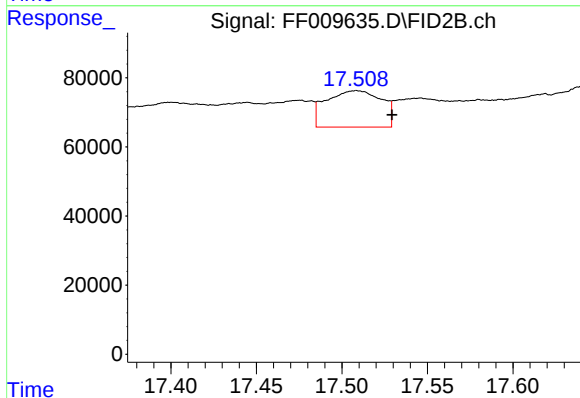


#13 N-TRIACONTANE

R.T.: 17.509 min
Delta R.T.: -0.021 min
Response: 236519
Conc: 2.06 ug/ml

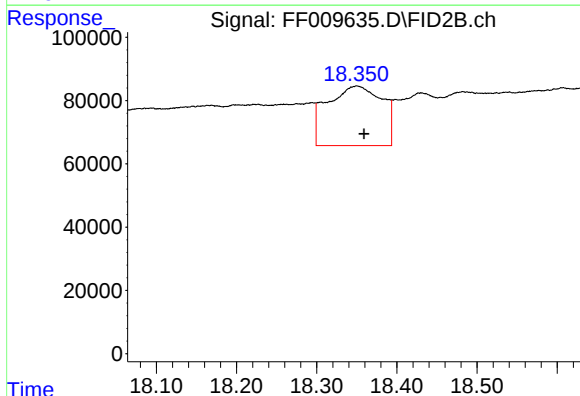


#14 N-DOTRIACONTANE

R.T.: 18.350 min
Delta R.T.: -0.009 min
Response: 894938
Conc: 8.19 ug/ml

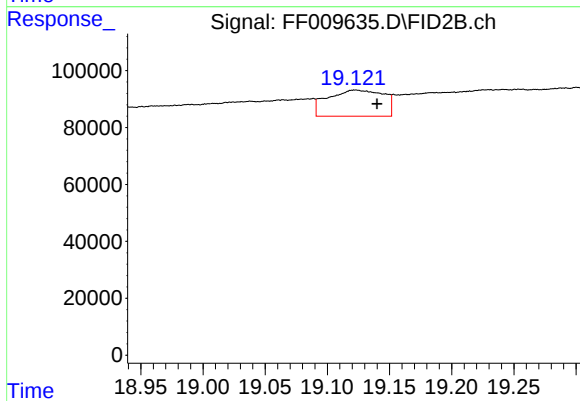

#15 N-TETRATRIACONTANE


R.T.: 19.123 min
Delta R.T.: -0.017 min
Response: 286676
Conc: 2.71 ug/ml

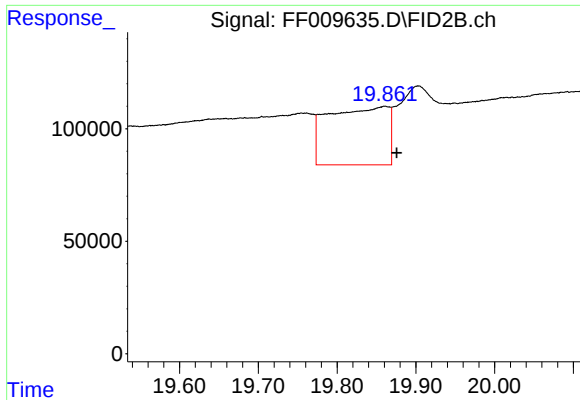

#16 N-HEXATRIACONTANE

R.T.: 19.861 min
Delta R.T.: -0.015 min
Response: 1367419
Conc: 13.65 ug/ml

Instrument :
FID_F
ClientSampleId :

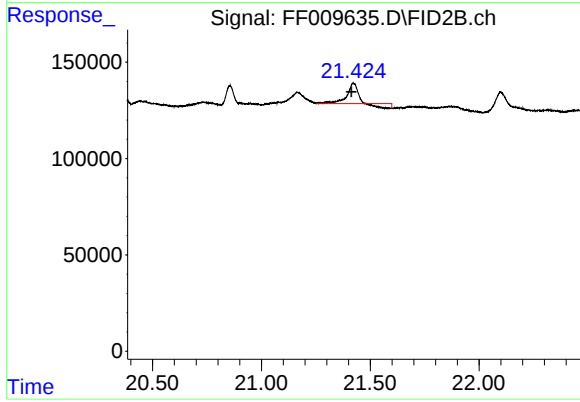

#18 N-TETRACONTANE

R.T.: 21.420 min
Delta R.T.: 0.006 min
Response: 265576
Conc: 2.63 ug/ml