

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010719\
 Data File : FF003161.D
 Signal(s) : FID2B.ch
 Acq On : 07 Jan 2019 20:03
 Operator : AJ\SJ
 Sample : K1062-05 5X
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jan 07 23:55:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Fri Jan 04 16:10:51 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.630	436158	3.281 ug/ml
Target Compounds			
3) N-DODECANE	6.382	55628	0.368 ug/ml
4) N-TETRADECANE	8.230f	64638	0.424 ug/ml
7) N-EICOSANE	12.580f	779075	5.116 ug/ml
10) N-TETRACOSANE	14.803	471148	3.162 ug/ml
12) N-OCTACOSANE	16.808	181413	1.246 ug/ml
13) N-TRIACONTANE	17.701	182365	1.277 ug/ml
14) N-DOTRIACONTANE	18.535	158243	1.188 ug/ml
15) N-TETRATRIACONTANE	19.381f	54351	0.439 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010719\
Data File : FF003161.D
Signal(s) : FID2B.ch
Acq On : 07 Jan 2019 20:03
Operator : AJ\SJ
Sample : K1062-05 5X
Misc :
ALS Vial : 64 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jan 07 23:55:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Fri Jan 04 16:10:51 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

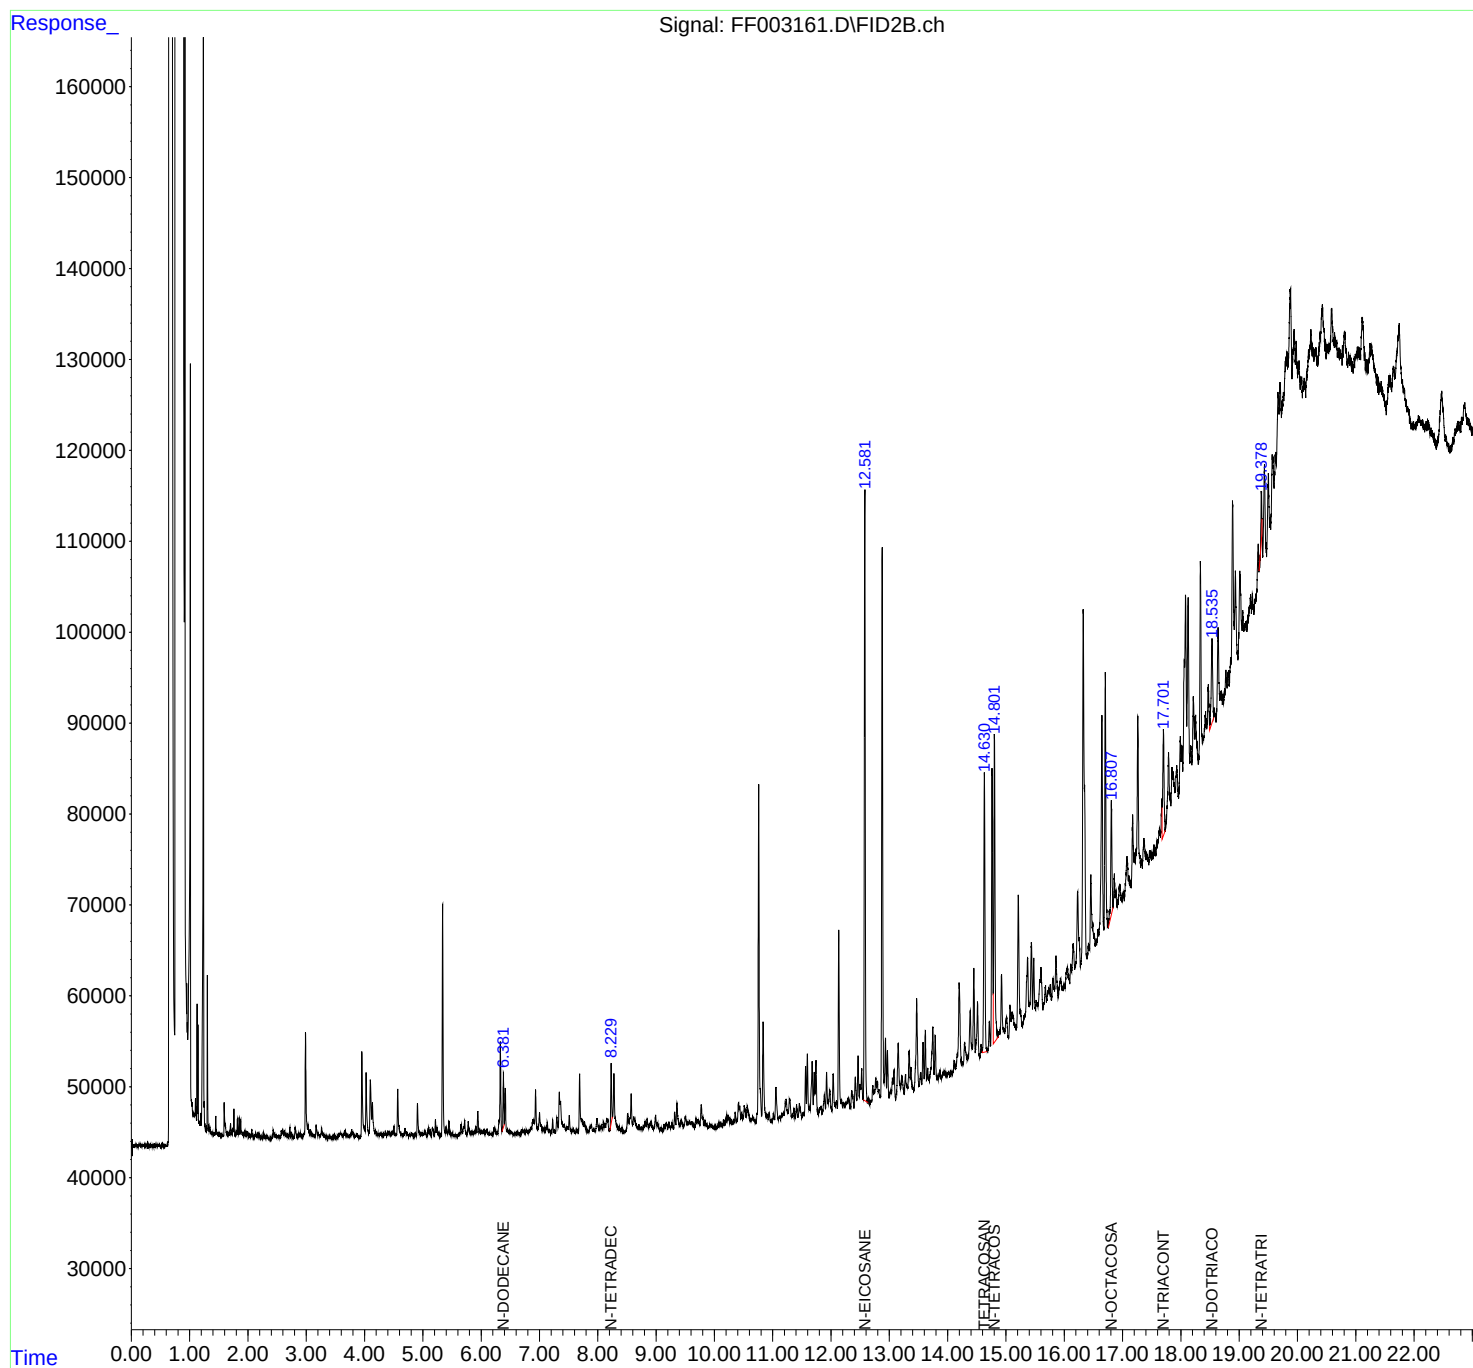

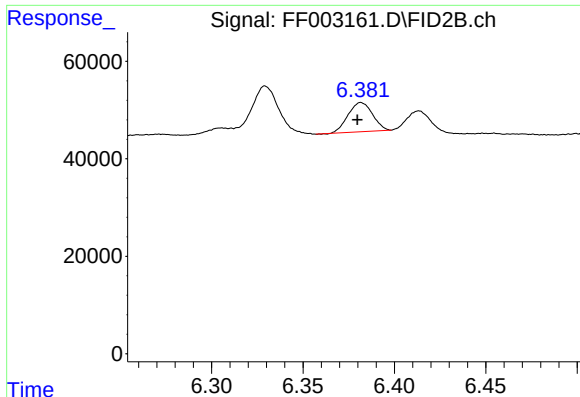


#3 N-DODECANE

R.T.: 6.382 min
Delta R.T.: 0.002 min
Response: 55628
Conc: 0.37 ug/ml

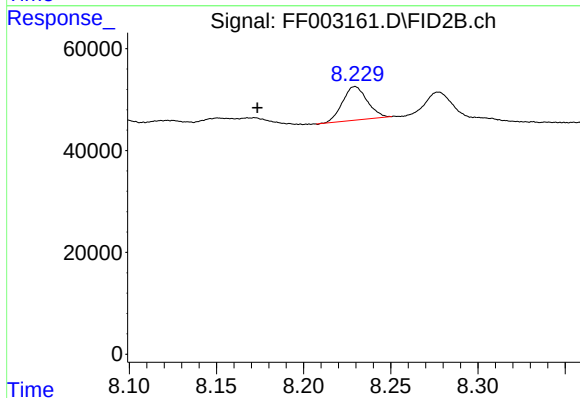


#4 N-TETRADECANE

R.T.: 8.230 min
Delta R.T.: 0.056 min
Response: 64638
Conc: 0.42 ug/ml

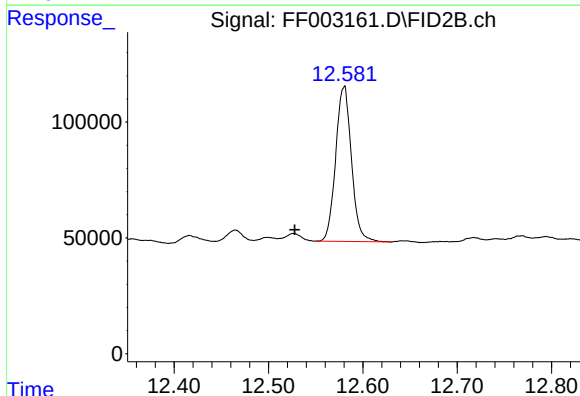


#7 N-EICOSANE

R.T.: 12.580 min
Delta R.T.: 0.052 min
Response: 779075
Conc: 5.12 ug/ml

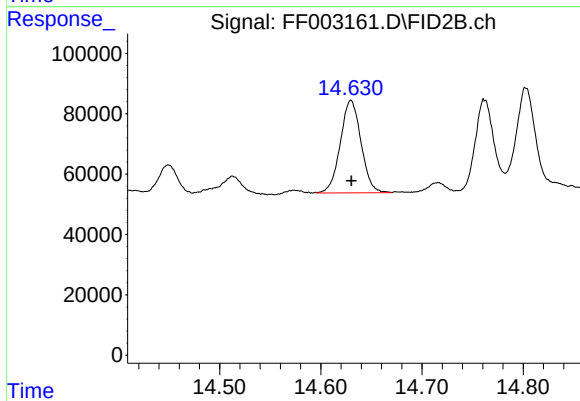


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.630 min
Delta R.T.: 0.000 min
Response: 436158
Conc: 3.28 ug/ml

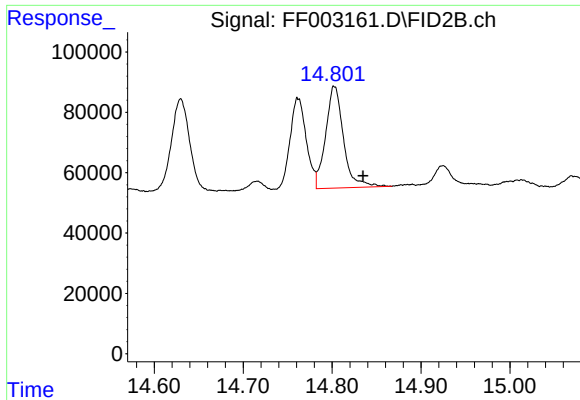


#10 N-TETRACOSANE

R.T.: 14.803 min
Delta R.T.: -0.032 min
Response: 471148
Conc: 3.16 ug/ml

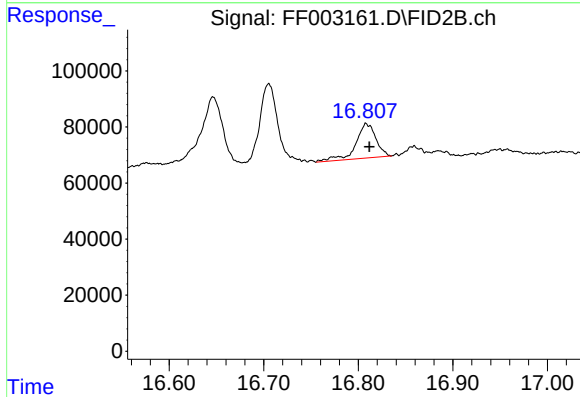


#12 N-OCTACOSANE

R.T.: 16.808 min
Delta R.T.: -0.004 min
Response: 181413
Conc: 1.25 ug/ml

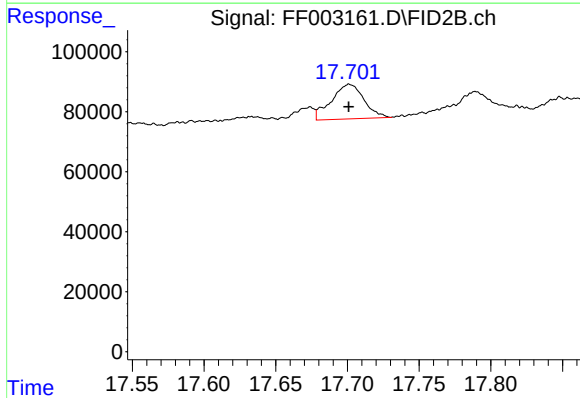


#13 N-TRIACONTANE

R.T.: 17.701 min
Delta R.T.: 0.000 min
Response: 182365
Conc: 1.28 ug/ml

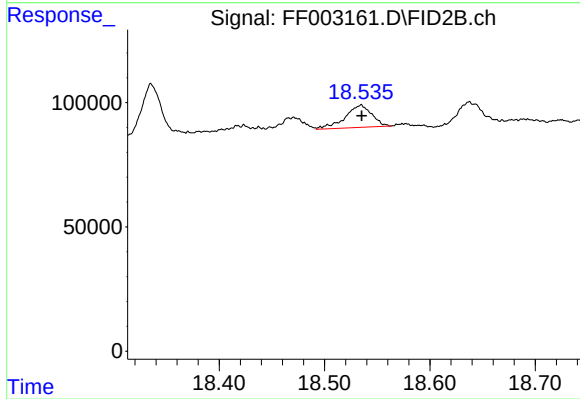

#14 N-DOTRIACONTANE

R.T.: 18.535 min
Delta R.T.: 0.000 min
Response: 158243
Conc: 1.19 ug/ml

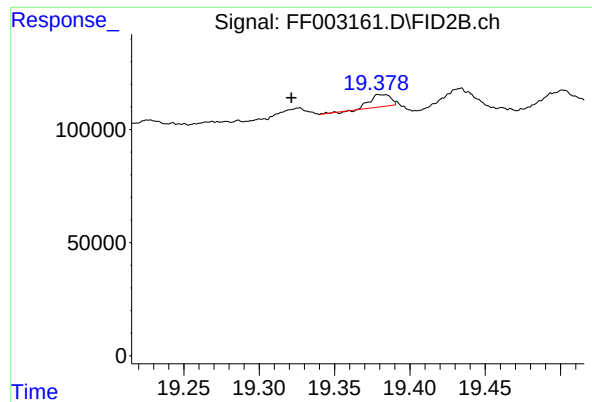

#15 N-TETRATRIACONTANE

R.T.: 19.381 min
Delta R.T.: 0.059 min
Response: 54351
Conc: 0.44 ug/ml