

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010721\
Data File : FF008071.D
Signal(s) : FID2B.ch
Acq On : 07 Jan 2021 10:26
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jan 08 00:24:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010421.M
Quant Title :
QLast Update : Tue Jan 05 12:03:34 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.418	2727872	21.219 ug/ml
12)	N-OCTACOSANE	16.853	2717926	19.881 ug/ml
14)	N-DOTRIACONTANE	18.577	110135	0.936 ug/ml
16)	N-HEXATRIACONTANE	20.148	138163	1.906 ug/ml
18)	N-TETRACONTANE	21.813	389036	6.750 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010721\
Data File : FF008071.D
Signal(s) : FID2B.ch
Acq On : 07 Jan 2021 10:26
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jan 08 00:24:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010421.M
Quant Title :
QLast Update : Tue Jan 05 12:03:34 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

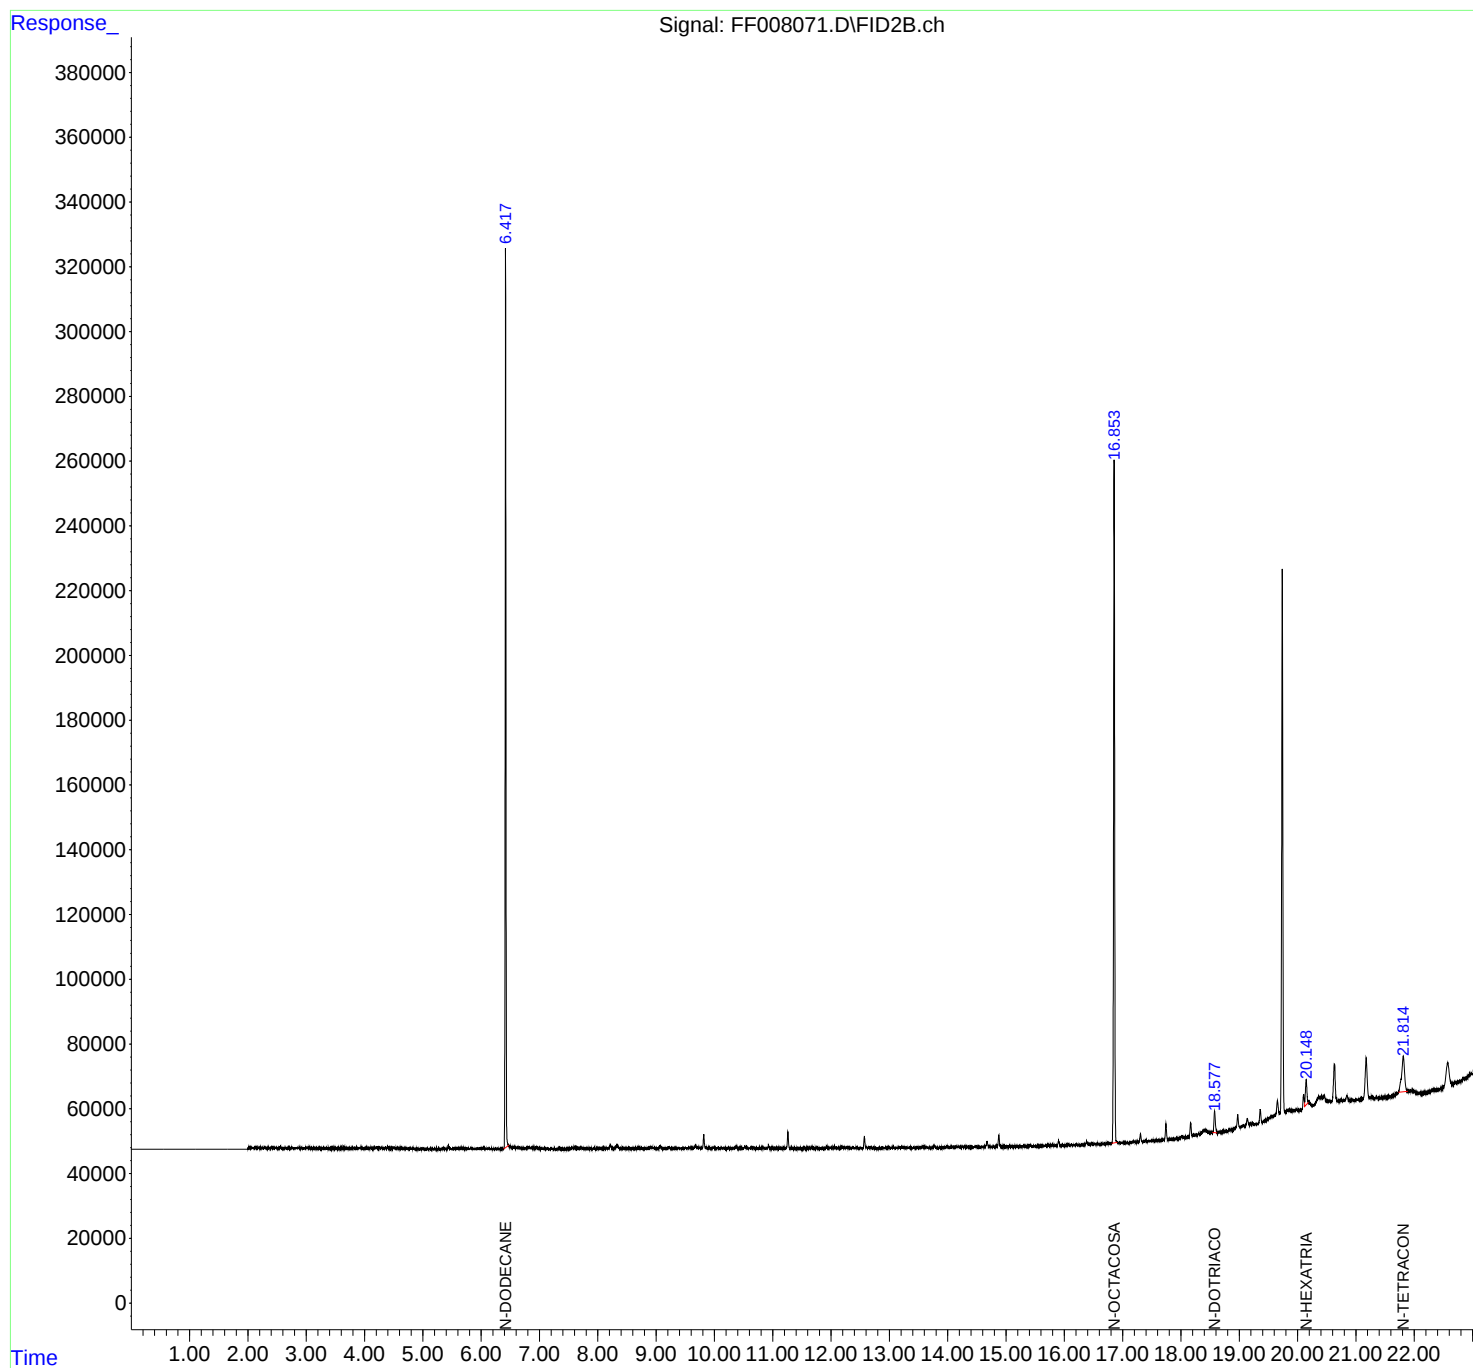

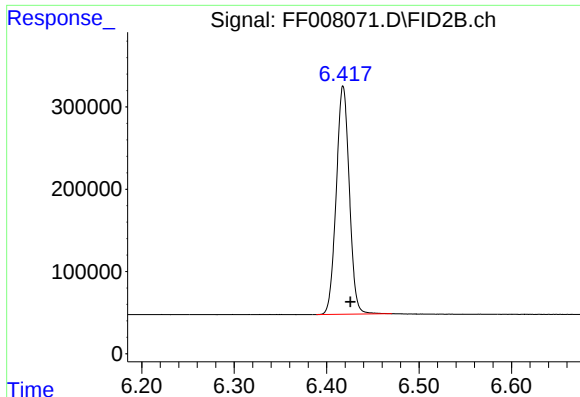


#3 N-DODECANE

R.T.: 6.418 min
Delta R.T.: -0.008 min
Response: 2727872
Conc: 21.22 ug/ml

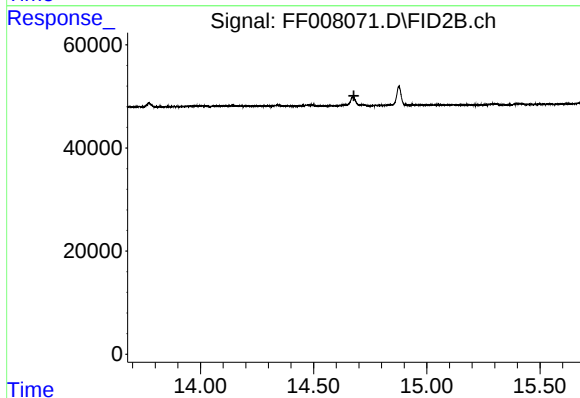


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.678 min
Response: 0
Conc: N.D.

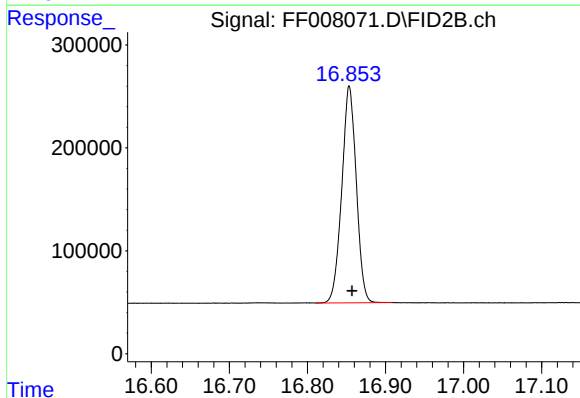


#12 N-OCTACOSANE

R.T.: 16.853 min
Delta R.T.: -0.004 min
Response: 2717926
Conc: 19.88 ug/ml

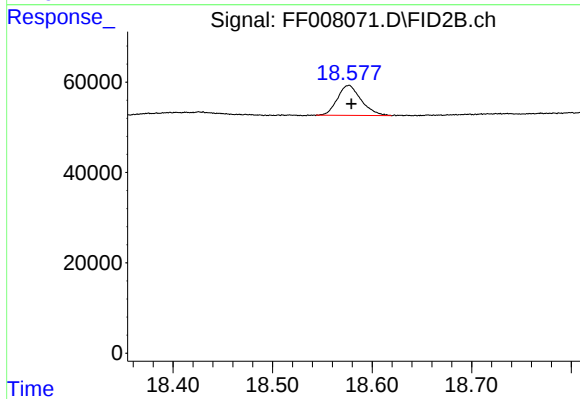


#14 N-DOTRIACONTANE

R.T.: 18.577 min
Delta R.T.: -0.002 min
Response: 110135
Conc: 0.94 ug/ml

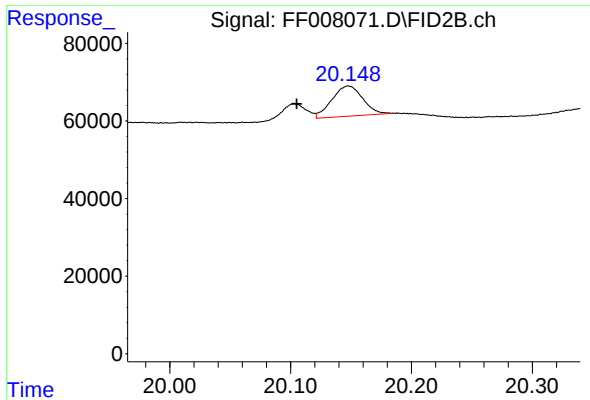

#16 N-HEXATRIACONTANE

R.T.: 20.148 min
Delta R.T.: 0.043 min
Response: 138163
Conc: 1.91 ug/ml

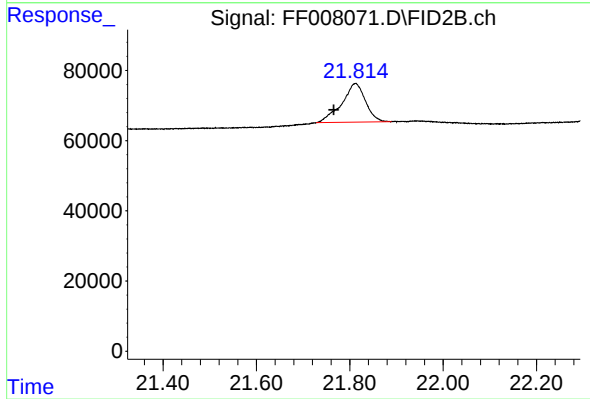

#18 N-TETRACONTANE

R.T.: 21.813 min
Delta R.T.: 0.047 min
Response: 389036
Conc: 6.75 ug/ml