

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010721\
 Data File : FF008078.D
 Signal(s) : FID2B.ch
 Acq On : 07 Jan 2021 16:49
 Operator : DD\AJ
 Sample : PB133980BS
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jan 08 00:25:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010421.M
 Quant Title :
 QLast Update : Tue Jan 05 12:03:34 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.674	3132440	25.298 ug/ml
Target Compounds			
2) N-DECANE	4.400	3237458	26.200 ug/ml
3) N-DODECANE	6.422	3399866	26.446 ug/ml
4) N-TETRADECANE	8.217	3548500	26.249 ug/ml
5) N-HEXADECANE	9.819	3614847	26.051 ug/ml
6) N-OCTADECANE	11.262	3689929	25.763 ug/ml
7) N-EICOSANE	12.573	3757256	26.033 ug/ml
8) N-DOCOSANE	13.773	3710948	26.044 ug/ml
10) N-TETRACOSANE	14.878	3603866	25.256 ug/ml
11) N-HEXACOSANE	15.901	3479834	24.884 ug/ml
12) N-OCTACOSANE	16.855	3355808	24.547 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010721\
Data File : FF008078.D
Signal(s) : FID2B.ch
Acq On : 07 Jan 2021 16:49
Operator : DD\AJ
Sample : PB133980BS
Misc :
ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jan 08 00:25:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010421.M
Quant Title :
QLast Update : Tue Jan 05 12:03:34 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

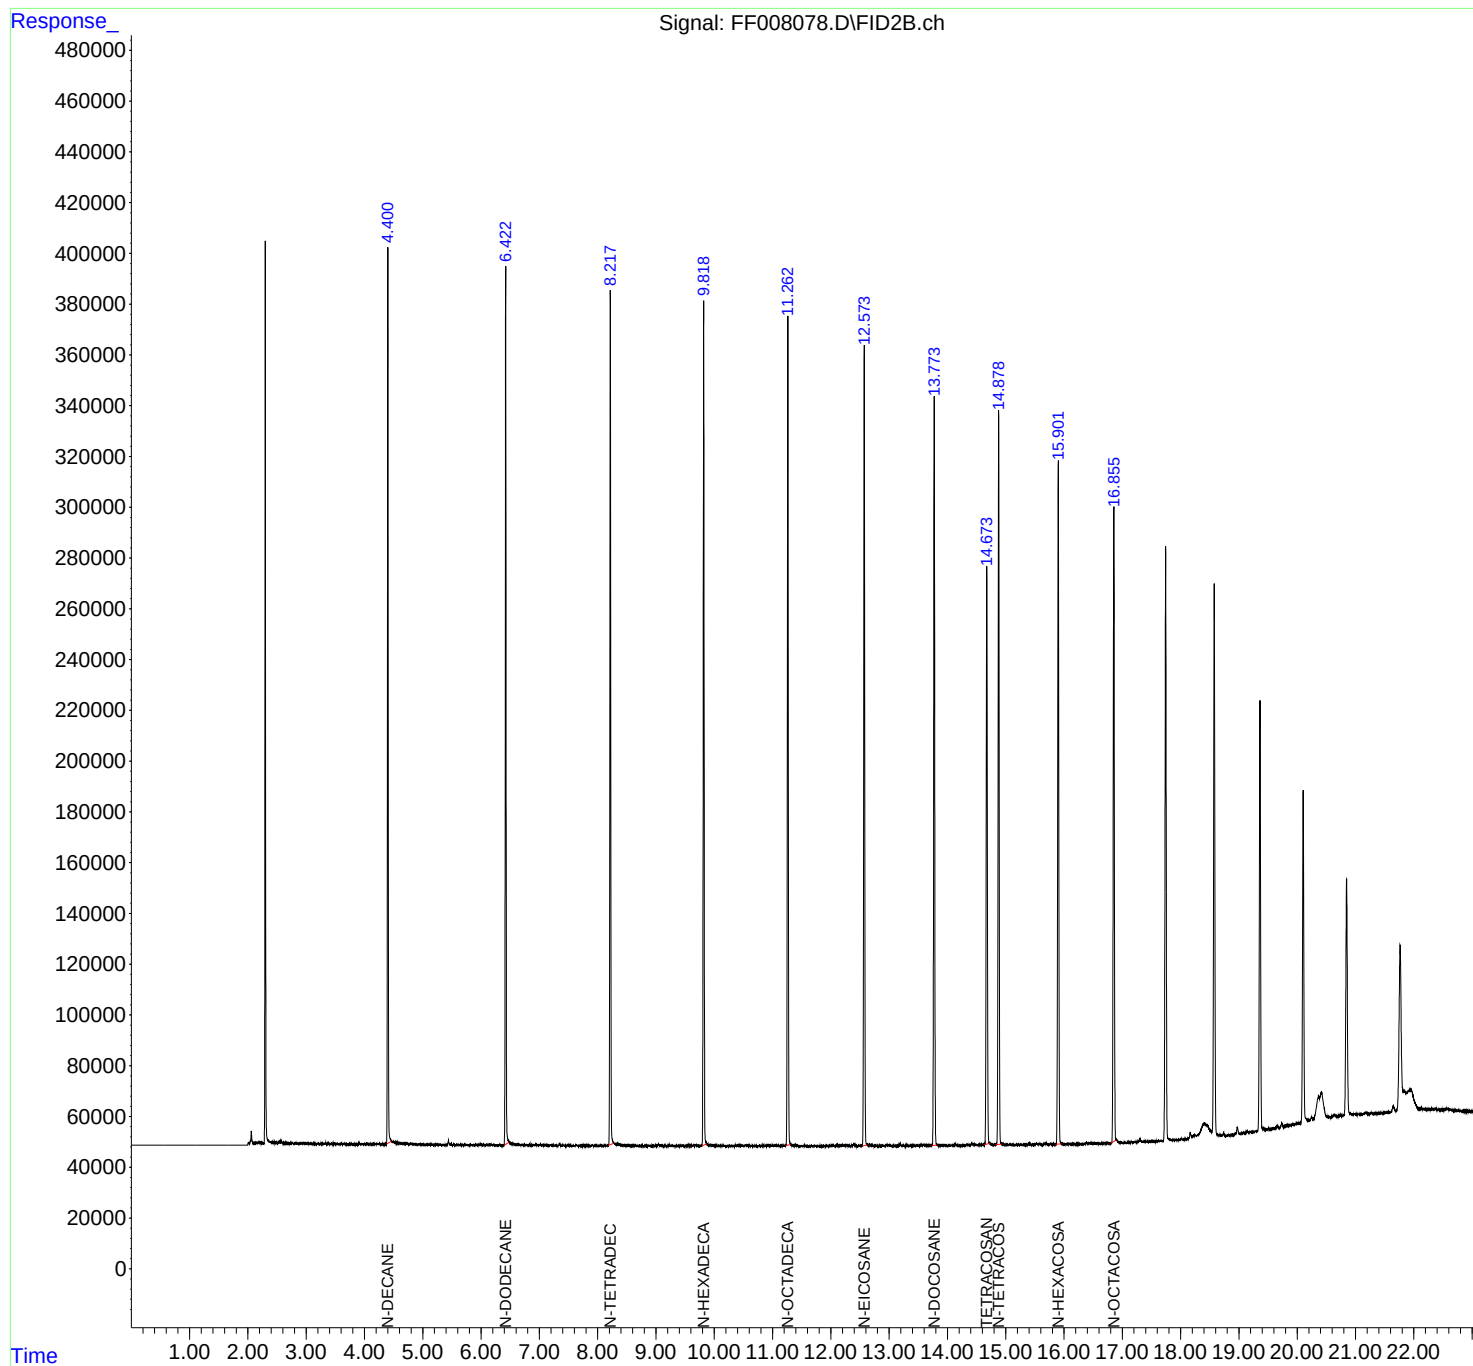

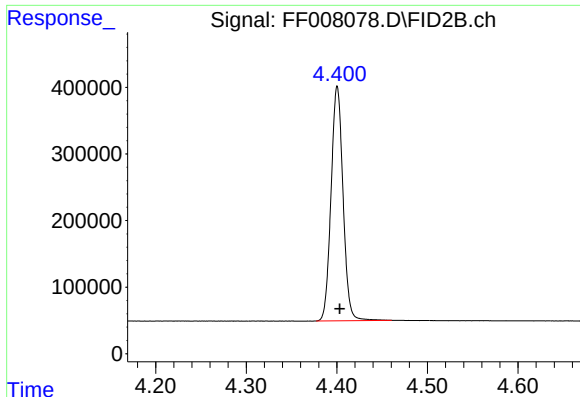


#2 N-DECANE

R.T.: 4.400 min
Delta R.T.: -0.003 min
Response: 3237458
Conc: 26.20 ug/ml

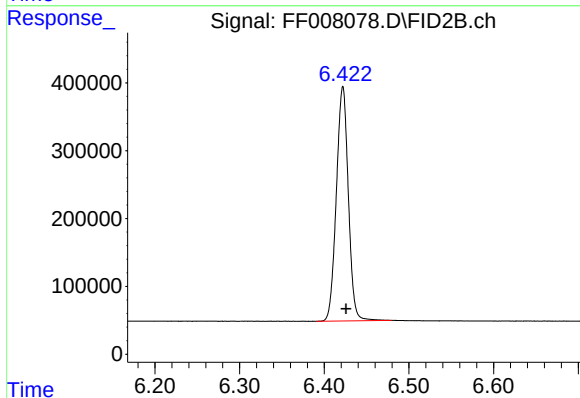


#3 N-DODECANE

R.T.: 6.422 min
Delta R.T.: -0.004 min
Response: 3399866
Conc: 26.45 ug/ml

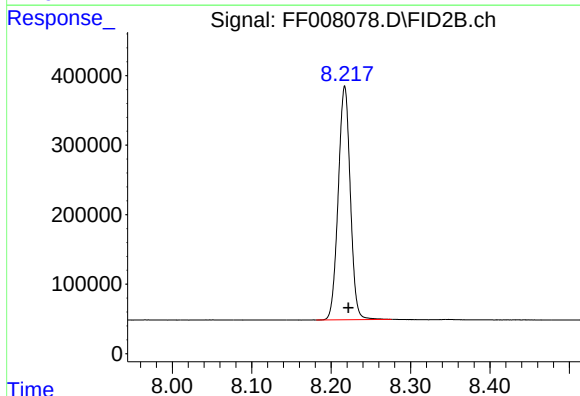


#4 N-TETRADECANE

R.T.: 8.217 min
Delta R.T.: -0.005 min
Response: 3548500
Conc: 26.25 ug/ml

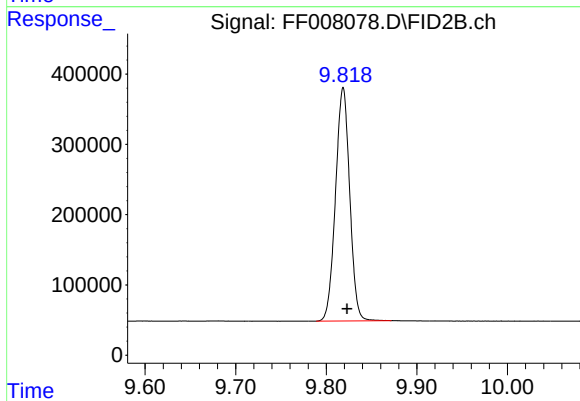


#5 N-HEXADECANE

R.T.: 9.819 min
Delta R.T.: -0.004 min
Response: 3614847
Conc: 26.05 ug/ml

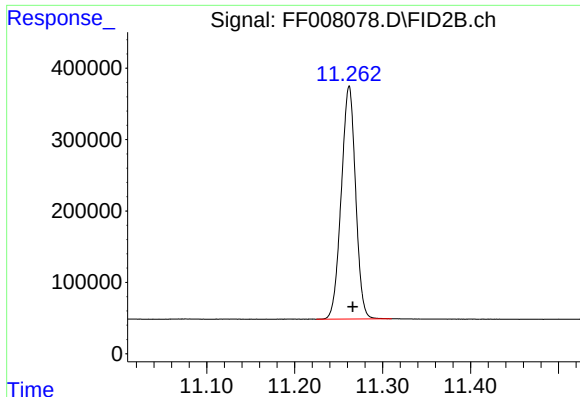


#6 N-OCTADECANE

R.T.: 11.262 min
Delta R.T.: -0.004 min
Response: 3689929
Conc: 25.76 ug/ml

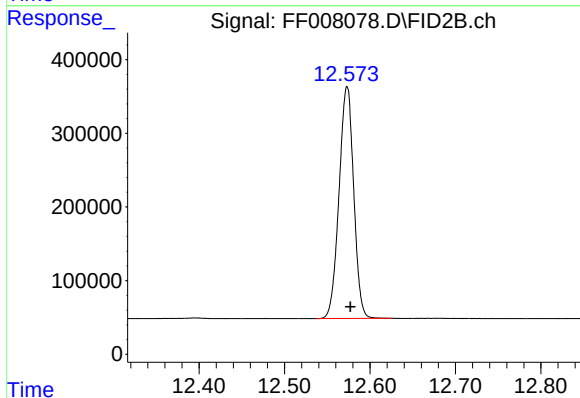


#7 N-EICOSANE

R.T.: 12.573 min
Delta R.T.: -0.004 min
Response: 3757256
Conc: 26.03 ug/ml

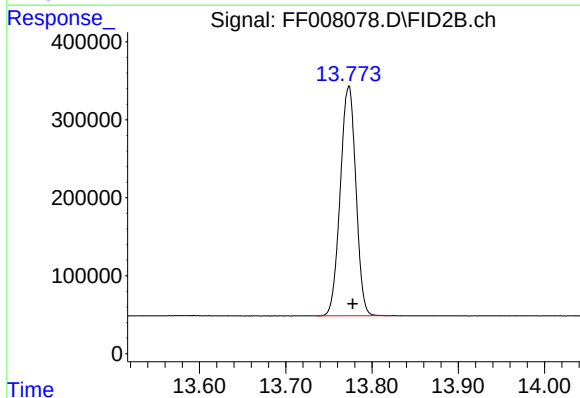


#8 N-DOCOSANE

R.T.: 13.773 min
Delta R.T.: -0.004 min
Response: 3710948
Conc: 26.04 ug/ml

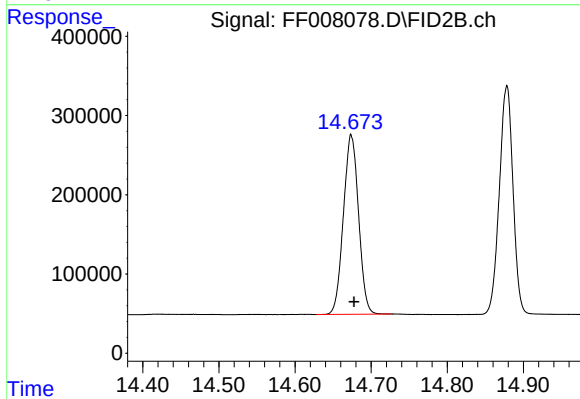


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.674 min
Delta R.T.: -0.004 min
Response: 3132440
Conc: 25.30 ug/ml

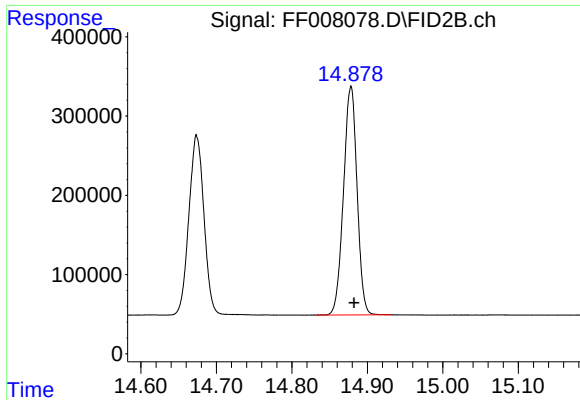


#10 N-TETRACOSANE

R.T.: 14.878 min
Delta R.T.: -0.004 min
Response: 3603866
Conc: 25.26 ug/ml

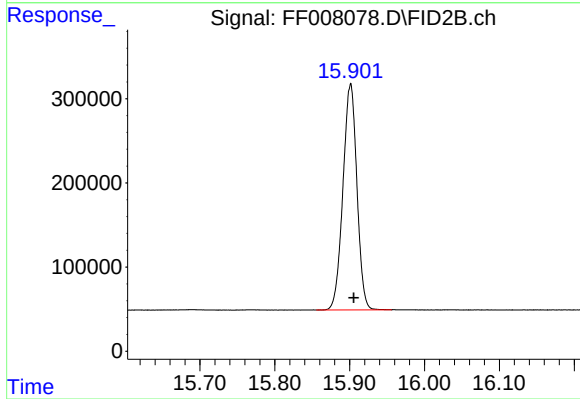

#11 N-HEXACOSANE

R.T.: 15.901 min
Delta R.T.: -0.004 min
Response: 3479834
Conc: 24.88 ug/ml

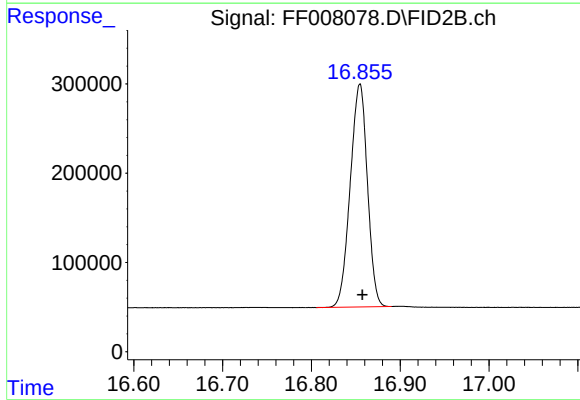

#12 N-OCTACOSANE

R.T.: 16.855 min
Delta R.T.: -0.003 min
Response: 3355808
Conc: 24.55 ug/ml