

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011019\
 Data File : FF003195.D
 Signal(s) : FID2B.ch
 Acq On : 10 Jan 2019 13:13
 Operator : AJ\SJ
 Sample : K1006-07 5X
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 11 01:06:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Fri Jan 04 16:10:51 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.612	242456	1.824 ug/ml
Target Compounds			
4) N-TETRADECANE	8.217	143852	0.944 ug/ml
12) N-OCTACOSANE	16.794	207103	1.423 ug/ml
13) N-TRIACONTANE	17.684	530840	3.717 ug/ml
14) N-DOTRIACONTANE	18.521	688746	5.169 ug/ml
15) N-TETRATRIACONTANE	19.307	439597	3.547 ug/ml
16) N-HEXATRIACONTANE	20.053	214217	1.899 ug/ml
17) N-OCTATRIACONTANE	20.790	192296	1.919 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011019\
Data File : FF003195.D
Signal(s) : FID2B.ch
Acq On : 10 Jan 2019 13:13
Operator : AJ\SJ
Sample : K1006-07 5X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 11 01:06:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Fri Jan 04 16:10:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

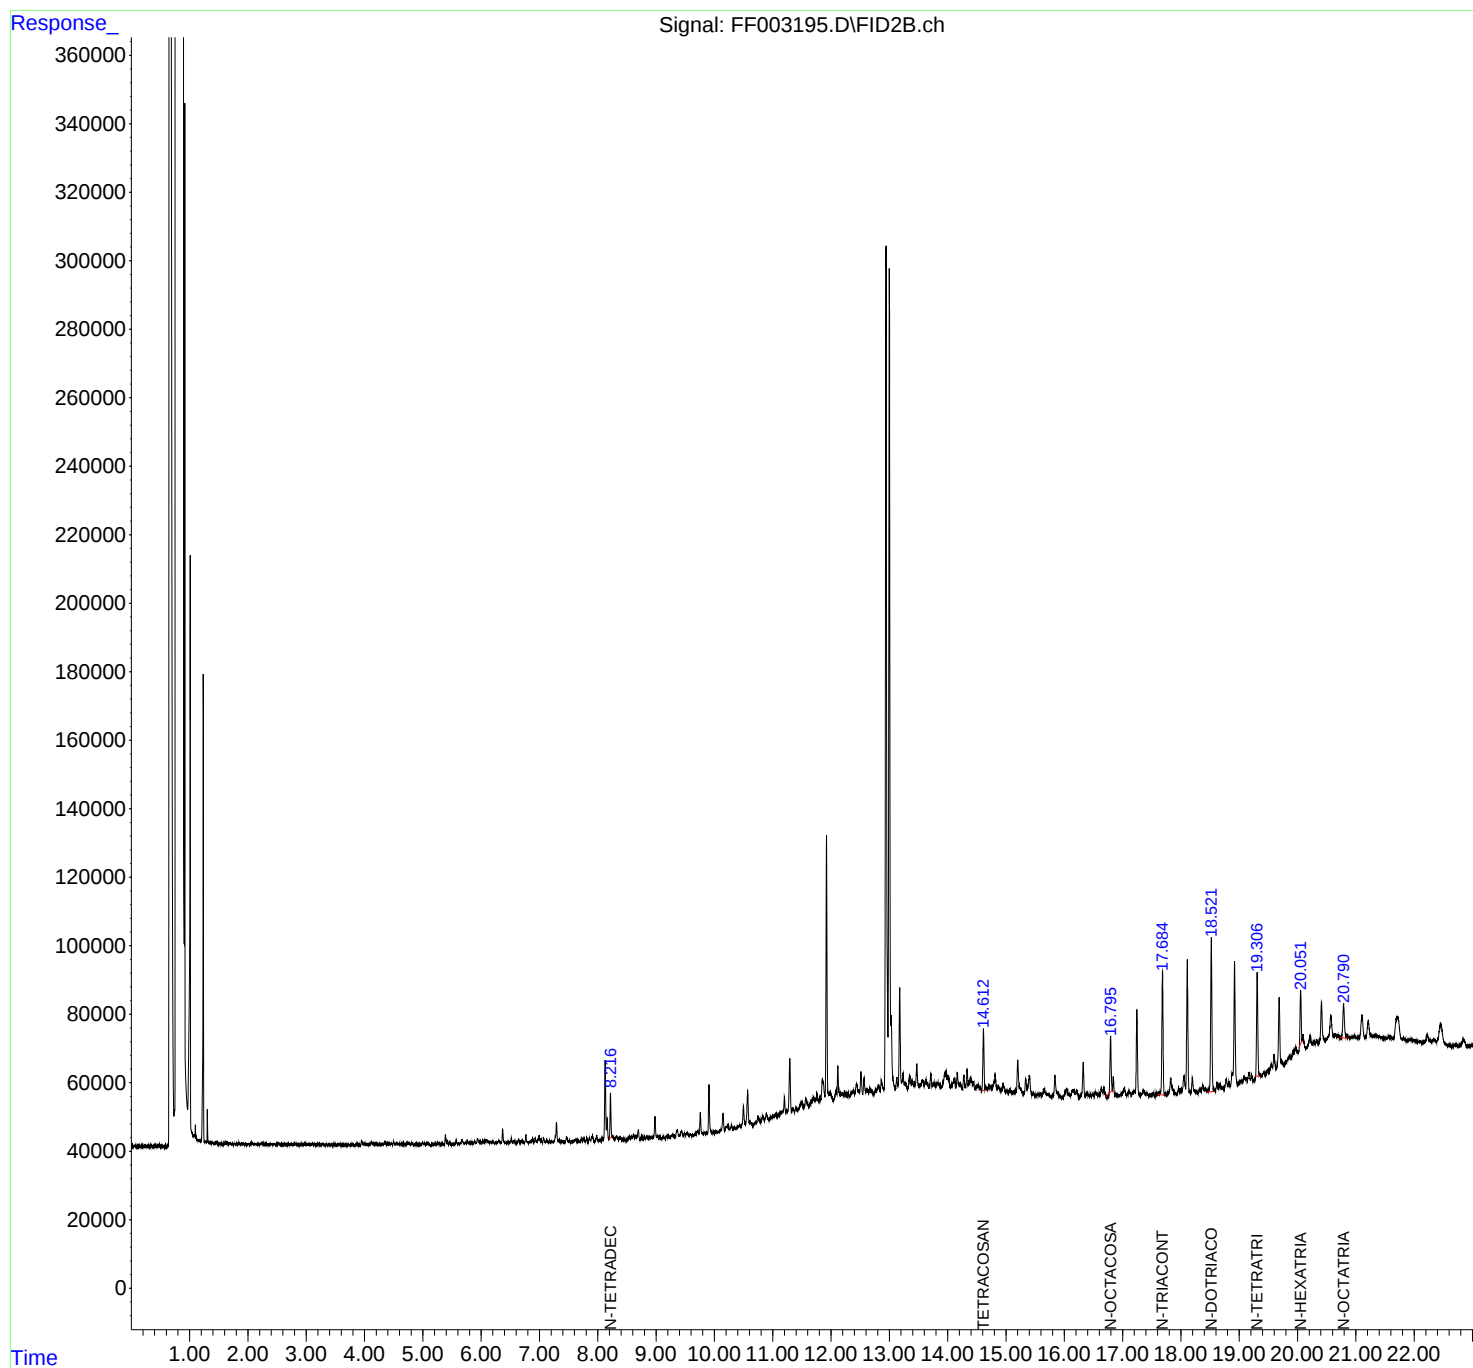


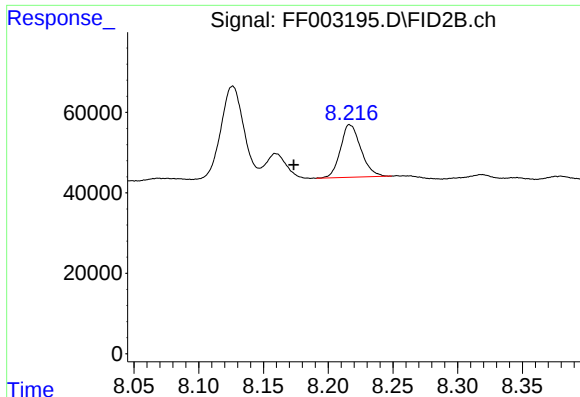

#4 N-TETRADECANE


R.T.: 8.217 min
Delta R.T.: 0.043 min
Response: 143852
Conc: 0.94 ug/ml

Instrument :
FID_F
ClientSampleId :

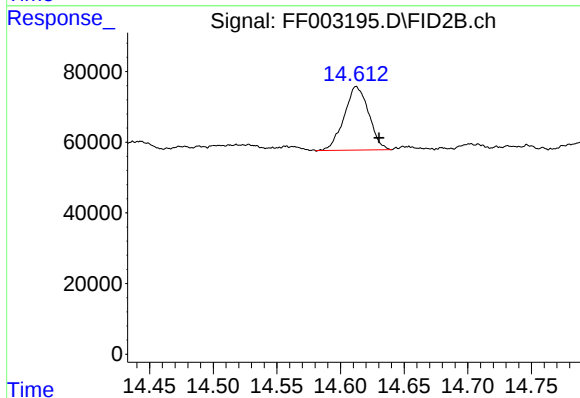


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.612 min
Delta R.T.: -0.018 min
Response: 242456
Conc: 1.82 ug/ml

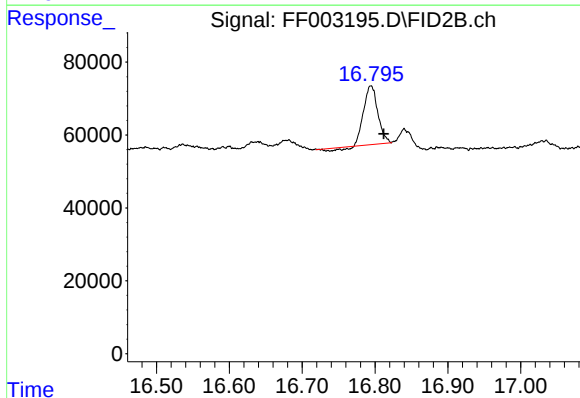


#12 N-OCTACOSANE

R.T.: 16.794 min
Delta R.T.: -0.018 min
Response: 207103
Conc: 1.42 ug/ml

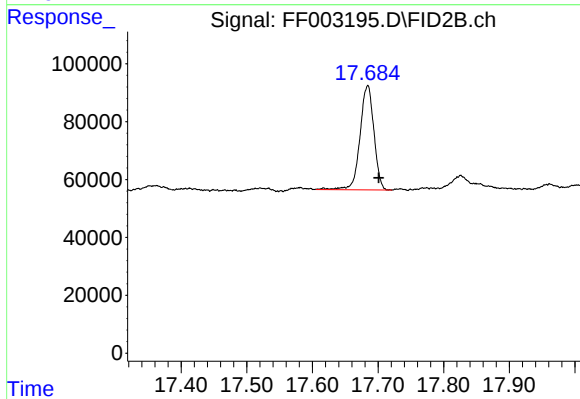

#13 N-TRIACONTANE


R.T.: 17.684 min
Delta R.T.: -0.016 min
Response: 530840
Conc: 3.72 ug/ml

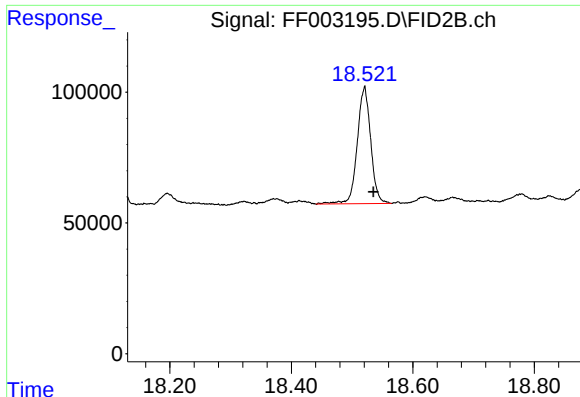

#14 N-DOTRIACONTANE


R.T.: 18.521 min
Delta R.T.: -0.015 min
Response: 688746
Conc: 5.17 ug/ml

Instrument :
FID_F
ClientSampleId :

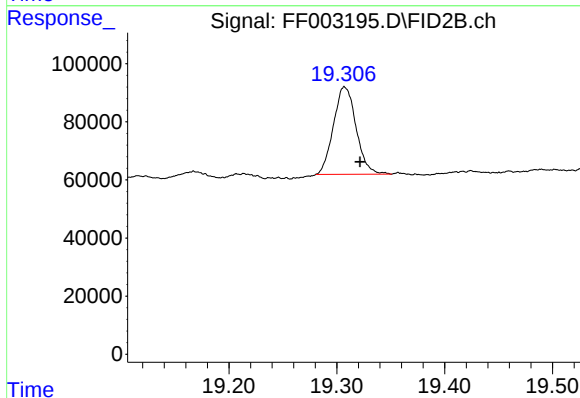


#15 N-TETRATRIACONTANE

R.T.: 19.307 min
Delta R.T.: -0.014 min
Response: 439597
Conc: 3.55 ug/ml

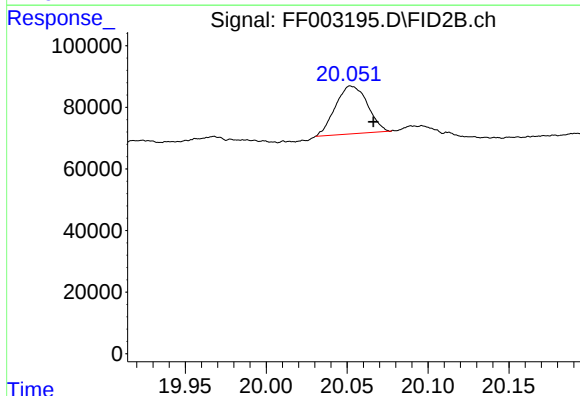

#16 N-HEXATRIACONTANE

R.T.: 20.053 min
Delta R.T.: -0.014 min
Response: 214217
Conc: 1.90 ug/ml

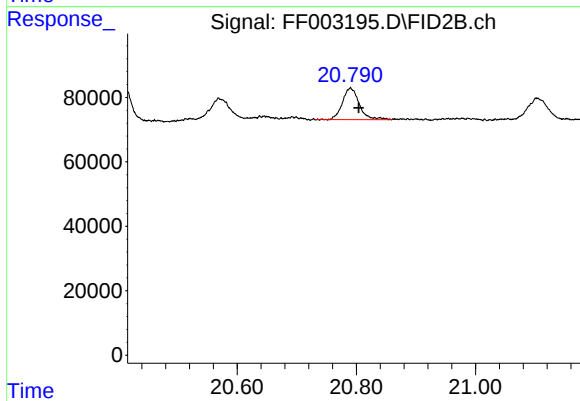

#17 N-OCTATRIACONTANE

R.T.: 20.790 min
Delta R.T.: -0.014 min
Response: 192296
Conc: 1.92 ug/ml